
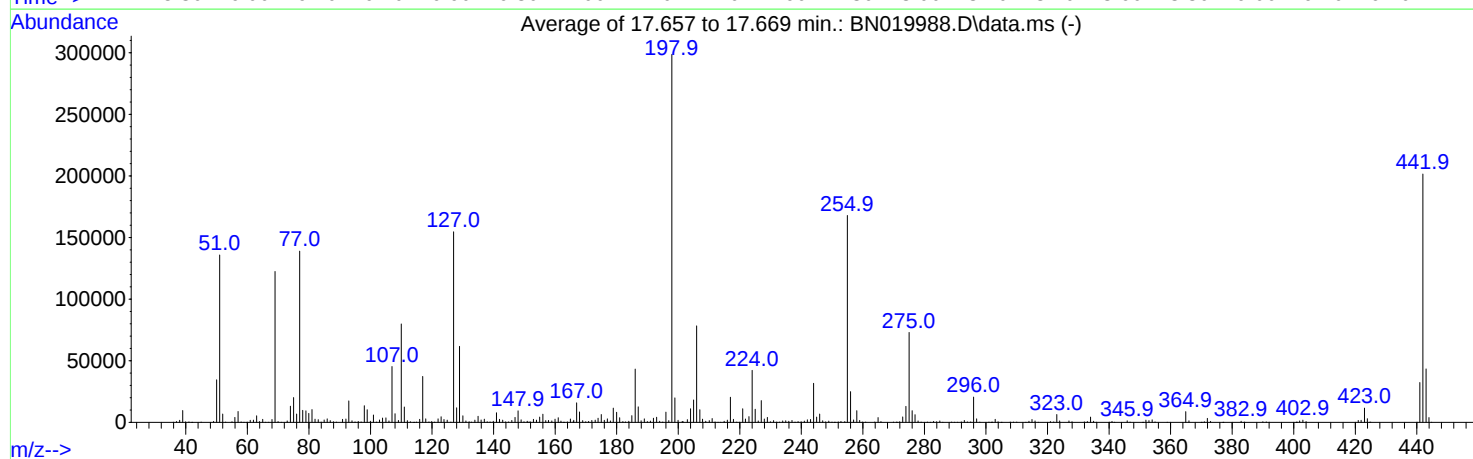


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052722\
 Data File : BN019988.D
 Acq On : 27 May 2022 13:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 18 07:42:52 2022

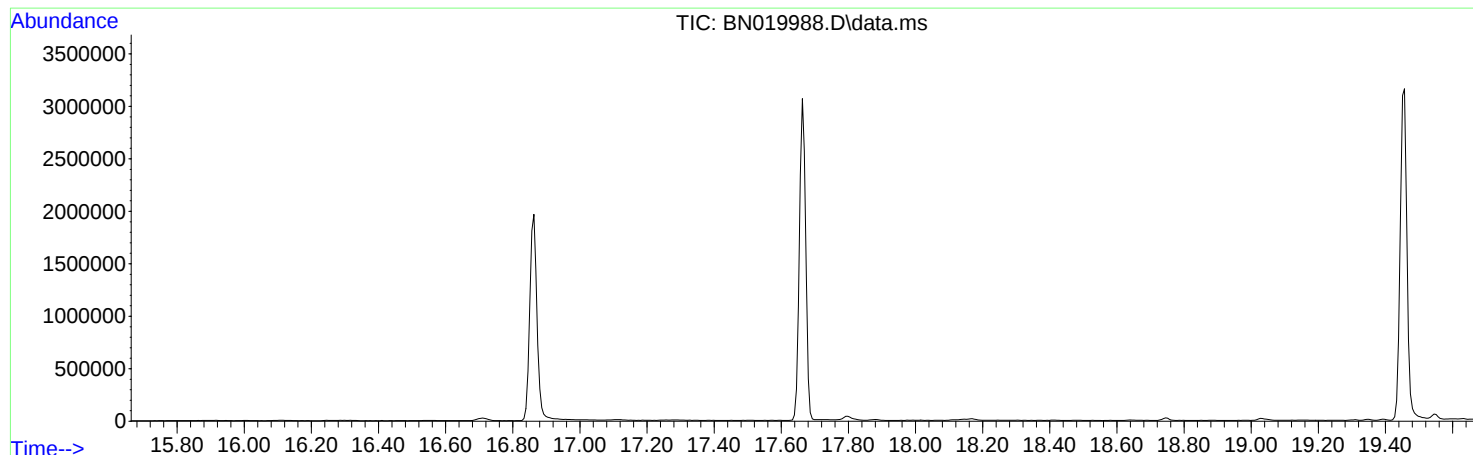




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	135856	PASS
68	69	0.00	2	2.0	2404	PASS
69	198	0.00	100	41.0	122464	PASS
70	69	0.00	2	0.5	602	PASS
127	198	10	80	51.8	154731	PASS
197	198	0.00	2	0.5	1467	PASS
198	198	100	100	100.0	298603	PASS
199	198	5	9	6.7	19867	PASS
275	198	10	60	24.4	72944	PASS
365	198	1	100	2.9	8768	PASS
441	198	0.01	100	10.9	32413	PASS
442	442	50	100	100.0	201579	PASS
443	442	15	24	21.5	43347	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052722\
Data File : BN019988.D
Acq On : 27 May 2022 13:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 28 06:20:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

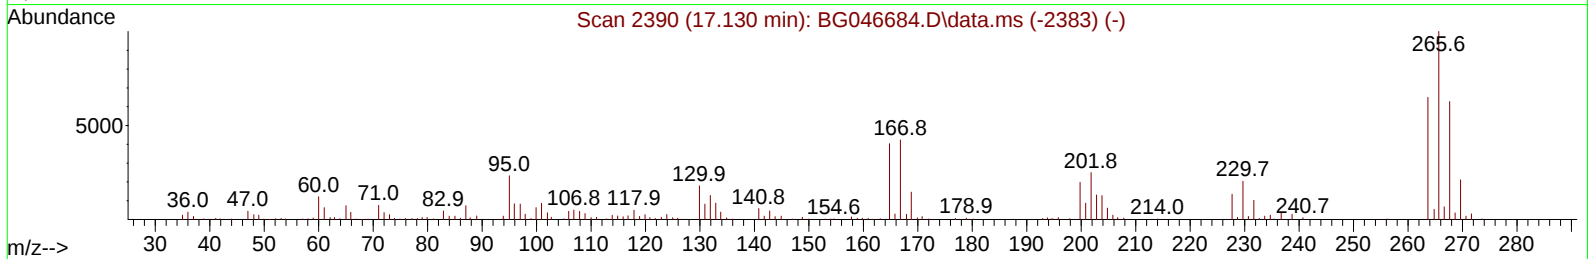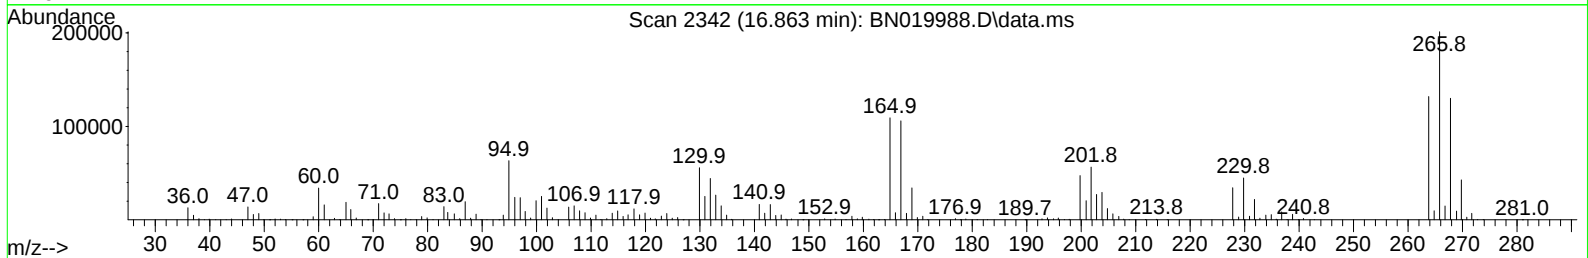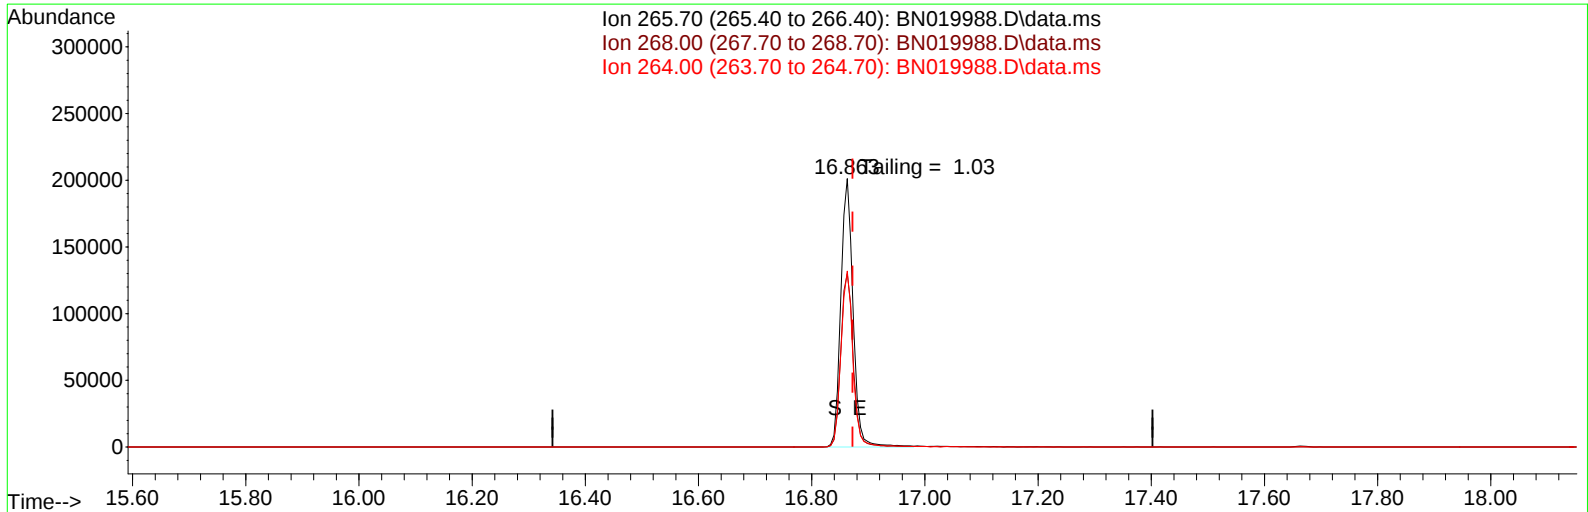

TIC: BN019988.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 19150.43 ng




response 303431

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.64
264.00	61.60	65.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052722\
 Data File : BN019988.D
 Acq On : 27 May 2022 13:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: May 28 06:20:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

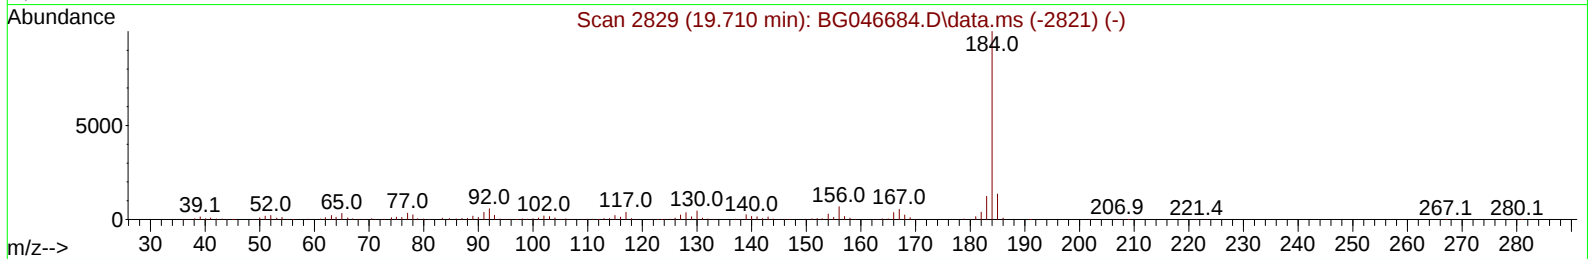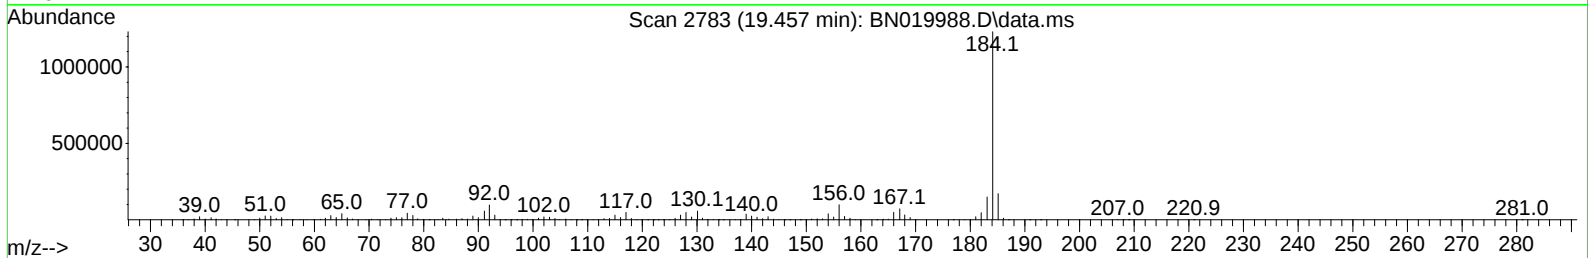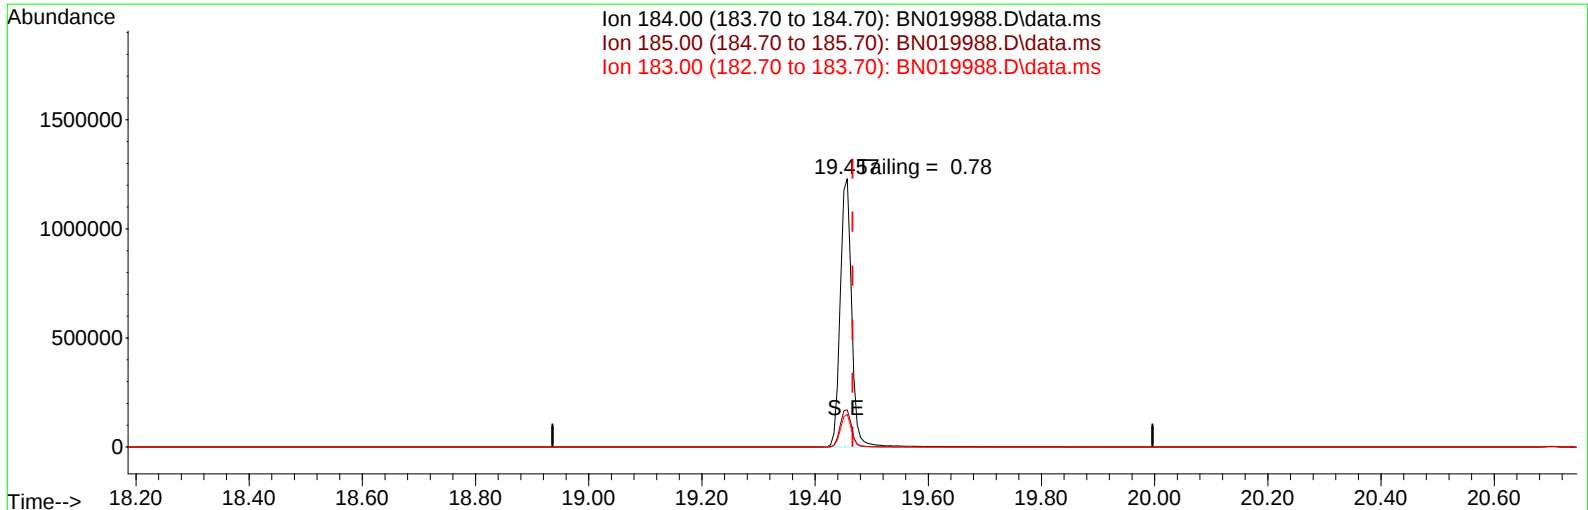

TIC: BN019988.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 1740982

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.86
183.00	13.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/27/2022	BNA_N	<u>BN019988.D</u>
Compound Name	Response	Retention Time
DDT	834289	20.704
DDD	130524	20.257
DDE	9419	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
139943	974232	14.36

Instrument :
BNA_N
ClientSampleId :
DFTPP