
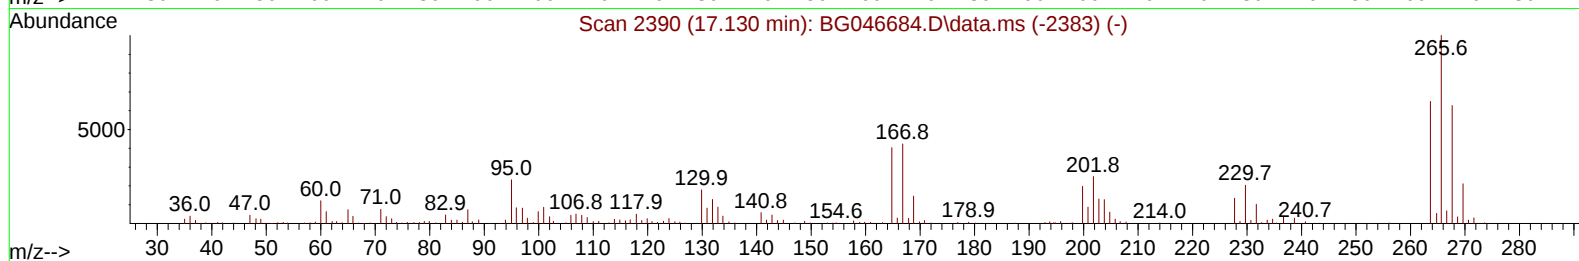
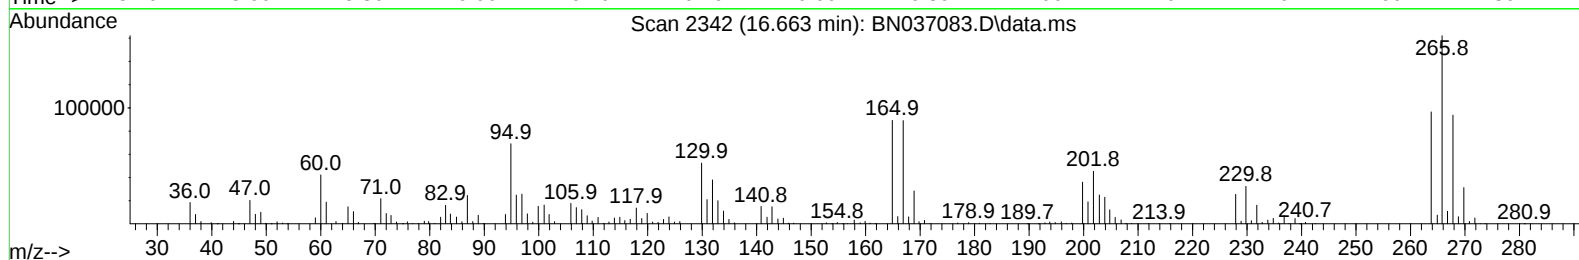


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052725\  
Data File : BN037083.D  
Acq On : 27 May 2025 12:38  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 15:00:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 27 07:40:28 2025  
Response via : Initial Calibration

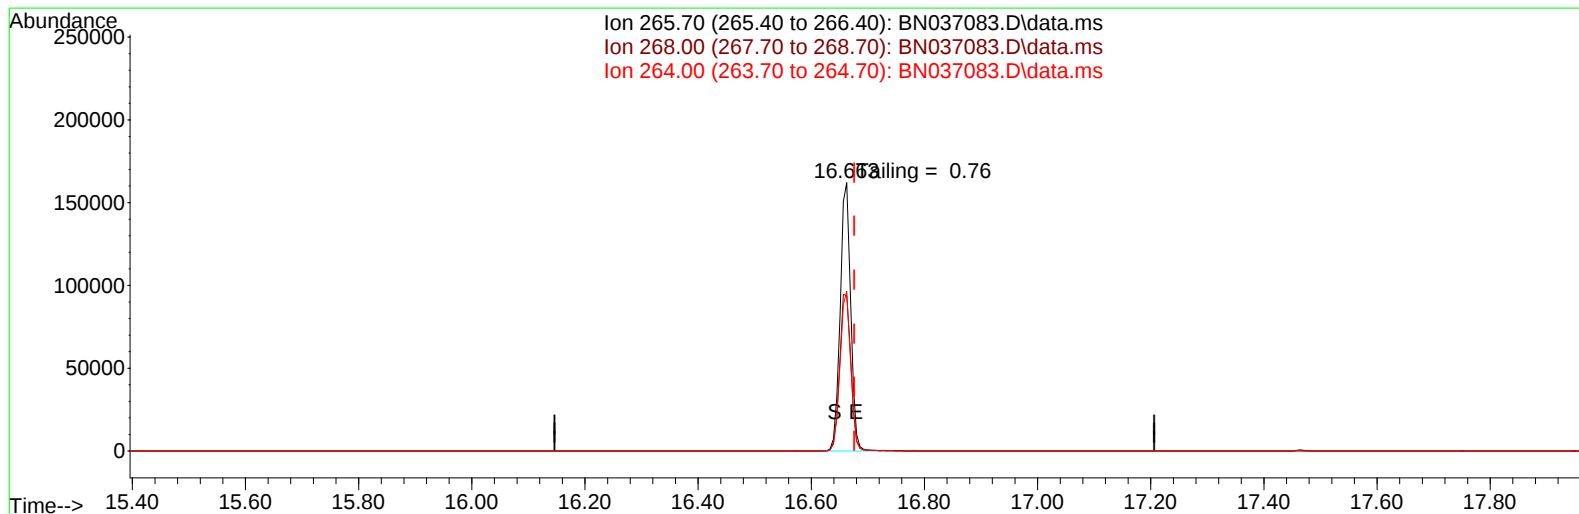

TIC: BN037083.D\data.ms

**(70) Pentachlorophenol (C)**




16.663min (-0.013) 16887.97 ng

response 209799

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 57.82  |
| 264.00 | 61.60  | 59.57  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN052725\  
Data File : BN037083.D  
Acq On : 27 May 2025 12:38  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 15:00:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 27 07:40:28 2025  
Response via : Initial Calibration

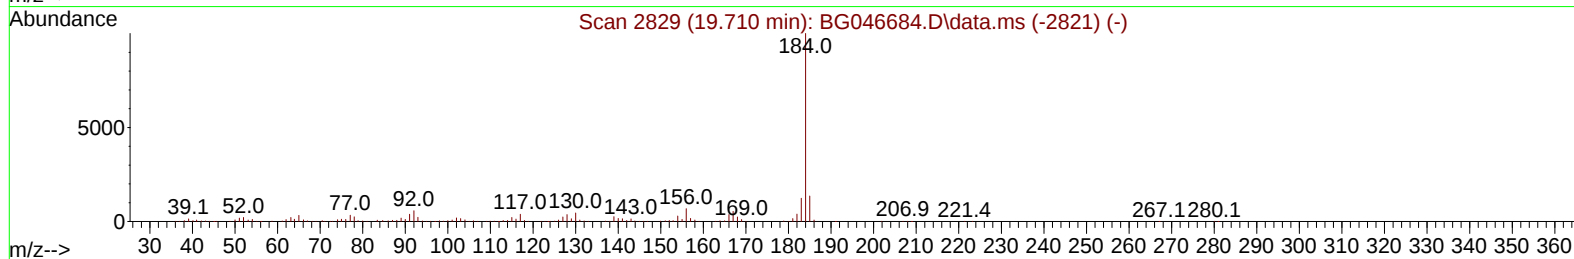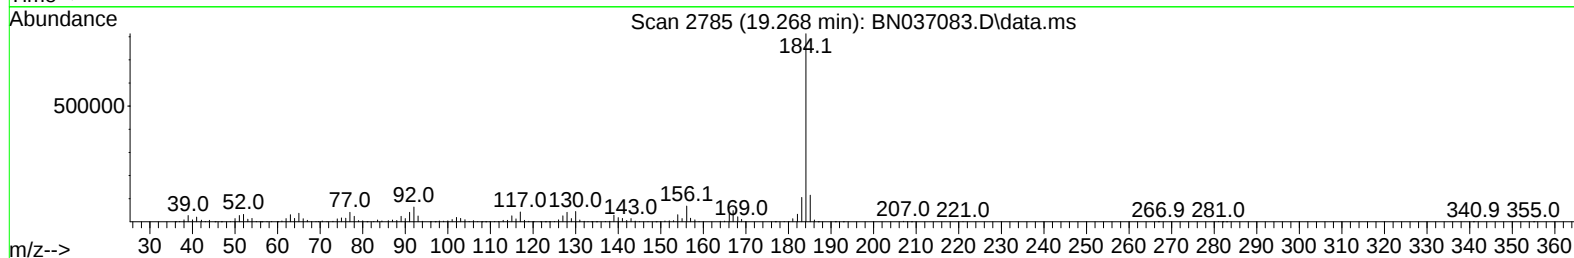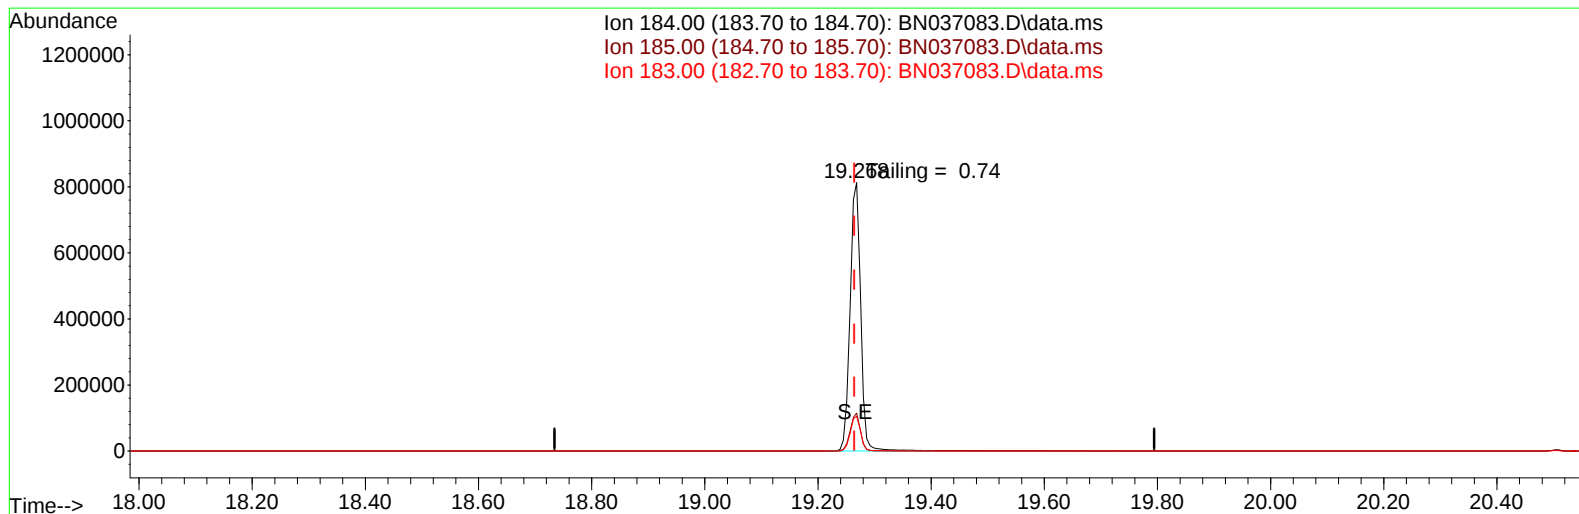

TIC: BN037083.D\data.ms

**(77) Benzidine****19.268min (+ 0.004) 0.00 ng****response 1062455**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.17  |
| 183.00 | 13.20  | 12.96  |
| 0.00   | 0.00   | 0.00   |