

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052819\
 Data File : BN005916.D
 Acq On : 29 May 2019 04:00
 Operator : JU/SJ
 Sample : K2692-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 29 05:16:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 29 02:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	606373	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	2798858	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	1617243	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	3411744	20.00	ng/ul	0.00
77) Chrysene-d12	21.32	240	2603475	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	2326934	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	41718	3.03	ng/uL	0.00
5) Phenol-d5	6.89	99	783921	14.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	511694	16.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	635050	15.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	307579	7.09	ng/ul	0.00
19) Nitrobenzene-d5	8.96	128	366	0.02	ng/ul	0.08
22) 2-Nitrophenol-d4	9.60	143	323976	19.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	596158	15.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	690148	13.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	2092692	17.55	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	2547239	17.08	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	295829	13.63	ng/ul	0.00
57) Fluorene-d10	15.36	176	1759751	17.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	154403	11.10	ng/ul	0.00
70) Anthracene-d10	17.22	188	2324042	16.01	ng/ul	0.00
78) Pyrene-d10	19.52	212	2674207	20.34	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.44	264	1783718	17.18	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	736414	6.180	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052819\
Data File : BN005916.D
Acq On : 29 May 2019 04:00
Operator : JU/SJ
Sample : K2692-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 29 05:16:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 29 02:28:30 2019
Response via : Initial Calibration

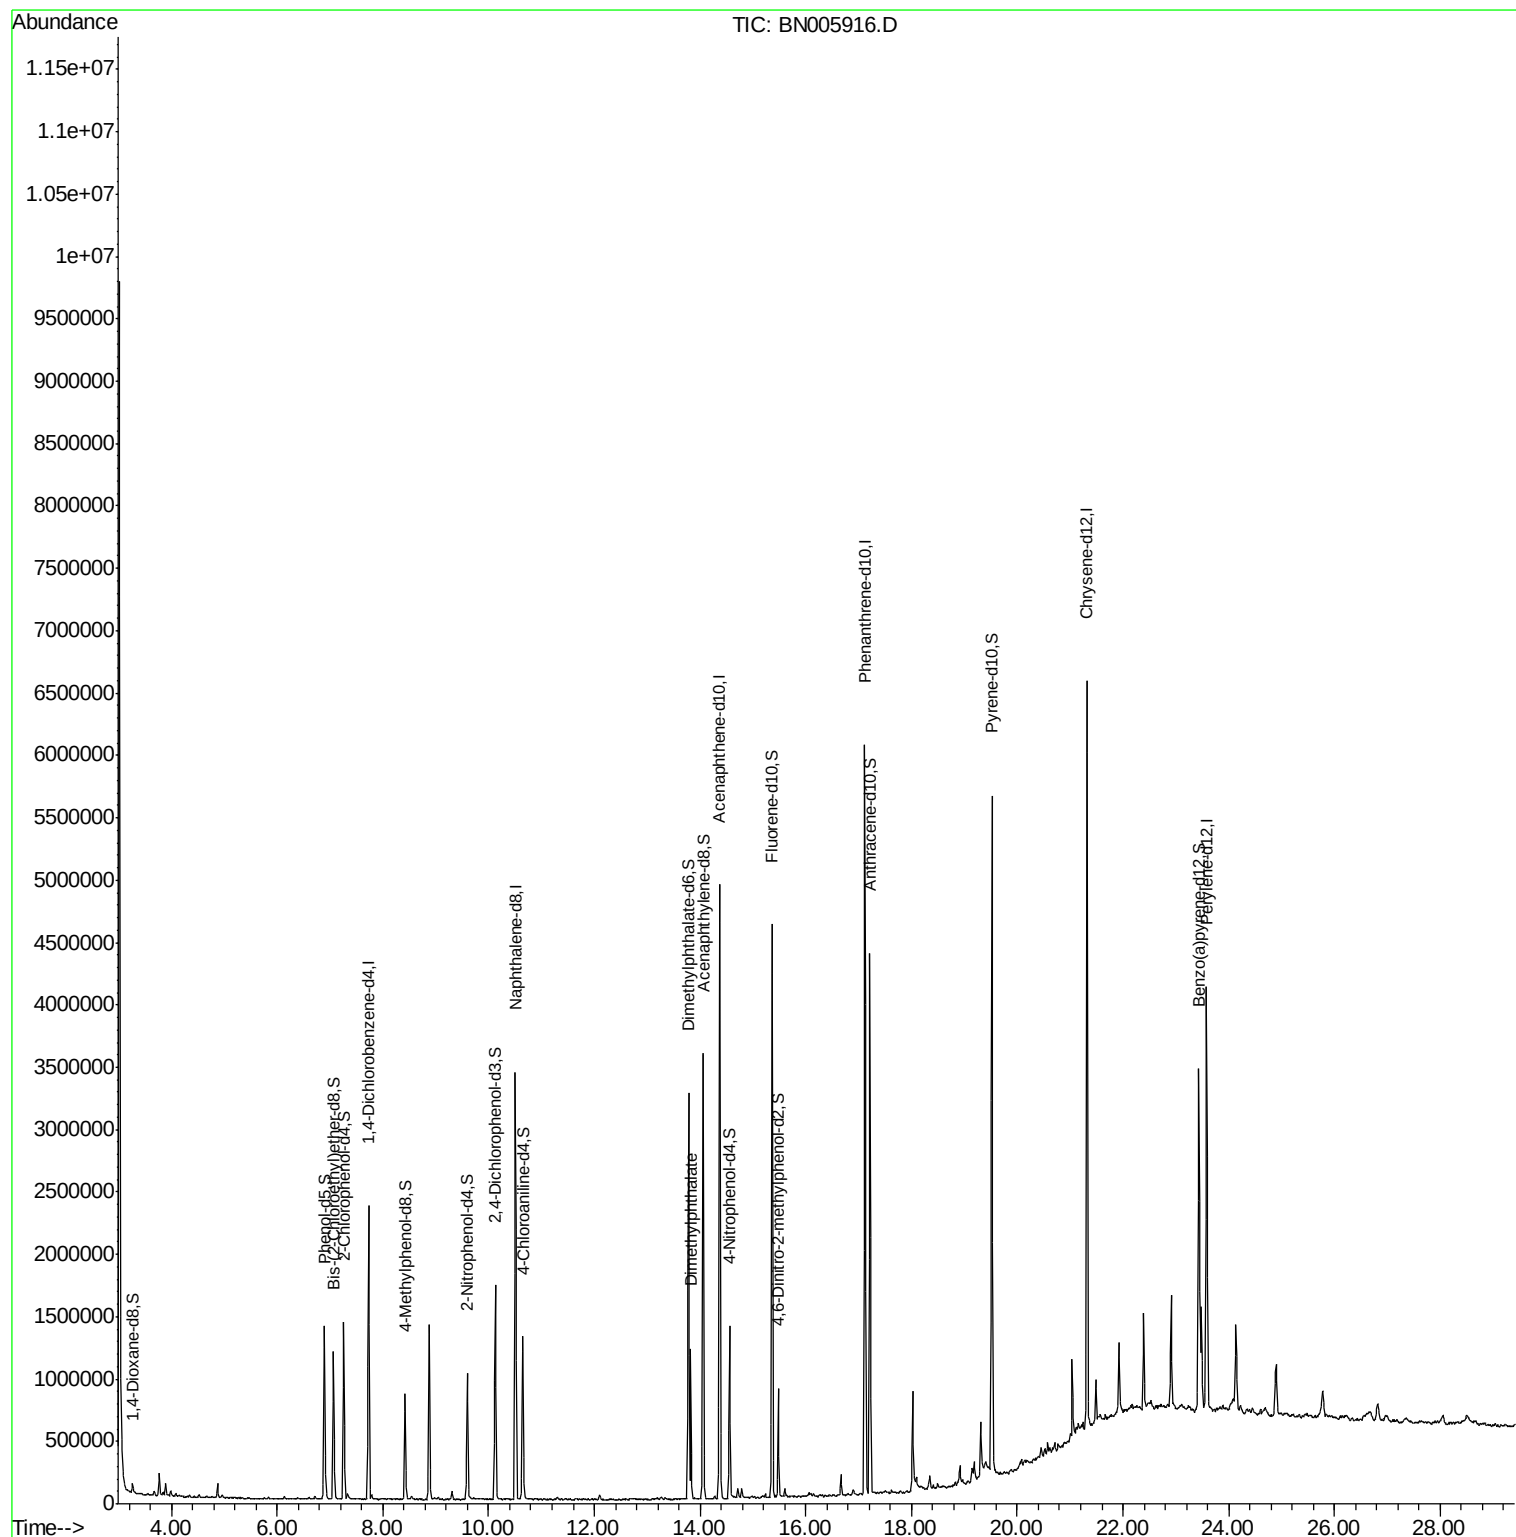

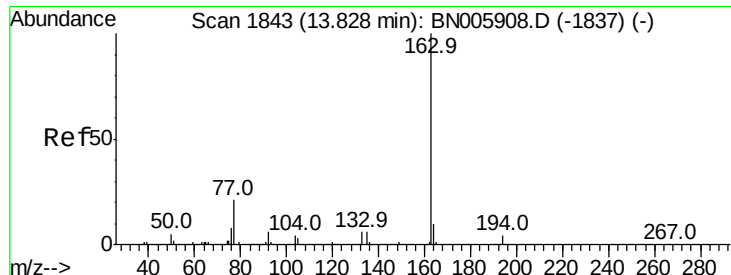

#44

Dimethylphthalate

Concen: 6.180 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BN005916.D

Acq: 29 May 2019 04:00

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 736414

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 9.9 8.1 12.1

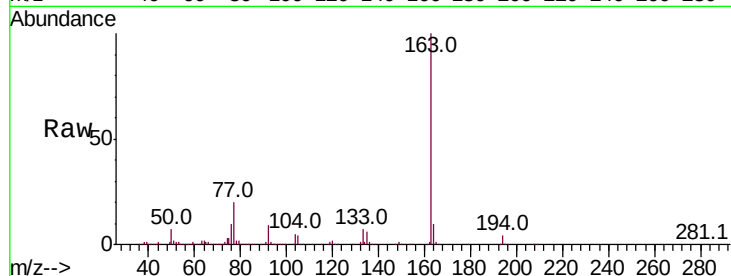

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

