

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN052819\
 Data File : BN005914.D
 Acq On : 29 May 2019 02:51
 Operator : JU/SJ
 Sample : K2692-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5178

Quant Time: May 29 04:25:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 29 02:28:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	536820	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	2471662	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	1401597	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	2967946	20.00	ng/ul	0.00
77) Chrysene-d12	21.32	240	2466519	20.00	ng/ul	0.00
85) Perylene-d12	23.59	264	2245050	20.00	ng/ul	0.00


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	62566	5.13	ng/uL	0.00
5) Phenol-d5	6.89	99	1355982	28.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	818588	30.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	1058723	29.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	730310	19.01	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	529379	33.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	532933	36.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	1026517	29.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	928987	20.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	3278135	31.73	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	4076223	31.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	477662	25.40	ng/ul	0.00
57) Fluorene-d10	15.36	176	2807505	32.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	323349	26.73	ng/ul	0.00
70) Anthracene-d10	17.22	188	3849525	30.48	ng/ul	0.00
78) Pyrene-d10	19.52	212	4421202	35.49	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.44	264	3282980	32.77	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83					

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN052819\
Data File : BN005914.D
Acq On : 29 May 2019 02:51
Operator : JU/SJ
Sample : K2692-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5178

Quant Time: May 29 04:25:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 29 02:28:30 2019
Response via : Initial Calibration

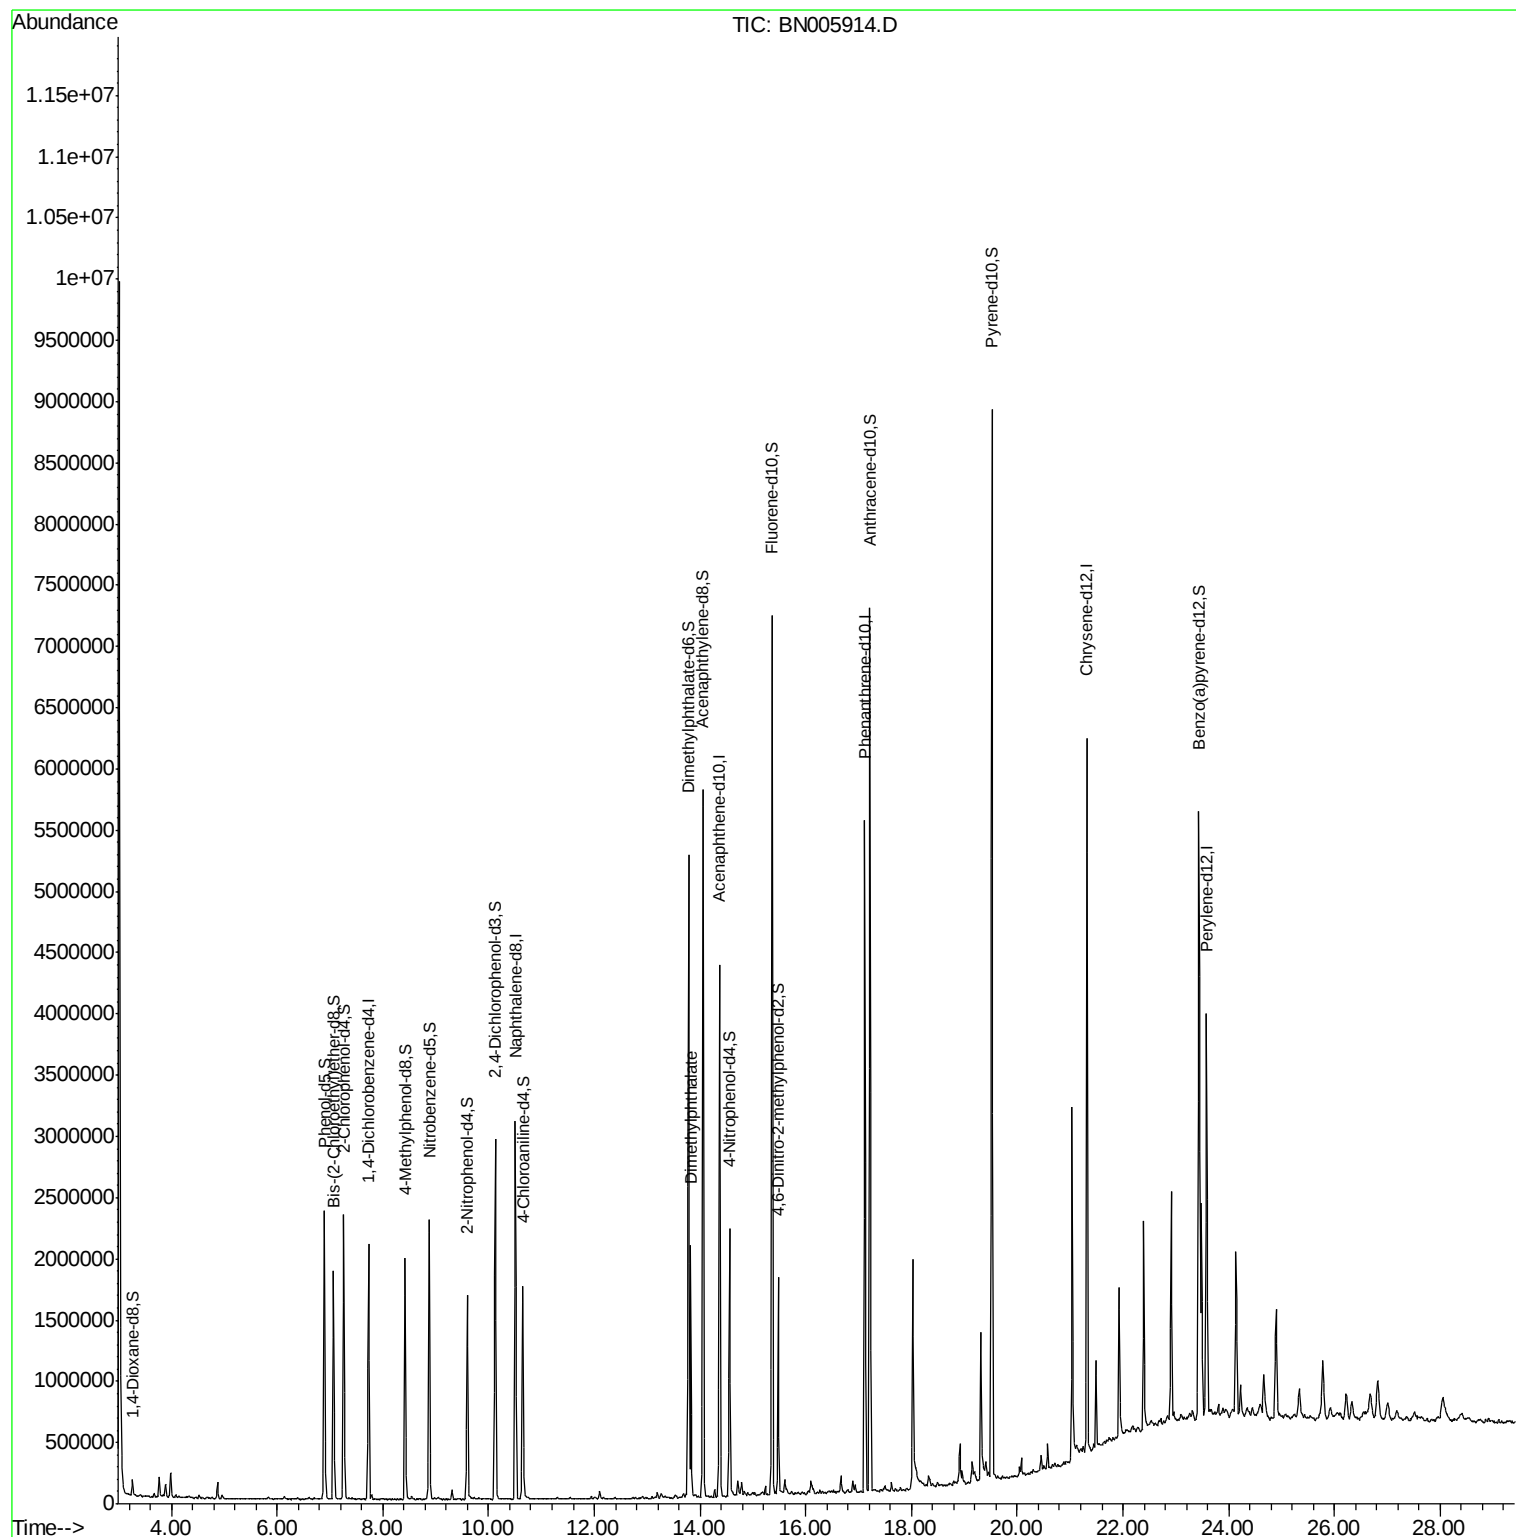

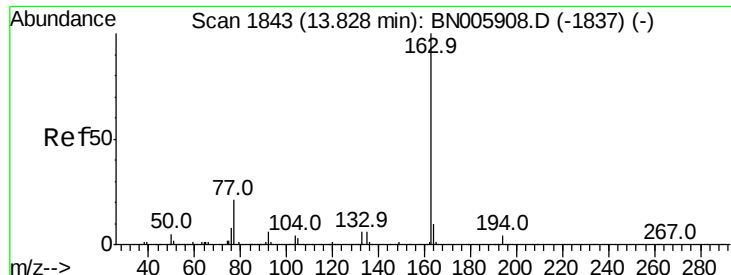

#44

Dimethylphthalate

Concen: 12.059 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BN005914.D

Acq: 29 May 2019 02:51

Instrument :

BNA_N

ClientSampleId :

A5178


Tot Ion:163 Resp: 1245391

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.2 8.1 12.1

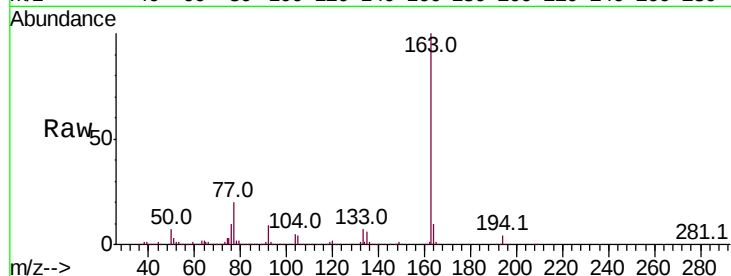

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

