
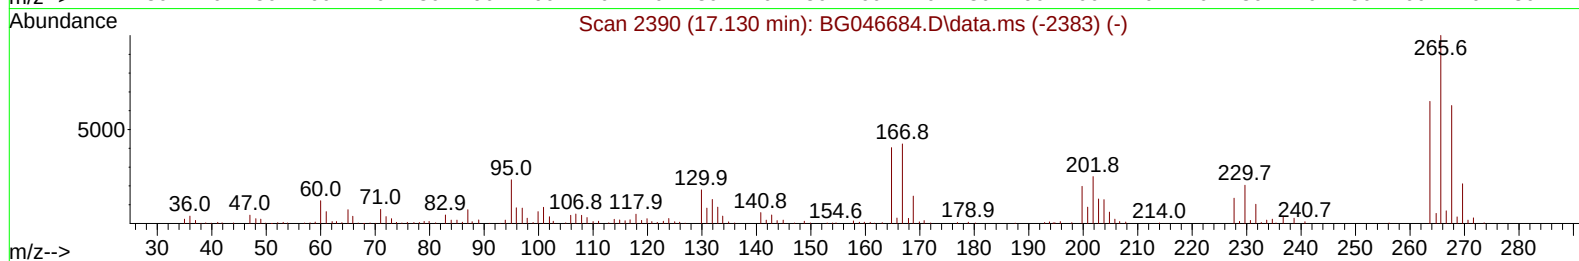
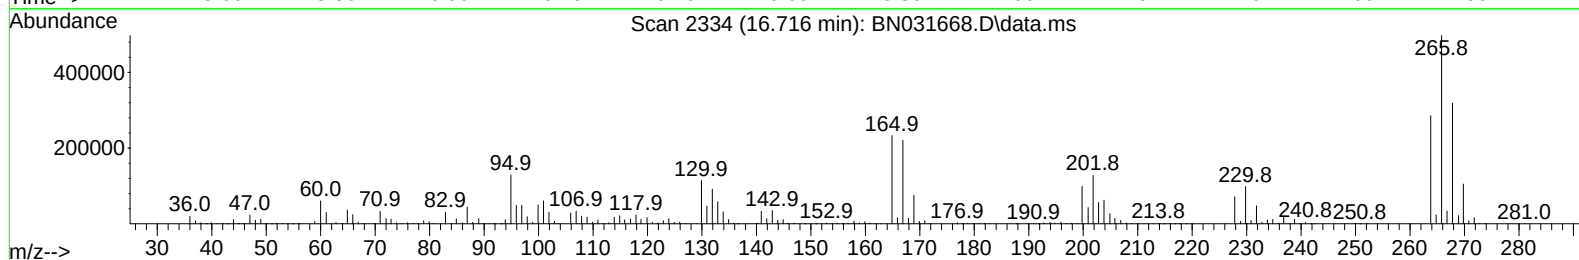


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052824\
Data File : BN031668.D
Acq On : 28 May 2024 09:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 13:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

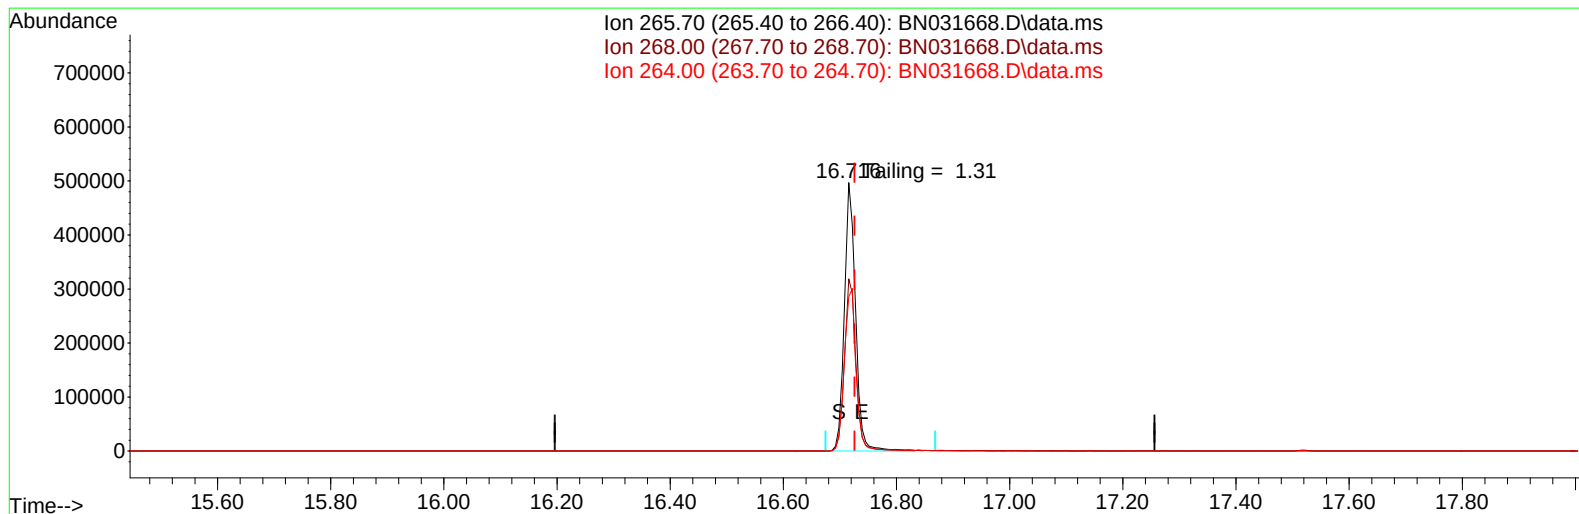

TIC: BN031668.D\data.ms

(70) Pentachlorophenol (C)




16.716min (-0.010) 24296.16 ng m

response 682599

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.15
264.00	61.60	57.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052824\
Data File : BN031668.D
Acq On : 28 May 2024 09:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 28 13:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

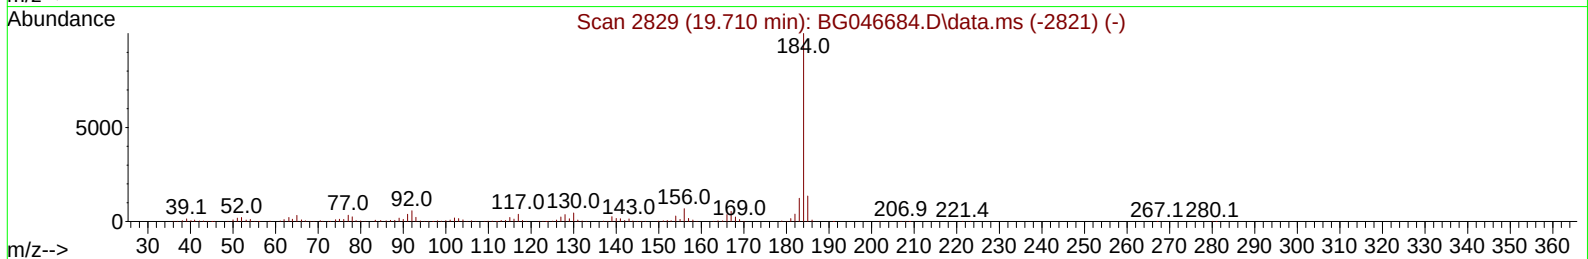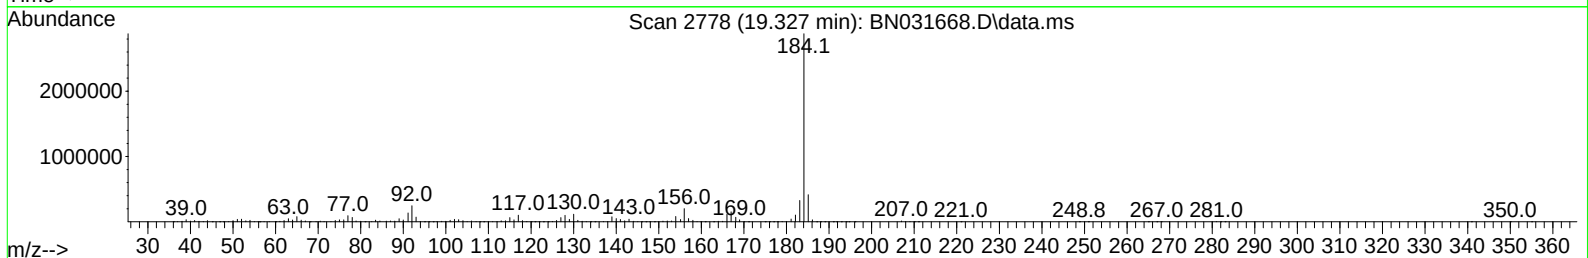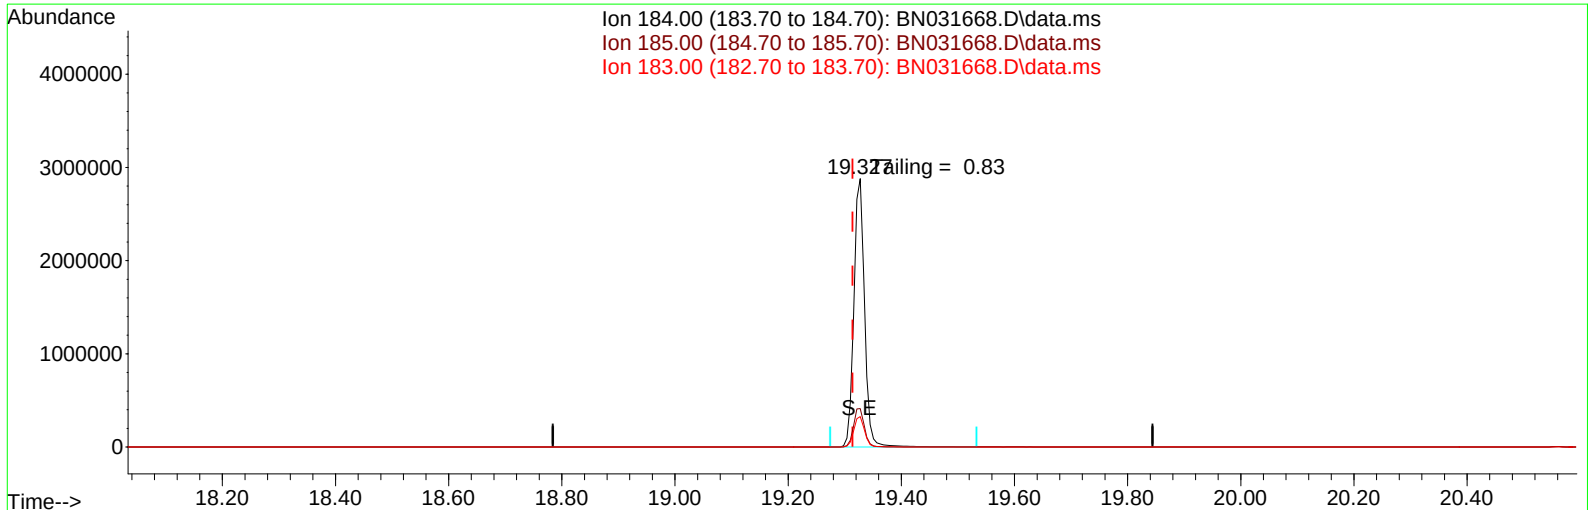

TIC: BN031668.D\data.ms

(77) Benzidine**19.327min (+ 0.013) 2198526.96 ng****response 3795143**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	11.35
0.00	0.00	0.00