
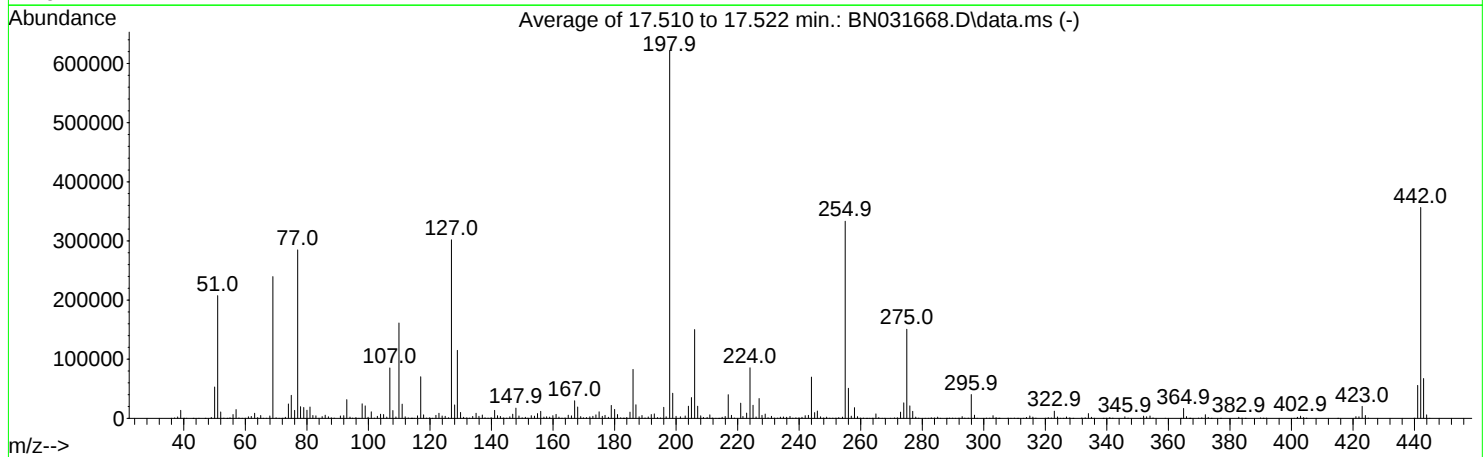


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052824\
Data File : BN031668.D
Acq On : 28 May 2024 09:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

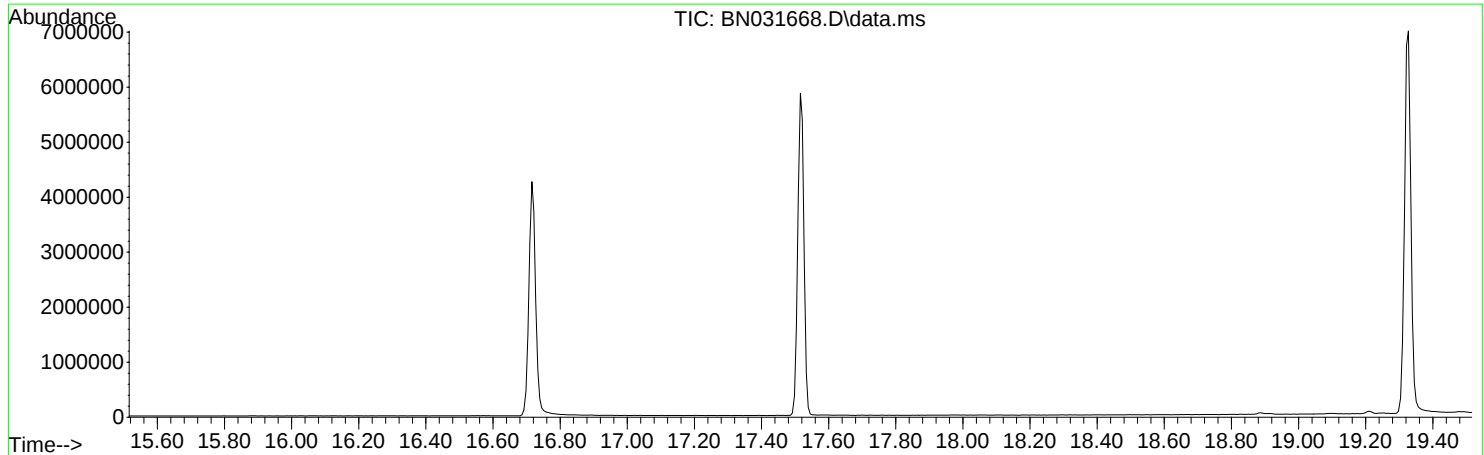

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.4	207536	PASS
68	69	0.00	2	1.7	4000	PASS
69	198	0.00	100	38.5	239701	PASS
70	69	0.00	2	0.5	1205	PASS
127	198	10	80	48.5	301909	PASS
197	198	0.00	2	0.4	2685	PASS
198	198	100	100	100.0	622016	PASS
199	198	5	9	6.8	42429	PASS
275	198	10	60	24.2	150728	PASS
365	198	1	100	2.7	16719	PASS
441	198	0.01	100	9.0	55883	PASS
442	442	50	100	100.0	356459	PASS
443	442	15	24	18.9	67405	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/28/2024	BNA_N	<u>BN031668.D</u>
Compound Name	Response	Retention Time
DDT	1355233	20.563
DDD	178001	20.121
DDE	16576	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
194577	1549810	12.55

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052824\
Data File : BN031668.D
Acq On : 28 May 2024 09:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 28 13:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

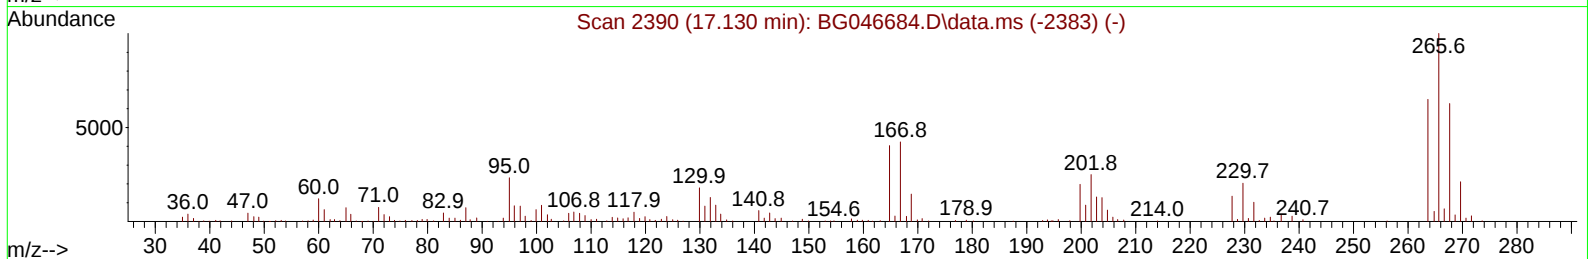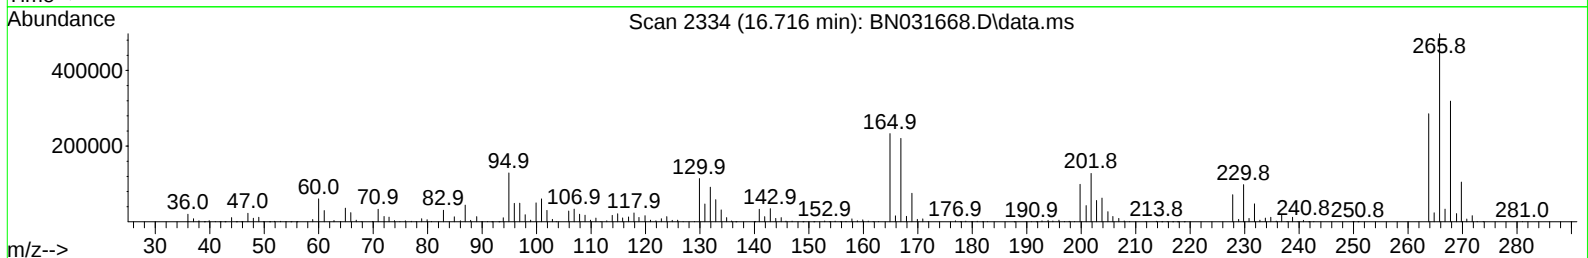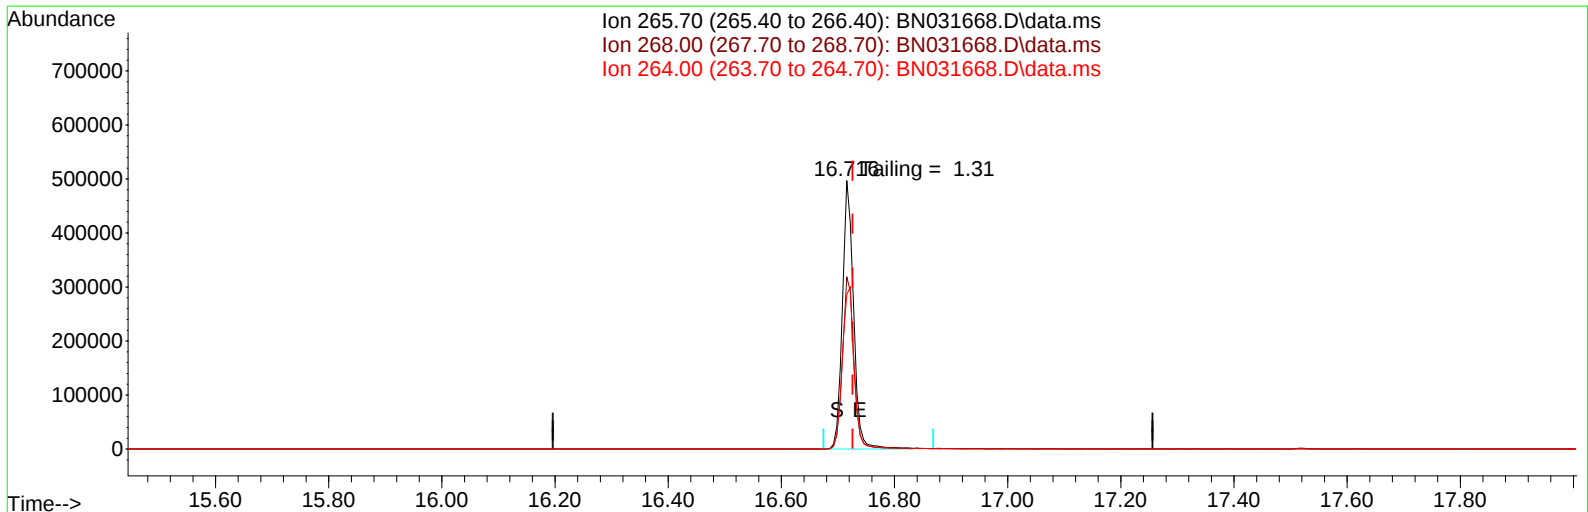

TIC: BN031668.D\data.ms

(70) Pentachlorophenol (C)

16.716min (-0.010) 24296.16 ng m




response 682599

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.15
264.00	61.60	57.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052824\
Data File : BN031668.D
Acq On : 28 May 2024 09:11
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: May 28 13:30:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

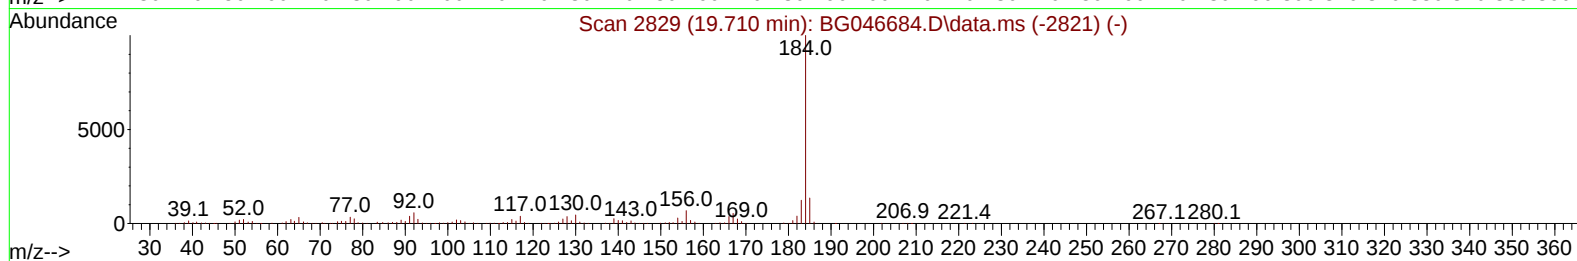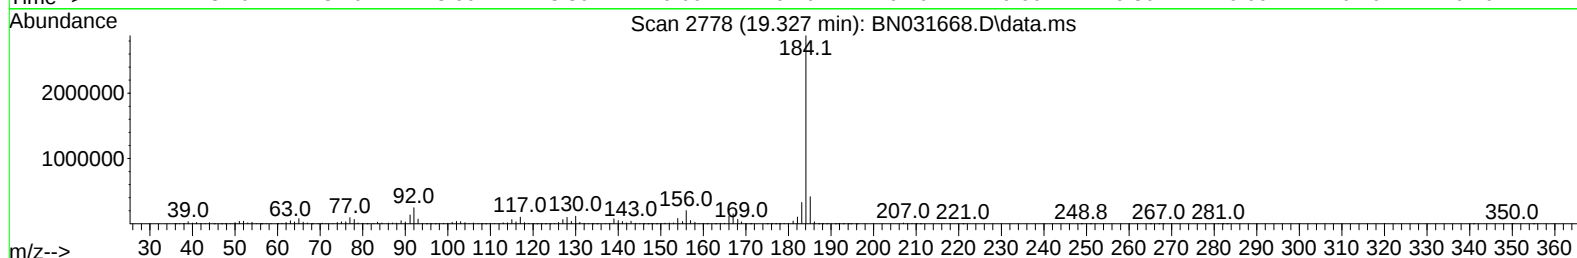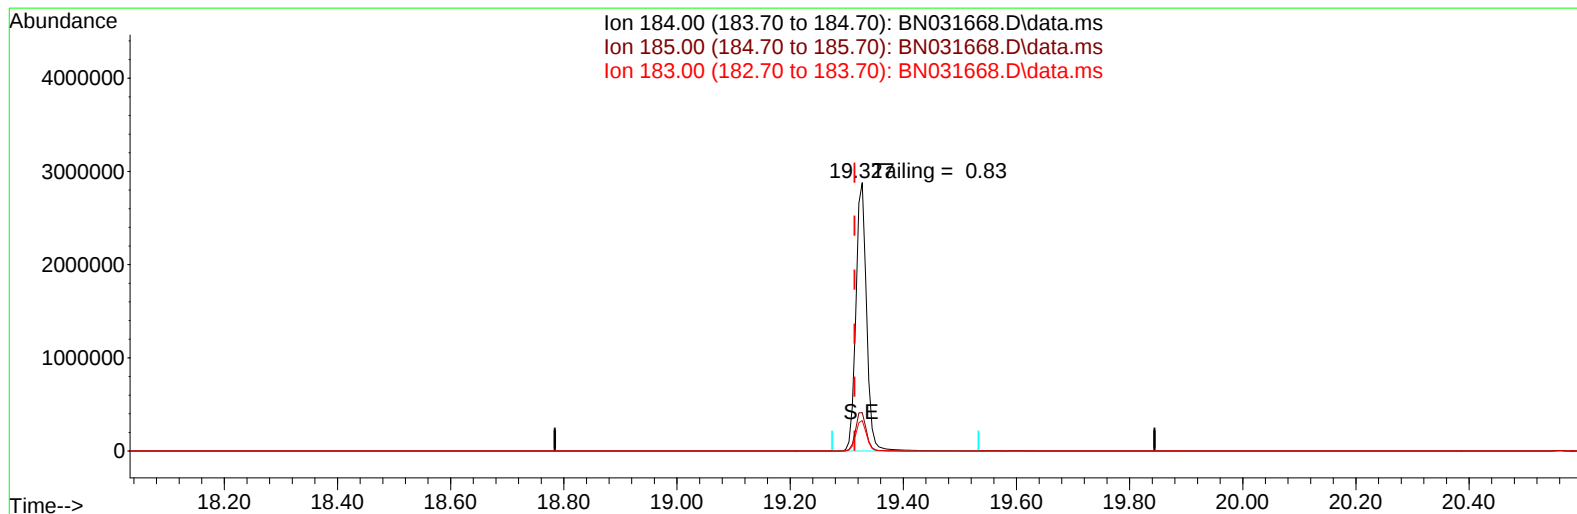

TIC: BN031668.D\data.ms

(77) Benzidine

19.327min (+ 0.013) 2198526.96 ng

response 3795143

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	11.35
0.00	0.00	0.00