

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
 Data File : BN031692.D
 Acq On : 29 May 2024 15:59
 Operator : MA/JU
 Sample : PB161084BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK084

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031692.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	105248	159717	1.19%	0.119%
2	3.593	100	103	124	rBV	1443561	2370295	17.70%	1.763%
3	3.917	154	158	164	rBV2	28539	49788	0.37%	0.037%
4	4.134	192	195	199	rVB5	15303	20276	0.15%	0.015%
5	4.540	259	264	269	rVB6	13850	25085	0.19%	0.019%
6	6.852	649	657	671	rVB	1832358	2922307	21.83%	2.173%
7	7.028	680	687	698	rVB	1575982	2485480	18.56%	1.848%
8	7.216	711	719	729	rBV	1873376	2964925	22.15%	2.205%
9	7.687	791	799	806	rVB	1775327	2839783	21.21%	2.112%
10	8.387	908	918	933	rBV	2304745	3815068	28.50%	2.837%
11	8.840	986	995	1004	rBV	1797495	2958116	22.09%	2.200%
12	9.558	1106	1117	1131	rBV	1376260	2308768	17.24%	1.717%
13	10.087	1199	1207	1217	rBV	2264747	3721669	27.80%	2.767%
14	10.469	1264	1272	1282	rVB	2605305	4426733	33.06%	3.292%
15	10.605	1287	1295	1304	rBV	2454315	4196268	31.34%	3.120%
16	11.246	1399	1404	1407	rBV7	9310	16179	0.12%	0.012%
17	12.057	1536	1542	1547	rBV	47005	78075	0.58%	0.058%
18	12.687	1643	1649	1653	rBV8	7363	16540	0.12%	0.012%
19	13.740	1821	1828	1839	rVB	4642760	6477922	48.38%	4.817%
20	14.016	1867	1875	1883	rBV	5000486	7359694	54.97%	5.473%
21	14.322	1920	1927	1935	rBV	4320536	6319283	47.20%	4.699%
22	14.522	1953	1961	1978	rBV	2283358	3308435	24.71%	2.460%
23	15.316	2088	2096	2103	rBV	6216273	9273499	69.26%	6.896%
24	15.434	2109	2116	2126	rBV	1828222	2425504	18.12%	1.804%
25	15.557	2133	2137	2144	rVB3	35477	59938	0.45%	0.045%
26	16.004	2208	2213	2219	rBV10	7182	16940	0.13%	0.013%
27	16.745	2335	2339	2345	rVB8	12700	18209	0.14%	0.014%
28	16.857	2354	2358	2364	rVB3	15285	23069	0.17%	0.017%
29	16.939	2367	2372	2375	rBV7	8014	17263	0.13%	0.013%
30	17.069	2387	2394	2404	rBV	5513451	7955348	59.42%	5.915%
31	17.169	2404	2411	2422	rBV	7030345	10139792	75.74%	7.540%
32	17.445	2454	2458	2461	rBV4	10895	17868	0.13%	0.013%
33	17.969	2543	2547	2550	rBV5	25559	37267	0.28%	0.028%
34	18.298	2598	2603	2609	rVB8	20347	39843	0.30%	0.030%
35	18.863	2696	2699	2708	rVB8	15787	28410	0.21%	0.021%
36	19.028	2723	2727	2733	rVB2	101255	135852	1.01%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031692.D
Acq On : 29 May 2024 15:59
Operator : MA/JU
Sample : PB161084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK084

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.098	2734	2739	2743	rBV	102705	142364	1.06%	0.106%
38	19.251	2763	2765	2769	rBV4	12159	15728	0.12%	0.012%
39	19.410	2789	2792	2795	rBV2	41091	44094	0.33%	0.033%
40	19.463	2795	2801	2811	rBV	8540340	12496193	93.34%	9.292%
41	20.463	2968	2971	2978	rVB3	62803	74476	0.56%	0.055%
42	21.304	3108	3114	3125	rVB	6086377	9209178	68.78%	6.848%
43	24.039	3569	3579	3591	rBV	5646841	13388476	100.00%	9.955%
44	24.239	3604	3613	3628	rVB	3952792	10083821	75.32%	7.498%




Sum of corrected areas: 134483538

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031692.D
Acq On : 29 May 2024 15:59
Operator : MA/JU
Sample : PB161084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK084

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

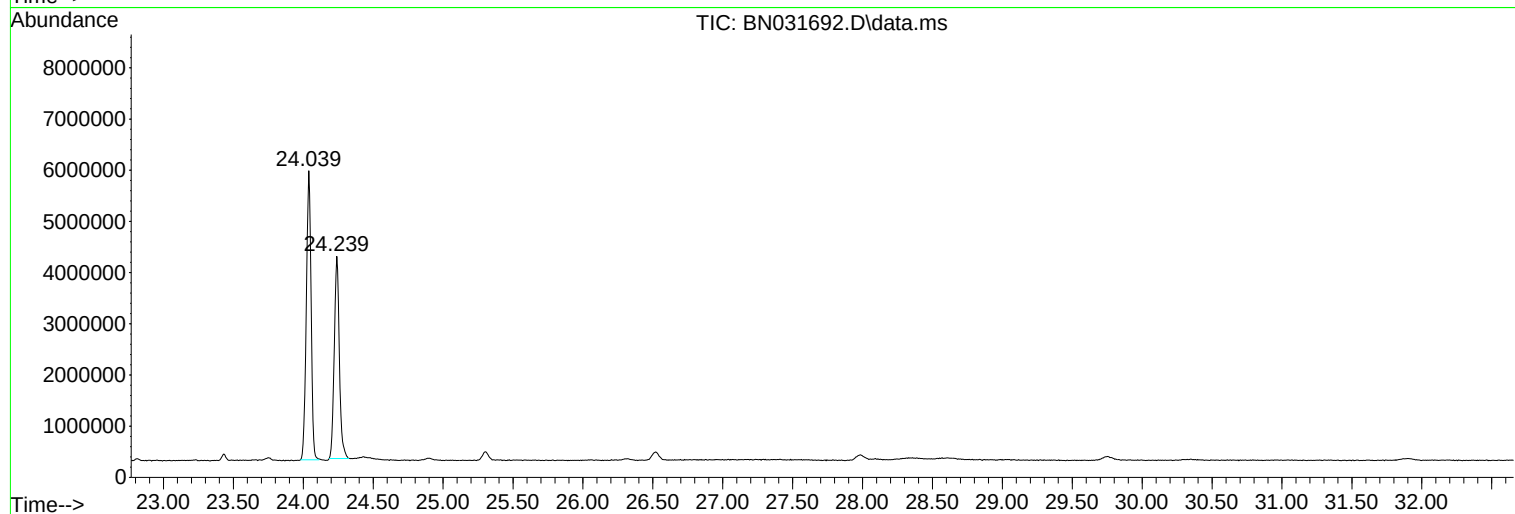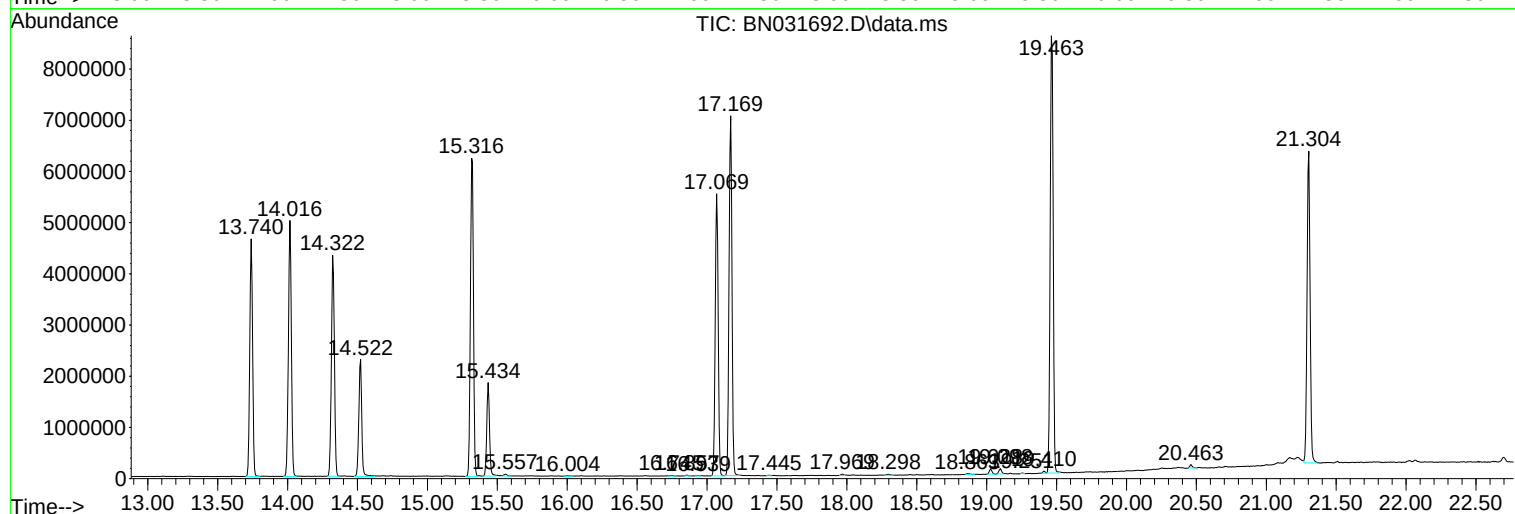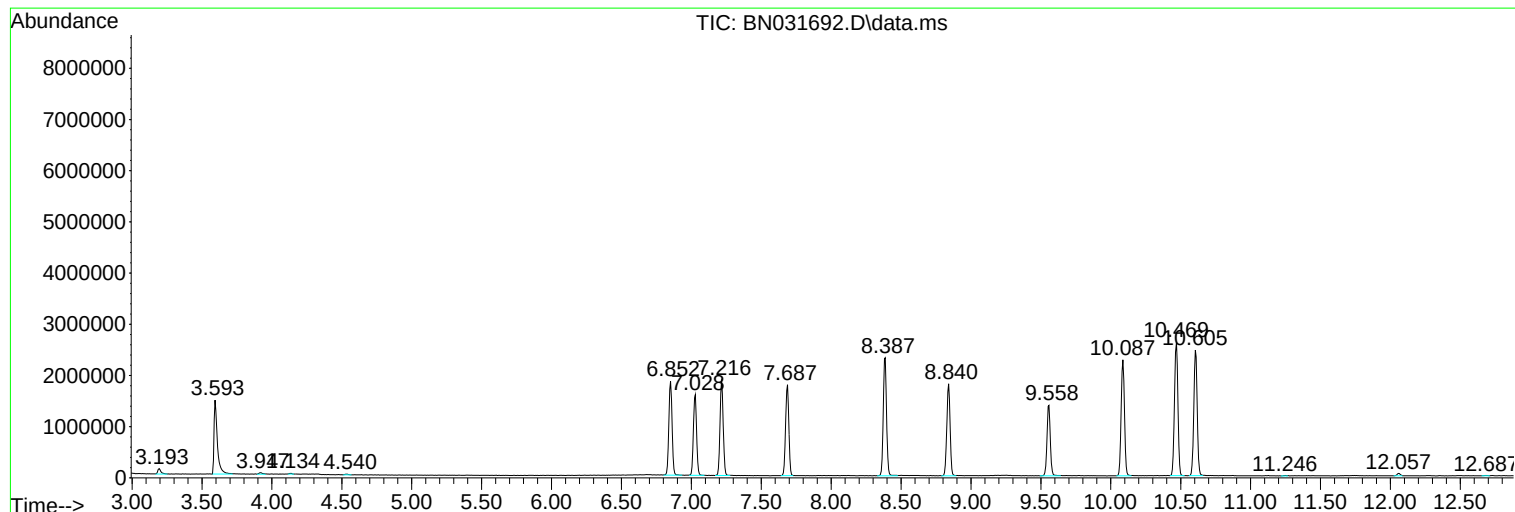

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031692.D
Acq On : 29 May 2024 15:59
Operator : MA/JU
Sample : PB161084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK084

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031692.D
Acq On : 29 May 2024 15:59
Operator : MA/JU
Sample : PB161084BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK084

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------