

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
 Data File : BN031694.D
 Acq On : 29 May 2024 17:21
 Operator : MA/JU
 Sample : PB161110BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	44	rVB	88116	121680	1.22%	0.124%
2	3.593	100	103	120	rBV	1145258	1809675	18.12%	1.847%
3	3.916	155	158	164	rVB3	17738	29748	0.30%	0.030%
4	6.852	650	657	666	rVB	1373621	2194784	21.98%	2.241%
5	7.022	680	686	695	rVB	1205288	1901602	19.04%	1.941%
6	7.216	712	719	728	rBV	1428770	2232361	22.36%	2.279%
7	7.687	791	799	810	rVB	1132368	1840902	18.44%	1.879%
8	8.381	910	917	926	rBV	1756435	2863207	28.68%	2.923%
9	8.840	988	995	1004	rBV	1348227	2221479	22.25%	2.268%
10	9.551	1107	1116	1128	rBV	1001753	1685291	16.88%	1.720%
11	10.087	1200	1207	1218	rBV	1658392	2788725	27.93%	2.847%
12	10.469	1264	1272	1280	rVB	1720292	2905853	29.10%	2.967%
13	10.604	1288	1295	1310	rBV	1919597	3178384	31.83%	3.245%
14	11.245	1400	1404	1411	rBV9	5477	10666	0.11%	0.011%
15	12.057	1536	1542	1550	rVB3	36762	68539	0.69%	0.070%
16	12.681	1643	1648	1654	rBV7	7571	16204	0.16%	0.017%
17	13.739	1821	1828	1840	rVB	3526987	4896749	49.04%	4.999%
18	14.016	1868	1875	1888	rBV2	3771024	5665217	56.74%	5.783%
19	14.322	1920	1927	1938	rVB	2879981	4265297	42.72%	4.354%
20	14.516	1951	1960	1972	rBV	1613710	2411905	24.16%	2.462%
21	14.745	1994	1999	2004	rBV9	6436	12079	0.12%	0.012%
22	14.981	2038	2039	2045	rVB6	8808	14049	0.14%	0.014%
23	15.322	2089	2097	2108	rBV	4739042	7122987	71.34%	7.272%
24	15.433	2110	2116	2126	rBV	1245297	1693319	16.96%	1.729%
25	15.557	2133	2137	2143	rVB2	25374	38872	0.39%	0.040%
26	15.998	2208	2212	2216	rBV6	6249	10542	0.11%	0.011%
27	16.110	2226	2231	2234	rVB5	5549	10182	0.10%	0.010%
28	16.563	2304	2308	2313	rVB7	6771	13271	0.13%	0.014%
29	16.751	2336	2340	2345	rVB8	7561	14028	0.14%	0.014%
30	16.857	2352	2358	2363	rBV4	11189	19979	0.20%	0.020%
31	16.933	2367	2371	2374	rBV6	6918	10204	0.10%	0.010%
32	17.069	2387	2394	2404	rBV	3673872	5347616	53.56%	5.459%
33	17.169	2404	2411	2424	rVV2	5492849	8042700	80.55%	8.211%
34	17.451	2454	2459	2463	rBV6	7584	14027	0.14%	0.014%
35	17.633	2485	2490	2493	rBV7	7335	11406	0.11%	0.012%
36	17.969	2544	2547	2555	rBV6	14560	26409	0.26%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031694.D
Acq On : 29 May 2024 17:21
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.027	2723	2727	2732	rBV2	72762	99794	1.00%	0.102%
38	19.098	2734	2739	2747	rVV	72498	111568	1.12%	0.114%
39	19.410	2789	2792	2795	rBV2	28803	33818	0.34%	0.035%
40	19.463	2795	2801	2810	rVV	7122426	9671249	96.86%	9.873%
41	21.298	3107	3113	3128	rBV2	4024556	6064363	60.74%	6.191%
42	24.033	3569	3578	3592	rVB	4056633	9984822	100.00%	10.193%
43	24.233	3603	3612	3629	rVB2	2591618	6479839	64.90%	6.615%




Sum of corrected areas: 97955391

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031694.D
Acq On : 29 May 2024 17:21
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

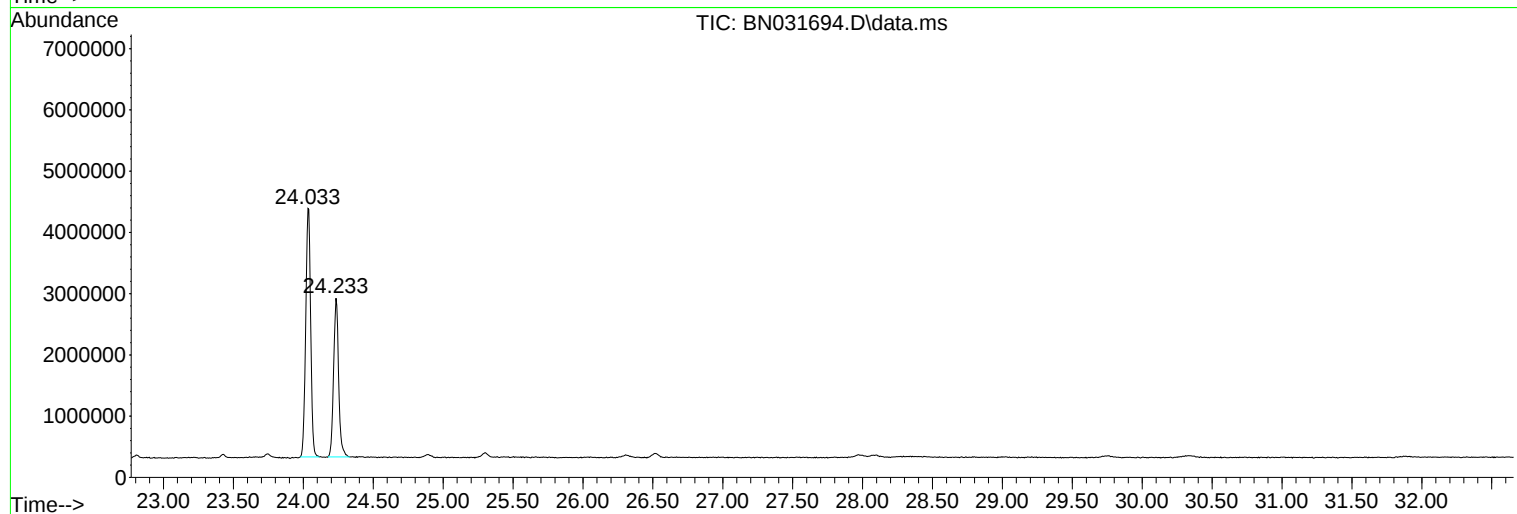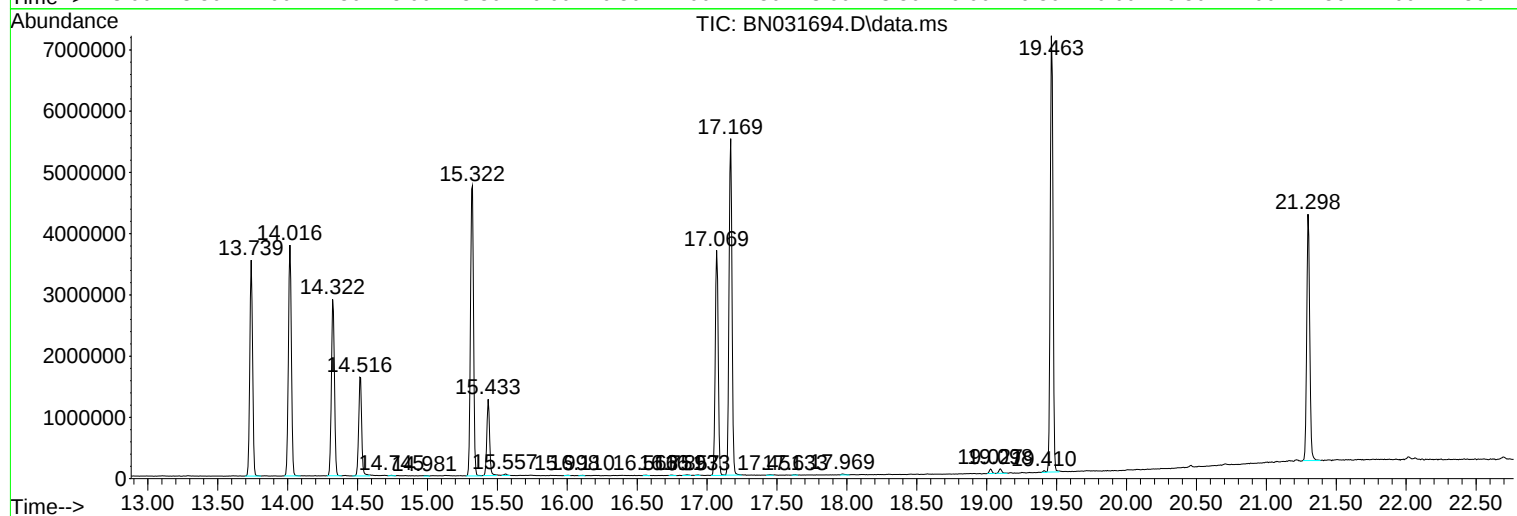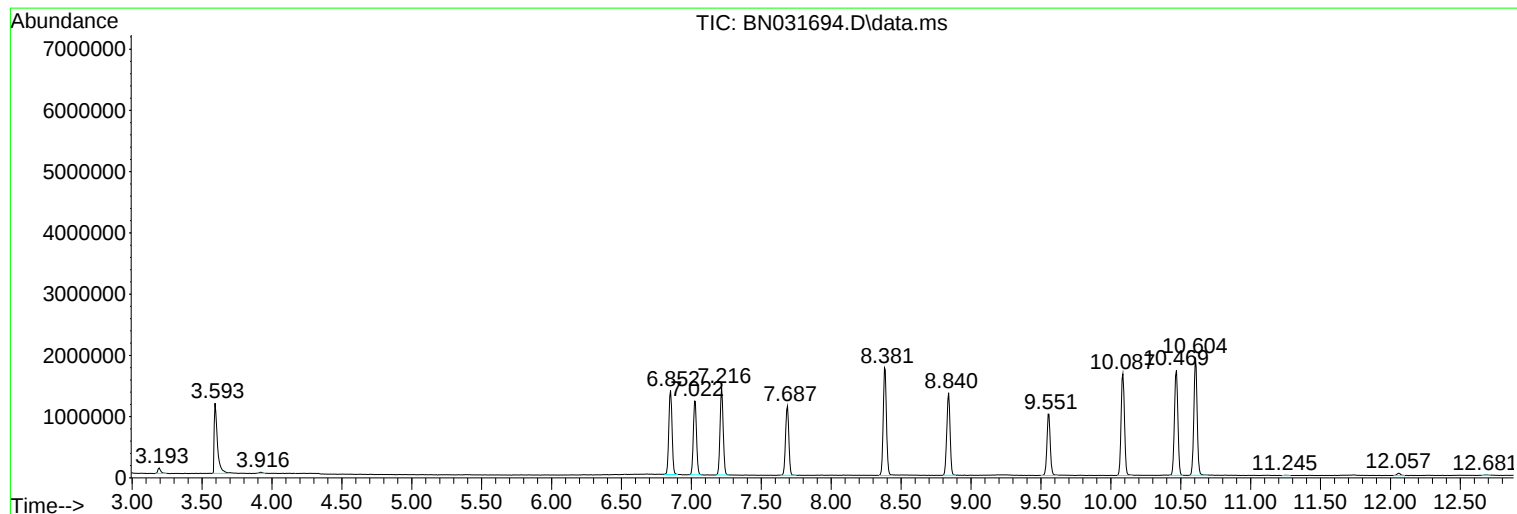

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031694.D
Acq On : 29 May 2024 17:21
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031694.D
Acq On : 29 May 2024 17:21
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc