

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
 Data File : BN031705.D
 Acq On : 30 May 2024 03:10
 Operator : MA/JU
 Sample : PB161110BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	44	rVB	120906	173361	1.43%	0.138%
2	3.593	100	103	119	rBV	1649022	2638913	21.69%	2.103%
3	3.917	155	158	165	rVB	21690	31754	0.26%	0.025%
4	6.852	650	657	667	rVB	2204022	3433171	28.22%	2.736%
5	7.028	677	687	696	rVB	1840312	2901028	23.85%	2.311%
6	7.216	711	719	728	rBV	2213097	3496725	28.74%	2.786%
7	7.687	792	799	807	rVB	1406190	2303006	18.93%	1.835%
8	8.387	910	918	929	rBV	2753022	4515664	37.12%	3.598%
9	8.840	987	995	1003	rBV	2169057	3475579	28.57%	2.769%
10	9.557	1109	1117	1128	rBV	1641385	2732717	22.46%	2.177%
11	10.087	1197	1207	1222	rBV	2724377	4513895	37.10%	3.597%
12	10.469	1263	1272	1281	rVB	2193825	3689659	30.33%	2.940%
13	10.604	1285	1295	1310	rBV	2828630	4844151	39.82%	3.860%
14	12.057	1537	1542	1551	rVB	55766	95028	0.78%	0.076%
15	13.287	1745	1751	1760	rVB8	9844	21351	0.18%	0.017%
16	13.740	1821	1828	1838	rBV	4902906	6822233	56.08%	5.436%
17	14.016	1868	1875	1884	rBV	5492131	8368873	68.79%	6.668%
18	14.322	1920	1927	1937	rBV	3561981	5133724	42.20%	4.090%
19	14.522	1953	1961	1977	rBV	2305917	3377890	27.77%	2.691%
20	14.734	1993	1997	2005	rVB10	11304	23564	0.19%	0.019%
21	15.316	2085	2096	2104	rBV	6771710	10147181	83.41%	8.085%
22	15.434	2109	2116	2130	rVV	1751503	2483834	20.42%	1.979%
23	15.557	2132	2137	2143	rVB2	37925	63459	0.52%	0.051%
24	15.887	2189	2193	2198	rBV8	9377	12761	0.10%	0.010%
25	16.557	2302	2307	2310	rBV6	7665	12986	0.11%	0.010%
26	16.751	2335	2340	2344	rVB6	11323	17777	0.15%	0.014%
27	16.857	2353	2358	2361	rBV3	10633	15571	0.13%	0.012%
28	17.069	2387	2394	2403	rBV	4235641	6112694	50.25%	4.871%
29	17.169	2404	2411	2427	rVB2	7569715	10947816	89.99%	8.723%
30	17.445	2453	2458	2461	rBV3	11669	20039	0.16%	0.016%
31	17.969	2543	2547	2552	rVB7	10695	17734	0.15%	0.014%
32	18.292	2599	2602	2607	rVB6	11534	14465	0.12%	0.012%
33	19.028	2722	2727	2732	rBV2	97640	141015	1.16%	0.112%
34	19.098	2734	2739	2743	rVV	94007	132744	1.09%	0.106%
35	19.410	2788	2792	2795	rBV2	42785	47090	0.39%	0.038%
36	19.463	2795	2801	2808	rBV	8649950	12165654	100.00%	9.693%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031705.D
Acq On : 30 May 2024 03:10
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	20.457	2967	2970	2974	rBV3	47169	56214	0.46%	0.045%
38	21.298	3107	3113	3122	rBV	3930525	5614054	46.15%	4.473%
39	24.033	3568	3578	3591	rBV2	3999822	9641582	79.25%	7.682%
40	24.233	3603	3612	3630	rVB	1968334	5247358	43.13%	4.181%




Sum of corrected areas: 125504314

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031705.D
Acq On : 30 May 2024 03:10
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

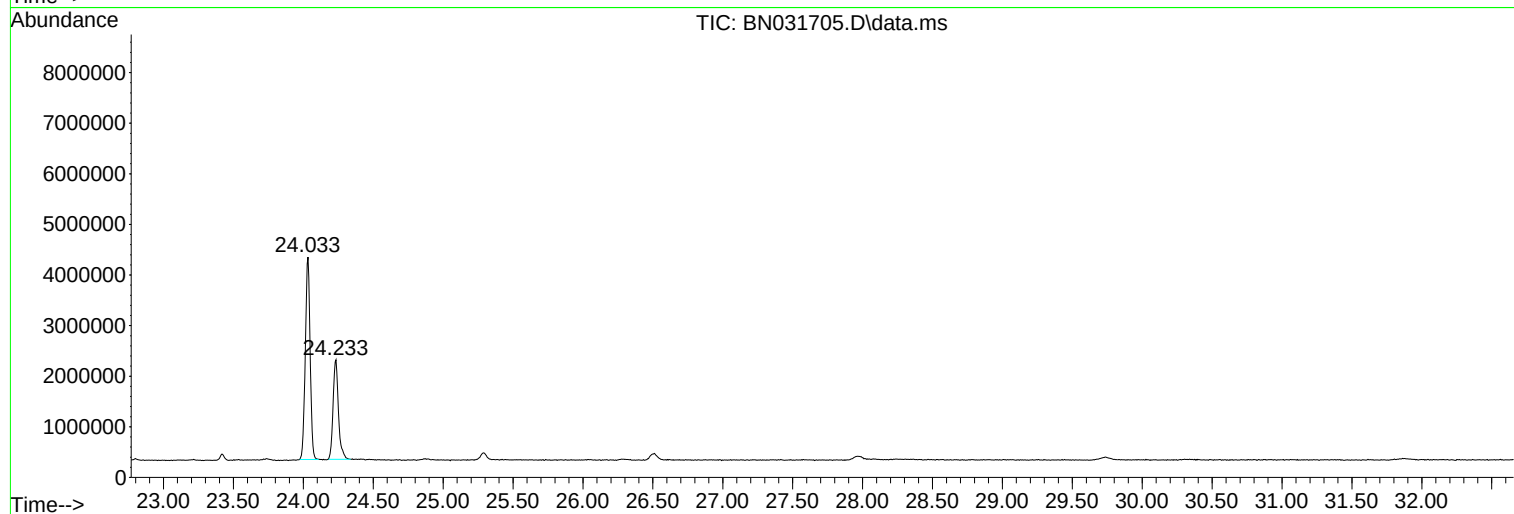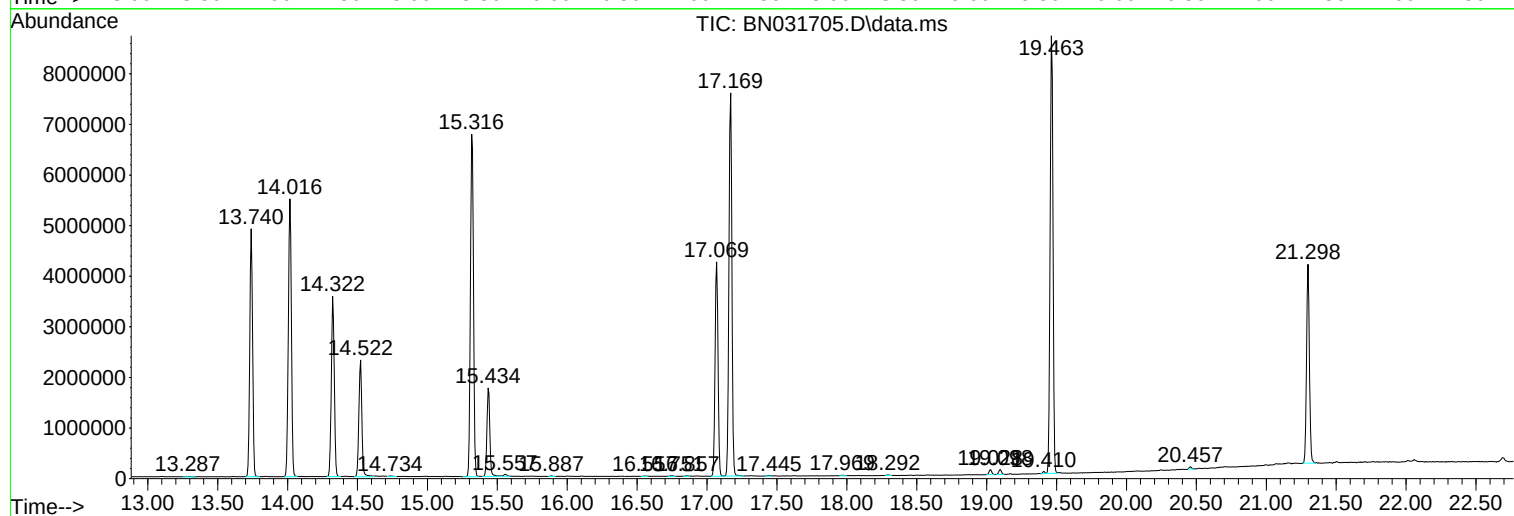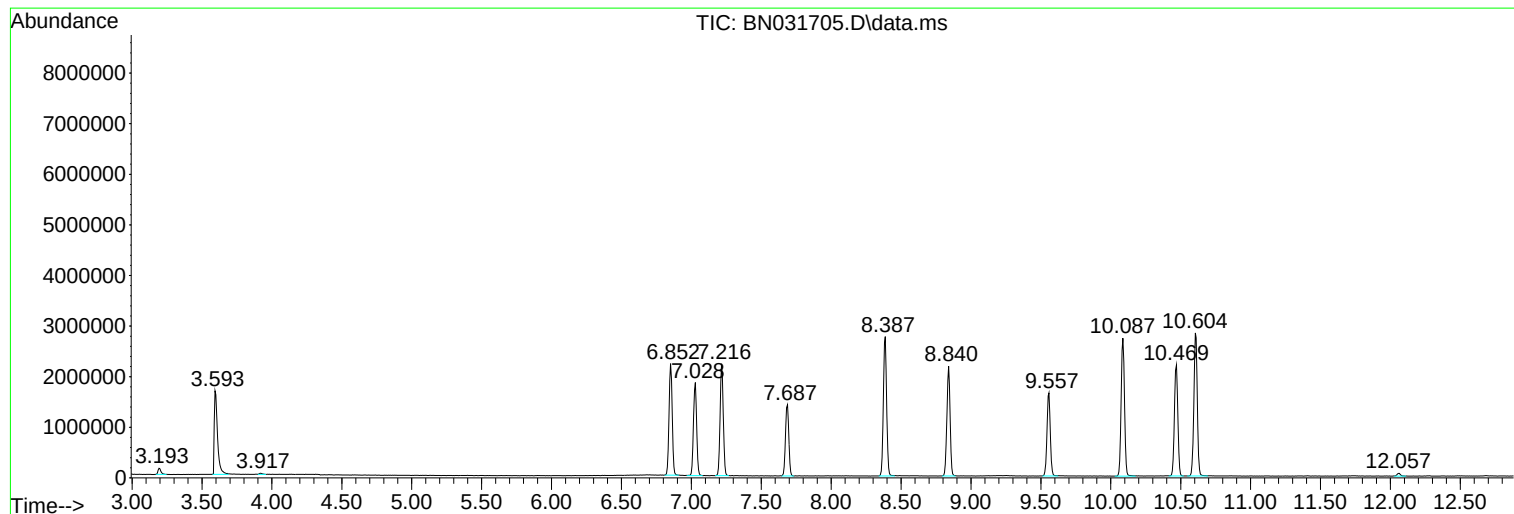

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031705.D
Acq On : 30 May 2024 03:10
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN052924\
Data File : BN031705.D
Acq On : 30 May 2024 03:10
Operator : MA/JU
Sample : PB161110BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK110

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc