

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053024\
 Data File : BN031721.D
 Acq On : 30 May 2024 18:20
 Operator : MA/JU
 Sample : PB161108BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	43	rVB	93701	132102	1.25%	0.117%
2	3.593	99	103	124	rBV	1253813	1900240	18.01%	1.676%
3	3.917	154	158	165	rVB	26615	38159	0.36%	0.034%
4	4.369	231	235	242	rBV	15721	32106	0.30%	0.028%
5	6.852	649	657	665	rBV	1483949	2346781	22.24%	2.070%
6	7.028	679	687	698	rVB	1263198	2030021	19.24%	1.791%
7	7.216	712	719	727	rBV	1513422	2427335	23.00%	2.141%
8	7.687	791	799	808	rVB	1476687	2345119	22.22%	2.069%
9	8.387	910	918	928	rBV	1978164	3142377	29.78%	2.772%
10	8.840	987	995	1004	rBV	1488863	2451652	23.23%	2.163%
11	9.557	1109	1117	1132	rVB	1210415	1983740	18.80%	1.750%
12	10.087	1196	1207	1219	rBV	1855204	3153293	29.88%	2.782%
13	10.469	1263	1272	1283	rVB	2175170	3677668	34.85%	3.245%
14	10.610	1288	1296	1312	rBV	2082680	3556628	33.71%	3.138%
15	12.063	1536	1543	1552	rVB	40583	73009	0.69%	0.064%
16	13.292	1746	1752	1756	rBV5	9297	14821	0.14%	0.013%
17	13.740	1820	1828	1837	rBV	3867181	5575045	52.84%	4.918%
18	14.022	1865	1876	1884	rBV	4380989	6470815	61.32%	5.709%
19	14.328	1919	1928	1937	rBV	3870879	5522629	52.34%	4.872%
20	14.528	1953	1962	1978	rBV	2005920	2925556	27.73%	2.581%
21	14.739	1996	1998	2003	rVB5	9330	10982	0.10%	0.010%
22	15.322	2090	2097	2106	rBV	5594817	8032714	76.13%	7.087%
23	15.445	2111	2118	2133	rBV	1601509	2316904	21.96%	2.044%
24	15.563	2134	2138	2144	rVB	30763	50383	0.48%	0.044%
25	16.104	2226	2230	2239	rVB9	10044	18617	0.18%	0.016%
26	16.204	2243	2247	2252	rBV8	8259	17593	0.17%	0.016%
27	16.745	2336	2339	2344	rBV7	9491	14331	0.14%	0.013%
28	16.863	2354	2359	2365	rVB3	11938	20696	0.20%	0.018%
29	17.010	2380	2384	2387	rBV4	14013	18593	0.18%	0.016%
30	17.075	2388	2395	2405	rVB	4822268	6941582	65.79%	6.124%
31	17.175	2405	2412	2421	rBV	6244821	9073286	85.99%	8.005%
32	17.445	2456	2458	2462	rBV2	11584	11638	0.11%	0.010%
33	17.610	2483	2486	2489	rBV5	8744	11895	0.11%	0.010%
34	17.751	2507	2510	2515	rVB7	14762	17734	0.17%	0.016%
35	17.986	2544	2550	2563	rBV	210595	585084	5.54%	0.516%
36	18.451	2626	2629	2633	rVB3	27670	33323	0.32%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053024\
Data File : BN031721.D
Acq On : 30 May 2024 18:20
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	19.033	2724	2728	2732	rBV2	90920	117113	1.11%	0.103%
38	19.104	2736	2740	2745	rVB	86090	118559	1.12%	0.105%
39	19.275	2764	2769	2784	rBV	216272	691140	6.55%	0.610%
40	19.475	2796	2803	2809	rBV	7594397	10551793	100.00%	9.309%
41	21.310	3109	3115	3122	rBV2	5186139	7486935	70.95%	6.605%
42	24.057	3573	3582	3595	rVB2	3915033	9920608	94.02%	8.752%
43	24.251	3607	3615	3629	rVB	2958535	7488900	70.97%	6.607%




Sum of corrected areas: 113349499

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053024\
Data File : BN031721.D
Acq On : 30 May 2024 18:20
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

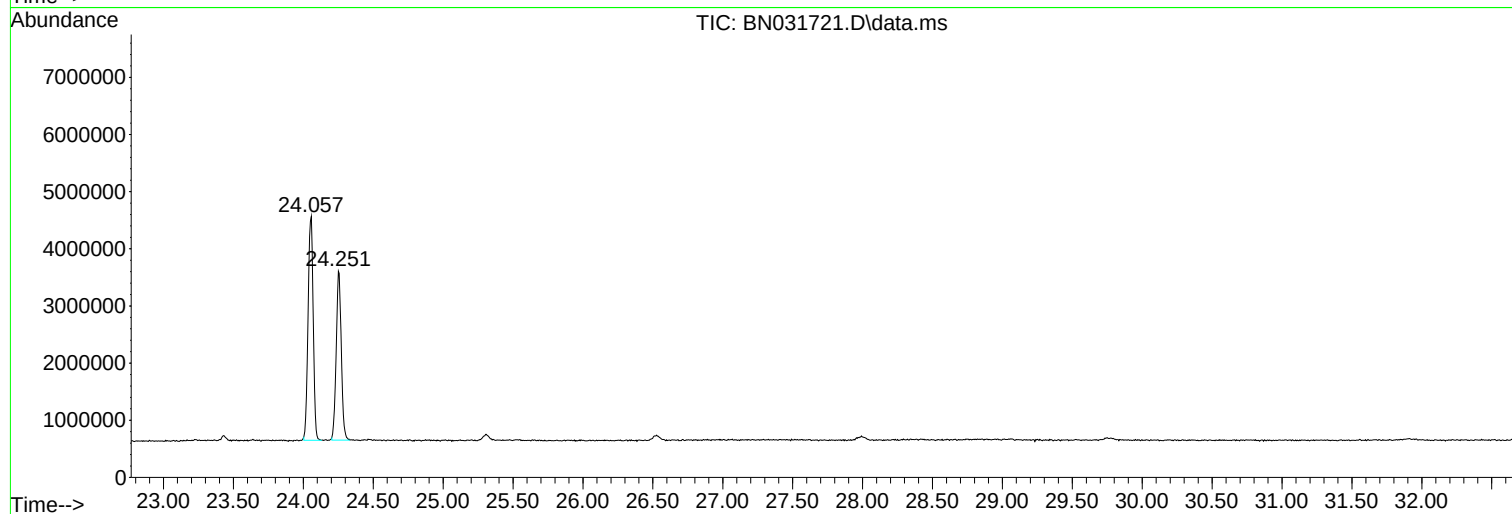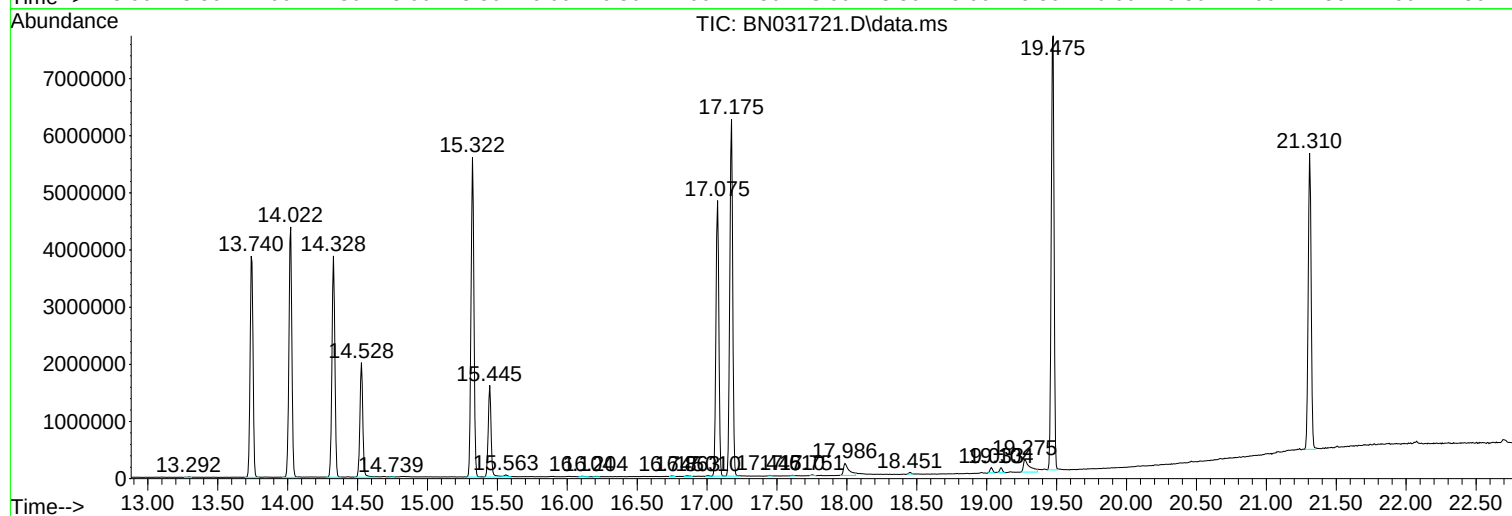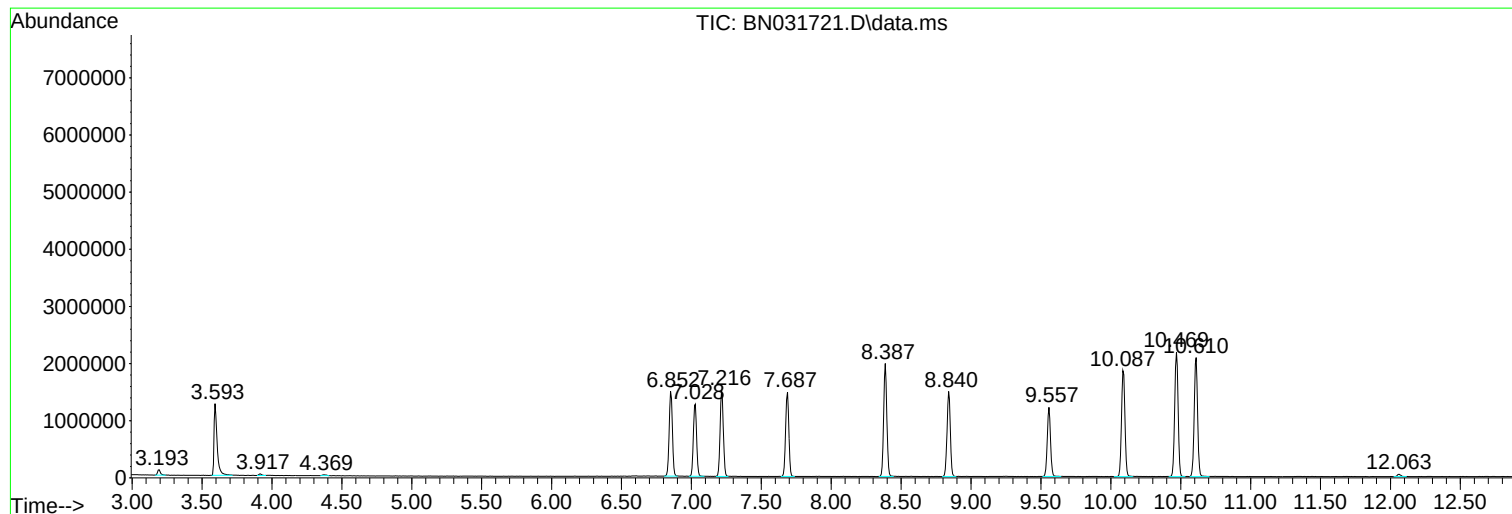

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053024\
Data File : BN031721.D
Acq On : 30 May 2024 18:20
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053024\
Data File : BN031721.D
Acq On : 30 May 2024 18:20
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------