
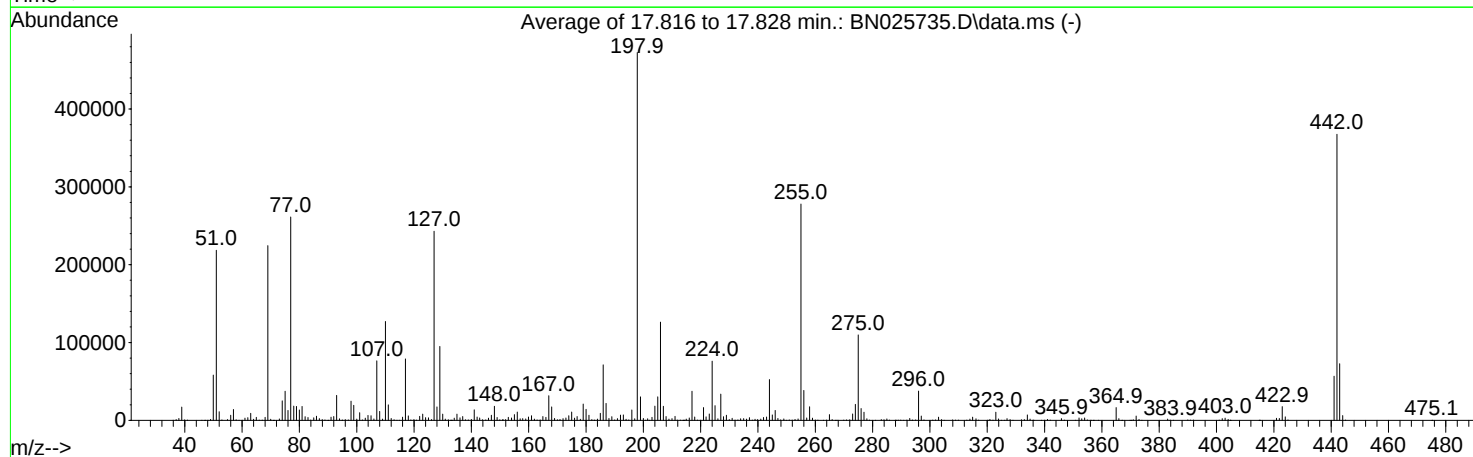


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053123\
 Data File : BN025735.D
 Acq On : 31 May 2023 12:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN053123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 01 01:04:04 2023

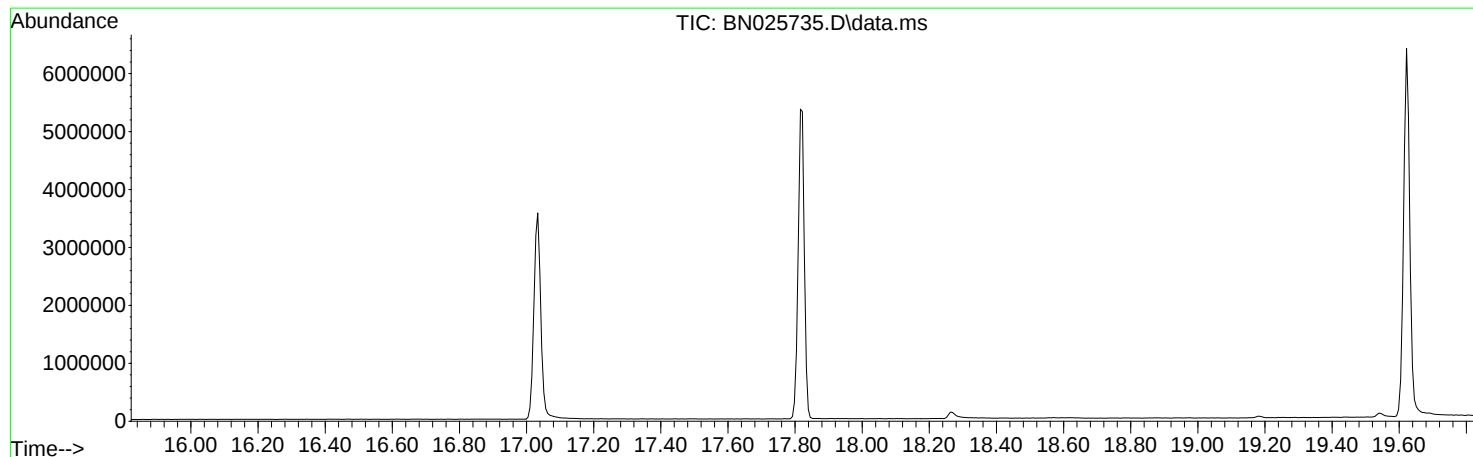

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	218507	PASS
68	69	0.00	2	1.7	3827	PASS
69	198	0.00	100	47.5	224600	PASS
70	69	0.00	2	0.6	1350	PASS
127	198	10	80	51.4	243051	PASS
197	198	0.00	2	0.4	2116	PASS
198	198	100	100	100.0	472661	PASS
199	198	5	9	6.4	30168	PASS
275	198	10	60	23.2	109819	PASS
365	198	1	100	3.5	16370	PASS
441	198	0.01	100	12.0	56819	PASS
442	442	50	100	100.0	367531	PASS
443	442	15	24	19.8	72720	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/31/2023	BNA_N	<u>BN025735.D</u>
Compound Name	Response	Retention Time
DDT	1306328	20.863
DDD	19869	20.469
DDE	558	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20427	1326755	1.54

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053123\
Data File : BN025735.D
Acq On : 31 May 2023 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 01 04:45:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 04:45:05 2023
Response via : Initial Calibration

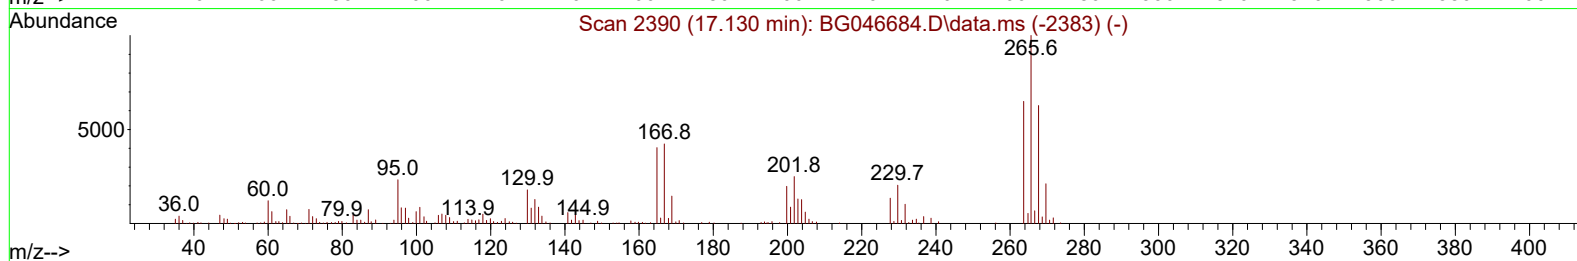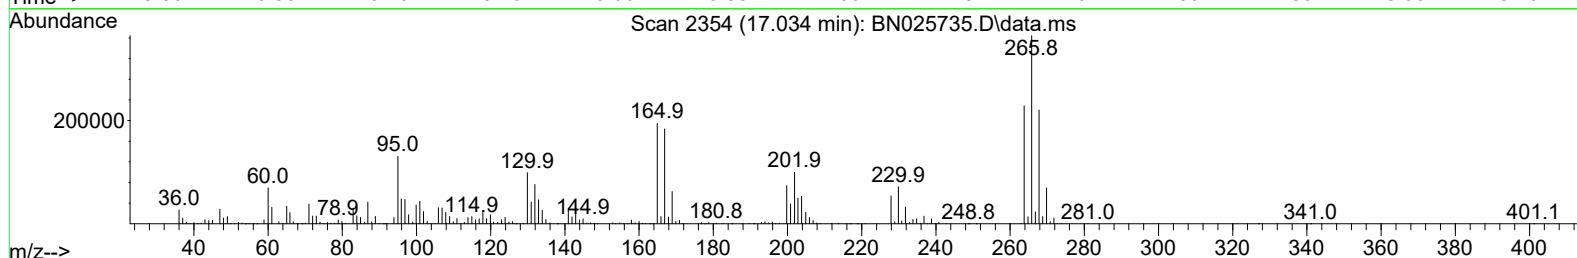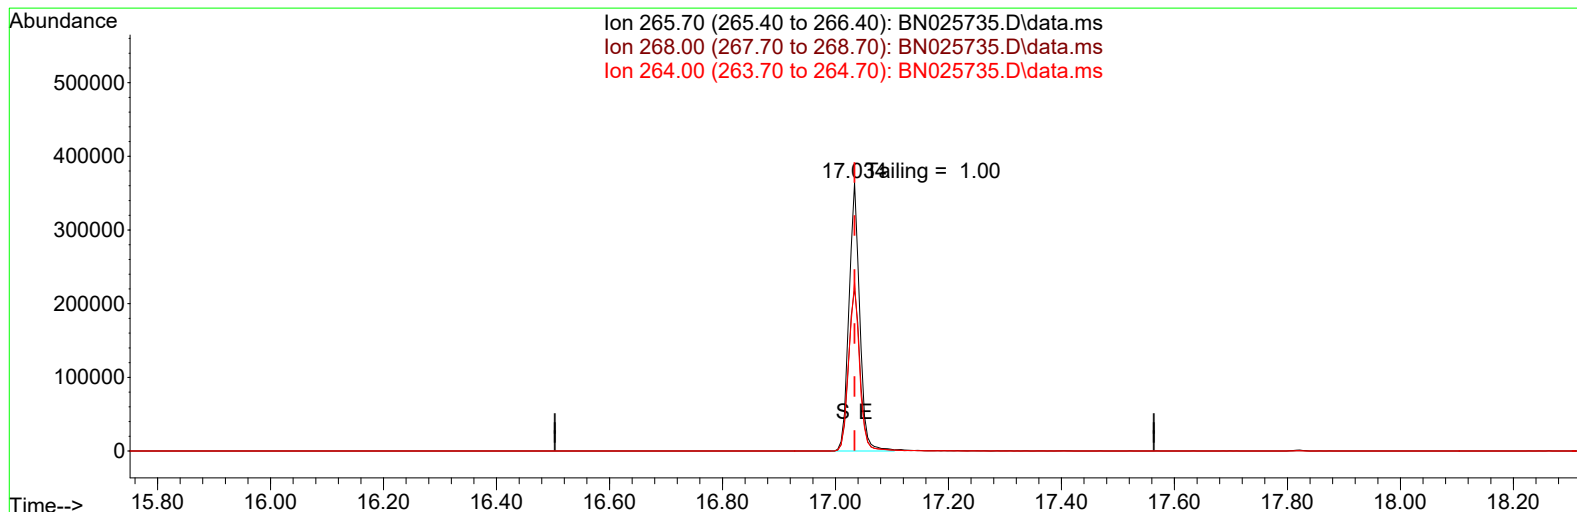

TIC: BN025735.D\data.ms

(70) Pentachlorophenol (C)

17.034min (0.000) 16236.06 ng




response 486094

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.56
264.00	61.60	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053123\
 Data File : BN025735.D
 Acq On : 31 May 2023 12:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 01 04:45:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 01 04:45:05 2023
 Response via : Initial Calibration

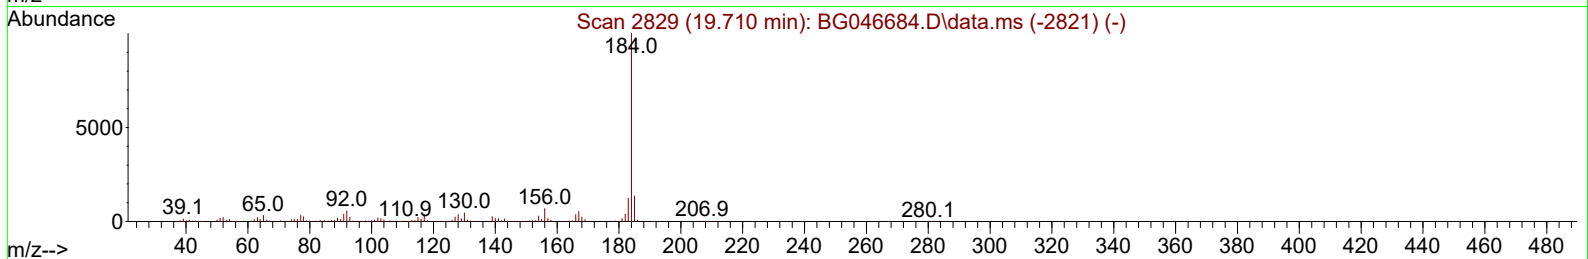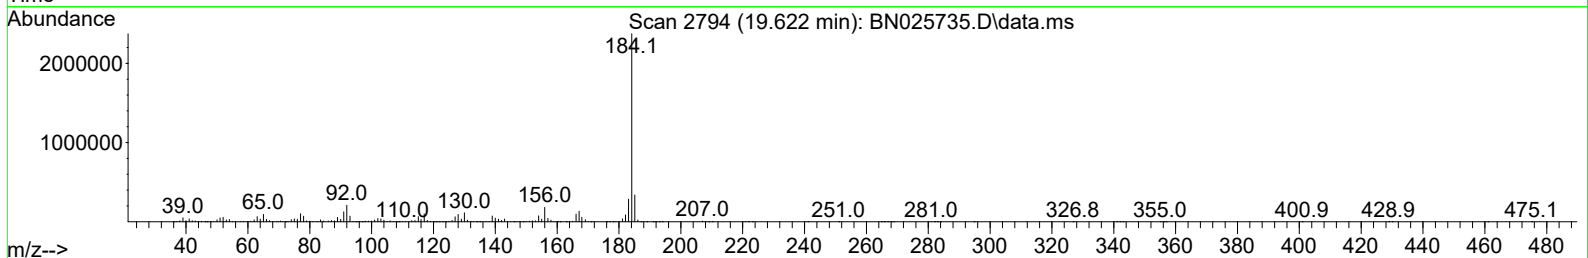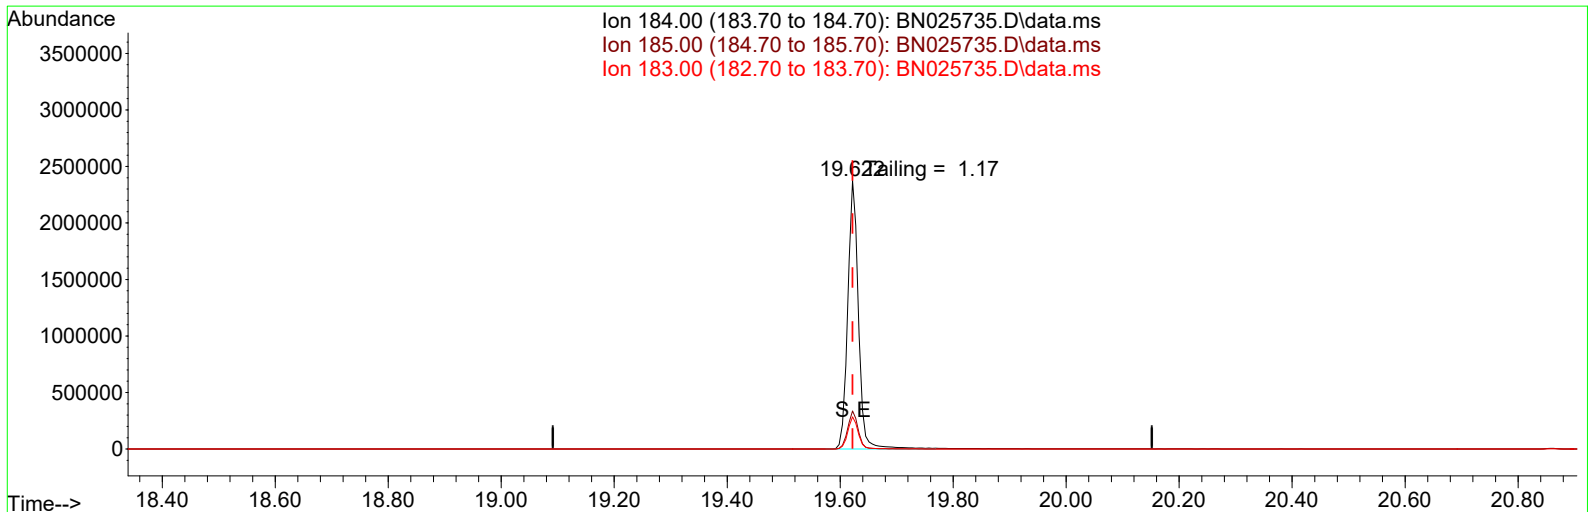

TIC: BN025735.D\data.ms

(77) Benzidine

19.622min (0.000) 0.00 ng

response 3152815

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.23
183.00	13.20	11.99
0.00	0.00	0.00