

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
 Data File : BN031736.D
 Acq On : 31 May 2024 11:04
 Operator : MA/JU
 Sample : PB161108BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK108

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	43	rVB	108832	158418	1.38%	0.131%
2	3.593	100	103	124	rBV	1411906	2192825	19.13%	1.812%
3	3.916	153	158	163	rBV	30355	43996	0.38%	0.036%
4	4.369	229	235	236	rBV4	8929	12122	0.11%	0.010%
5	6.851	646	657	668	rBV	1693591	2720968	23.73%	2.249%
6	7.022	677	686	698	rVB	1495348	2317683	20.22%	1.916%
7	7.216	708	719	726	rBV	1714440	2790255	24.34%	2.306%
8	7.681	791	798	807	rBV	1687923	2662734	23.23%	2.201%
9	8.381	910	917	929	rBV	2197837	3568437	31.13%	2.949%
10	8.834	986	994	1002	rBV	1676097	2778793	24.24%	2.297%
11	9.551	1109	1116	1126	rBV	1373793	2261981	19.73%	1.870%
12	10.086	1198	1207	1224	rBV	2079166	3548568	30.95%	2.933%
13	10.463	1262	1271	1280	rVB	2466066	4156365	36.26%	3.435%
14	10.604	1286	1295	1308	rBV	2332863	3956598	34.51%	3.270%
15	12.057	1534	1542	1549	rVB2	45014	72732	0.63%	0.060%
16	13.739	1821	1828	1837	rBV	4463258	6141787	53.57%	5.076%
17	14.016	1868	1875	1886	rBV2	4683078	7116690	62.08%	5.882%
18	14.322	1918	1927	1938	rBV	4172285	6181887	53.92%	5.109%
19	14.416	1941	1943	1949	rVB7	7324	13337	0.12%	0.011%
20	14.522	1955	1961	1982	rBV	2170734	3199205	27.91%	2.644%
21	14.739	1994	1998	2001	rBV6	7414	12680	0.11%	0.010%
22	15.316	2089	2096	2104	rBV	5939501	8906428	77.69%	7.361%
23	15.439	2110	2117	2133	rBV	1951786	2723055	23.75%	2.251%
24	15.557	2133	2137	2142	rVB	32408	48243	0.42%	0.040%
25	16.104	2225	2230	2233	rBV5	8914	11708	0.10%	0.010%
26	16.751	2336	2340	2344	rVB6	11078	16221	0.14%	0.013%
27	16.851	2354	2357	2364	rVB3	12588	22576	0.20%	0.019%
28	17.068	2387	2394	2404	rBV	5290037	7637679	66.62%	6.313%
29	17.168	2404	2411	2421	rBV2	6704213	9869391	86.09%	8.157%
30	17.445	2454	2458	2464	rBV3	10205	16203	0.14%	0.013%
31	17.974	2544	2548	2558	rBV2	138713	318177	2.78%	0.263%
32	19.027	2723	2727	2733	rBV2	98202	133893	1.17%	0.111%
33	19.098	2735	2739	2744	rBV	92201	133410	1.16%	0.110%
34	19.262	2764	2767	2777	rBV4	75437	170583	1.49%	0.141%
35	19.468	2795	2802	2808	rBV	8363235	11464056	100.00%	9.475%
36	21.304	3108	3114	3122	rBV	5336814	7545458	65.82%	6.236%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031736.D
Acq On : 31 May 2024 11:04
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	24.039	3570	3579	3590	rVB	3646312	9018574	78.67%	7.454%
38	24.245	3605	3614	3632	rVB	2671178	7045708	61.46%	5.823%




Sum of corrected areas: 120989424

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031736.D
Acq On : 31 May 2024 11:04
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

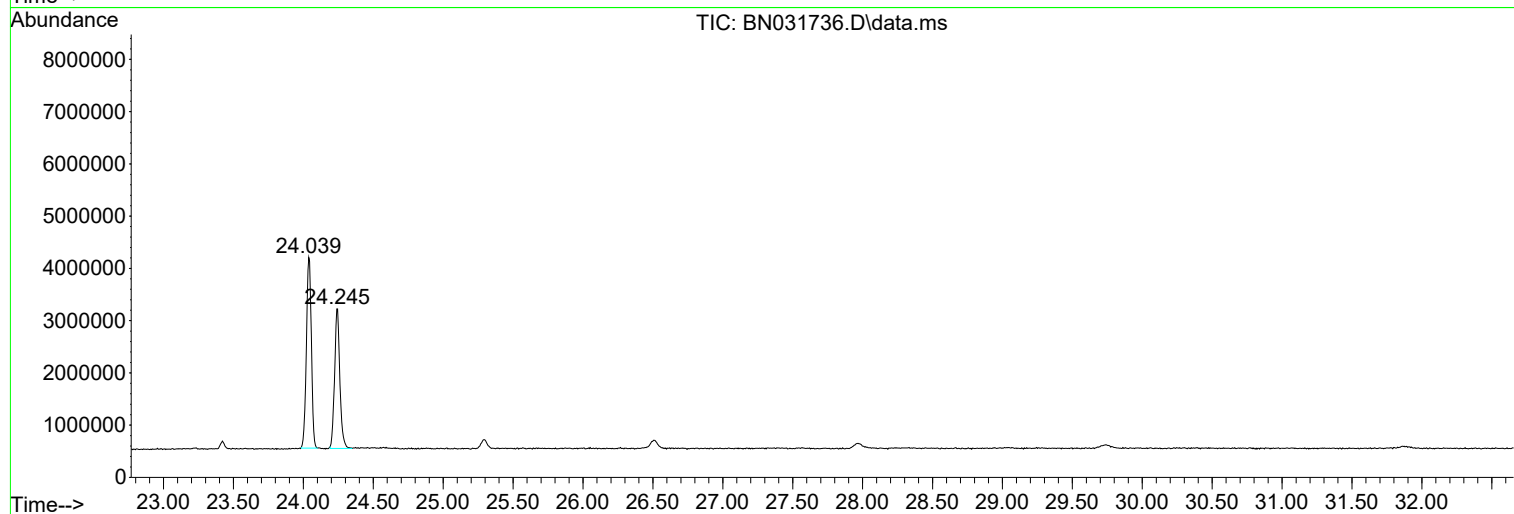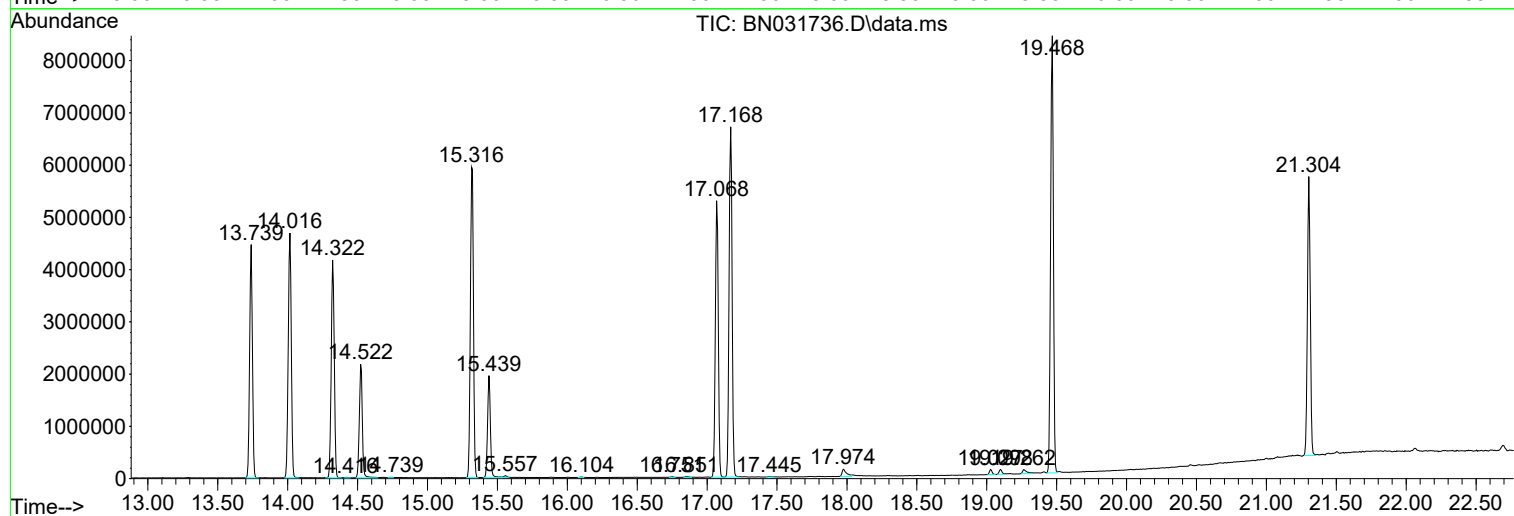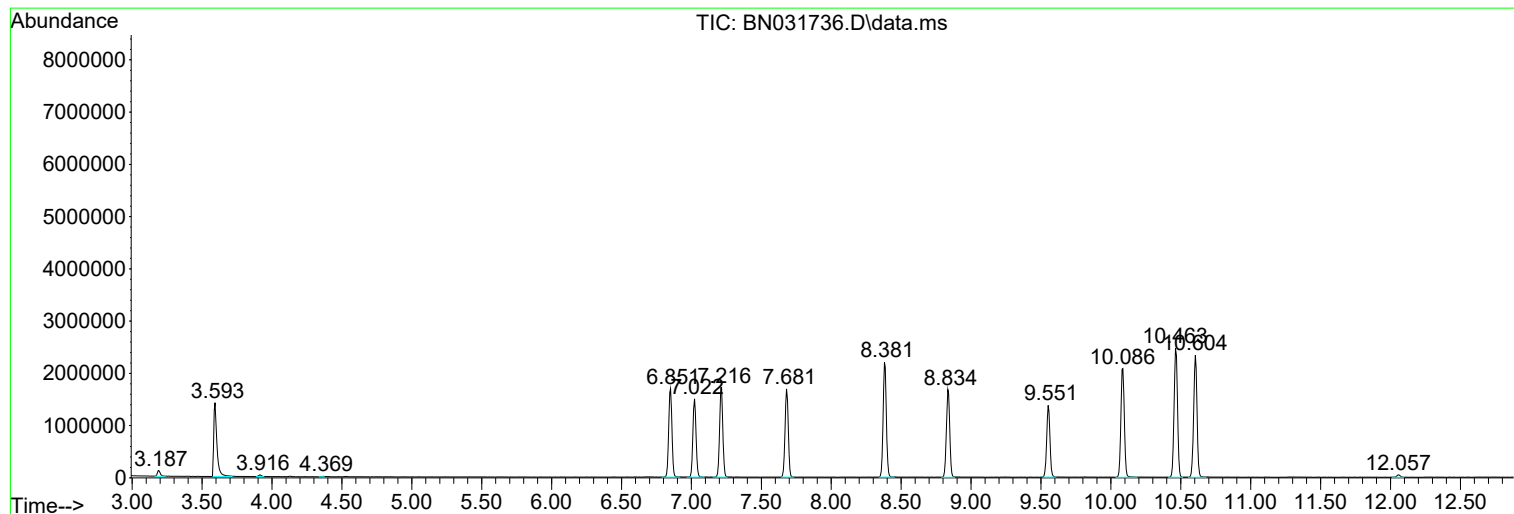

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031736.D
Acq On : 31 May 2024 11:04
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031736.D
Acq On : 31 May 2024 11:04
Operator : MA/JU
Sample : PB161108BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK108

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------