

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
 Data File : BN031739.D
 Acq On : 31 May 2024 13:02
 Operator : MA/JU
 Sample : P2569-07DL2 20X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH647DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.705	118	122	129	rVB	31620	43658	0.24%	0.076%
2	3.917	153	158	163	rBV	54489	83823	0.46%	0.146%
3	4.370	228	235	241	rVB2	9274	21990	0.12%	0.038%
4	4.911	322	327	334	rVB5	8843	19369	0.11%	0.034%
5	6.852	647	657	667	rVB	90952	169132	0.92%	0.294%
6	7.022	680	686	693	rBV	80780	127711	0.70%	0.222%
7	7.216	713	719	726	rBV	95913	161882	0.88%	0.282%
8	7.681	790	798	805	rBV	2073021	3266619	17.83%	5.683%
9	7.746	805	809	816	rVB	50394	83535	0.46%	0.145%
10	8.381	912	917	926	rVB	57537	96715	0.53%	0.168%
11	8.834	988	994	1001	rBV	88730	149297	0.81%	0.260%
12	9.552	1109	1116	1125	rBV	62323	112652	0.61%	0.196%
13	10.087	1199	1207	1215	rVB	112404	188738	1.03%	0.328%
14	10.463	1263	1271	1284	rVB	2972928	5228944	28.54%	9.096%
15	10.604	1289	1295	1308	rVB	59596	119836	0.65%	0.208%
16	11.210	1392	1398	1403	rBV2	12955	22880	0.12%	0.040%
17	13.740	1821	1828	1837	rVB	232126	324180	1.77%	0.564%
18	14.016	1863	1875	1880	rBV	264073	427868	2.33%	0.744%
19	14.228	1908	1911	1916	rVB4	14559	21037	0.11%	0.037%
20	14.322	1920	1927	1944	rVB	4629601	7155748	39.05%	12.448%
21	14.528	1957	1962	1969	rBV5	41766	82653	0.45%	0.144%
22	15.316	2090	2096	2103	rBV	352382	514281	2.81%	0.895%
23	16.045	2216	2220	2228	rVB4	16862	31029	0.17%	0.054%
24	16.851	2352	2357	2362	rBV3	18645	40810	0.22%	0.071%
25	17.069	2388	2394	2400	rBV	5422692	7871019	42.95%	13.693%
26	17.110	2400	2401	2406	rVB	97834	94626	0.52%	0.165%
27	17.169	2406	2411	2416	rBV	323266	460837	2.51%	0.802%
28	17.463	2457	2461	2467	rVB4	48776	74365	0.41%	0.129%
29	17.751	2506	2510	2515	rBV	53953	72812	0.40%	0.127%
30	17.975	2544	2548	2557	rBV2	177890	328007	1.79%	0.571%
31	18.839	2692	2695	2699	rBV3	78229	98913	0.54%	0.172%
32	19.063	2731	2733	2736	rVB	55455	50217	0.27%	0.087%
33	19.133	2741	2745	2750	rVB	270492	347651	1.90%	0.605%
34	19.269	2764	2768	2774	rBV5	116605	279003	1.52%	0.485%
35	19.463	2797	2801	2804	rBV	413847	584065	3.19%	1.016%
36	21.222	3095	3100	3106	rVB	13741596	18324324	100.00%	31.877%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031739.D
Acq On : 31 May 2024 13:02
Operator : MA/JU
Sample : P2569-07DL2 20X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH647DL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	21.304	3109	3114	3120	rVB2	3506634	5314472	29.00%	9.245%
38	24.245	3607	3614	3624	rVB	1991862	5089378	27.77%	8.854%




Sum of corrected areas: 57484076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031739.D
Acq On : 31 May 2024 13:02
Operator : MA/JU
Sample : P2569-07DL2 20X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH647DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

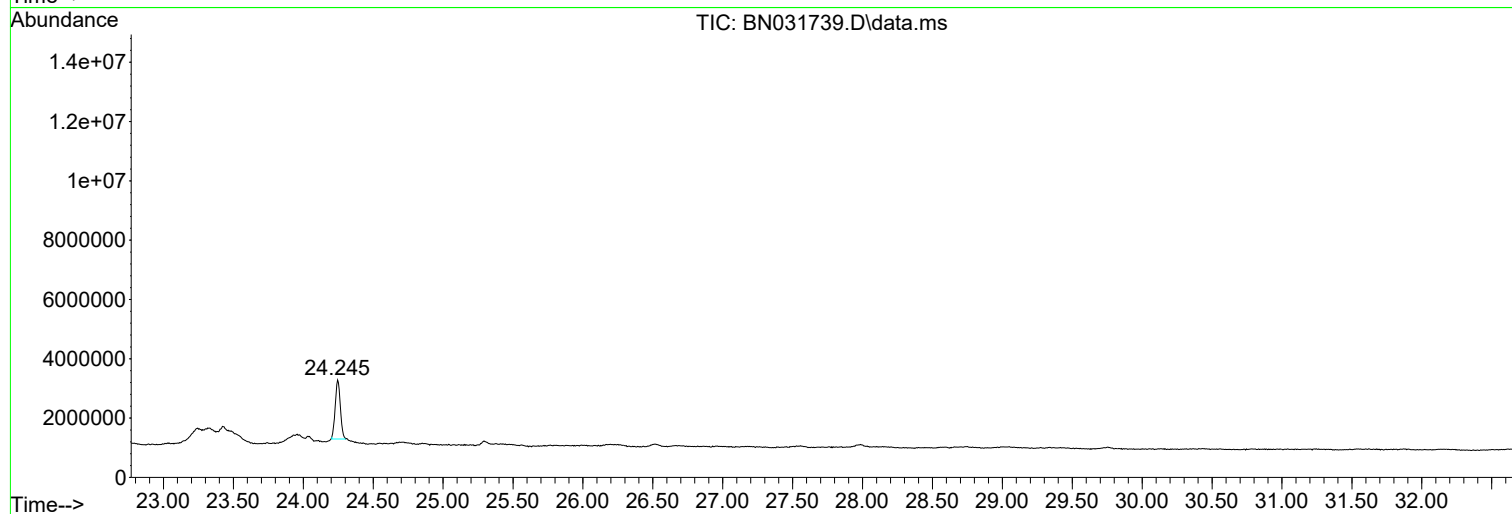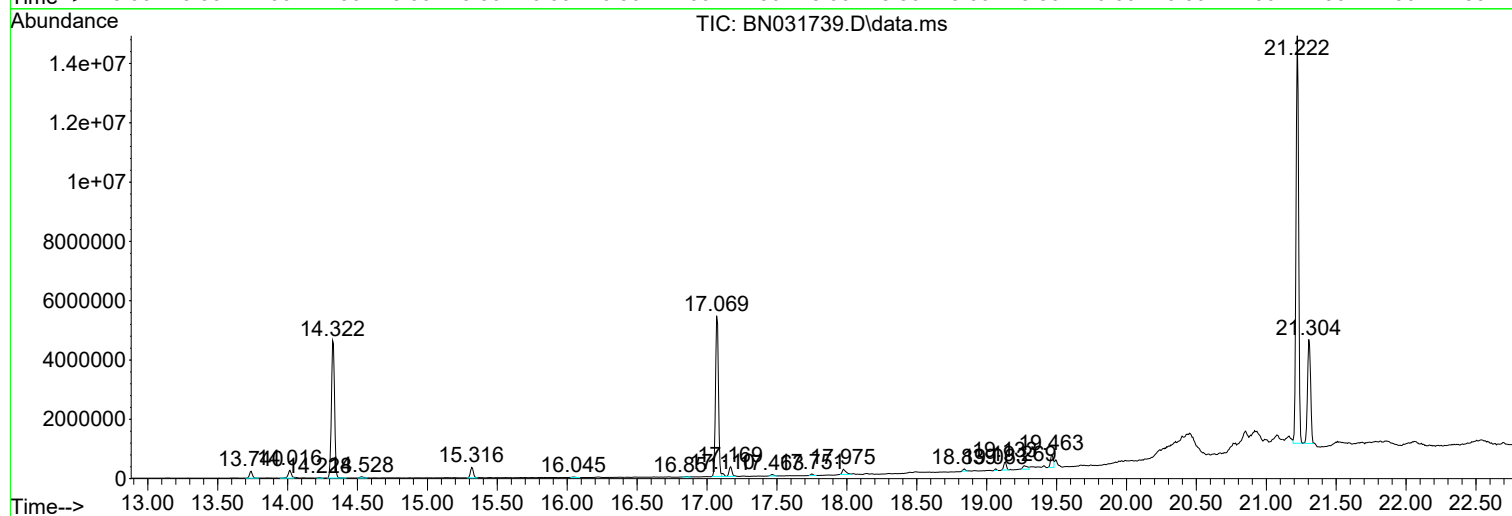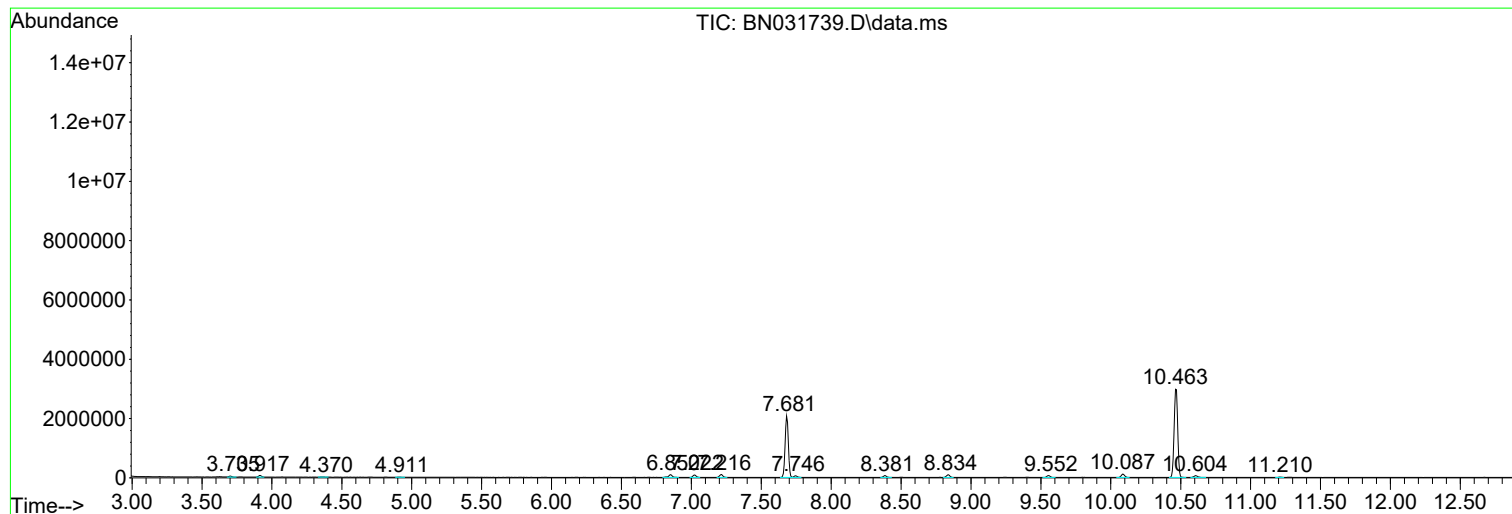

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031739.D
Acq On : 31 May 2024 13:02
Operator : MA/JU
Sample : P2569-07DL2 20X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH647DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN053124\
Data File : BN031739.D
Acq On : 31 May 2024 13:02
Operator : MA/JU
Sample : P2569-07DL2 20X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH647DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc