

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
 Data File : BN006011.D
 Acq On : 02 Jun 2019 01:31
 Operator : JU/SJ
 Sample : K2846-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 03 01:07:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 01 01:49:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	352302	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.52	136	1603419	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.38	164	993927	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.14	188	2239704	20.00	ng/ul	-0.02
77) Chrysene-d12	21.35	240	2134194	20.00	ng/ul	-0.02
85) Perylene-d12	23.64	264	2369214	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	53050	6.63	ng/uL	0.00
5) Phenol-d5	6.89	99	946128	30.30	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.06	67	633525	35.56	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	762887	32.07	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	813024	32.25	ng/ul	-0.02
19) Nitrobenzene-d5	8.88	128	427399	41.53	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	476947	49.76	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.14	165	755189	33.37	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.65	131	1153801	38.89	ng/ul	-0.02
43) Dimethylphthalate-d6	13.79	166	2961130	40.41	ng/ul	-0.01
46) Acenaphthylene-d8	14.08	160	3232134	35.26	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.59	143	423507	31.76	ng/ul	-0.02
57) Fluorene-d10	15.38	176	2318990	37.74	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.51	200	394838	43.25	ng/ul	-0.02
70) Anthracene-d10	17.24	188	3519808	36.93	ng/ul	-0.02
78) Pyrene-d10	19.55	212	3691203	34.25	ng/ul	-0.02
89) Benzo(a)pyrene-d12	23.49	264	3578451	33.85	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.92	94	84031	2.612	ng/ul	95
44) Dimethylphthalate	13.84	163	541314	7.391	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
Data File : BN006011.D
Acq On : 02 Jun 2019 01:31
Operator : JU/SJ
Sample : K2846-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 03 01:07:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 01 01:49:29 2019
Response via : Initial Calibration

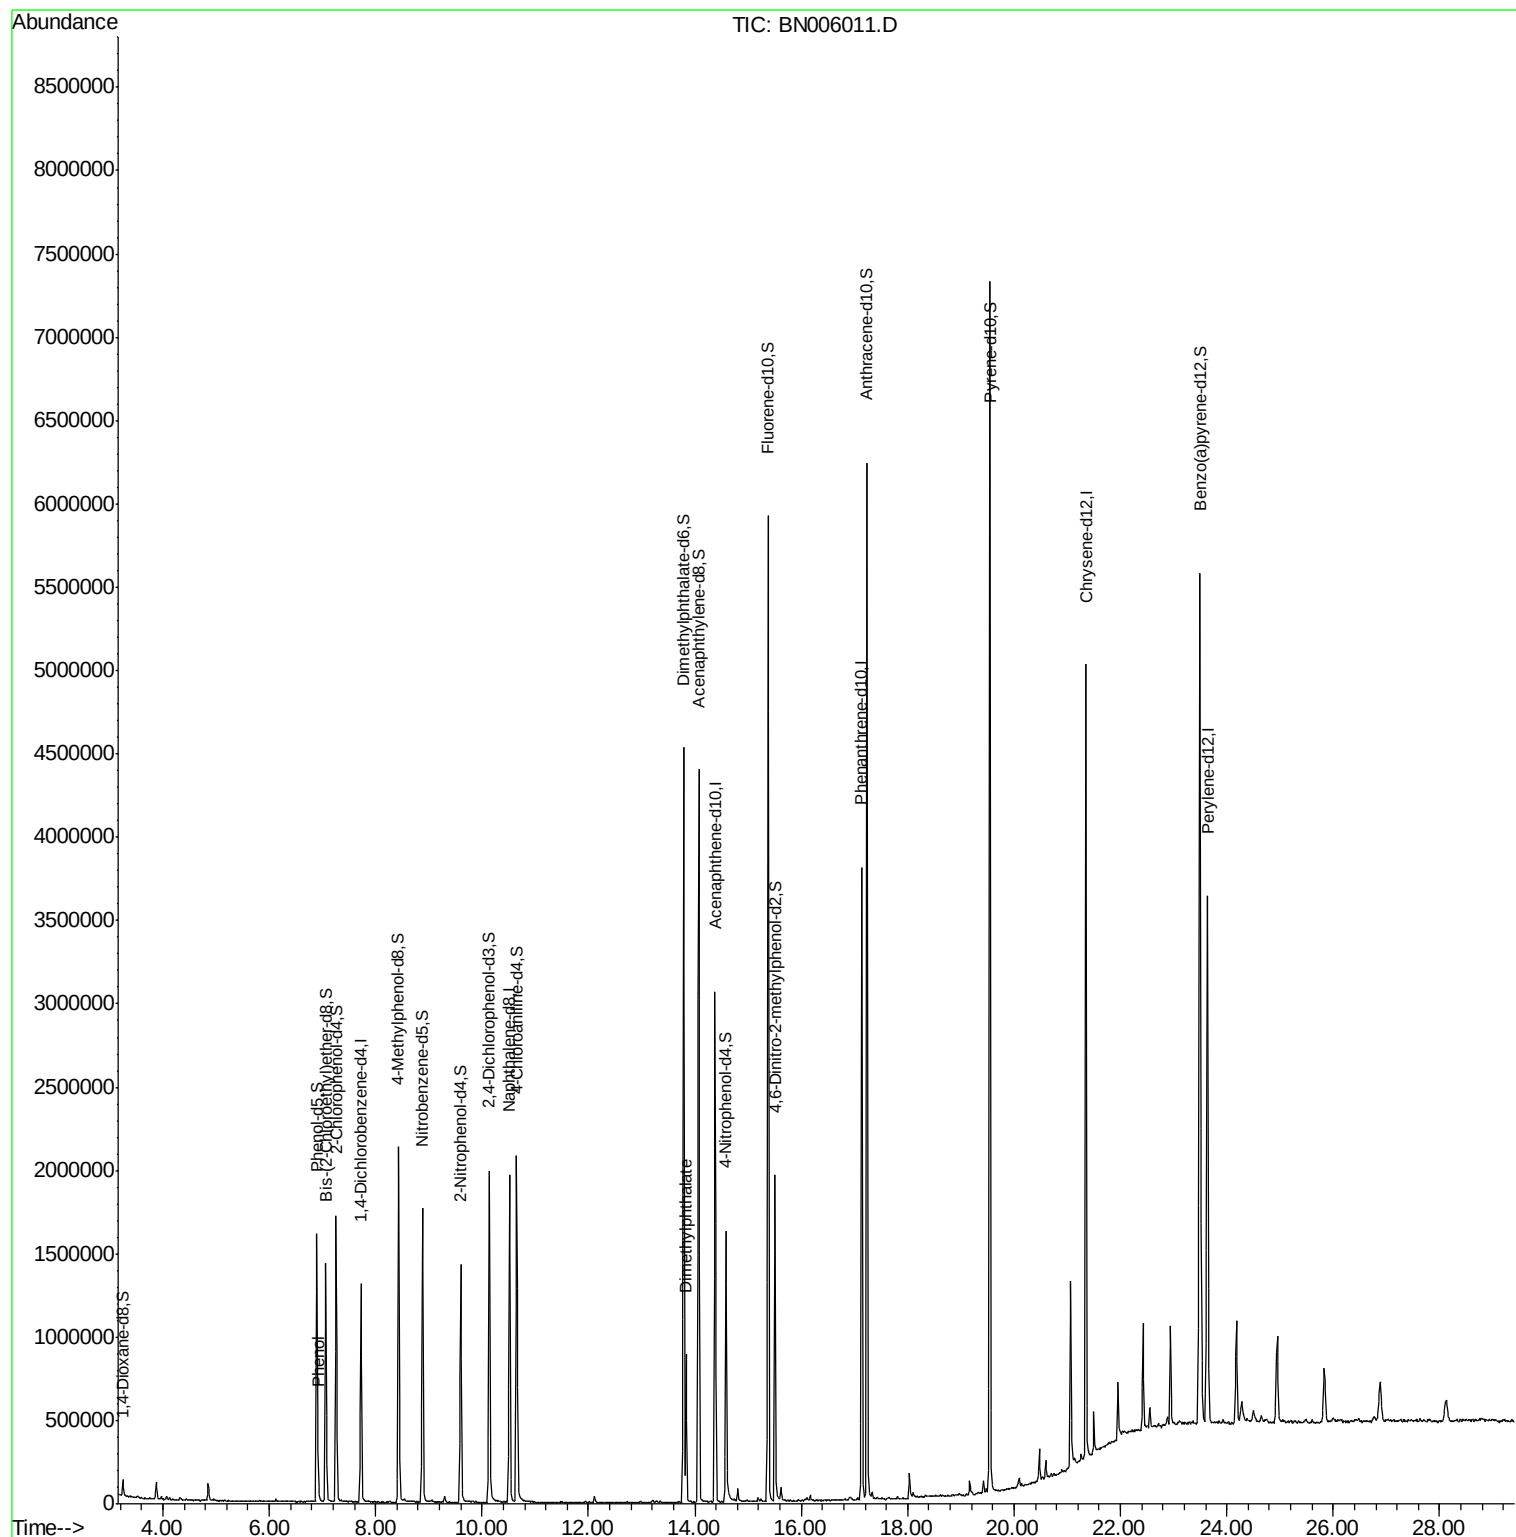

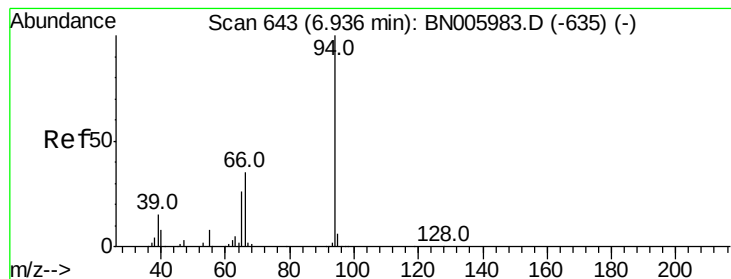





#6

Phenol

Concen: 2.612 ng/ul
 RT: 6.92 min Scan# 641
 Delta R.T. -0.01 min
 Lab File: BN006011.D
 Acq: 02 Jun 2019 01:31

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 94 Resp: 84031
 Ion Ratio Lower Upper
 94 100
 65 27.6 24.2 36.4
 66 39.0 33.8 50.6

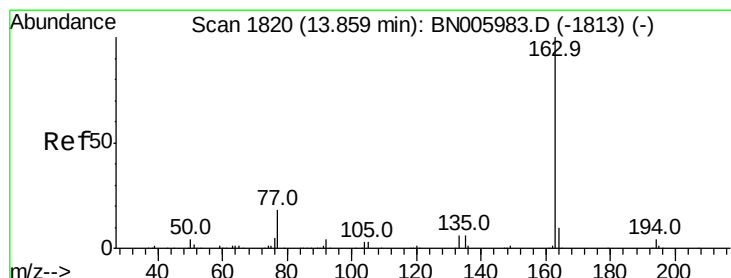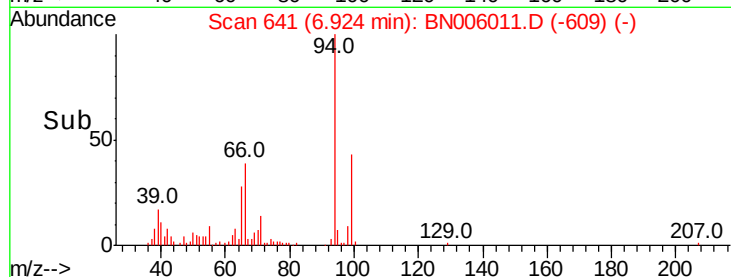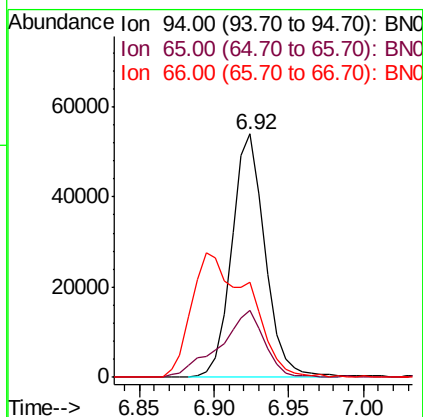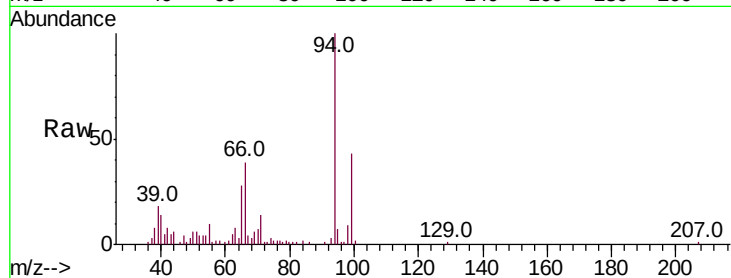

#44

Dimethylphthalate

Concen: 7.391 ng/ul
 RT: 13.84 min Scan# 1816
 Delta R.T. -0.02 min
 Lab File: BN006011.D
 Acq: 02 Jun 2019 01:31

Tgt Ion:163 Resp: 541314
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.0
 164 10.5 8.1 12.1

