

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060119\
 Data File : BN006027.D
 Acq On : 02 Jun 2019 11:51
 Operator : JU/SJ
 Sample : K2846-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jun 03 01:09:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jun 01 01:49:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	507775	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.52	136	2171349	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.38	164	1196338	20.00	ng/ul	-0.02
61) Phenanthrene-d10	17.14	188	2356140	20.00	ng/ul	-0.02
77) Chrysene-d12	21.36	240	1517422	20.00	ng/ul	-0.02
85) Perylene-d12	23.65	264	1618314	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	35891	3.11	ng/uL	0.00
5) Phenol-d5	6.89	99	699036	15.53	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	7.06	67	455092	17.72	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.26	132	570457	16.64	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	534623	14.72	ng/ul	-0.02
19) Nitrobenzene-d5	8.88	128	301792	21.66	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	313225	24.13	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.14	165	527015	17.20	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.65	131	721517	17.96	ng/ul	-0.02
43) Dimethylphthalate-d6	13.79	166	1767551	20.04	ng/ul	-0.01
46) Acenaphthylene-d8	14.07	160	1997961	18.11	ng/ul	-0.02
51) 4-Nitrophenol-d4	14.59	143	199952	12.46	ng/ul	-0.02
57) Fluorene-d10	15.38	176	1384290	18.72	ng/ul	-0.02
62) 4,6-Dinitro-2-methylphenol	15.51	200	45361	4.72	ng/ul	-0.02
70) Anthracene-d10	17.24	188	1856188	18.51	ng/ul	-0.02
78) Pyrene-d10	19.55	212	1671420	21.81	ng/ul	-0.02
89) Benzo(a)pyrene-d12	23.50	264	1316507	18.23	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.84	163	458047	5.196	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
Data File : BN006027.D
Acq On : 02 Jun 2019 11:51
Operator : JU/SJ
Sample : K2846-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jun 03 01:09:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jun 01 01:49:29 2019
Response via : Initial Calibration

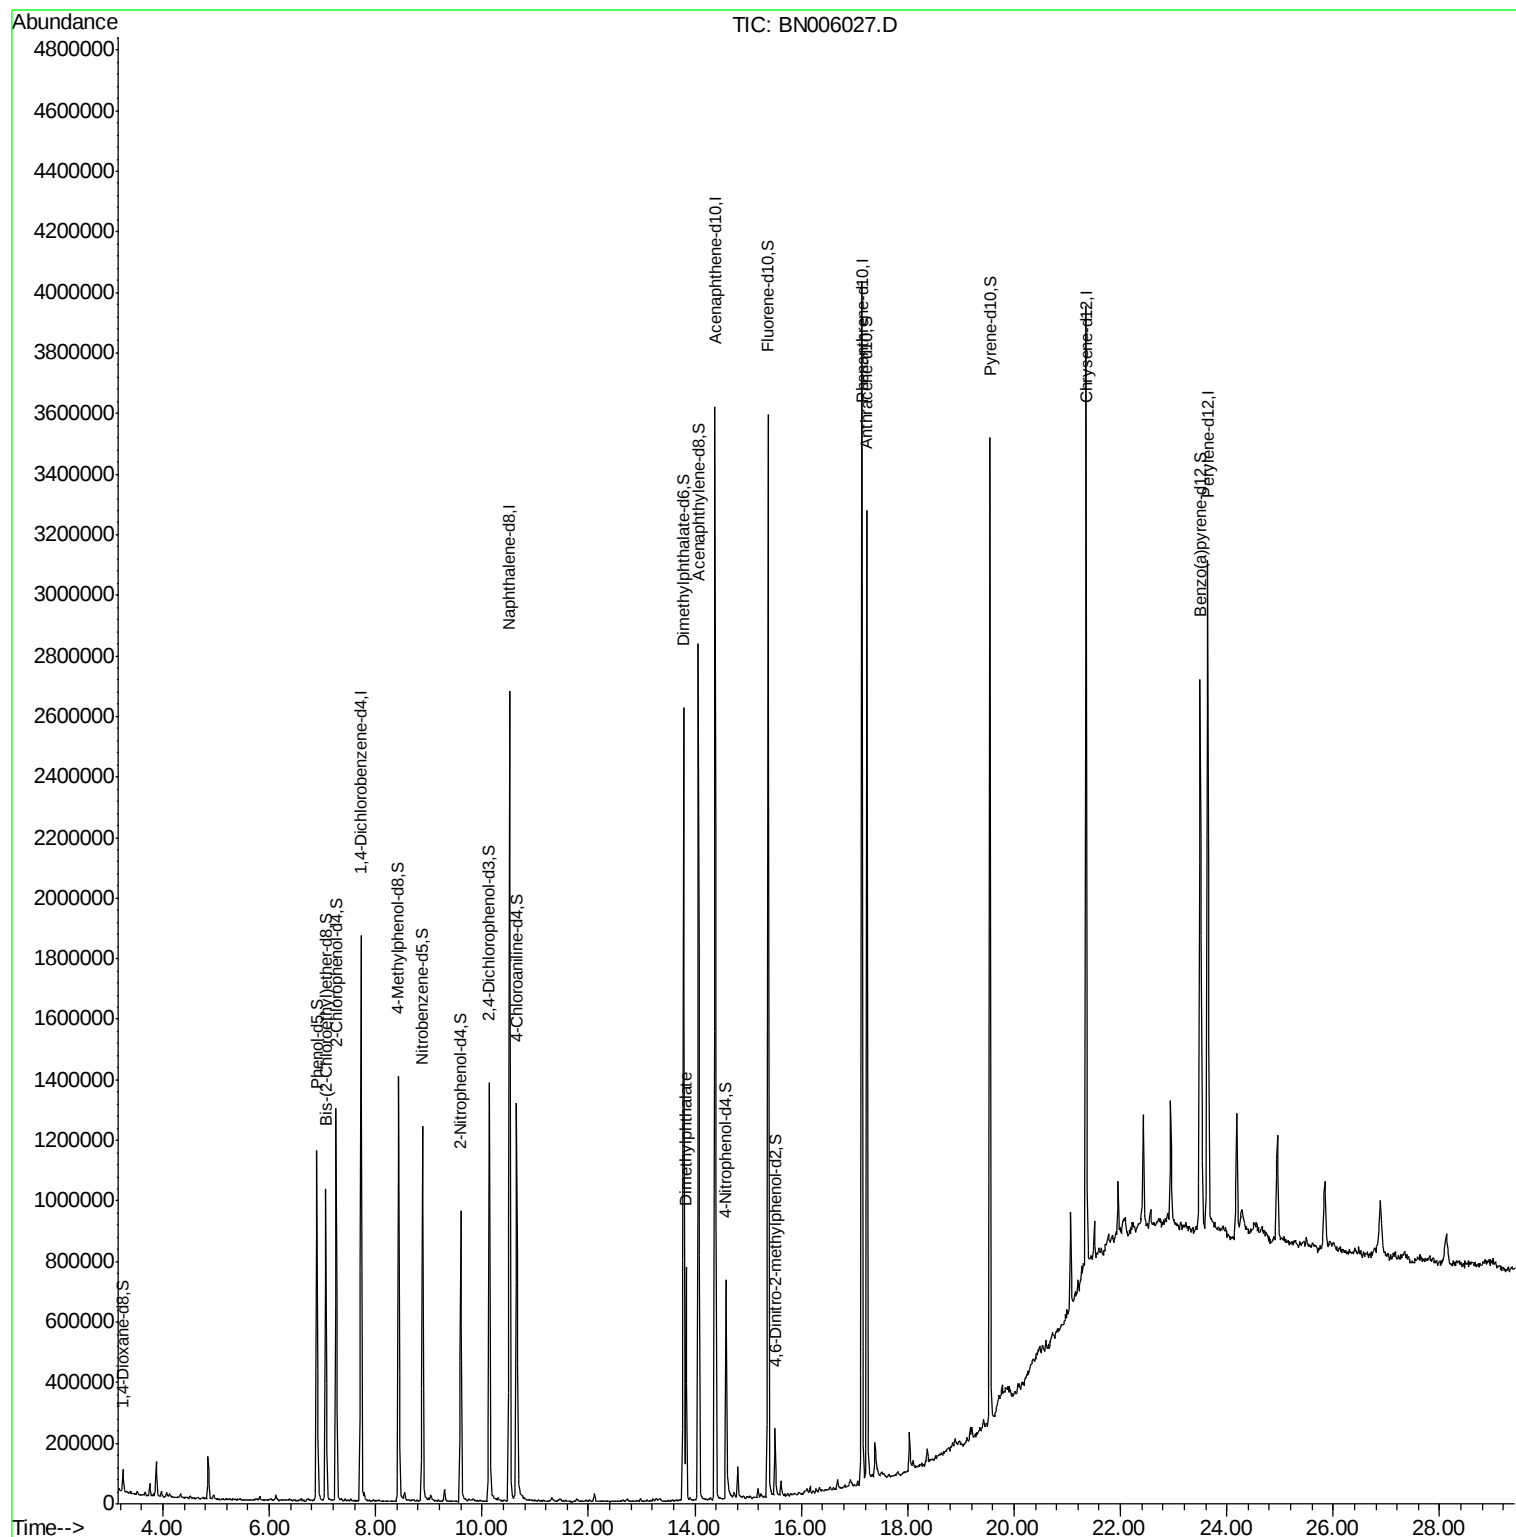

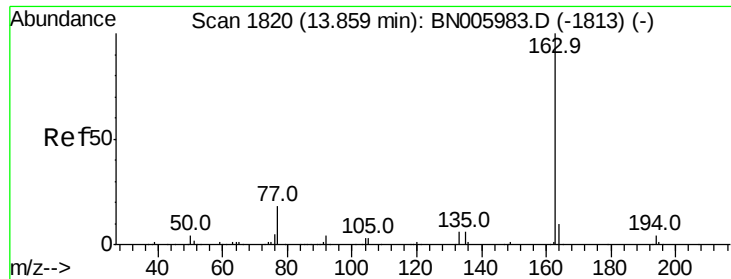

#44

Dimethylphthalate

Concen: 5.196 ng/ul

RT: 13.84 min Scan# 1816

Delta R.T. -0.02 min

Lab File: BN006027.D

Acq: 02 Jun 2019 11:51

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 458047

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.2 8.1 12.1

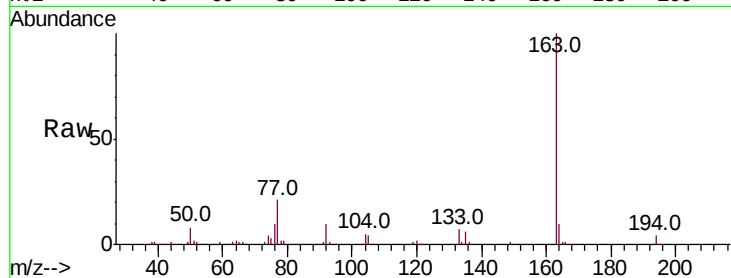

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

