

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060119\
 Data File : BN006023.D
 Acq On : 02 Jun 2019 09:33
 Operator : JU/SJ
 Sample : K2846-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.248	13	16	26	rVB	67381	99135	1.85%	0.150%
2	3.666	82	87	91	rVB2	12513	18567	0.35%	0.028%
3	3.754	98	102	111	rVB	63928	87026	1.62%	0.132%
4	3.824	111	114	117	rBV3	9545	12972	0.24%	0.020%
5	3.877	117	123	128	rVB	94236	137279	2.56%	0.208%
6	3.971	135	139	145	rVB	23914	36448	0.68%	0.055%
7	4.066	151	155	161	rBV3	14467	21165	0.39%	0.032%
8	4.130	162	166	170	rVB6	7409	11497	0.21%	0.017%
9	4.324	194	199	205	rBV4	14298	23466	0.44%	0.036%
10	4.507	227	230	235	rVB3	16265	21594	0.40%	0.033%
11	4.648	252	254	258	rVB5	4628	5767	0.11%	0.009%
12	4.748	269	271	274	rBV3	5107	5708	0.11%	0.009%
13	4.854	284	289	296	rBV	108765	166251	3.10%	0.252%
14	4.954	301	306	311	rBV5	16120	25375	0.47%	0.038%
15	5.442	388	389	395	rVB6	6102	8047	0.15%	0.012%
16	5.801	446	450	451	rBV4	5284	7085	0.13%	0.011%
17	5.818	451	453	460	rVB	13780	19926	0.37%	0.030%
18	6.130	501	506	511	rVB	15633	23663	0.44%	0.036%
19	6.377	544	548	553	rVB4	6487	9894	0.18%	0.015%
20	6.601	582	586	591	rBV5	8379	12767	0.24%	0.019%
21	6.718	602	606	609	rBV5	5605	7346	0.14%	0.011%
22	6.895	626	636	651	rBV	1018490	1919988	35.82%	2.906%
23	7.060	658	664	679	rVB	933694	1473660	27.49%	2.230%
24	7.260	691	698	709	rBV	1173571	1825882	34.07%	2.764%
25	7.724	770	777	785	rBV	1837914	2974553	55.50%	4.502%
26	7.783	785	787	793	rVB5	18504	27660	0.52%	0.042%
27	8.148	846	849	855	rVB7	6582	9558	0.18%	0.014%
28	8.283	867	872	874	rBV5	3733	5680	0.11%	0.009%
29	8.430	890	897	911	rBV	1292016	2109218	39.35%	3.192%
30	8.548	913	917	922	rVB	35694	52139	0.97%	0.079%
31	8.683	936	940	944	rBV6	3090	5898	0.11%	0.009%
32	8.883	967	974	984	rBV	1093458	1811532	33.80%	2.742%
33	8.989	990	992	995	rVB4	5101	5365	0.10%	0.008%
34	9.036	997	1000	1007	rVV8	10562	21601	0.40%	0.033%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060119\
 Data File : BN006023.D
 Acq On : 02 Jun 2019 09:33
 Operator : JU/SJ
 Sample : K2846-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFHB6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
 Title : SVOA CALIBRATION

35	9.301	1037	1045	1050	rVB	16118	27837	0.52%	0.042%
36	9.436	1065	1068	1072	rVB6	3741	5669	0.11%	0.009%
37	9.601	1089	1096	1109	rBV	823860	1404614	26.21%	2.126%
38	9.689	1109	1111	1118	rVB7	6348	9303	0.17%	0.014%
39	9.748	1118	1121	1125	rBV5	5916	9887	0.18%	0.015%
40	9.865	1138	1141	1147	rVB7	6256	8958	0.17%	0.014%
41	9.953	1153	1156	1163	rVB6	8107	14968	0.28%	0.023%
42	10.136	1177	1187	1198	rBV	1242591	2181894	40.71%	3.302%
43	10.518	1240	1252	1263	rBV	2504234	4309432	80.40%	6.522%
44	10.653	1268	1275	1294	rVV	956965	1744325	32.54%	2.640%
45	10.912	1317	1319	1328	rVB8	6420	14199	0.26%	0.021%
46	11.000	1332	1334	1338	rVB4	5491	6121	0.11%	0.009%
47	11.059	1340	1344	1346	rVB4	6968	8929	0.17%	0.014%
48	11.118	1351	1354	1359	rVB7	3458	5441	0.10%	0.008%
49	11.306	1382	1386	1390	rBV4	12514	18149	0.34%	0.027%
50	11.348	1390	1393	1399	rVB8	6978	12207	0.23%	0.018%
51	11.430	1403	1407	1413	rVB8	8782	15759	0.29%	0.024%
52	11.559	1422	1429	1430	rBV7	7054	13051	0.24%	0.020%
53	11.571	1430	1431	1436	rVB5	10295	12420	0.23%	0.019%
54	11.706	1449	1454	1459	rBV6	9724	19989	0.37%	0.030%
55	11.795	1465	1469	1474	rBV6	5550	8734	0.16%	0.013%
56	11.848	1474	1478	1480	rBV4	6670	7926	0.15%	0.012%
57	11.947	1490	1495	1496	rBV4	4445	5791	0.11%	0.009%
58	12.006	1503	1505	1510	rVB6	5348	9007	0.17%	0.014%
59	12.112	1517	1523	1530	rBV2	27076	56199	1.05%	0.085%
60	12.259	1543	1548	1551	rBV6	7267	13810	0.26%	0.021%
61	12.324	1554	1559	1560	rVV5	5176	7028	0.13%	0.011%
62	12.353	1561	1564	1568	rVV4	8599	14286	0.27%	0.022%
63	12.383	1568	1569	1574	rVB5	5225	6272	0.12%	0.009%
64	12.571	1596	1601	1602	rBV4	7811	8178	0.15%	0.012%
65	12.724	1623	1627	1631	rVB6	13342	19465	0.36%	0.029%
66	12.812	1636	1642	1645	rVV7	13283	23543	0.44%	0.036%
67	12.977	1666	1670	1674	rVB5	11941	16055	0.30%	0.024%
68	13.047	1678	1682	1685	rBV6	4905	9022	0.17%	0.014%
69	13.153	1698	1700	1701	rBV2	5837	5653	0.11%	0.009%
70	13.183	1703	1705	1710	rVB6	8156	10714	0.20%	0.016%
71	13.271	1716	1720	1723	rBV7	8273	14360	0.27%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
Data File : BN006023.D
Acq On : 02 Jun 2019 09:33
Operator : JU/SJ
Sample : K2846-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHB6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Title : SVOA CALIBRATION

72	13.436	1744	1748	1750	rVB5	9595	11144	0.21%	0.017%
73	13.789	1802	1808	1813	rBV	2325698	3388864	63.23%	5.129%
74	13.836	1813	1816	1825	rVB	667251	854093	15.93%	1.293%
75	14.071	1850	1856	1869	rVB	2438594	3697368	68.98%	5.596%
76	14.277	1889	1891	1895	rVB5	13794	14170	0.26%	0.021%
77	14.383	1902	1909	1923	rBV2	3405318	5359863	100.00%	8.112%
78	14.594	1940	1945	1956	rVB	151453	288513	5.38%	0.437%
79	14.736	1967	1969	1975	rVB5	24325	34091	0.64%	0.052%
80	14.806	1976	1981	1989	rBV2	102869	167042	3.12%	0.253%
81	15.183	2041	2045	2052	rVB3	42704	88224	1.65%	0.134%
82	15.383	2073	2079	2084	rBV	3097308	4488643	83.75%	6.794%
83	17.135	2372	2377	2387	rBV2	3561105	5347015	99.76%	8.093%
84	17.235	2389	2394	2404	rVB2	2858748	4130676	77.07%	6.252%
85	19.541	2782	2786	2795	rBV	2587234	3762863	70.20%	5.695%
86	21.353	3089	3094	3103	rBV	2968520	3859207	72.00%	5.841%
87	23.494	3453	3458	3468	rVB3	1641970	3784746	70.61%	5.728%
88	23.641	3477	3483	3491	rVB2	1922056	3711031	69.24%	5.617%


Sum of corrected areas: 66070460

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN060119\
Data File : BN006023.D
Acq On : 02 Jun 2019 09:33
Operator : JU/SJ
Sample : K2846-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

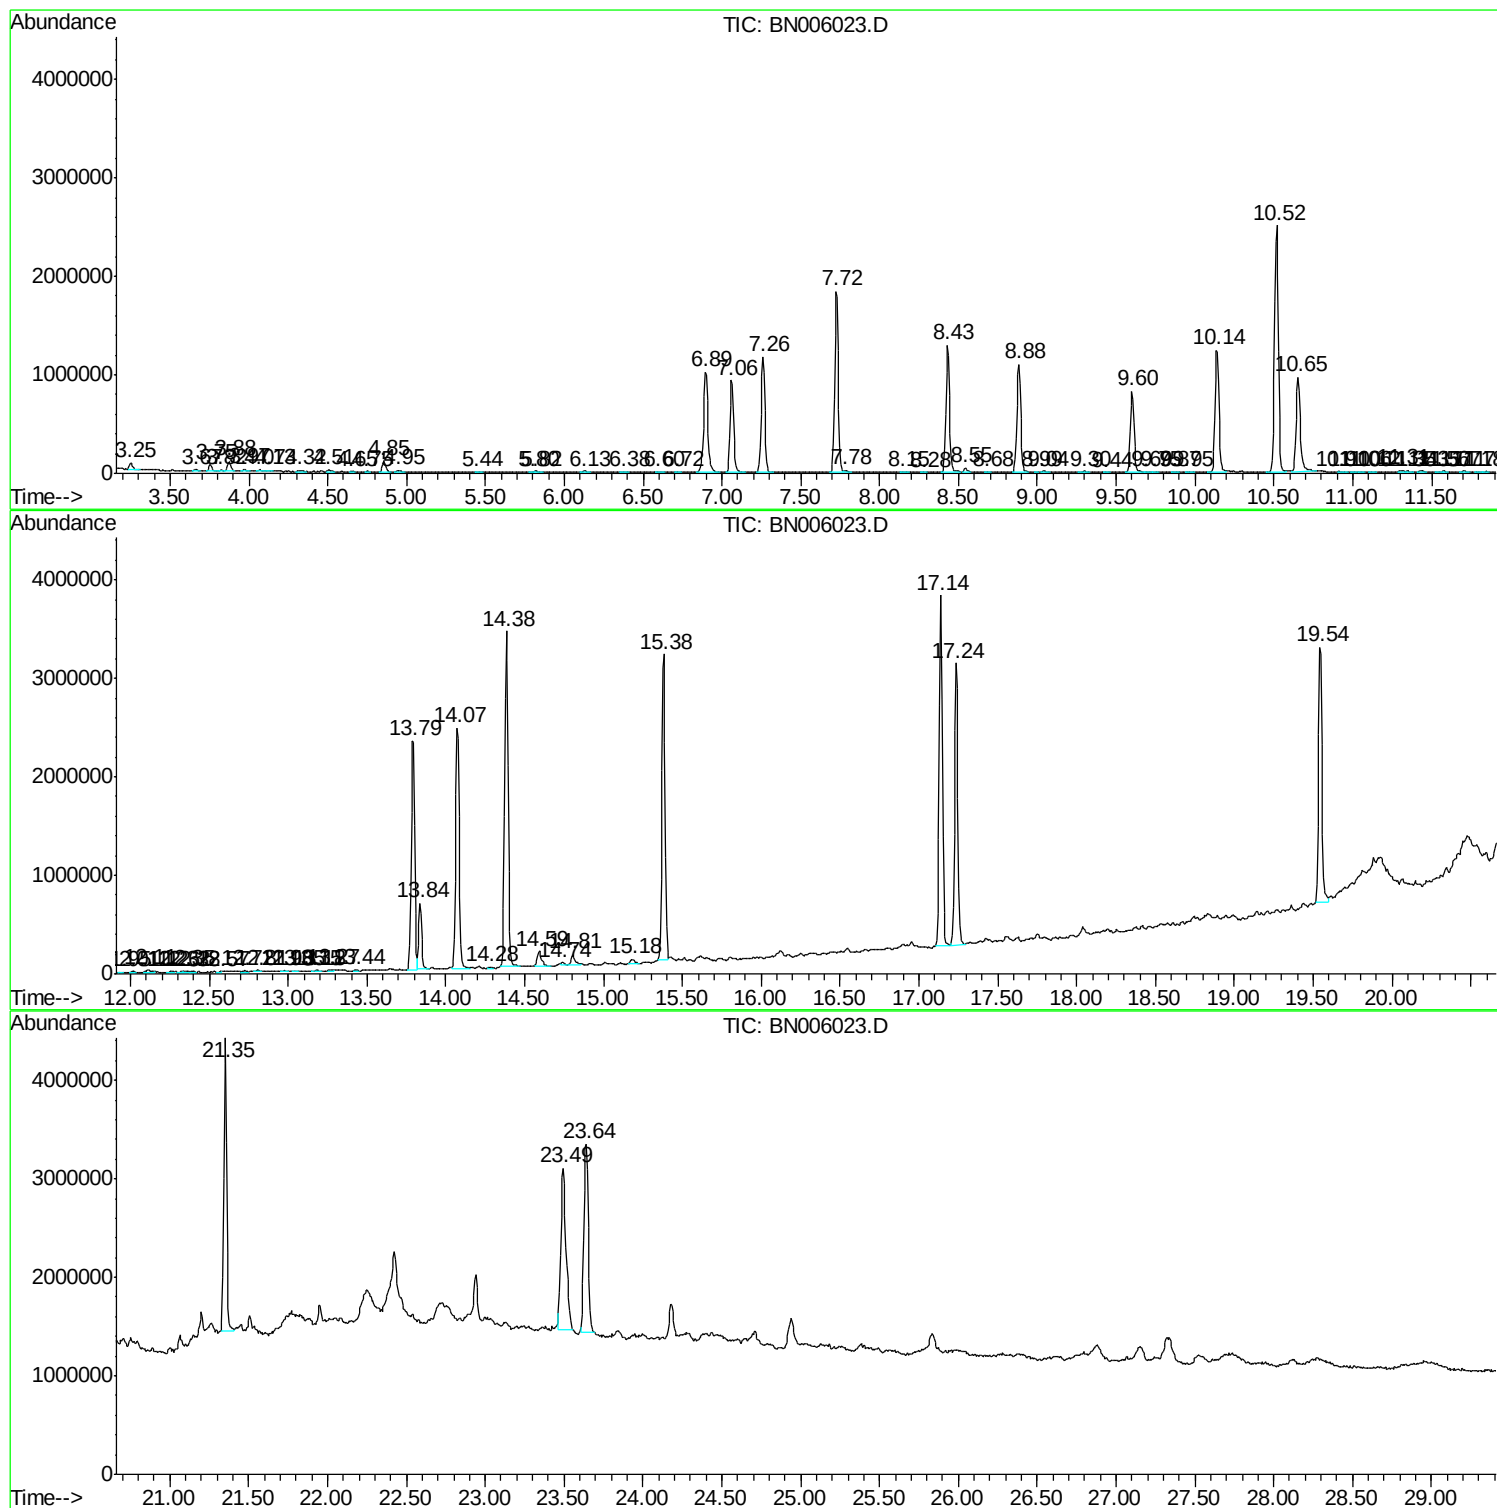

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
Data File : BN006023.D
Acq On : 02 Jun 2019 09:33
Operator : JU/SJ
Sample : K2846-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN060119\
Data File : BN006023.D
Acq On : 02 Jun 2019 09:33
Operator : JU/SJ
Sample : K2846-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFHB6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN052819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc