

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
 Data File : BN014810.D
 Acq On : 01 Jun 2021 12:55
 Operator : CG/JU
 Sample : SSTDIC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.1

Quant Time: Jun 01 14:45:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 01 14:44:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	571	0.40	ng	0.00
7) Naphthalene-d8	10.492	136	2008	0.40	ng	0.00
13) Acenaphthene-d10	14.359	164	1474	0.40	ng	0.01
19) Phenanthrene-d10	17.104	188	3487	0.40	ng	# 0.00
29) Chrysene-d12	21.311	240	4569	0.40	ng	# 0.00
35) Perylene-d12	23.569	264	4856	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.317	112	163	0.11	ng	0.00
5) Phenol-d6	6.895	99	211	0.10	ng	0.00
8) Nitrobenzene-d5	8.870	82	147	0.08	ng	0.01
11) 2-Methylnaphthalene-d10	12.093	152	380	0.09	ng	0.00
14) 2,4,6-Tribromophenol	15.856	330	66	0.08	ng	0.00
15) 2-Fluorobiphenyl	12.976	172	524	0.10	ng	0.00
27) Fluoranthene-d10	19.151	212	1334	0.10	ng	0.00
31) Terphenyl-d14	19.752	244	1117	0.10	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.271	88	153	0.23	ng	# 74
3) n-Nitrosodimethylamine	3.642	42	28	0.13	ng	# 61
6) bis(2-Chloroethyl)ether	7.145	93	182	0.10	ng	95
9) Naphthalene	10.543	128	539	0.09	ng	# 81
10) Hexachlorobutadiene	10.835	225	162	0.11	ng	# 90
12) 2-Methylnaphthalene	12.169	142	371	0.09	ng	# 91
16) Acenaphthylene	14.067	152	532	0.09	ng	97
17) Acenaphthene	14.422	154	417	0.10	ng	100
18) Fluorene	15.412	166	571	0.09	ng	97
20) 4,6-Dinitro-2-methylph...	15.514	198	39	0.11	ng	# 75
21) 4-Bromophenyl-phenylether	16.300	248	216	0.09	ng	# 82
22) Hexachlorobenzene	16.422	284	268	0.10	ng	# 87
23) Atrazine	16.580	200	154	0.10	ng	# 77
24) Pentachlorophenol	16.775	266	67	0.12	ng	# 77
25) Phenanthrene	17.152	178	1007	0.10	ng	97
26) Anthracene	17.250	178	762	0.09	ng	99
28) Fluoranthene	19.176	202	1336	0.09	ng	99
30) Pyrene	19.543	202	1404	0.11	ng	99
32) Benzo(a)anthracene	21.290	228	1282	0.09	ng	# 93
33) Chrysene	21.343	228	1583	0.10	ng	94
34) Bis(2-ethylhexyl)phtha...	21.226	149	654	0.17	ng	# 93
36) Indeno(1,2,3-cd)pyrene	25.852	276	1830	0.09	ng	# 96
37) Benzo(b)fluoranthene	22.891	252	1668	0.09	ng	# 65
38) Benzo(k)fluoranthene	22.935	252	1800	0.10	ng	# 71
39) Benzo(a)pyrene	23.469	252	1476	0.09	ng	# 49
40) Dibenzo(a,h)anthracene	25.872	278	1453	0.09	ng	# 70
41) Benzo(g,h,i)perylene	26.547	276	1781	0.10	ng	# 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
Data File : BN014810.D
Acq On : 01 Jun 2021 12:55
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Jun 01 14:45:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 14:44:32 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.708 min Scan# 612
 Delta R.T. 0.000 min
 Lab File: BN014810.D
 Acq: 01 Jun 2021 12:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 571
 Ion Ratio Lower Upper
 152 100
 150 156.5 123.4 185.2
 115 88.2 73.2 109.8



#2
 1,4-Dioxane
 Concen: 0.23 ng
 RT: 3.271 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN014810.D
 Acq: 01 Jun 2021 12:55

Tgt Ion: 88 Resp: 153
 Ion Ratio Lower Upper
 88 100
 58 32.7 44.7 67.1#
 43 19.6 21.0 31.6#









#3
n-Nitrosodimethylamine
Concen: 0.13 ng
RT: 3.642 min Scan# 107
Delta R.T. 0.008 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion: 42 Resp: 28
Ion Ratio Lower Upper
42 100
74 0.0 0.0 0.0
44 60.7 80.0 120.0#



#4
2-Fluorophenol
Concen: 0.11 ng
RT: 5.317 min Scan# 315
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion: 112 Resp: 163
Ion Ratio Lower Upper
112 100
64 60.7 43.6 65.4
63 33.1 25.0 37.6









#5
Phenol-d6
Concen: 0.10 ng
RT: 6.895 min Scan# 511
Delta R.T. 0.008 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion: 99 Resp: 211
Ion Ratio Lower Upper
99 100
42 19.4 10.2 15.2#
71 44.1 32.4 48.6



#6
bis(2-Chloroethyl)ether
Concen: 0.10 ng
RT: 7.145 min Scan# 542
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion: 93 Resp: 182
Ion Ratio Lower Upper
93 100
63 53.3 47.5 71.3
95 36.3 28.5 42.7









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	136	Resp:	2008
Ion	Ratio	Lower	Upper
136	100		
137	14.8	13.2	19.8
54	10.1	9.0	13.4
68	9.8	8.8	13.2



#8
Nitrobenzene-d5
Concen: 0.08 ng
RT: 8.870 min Scan# 731
Delta R.T. 0.013 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:	82	Resp:	147
Ion	Ratio	Lower	Upper
82	100		
128	59.3	34.2	51.2#
54	58.5	38.4	57.6#









#9
Naphthalene
Concen: 0.09 ng
RT: 10.543 min Scan# 863
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	128	Resp:	539
Ion	Ratio	Lower	Upper
128	100		
129	23.5	13.0	19.4#
127	27.8	15.0	22.6#



#10
Hexachlorobutadiene
Concen: 0.11 ng
RT: 10.835 min Scan# 886
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:	225	Resp:	162
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	71.0	50.8	76.2









#11
2-Methylnaphthalene-d10
Concen: 0.09 ng
RT: 12.093 min Scan# 1071
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:152 Resp: 380
Ion Ratio Lower Upper
152 100
151 20.8 16.8 25.2



#12
2-Methylnaphthalene
Concen: 0.09 ng
RT: 12.169 min Scan# 1088
Delta R.T. 0.005 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:142 Resp: 371
Ion Ratio Lower Upper
142 100
141 94.2 72.9 109.3
115 65.5 41.8 62.6#









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.359 min Scan# 1310
Delta R.T. 0.013 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:164 Resp: 1474
Ion Ratio Lower Upper
164 100
162 100.6 83.2 124.8
160 47.6 41.8 62.6



#14
2,4,6-Tribromophenol
Concen: 0.08 ng
RT: 15.856 min Scan# 1428
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:330 Resp: 66
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 45.5 21.8 32.6#









#15
2-Fluorobiphenyl
Concen: 0.10 ng
RT: 12.976 min Scan# 1201
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:172 Resp: 524
Ion Ratio Lower Upper
172 100
171 48.1 30.9 46.3#
170 36.5 21.4 32.0#



#16
Acenaphthylene
Concen: 0.09 ng
RT: 14.067 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:152 Resp: 532
Ion Ratio Lower Upper
152 100
151 22.0 17.1 25.7
153 14.3 9.9 14.9









#17
Acenaphthene
Concen: 0.10 ng
RT: 14.422 min Scan# 1315
Delta R.T. 0.013 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:154 Resp: 417
Ion Ratio Lower Upper
154 100
153 115.1 91.8 137.8
152 58.0 46.0 69.0



#18
Fluorene
Concen: 0.09 ng
RT: 15.412 min Scan# 1393
Delta R.T. 0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:166 Resp: 571
Ion Ratio Lower Upper
166 100
165 97.5 79.9 119.9
167 15.4 10.5 15.7







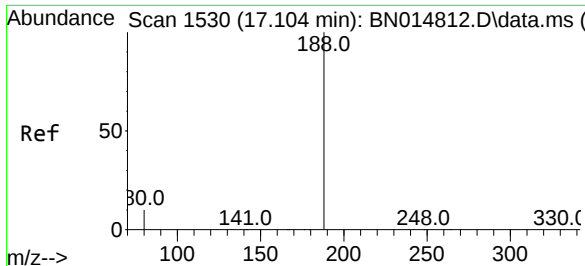

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.104 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:188 Resp: 3487
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.6 8.2 12.4#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.11 ng
RT: 15.514 min Scan# 1401
Delta R.T. 0.013 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:198 Resp: 39
Ion Ratio Lower Upper
198 100
51 150.0 96.4 144.6#
105 113.0 72.3 108.5#









#21
4-Bromophenyl-phenylether
Concen: 0.09 ng
RT: 16.300 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:248 Resp: 216
Ion Ratio Lower Upper
248 100
250 95.6 77.5 116.3
141 96.2 50.2 75.4#



#22
Hexachlorobenzene
Concen: 0.10 ng
RT: 16.422 min Scan# 1474
Delta R.T. 0.012 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:284 Resp: 268
Ion Ratio Lower Upper
284 100
142 35.8 20.3 30.5#
249 37.3 26.4 39.6









#23
Atrazine
Concen: 0.10 ng
RT: 16.580 min Scan# 1487
Delta R.T. 0.012 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:200 Resp: 154
Ion Ratio Lower Upper
200 100
173 53.7 29.1 43.7#
215 70.7 45.1 67.7#



#24
Pentachlorophenol
Concen: 0.12 ng
RT: 16.775 min Scan# 1503
Delta R.T. 0.012 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:266 Resp: 67
Ion Ratio Lower Upper
266 100
264 61.2 44.2 66.2
268 82.1 44.2 66.2#









#25
Phenanthrene
Concen: 0.10 ng
RT: 17.152 min Scan# 1534
Delta R.T. -0.000 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:178 Resp: 1007
Ion Ratio Lower Upper
178 100
176 20.0 16.0 24.0
179 18.7 12.6 19.0



#26
Anthracene
Concen: 0.09 ng
RT: 17.250 min Scan# 1542
Delta R.T. 0.012 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:178 Resp: 762
Ion Ratio Lower Upper
178 100
176 17.7 14.2 21.2
179 16.3 13.7 20.5







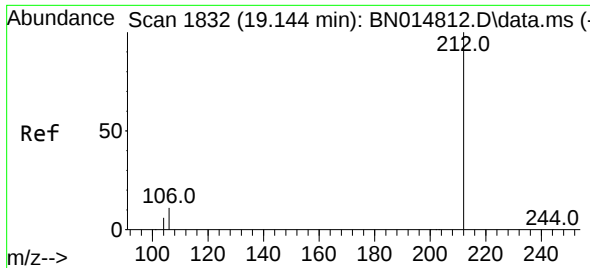

#27
Fluoranthene-d10
Concen: 0.10 ng
RT: 19.151 min Scan# 1835
Delta R.T. 0.007 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:212 Resp: 1334
Ion Ratio Lower Upper
212 100
106 9.5 7.4 11.2
104 5.5 4.1 6.1

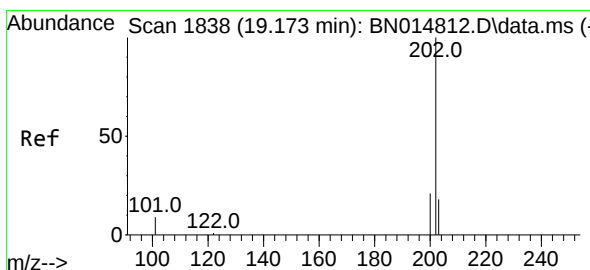

#28
Fluoranthene
Concen: 0.09 ng
RT: 19.176 min Scan# 1840
Delta R.T. 0.002 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:202 Resp: 1336
Ion Ratio Lower Upper
202 100
101 9.2 7.0 10.6
203 16.6 13.5 20.3





#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.311 min Scan# 2130

Delta R.T. 0.008 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1





Tgt Ion:240 Resp: 4569

Ion Ratio Lower Upper

240 100

120 8.0 5.2 7.8#

236 27.0 21.6 32.4



#30

Pyrene

Concen: 0.11 ng

RT: 19.543 min Scan# 1914

Delta R.T. 0.002 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55




Tgt Ion:202 Resp: 1404


Ion Ratio Lower Upper

202 100

200 20.5 16.6 24.8

203 17.8 13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.10 ng
 RT: 19.752 min Scan# 1956
 Delta R.T. 0.002 min
 Lab File: BN014810.D
 Acq: 01 Jun 2021 12:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:244 Resp: 1117
 Ion Ratio Lower Upper
 244 100
 212 14.5 6.8 10.2#
 122 13.8 6.6 9.8#



#32
 Benzo(a)anthracene
 Concen: 0.09 ng
 RT: 21.290 min Scan# 2128
 Delta R.T. -0.003 min
 Lab File: BN014810.D
 Acq: 01 Jun 2021 12:55

Tgt Ion:228 Resp: 1282
 Ion Ratio Lower Upper
 228 100
 226 31.6 22.9 34.3
 229 24.7 16.2 24.2#









#33
Chrysene
Concen: 0.10 ng
RT: 21.343 min Scan# 2133
Delta R.T. -0.003 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:228 Resp: 1583
Ion Ratio Lower Upper
228 100
226 32.7 24.3 36.5
229 24.4 16.4 24.6

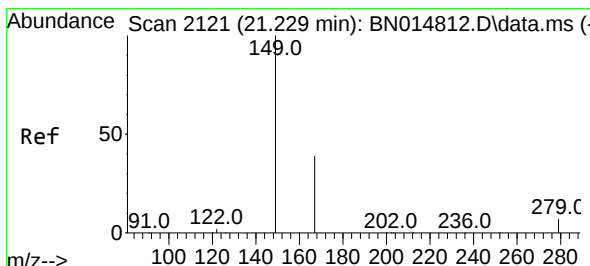

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.17 ng
RT: 21.226 min Scan# 2122
Delta R.T. -0.003 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:149 Resp: 654
Ion Ratio Lower Upper
149 100
167 39.1 28.3 42.5
279 9.3 5.5 8.3#





#35

Perylene-d12

Concen: 0.40 ng

RT: 23.569 min Scan# 2573

Delta R.T. 0.001 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55





Tgt Ion:264 Resp: 4856

Ion Ratio Lower Upper

264 100

260 26.5 21.4 32.2

265 53.2 40.9 61.3



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.09 ng

RT: 25.852 min Scan# 3240

Delta R.T. 0.008 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55




Tgt Ion:276 Resp: 1830


Ion Ratio Lower Upper

276 100

138 9.0 10.2 15.4#

277 24.9 20.4 30.6





#37

Benzo(b)fluoranthene

Concen: 0.09 ng

RT: 22.891 min Scan# 2375

Delta R.T. 0.004 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55





Tgt Ion:252 Resp: 1668

Ion Ratio Lower Upper

252 100

253 44.8 21.5 32.3#

125 21.8 6.6 10.0#



#38

Benzo(k)fluoranthene

Concen: 0.10 ng

RT: 22.935 min Scan# 2388

Delta R.T. 0.004 min

Lab File: BN014810.D

Acq: 01 Jun 2021 12:55




Tgt Ion:252 Resp: 1800


Ion Ratio Lower Upper

252 100

253 44.4 22.7 34.1#

125 16.5 6.4 9.6#









#39
Benzo(a)pyrene
Concen: 0.09 ng
RT: 23.469 min Scan# 2544
Delta R.T. 0.004 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:252 Resp: 1476
Ion Ratio Lower Upper
252 100
253 57.2 25.1 37.7#
125 35.9 9.4 14.0#



#40
Dibenzo(a,h)anthracene
Concen: 0.09 ng
RT: 25.872 min Scan# 3246
Delta R.T. 0.011 min
Lab File: BN014810.D
Acq: 01 Jun 2021 12:55

Tgt Ion:278 Resp: 1453
Ion Ratio Lower Upper
278 100
139 22.6 8.6 13.0#
279 44.2 22.8 34.2#





#41
 Benzo(g,h,i)perylene
 Concen: 0.10 ng
 RT: 26.547 min Scan# 3443
 Delta R.T. 0.011 min
 Lab File: BN014810.D
 Acq: 01 Jun 2021 12:55

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:	276	Resp:	1781
Ion	Ratio	Lower	Upper
276	100		
277	31.8	20.9	31.3#
138	19.4	10.3	15.5#

