

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
 Data File : BN014811.D
 Acq On : 01 Jun 2021 13:31
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Jun 01 14:45:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 01 14:44:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.708	152	563	0.40	ng	0.00
7) Naphthalene-d8	10.492	136	1933	0.40	ng	0.00
13) Acenaphthene-d10	14.346	164	1439	0.40	ng	0.00
19) Phenanthrene-d10	17.104	188	3369	0.40	ng	0.00
29) Chrysene-d12	21.311	240	4361	0.40	ng	0.00
35) Perylene-d12	23.569	264	4450	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.316	112	307	0.20	ng	0.00
5) Phenol-d6	6.887	99	385	0.19	ng	0.00
8) Nitrobenzene-d5	8.857	82	332	0.19	ng	0.00
11) 2-Methylnaphthalene-d10	12.093	152	775	0.20	ng	0.00
14) 2,4,6-Tribromophenol	15.856	330	135	0.16	ng	0.00
15) 2-Fluorobiphenyl	12.976	172	1022	0.19	ng	0.00
27) Fluoranthene-d10	19.146	212	2706	0.20	ng	0.00
31) Terphenyl-d14	19.751	244	2133	0.21	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.271	88	243	0.37	ng	Qvalue # 71
3) n-Nitrosodimethylamine	3.625	42	26	0.13	ng	# 85
6) bis(2-Chloroethyl)ether	7.145	93	304	0.18	ng	92
9) Naphthalene	10.543	128	1107	0.20	ng	95
10) Hexachlorobutadiene	10.834	225	299	0.21	ng	# 94
12) 2-Methylnaphthalene	12.164	142	738	0.18	ng	97
16) Acenaphthylene	14.067	152	1009	0.18	ng	99
17) Acenaphthene	14.410	154	795	0.19	ng	99
18) Fluorene	15.412	166	1099	0.18	ng	100
20) 4,6-Dinitro-2-methylph...	15.513	198	50	0.14	ng	83
21) 4-Bromophenyl-phenylether	16.300	248	418	0.18	ng	# 87
22) Hexachlorobenzene	16.410	284	554	0.22	ng	98
23) Atrazine	16.580	200	264	0.18	ng	88
24) Pentachlorophenol	16.775	266	99	0.18	ng	# 83
25) Phenanthrene	17.152	178	1865	0.18	ng	98
26) Anthracene	17.237	178	1500	0.18	ng	98
28) Fluoranthene	19.176	202	2500	0.18	ng	99
30) Pyrene	19.538	202	2600	0.21	ng	98
32) Benzo(a)anthracene	21.290	228	2346	0.18	ng	95
33) Chrysene	21.343	228	3011	0.21	ng	98
34) Bis(2-ethylhexyl)phtha...	21.226	149	830	0.22	ng	99
36) Indeno(1,2,3-cd)pyrene	25.852	276	3461	0.19	ng	99
37) Benzo(b)fluoranthene	22.887	252	3055	0.19	ng	# 90
38) Benzo(k)fluoranthene	22.932	252	3295	0.19	ng	# 89
39) Benzo(a)pyrene	23.469	252	2677	0.18	ng	# 83
40) Dibenzo(a,h)anthracene	25.869	278	2820	0.18	ng	# 90
41) Benzo(g,h,i)perylene	26.540	276	3367	0.21	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
Data File : BN014811.D
Acq On : 01 Jun 2021 13:31
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Jun 01 14:45:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 01 14:44:32 2021
Response via : Initial Calibration




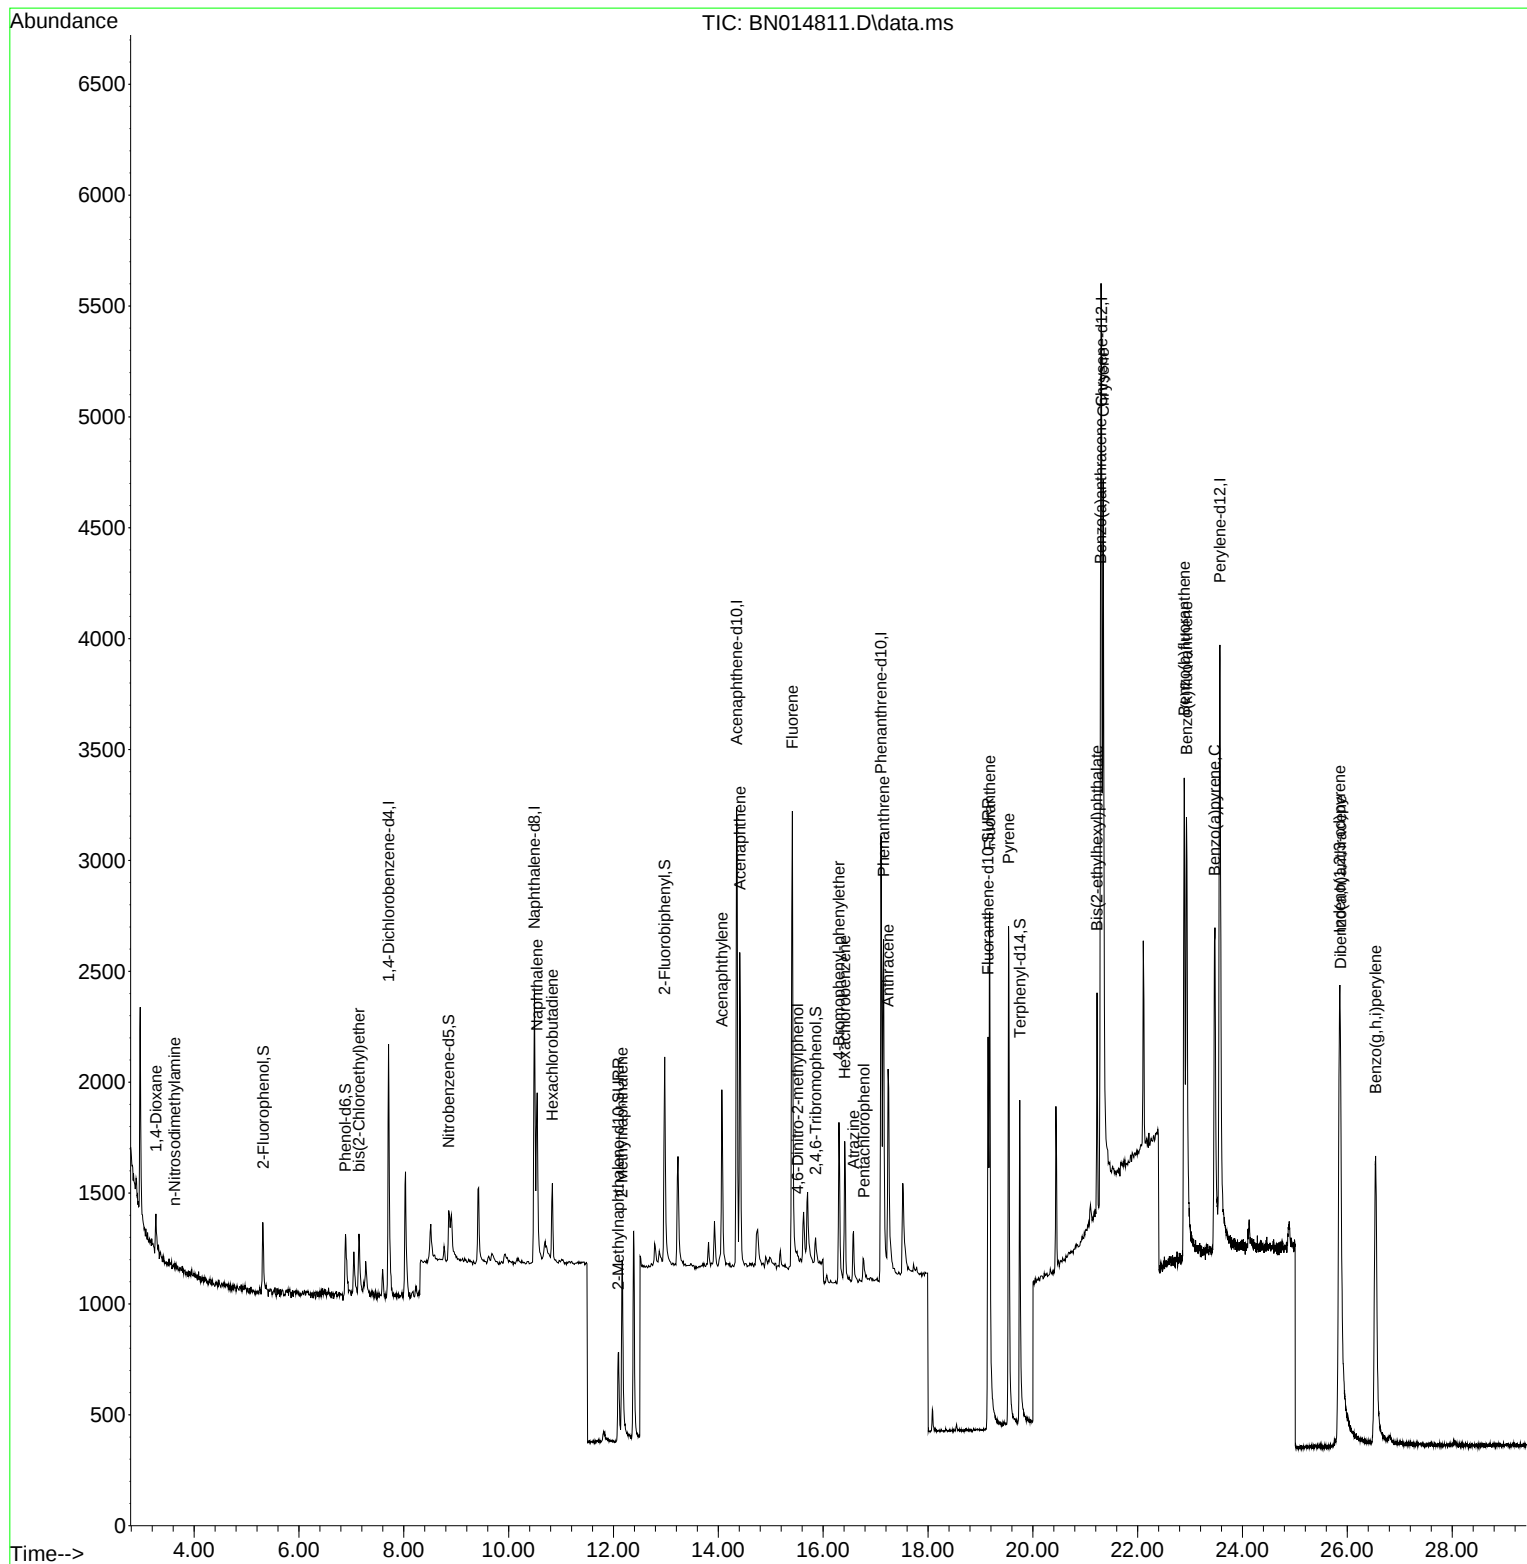




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.708 min Scan# 612
 Delta R.T. 0.000 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:152 Resp: 563
 Ion Ratio Lower Upper
 152 100
 150 149.6 123.4 185.2
 115 86.6 73.2 109.8

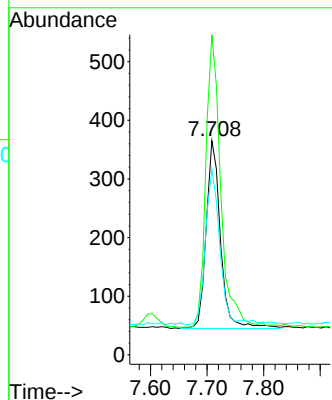

#2
 1,4-Dioxane
 Concen: 0.37 ng
 RT: 3.271 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31

Tgt Ion: 88 Resp: 243
 Ion Ratio Lower Upper
 88 100
 58 35.0 44.7 67.1#
 43 11.5 21.0 31.6#



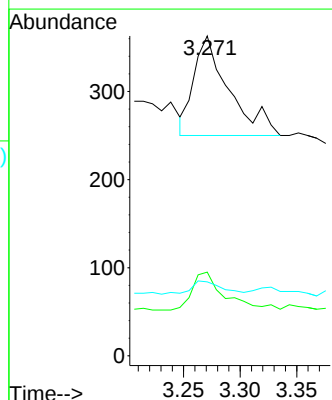
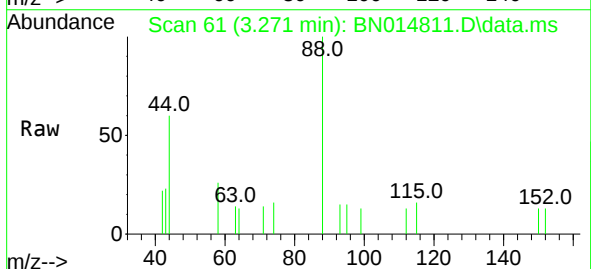




#3
n-Nitrosodimethylamine
Concen: 0.13 ng
RT: 3.625 min Scan# 105
Delta R.T. -0.008 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion: 42 Resp: 26
Ion Ratio Lower Upper
42 100
74 15.4 0.0 0.0#
44 84.6 80.0 120.0

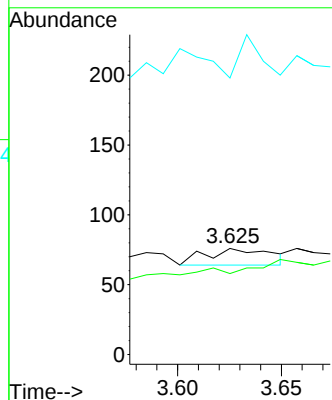

#4
2-Fluorophenol
Concen: 0.20 ng
RT: 5.316 min Scan# 315
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion: 112 Resp: 307
Ion Ratio Lower Upper
112 100
64 60.3 43.6 65.4
63 28.3 25.0 37.6



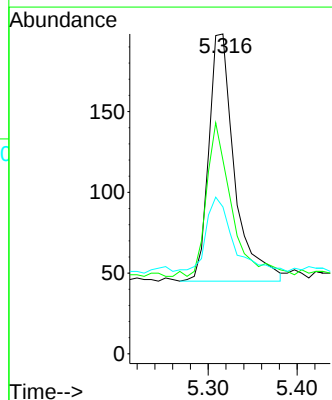
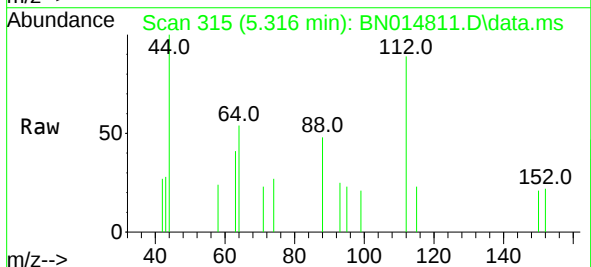




#5
Phenol-d6
Concen: 0.19 ng
RT: 6.887 min Scan# 510
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	99	Resp:	385
Ion	Ratio	Lower	Upper
99	100		
42	14.5	10.2	15.2
71	45.5	32.4	48.6



#6
bis(2-Chloroethyl)ether
Concen: 0.18 ng
RT: 7.145 min Scan# 542
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:	93	Resp:	304
Ion	Ratio	Lower	Upper
93	100		
63	66.1	47.5	71.3
95	38.8	28.5	42.7


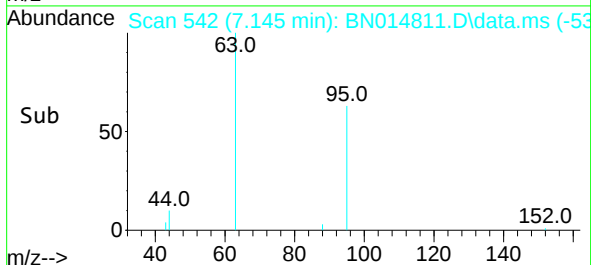
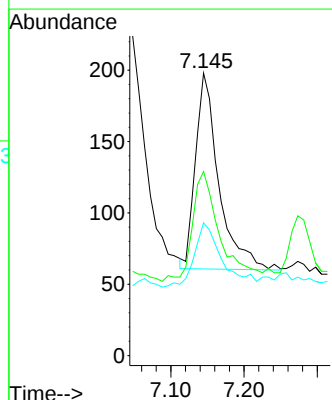
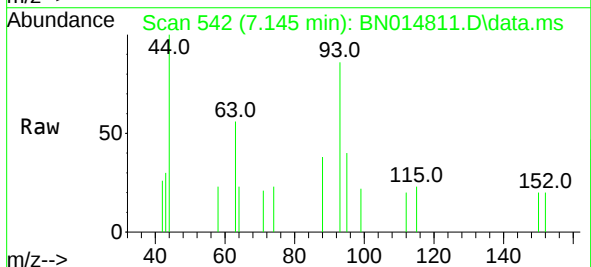




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	136	Resp:	1933
Ion	Ratio	Lower	Upper
136	100		
137	14.7	13.2	19.8
54	10.1	9.0	13.4
68	9.9	8.8	13.2

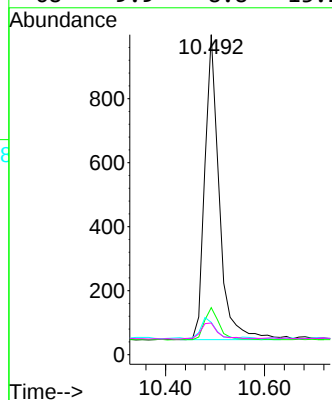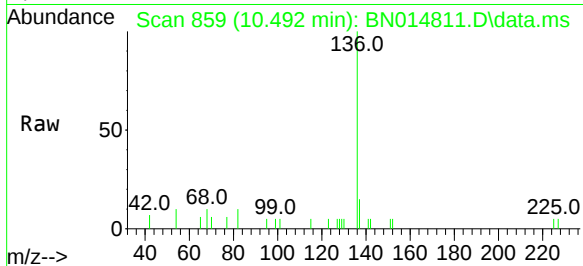

#8
Nitrobenzene-d5
Concen: 0.19 ng
RT: 8.857 min Scan# 730
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:	82	Resp:	332
Ion	Ratio	Lower	Upper
82	100		
128	52.1	34.2	51.2#
54	59.9	38.4	57.6#


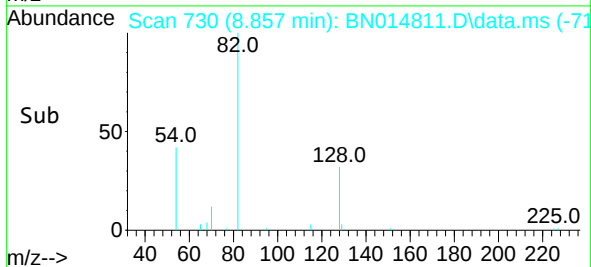
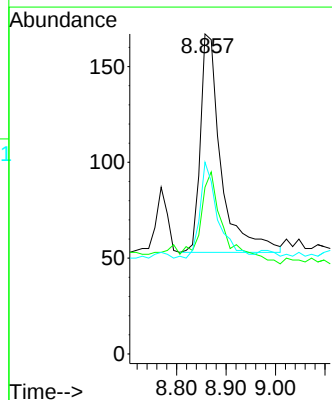
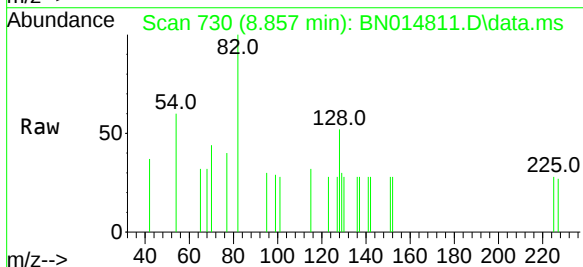




#9
Naphthalene
Concen: 0.20 ng
RT: 10.543 min Scan# 863
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	128	Resp:	1107
Ion	Ratio	Lower	Upper
128	100		
129	18.5	13.0	19.4
127	20.7	15.0	22.6



#10
Hexachlorobutadiene
Concen: 0.21 ng
RT: 10.834 min Scan# 886
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:	225	Resp:	299
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	67.9	50.8	76.2


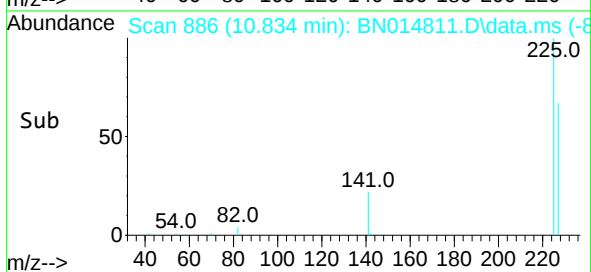






#11
2-Methylnaphthalene-d10
Concen: 0.20 ng
RT: 12.093 min Scan# 1071
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:152 Resp: 775
Ion Ratio Lower Upper
152 100
151 19.7 16.8 25.2



#12
2-Methylnaphthalene
Concen: 0.18 ng
RT: 12.164 min Scan# 1087
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:142 Resp: 738
Ion Ratio Lower Upper
142 100
141 92.7 72.9 109.3
115 55.4 41.8 62.6



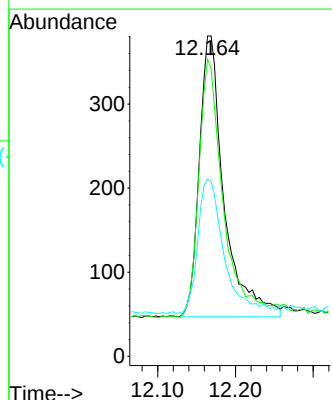
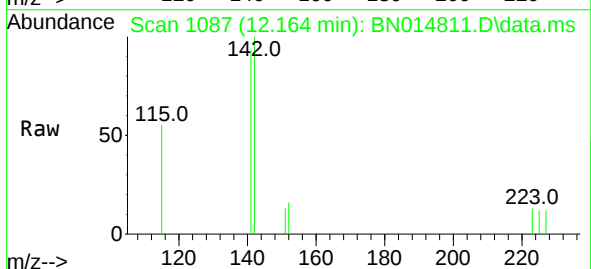




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:164 Resp: 1439
Ion Ratio Lower Upper
164 100
162 105.6 83.2 124.8
160 52.3 41.8 62.6



#14
2,4,6-Tribromophenol
Concen: 0.16 ng
RT: 15.856 min Scan# 1428
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:330 Resp: 135
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 33.3 21.8 32.6#




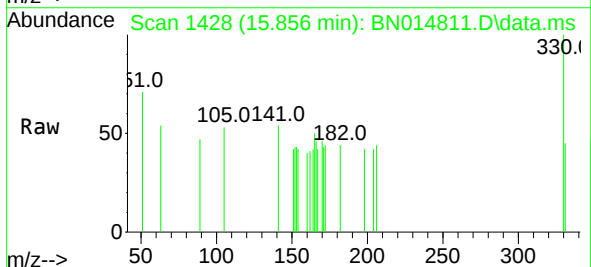


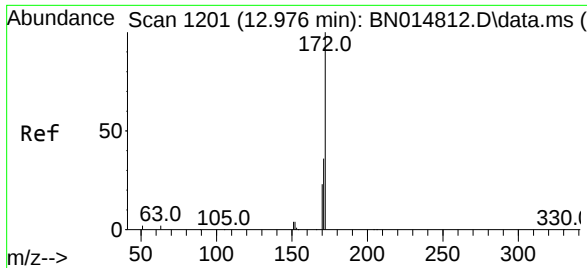

#15
2-Fluorobiphenyl
Concen: 0.19 ng
RT: 12.976 min Scan# 1201
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	172	Resp:	1022
Ion	Ratio	Lower	Upper
172	100		
171	43.0	30.9	46.3
170	30.9	21.4	32.0

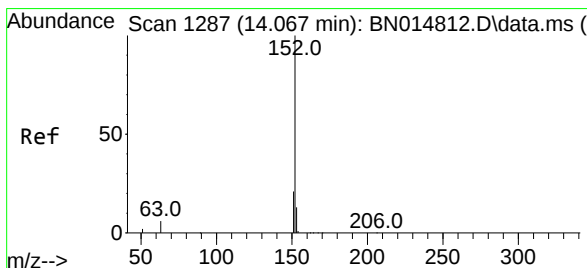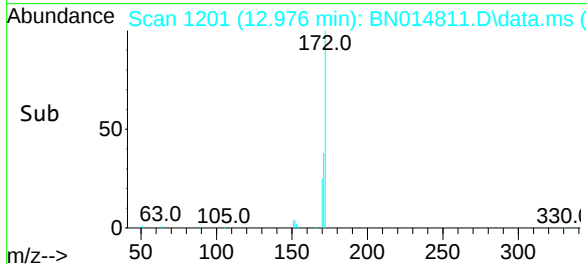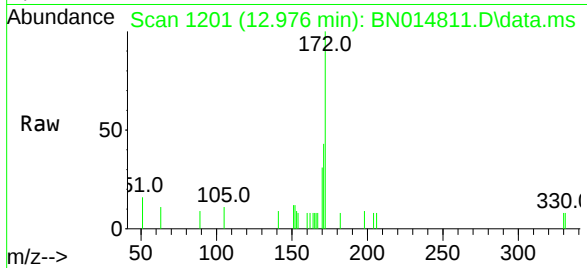

#16
Acenaphthylene
Concen: 0.18 ng
RT: 14.067 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:	152	Resp:	1009
Ion	Ratio	Lower	Upper
152	100		
151	21.8	17.1	25.7
153	13.3	9.9	14.9


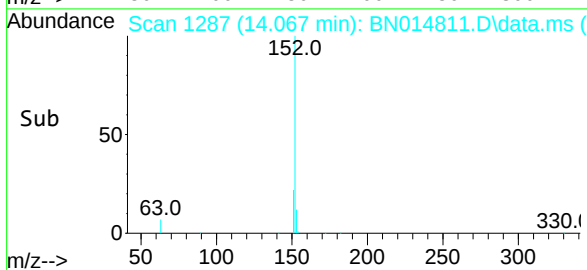

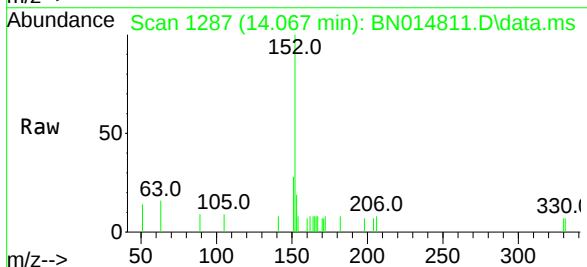


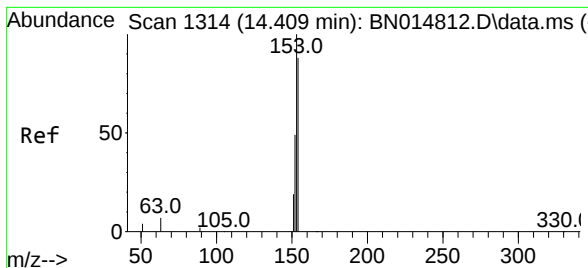

#17
Acenaphthene
Concen: 0.19 ng
RT: 14.410 min Scan# 1314
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:154 Resp: 795
Ion Ratio Lower Upper
154 100
153 115.3 91.8 137.8
152 59.0 46.0 69.0

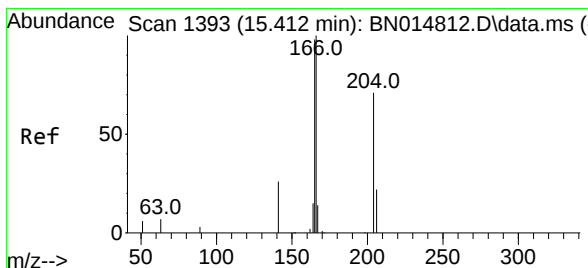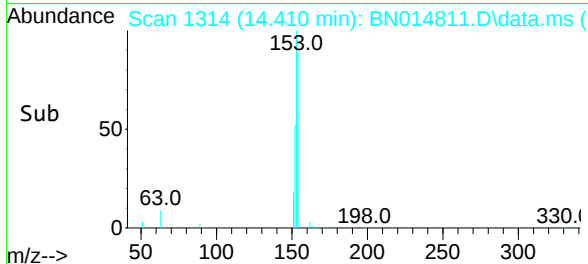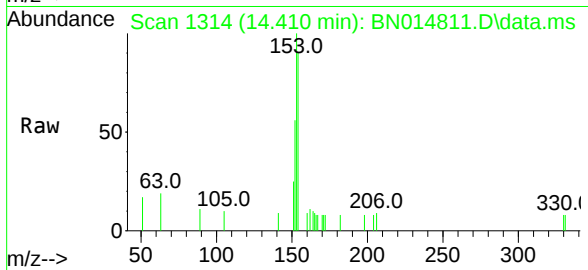

#18
Fluorene
Concen: 0.18 ng
RT: 15.412 min Scan# 1393
Delta R.T. 0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:166 Resp: 1099
Ion Ratio Lower Upper
166 100
165 99.7 79.9 119.9
167 14.1 10.5 15.7


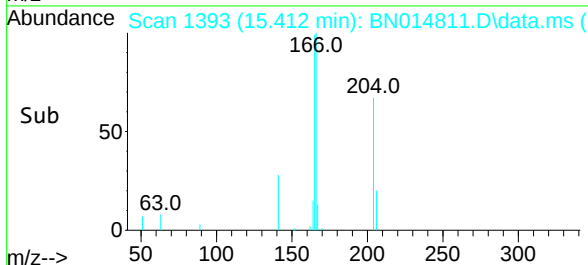

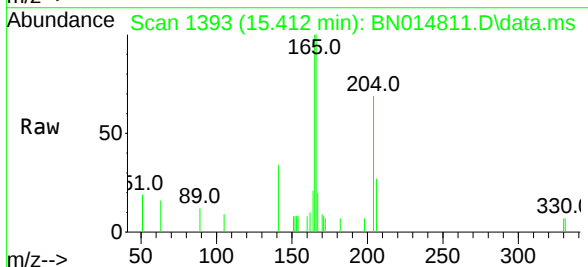


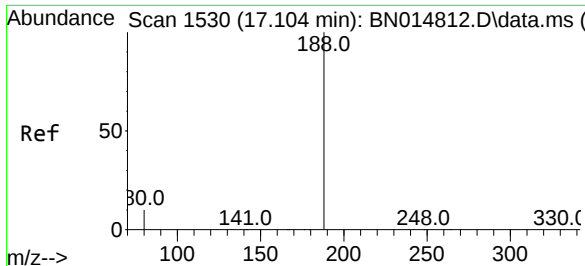

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.104 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:188 Resp: 3369
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.0 8.2 12.4

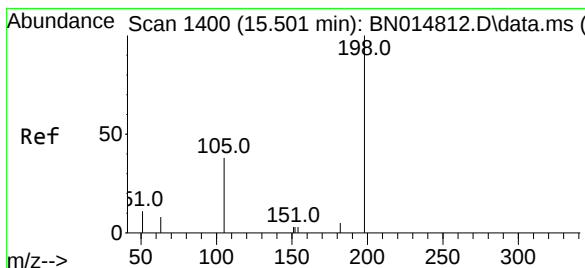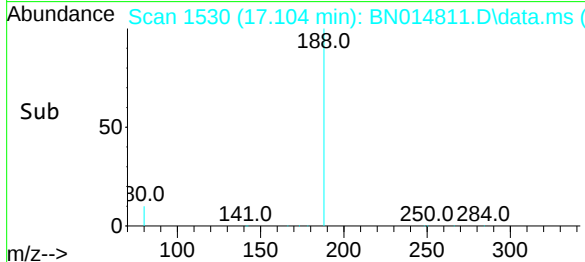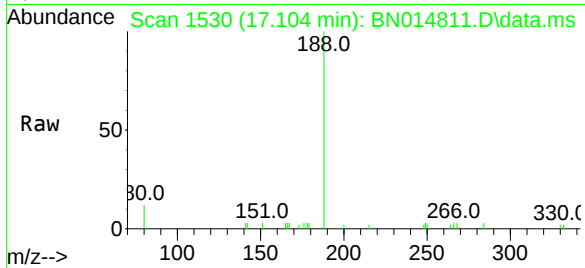

#20
4,6-Dinitro-2-methylphenol
Concen: 0.14 ng
RT: 15.513 min Scan# 1401
Delta R.T. 0.013 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:198 Resp: 50
Ion Ratio Lower Upper
198 100
51 141.4 96.4 144.6
105 103.4 72.3 108.5


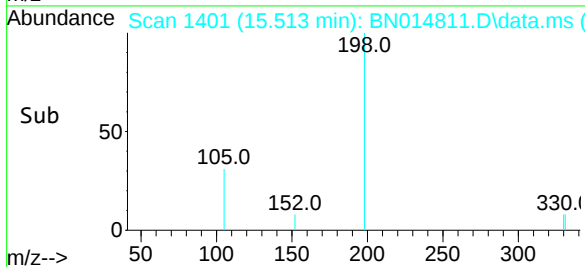

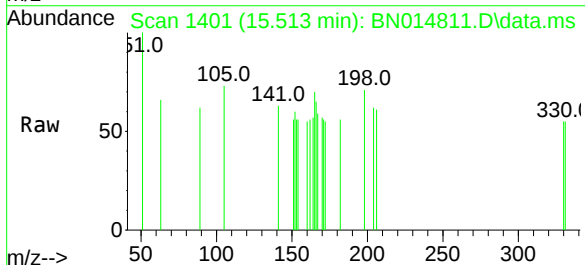




#21
4-Bromophenyl-phenylether
Concen: 0.18 ng
RT: 16.300 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:248 Resp: 418
Ion Ratio Lower Upper
248 100
250 97.5 77.5 116.3
141 87.6 50.2 75.4#



#22
Hexachlorobenzene
Concen: 0.22 ng
RT: 16.410 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:284 Resp: 554
Ion Ratio Lower Upper
284 100
142 25.6 20.3 30.5
249 30.9 26.4 39.6

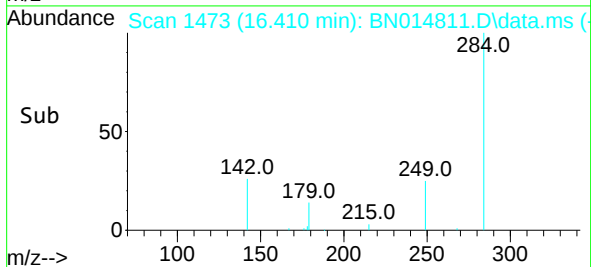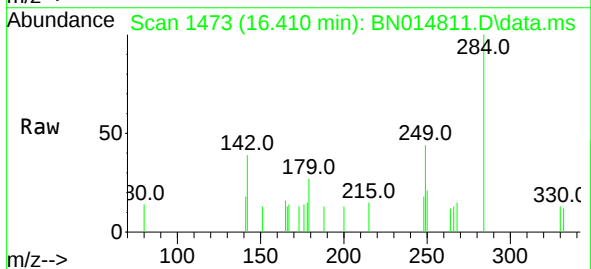

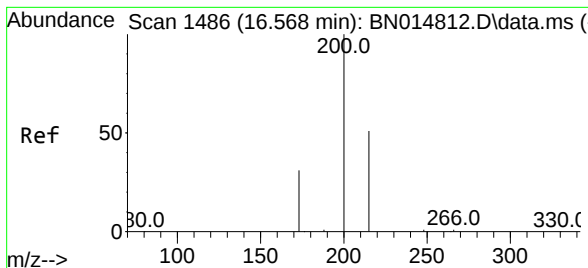

#23

Atrazine

Concen: 0.18 ng

RT: 16.580 min Scan# 1487

Delta R.T. 0.012 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31





Tgt Ion:	200	Resp:	264
Ion Ratio	Lower	Upper	
200	100		
173	41.9	29.1	43.7
215	66.9	45.1	67.7

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2

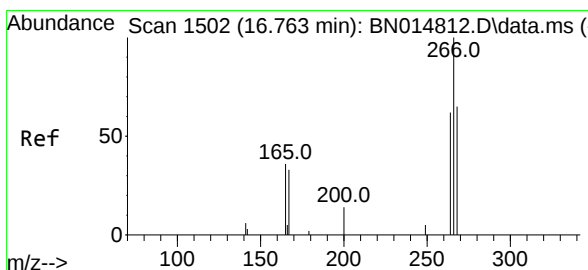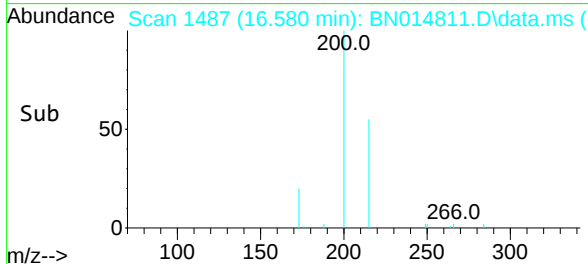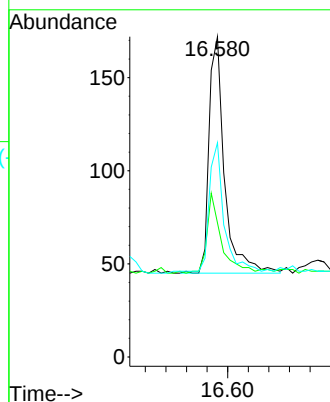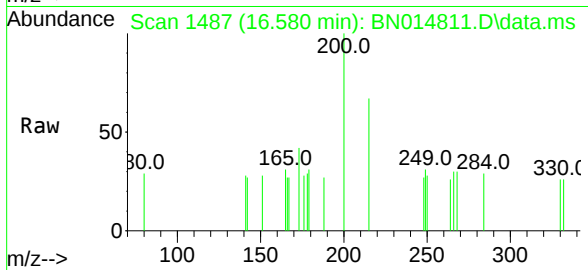

#24

Pentachlorophenol

Concen: 0.18 ng




RT: 16.775 min Scan# 1503


Delta R.T. 0.012 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31

Tgt Ion:	266	Resp:	99
Ion Ratio	Lower	Upper	
266	100		
264	53.5	44.2	66.2
268	77.8	44.2	66.2#


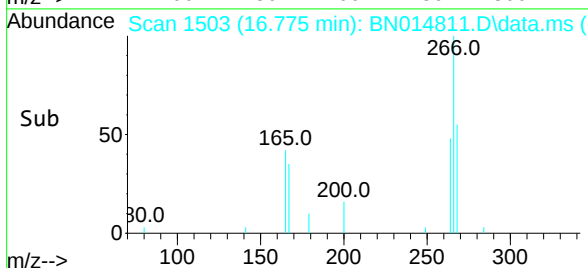

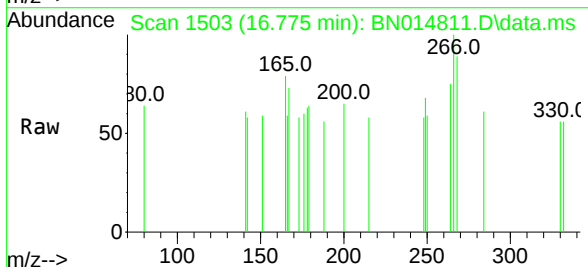


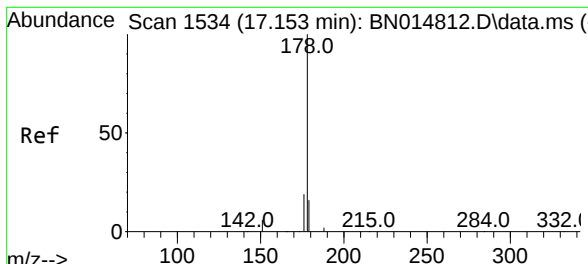

#25
Phenanthrene
Concen: 0.18 ng
RT: 17.152 min Scan# 1534
Delta R.T. -0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	178	Resp:	1865
Ion Ratio	Lower	Upper	
178	100		
176	19.5	16.0	24.0
179	16.9	12.6	19.0

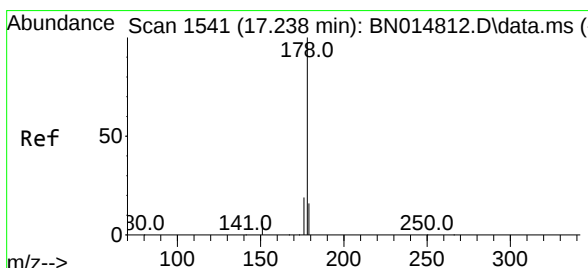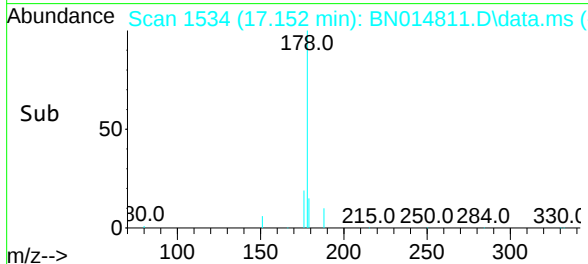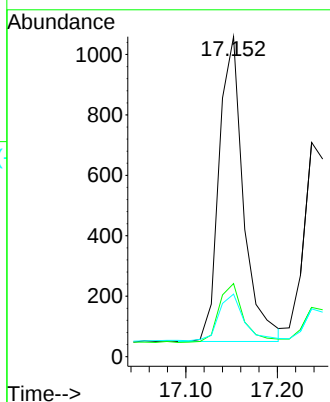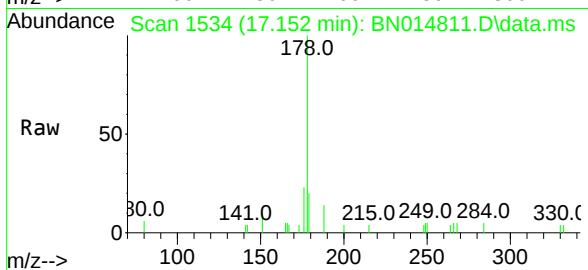

#26
Anthracene
Concen: 0.18 ng
RT: 17.237 min Scan# 1541
Delta R.T. -0.000 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:	178	Resp:	1500
Ion Ratio	Lower	Upper	
178	100		
176	17.8	14.2	21.2
179	15.3	13.7	20.5


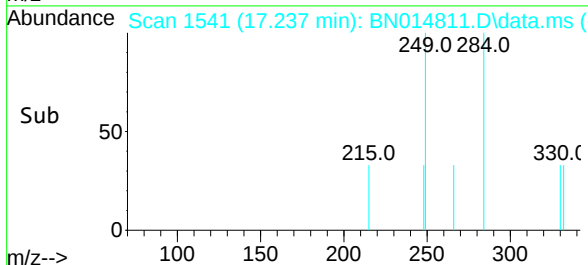

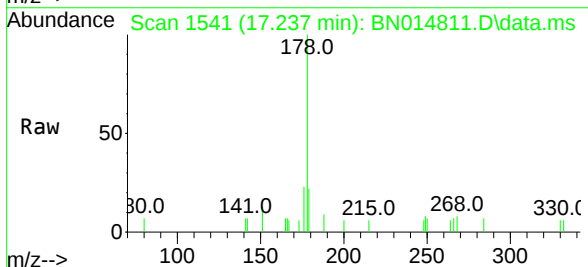


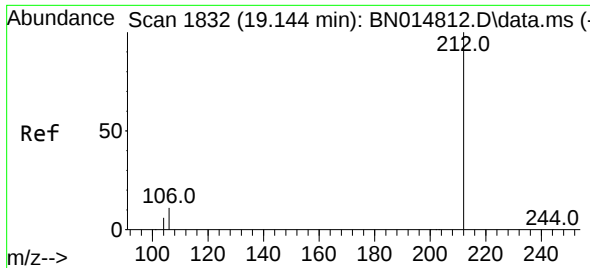

#27
Fluoranthene-d10
Concen: 0.20 ng
RT: 19.146 min Scan# 1834
Delta R.T. 0.002 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:212 Resp: 2706
Ion Ratio Lower Upper
212 100
106 10.4 7.4 11.2
104 5.3 4.1 6.1

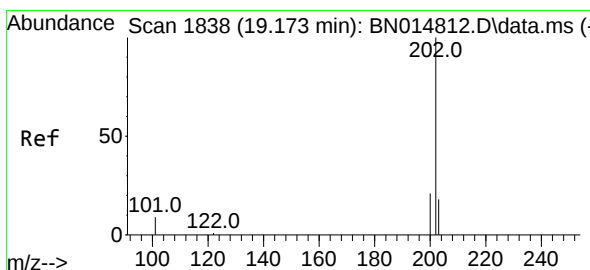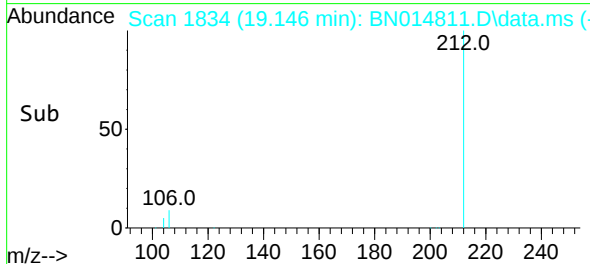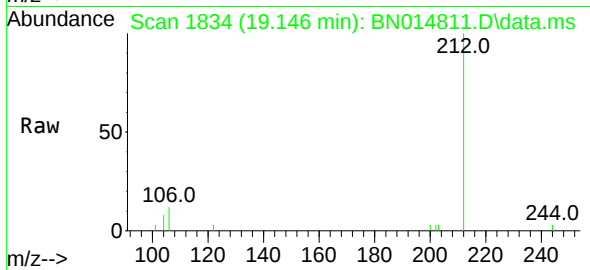

#28
Fluoranthene
Concen: 0.18 ng
RT: 19.176 min Scan# 1840
Delta R.T. 0.002 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:202 Resp: 2500
Ion Ratio Lower Upper
202 100
101 9.0 7.0 10.6
203 16.4 13.5 20.3

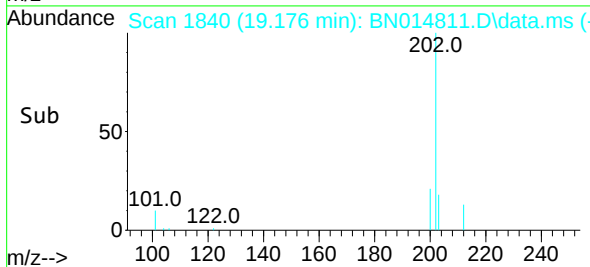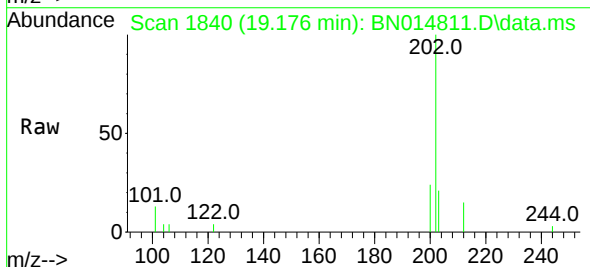



#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.311 min Scan# 2130

Delta R.T. 0.008 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31





Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2

Tgt Ion:240	Resp:	4361
Ion Ratio	Lower	Upper
240	100	
120	7.1	5.2 7.8
236	26.3	21.6 32.4

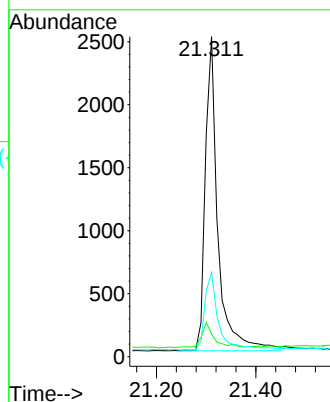

#30

Pyrene

Concen: 0.21 ng




RT: 19.538 min Scan# 1913


Delta R.T. -0.003 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31

Tgt Ion:202	Resp:	2600
Ion Ratio	Lower	Upper
202	100	
200	21.3	16.6 24.8
203	18.3	13.9 20.9









#31
 Terphenyl-d14
 Concen: 0.21 ng
 RT: 19.751 min Scan# 1956
 Delta R.T. 0.002 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:244 Resp: 2133
 Ion Ratio Lower Upper
 244 100
 212 9.7 6.8 10.2
 122 10.6 6.6 9.8#

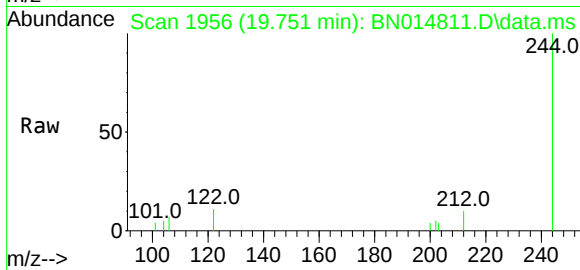

#32
 Benzo(a)anthracene
 Concen: 0.18 ng
 RT: 21.290 min Scan# 2128
 Delta R.T. -0.003 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31

Tgt Ion:228 Resp: 2346
 Ion Ratio Lower Upper
 228 100
 226 31.0 22.9 34.3
 229 22.5 16.2 24.2


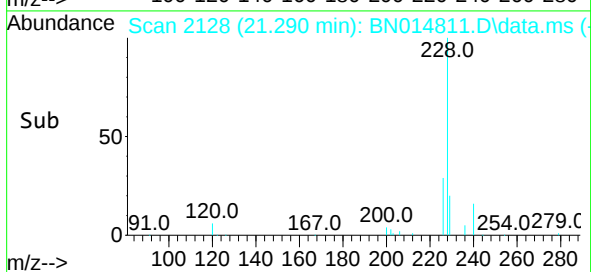

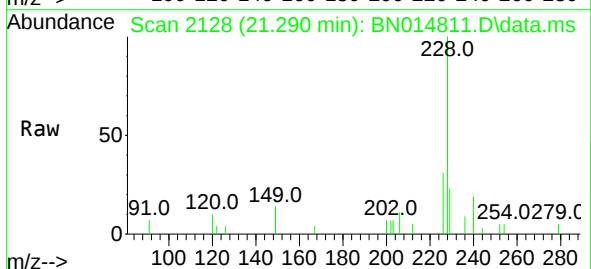


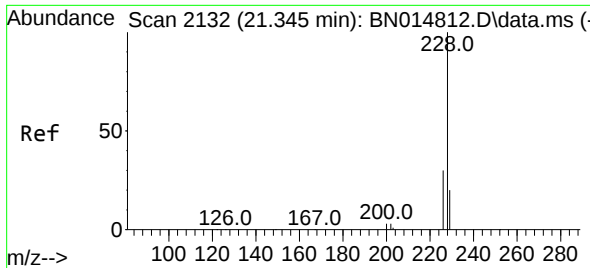

#33
Chrysene
Concen: 0.21 ng
RT: 21.343 min Scan# 2133
Delta R.T. -0.003 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:228	Resp:	3011
Ion Ratio	Lower	Upper
228	100	
226	31.3	24.3 36.5
229	22.0	16.4 24.6

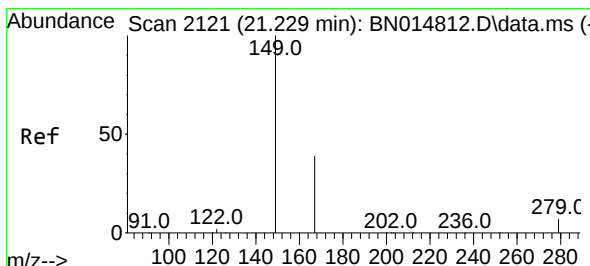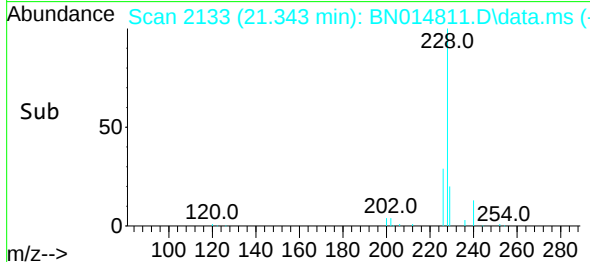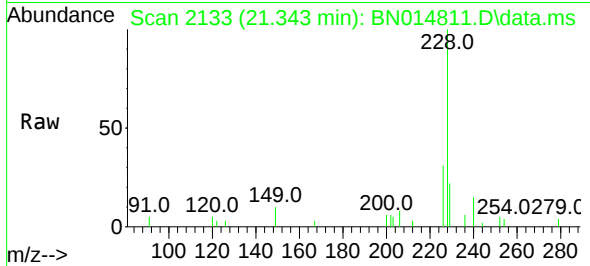

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.22 ng
RT: 21.226 min Scan# 2122
Delta R.T. -0.003 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31


Tgt Ion:149	Resp:	830
Ion Ratio	Lower	Upper
149	100	
167	36.0	28.3 42.5
279	8.0	5.5 8.3

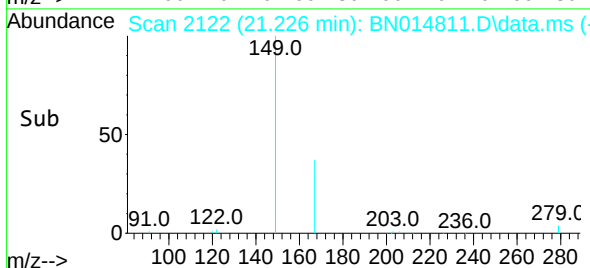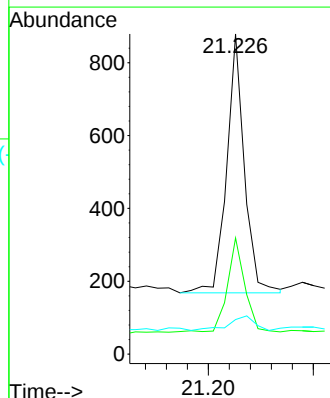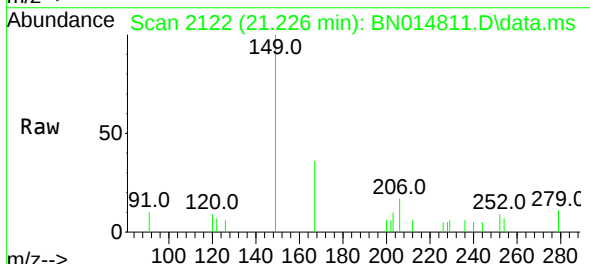






#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.569 min Scan# 2573
 Delta R.T. 0.001 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

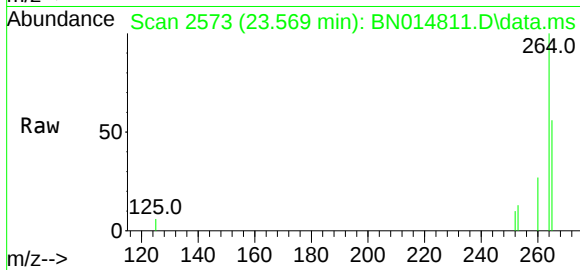


Tgt Ion:264 Resp: 4450

Ion	Ratio	Lower	Upper
264	100		
260	27.3	21.4	32.2
265	55.9	40.9	61.3

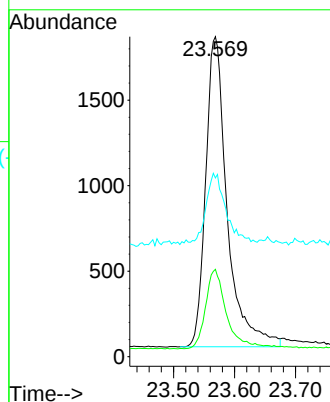
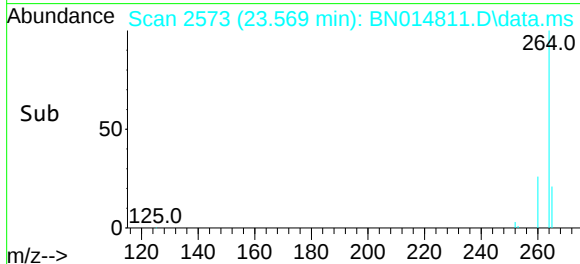



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.19 ng
 RT: 25.852 min Scan# 3240
 Delta R.T. 0.008 min
 Lab File: BN014811.D
 Acq: 01 Jun 2021 13:31

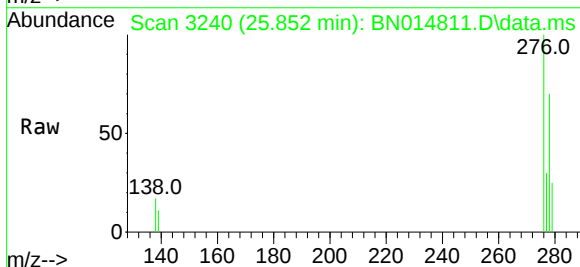

Tgt Ion:276 Resp: 3461

Ion	Ratio	Lower	Upper
276	100		
138	12.1	10.2	15.4
277	26.1	20.4	30.6




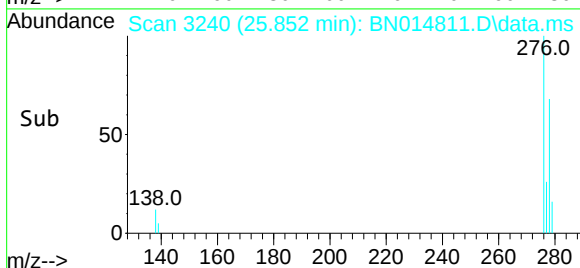




#37
Benzo(b)fluoranthene
Concen: 0.19 ng
RT: 22.887 min Scan# 2374
Delta R.T. 0.001 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:252 Resp: 3055
Ion Ratio Lower Upper
252 100
253 32.0 21.5 32.3
125 12.5 6.6 10.0#



#38
Benzo(k)fluoranthene
Concen: 0.19 ng
RT: 22.932 min Scan# 2387
Delta R.T. 0.001 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Tgt Ion:252 Resp: 3295
Ion Ratio Lower Upper
252 100
253 34.1 22.7 34.1#
125 11.3 6.4 9.6#

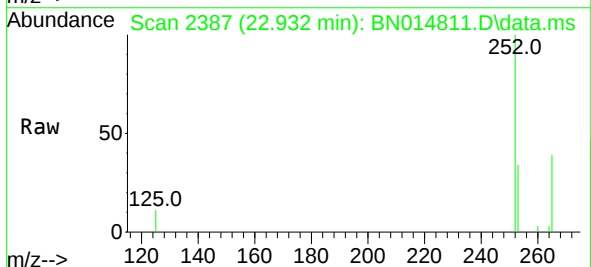



#39

Benzo(a)pyrene

Concen: 0.18 ng

RT: 23.469 min Scan# 2544

Delta R.T. 0.004 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31

Tgt Ion:252 Resp: 2677

Ion Ratio Lower Upper

252 100

253 40.8 25.1 37.7#





125 18.6 9.4 14.0#

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2



#40

Dibenzo(a,h)anthracene

Concen: 0.18 ng

RT: 25.869 min Scan# 3245

Delta R.T. 0.008 min

Lab File: BN014811.D

Acq: 01 Jun 2021 13:31




Tgt Ion:278 Resp: 2820


Ion Ratio Lower Upper

278 100

139 14.6 8.6 13.0#


279 34.0 22.8 34.2

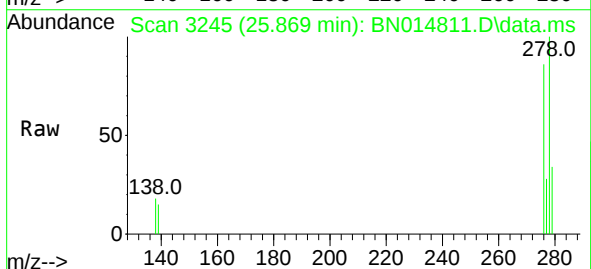

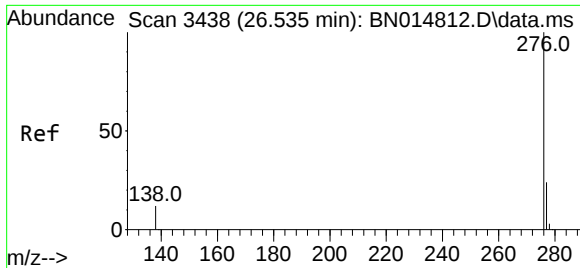

#41
Benzo(g,h,i)perylene
Concen: 0.21 ng
RT: 26.540 min Scan# 3441
Delta R.T. 0.004 min
Lab File: BN014811.D
Acq: 01 Jun 2021 13:31

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

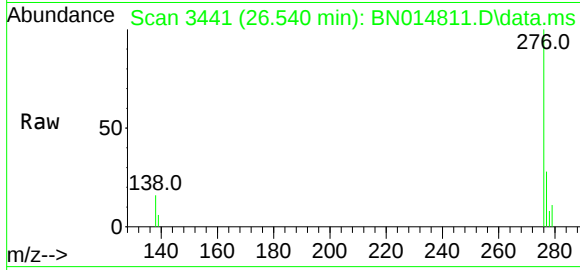

Tgt Ion:276 Resp: 3367
Ion Ratio Lower Upper
276 100
277 28.0 20.9 31.3
138 16.3 10.3 15.5#

