
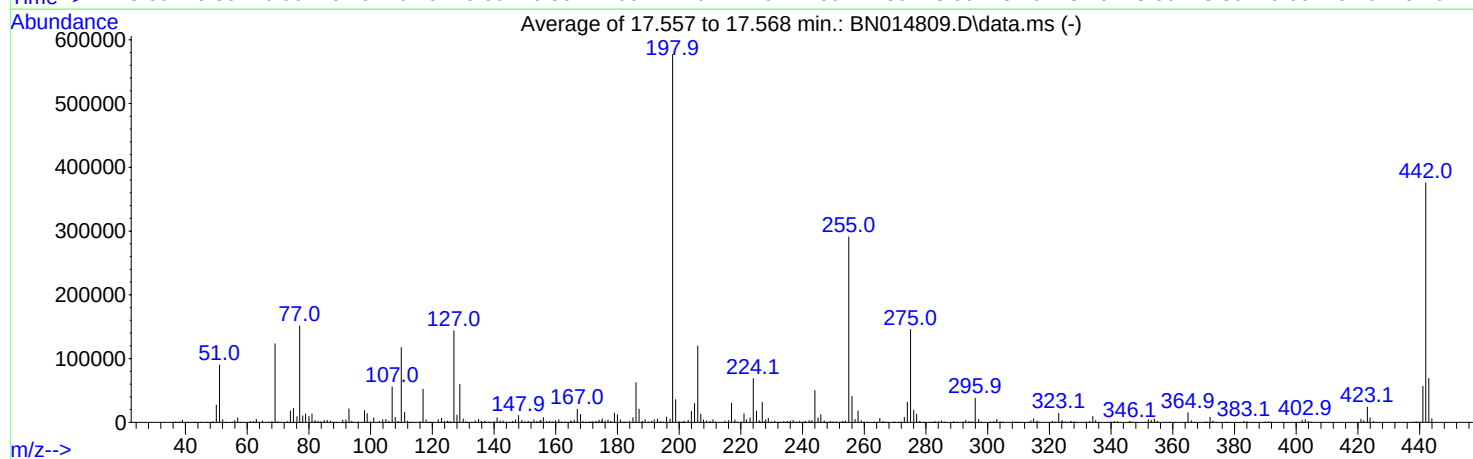


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
 Data File : BN014809.D
 Acq On : 01 Jun 2021 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 01 17:40:45 2021

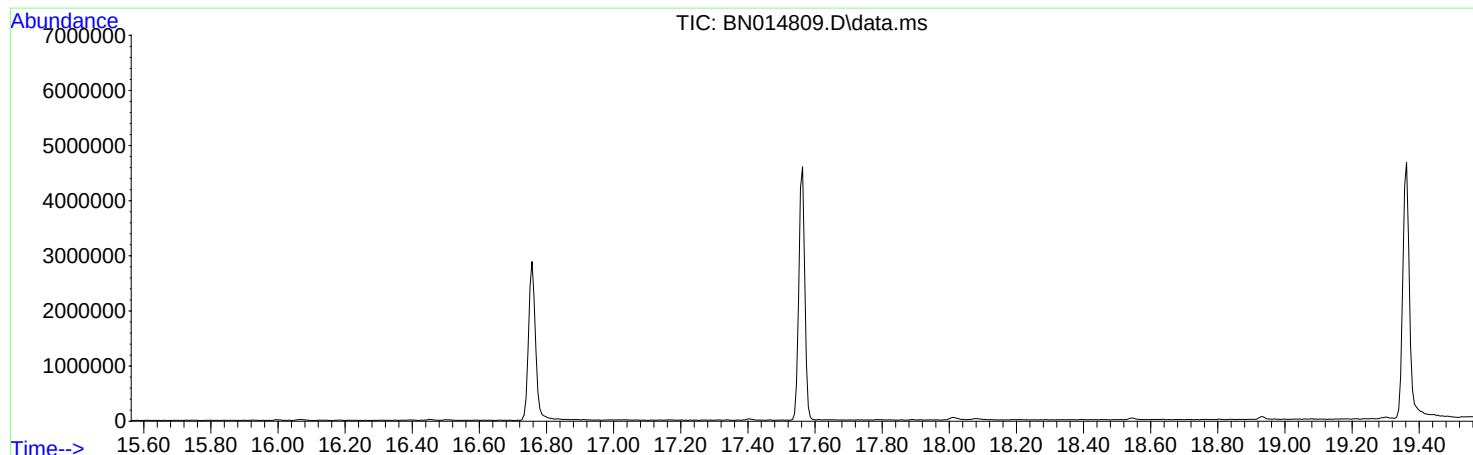




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.6	89760	PASS
68	69	0.00	2	1.1	1393	PASS
69	198	0.00	100	21.4	123285	PASS
70	69	0.00	2	1.0	1186	PASS
127	198	10	80	24.9	143776	PASS
197	198	0.00	2	0.9	5058	PASS
198	198	100	100	100.0	576939	PASS
199	198	5	9	6.2	35683	PASS
275	198	10	60	25.2	145488	PASS
365	198	1	100	2.6	15229	PASS
441	198	0.01	100	9.8	56811	PASS
442	442	50	100	100.0	375573	PASS
443	442	15	24	18.4	69136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
Data File : BN014809.D
Acq On : 01 Jun 2021 12:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 01 13:53:01 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

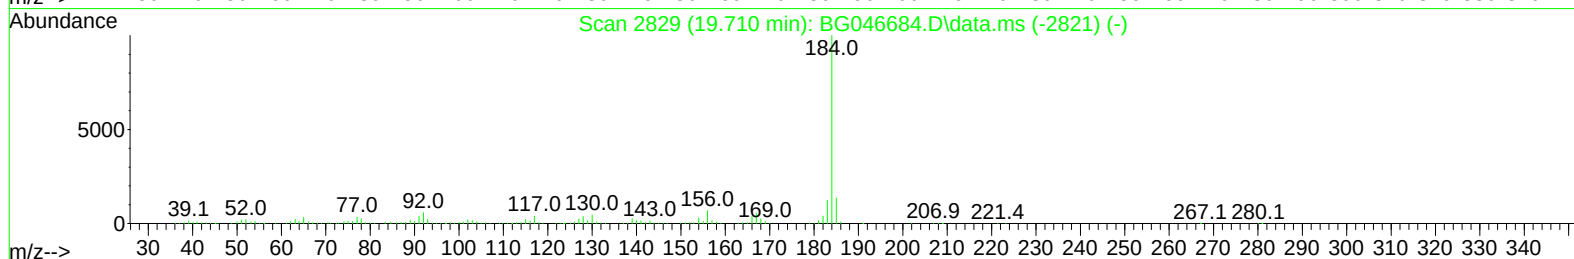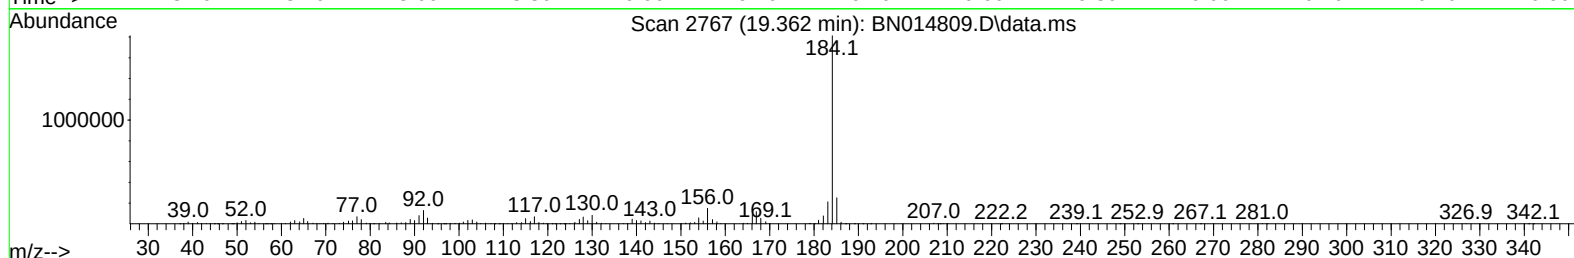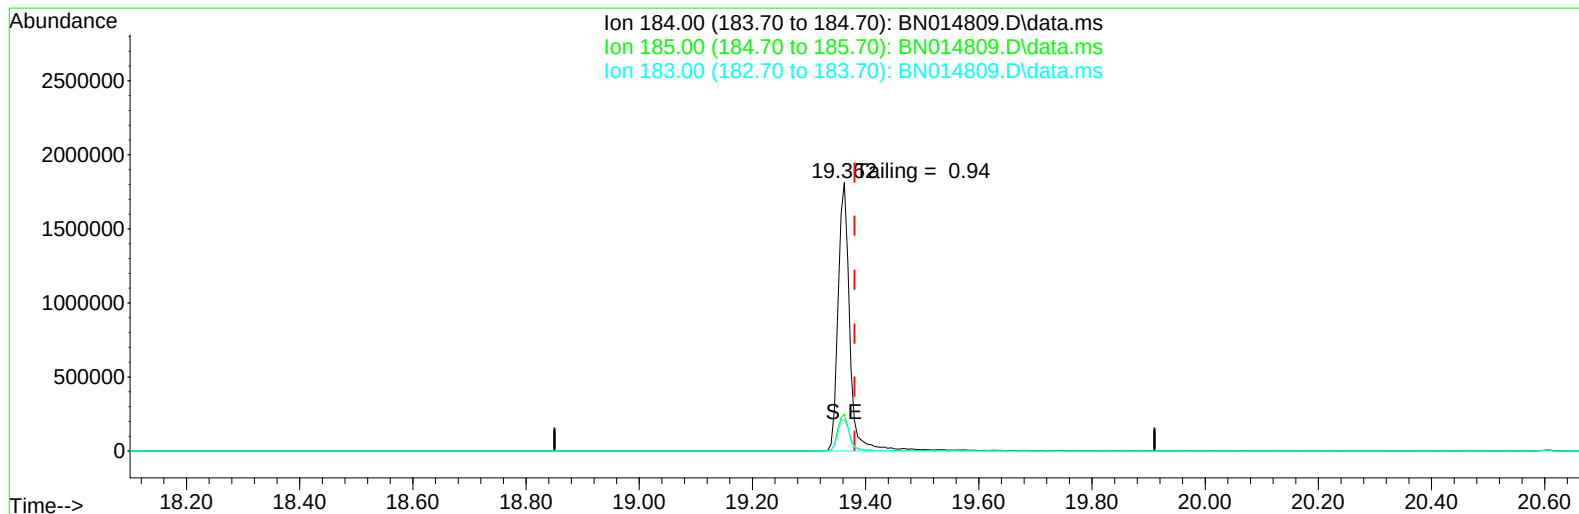

TIC: BN014809.D\data.ms

(77) Benzidine

19.362min (-0.018) 694789.99 ng




response 2548642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	11.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060121\
 Data File : BN014809.D
 Acq On : 01 Jun 2021 12:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 01 13:53:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

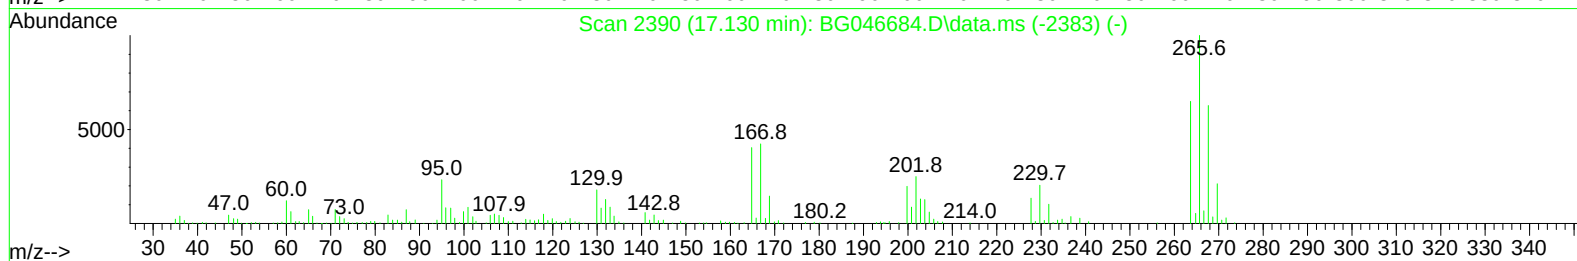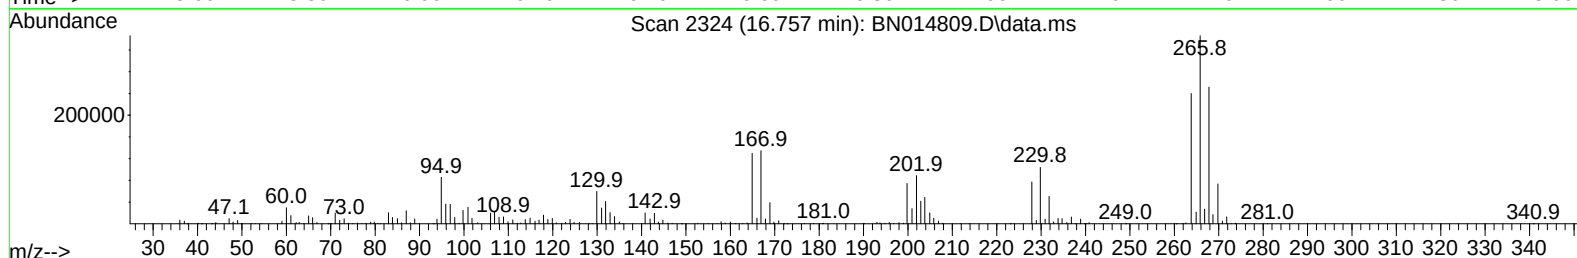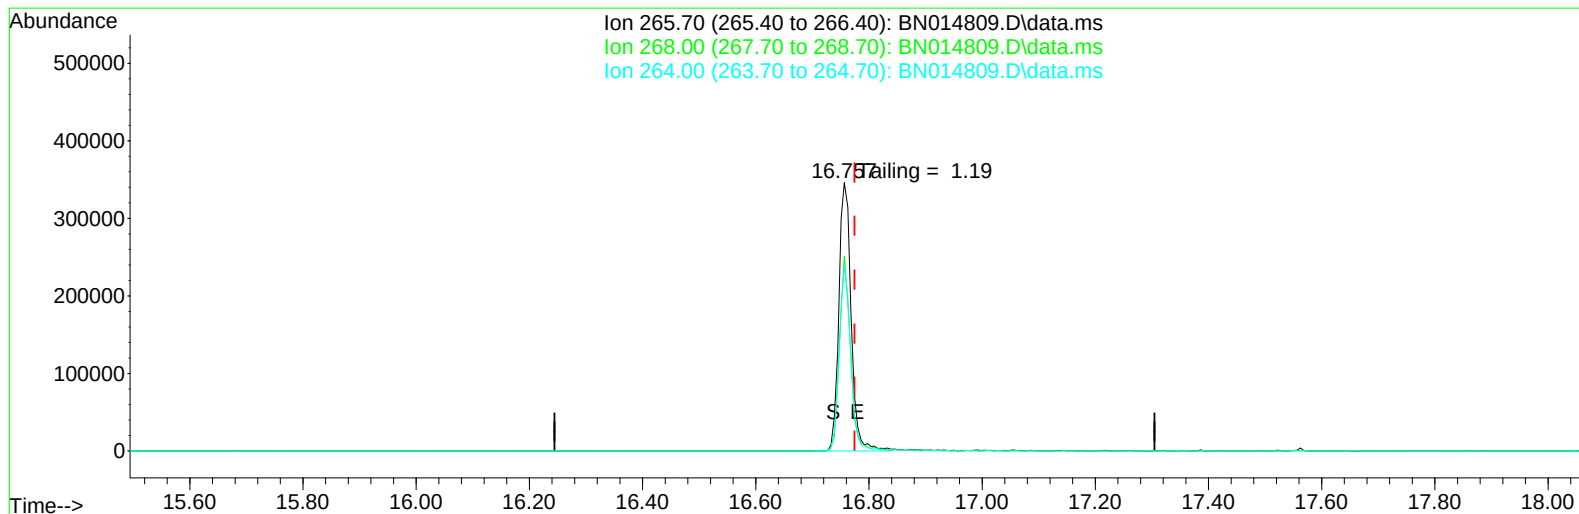

TIC: BN014809.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.018) 23476.90 ng

response 524902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	77.62#
264.00	61.60	69.30
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/1/2021	BNA_N	<u>BN014809.D</u>
Compound Name	Response	Retention Time
DDT	1528587	20.6
DDD	2063	20.15
DDE	2309	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4372	1532959	0.29