
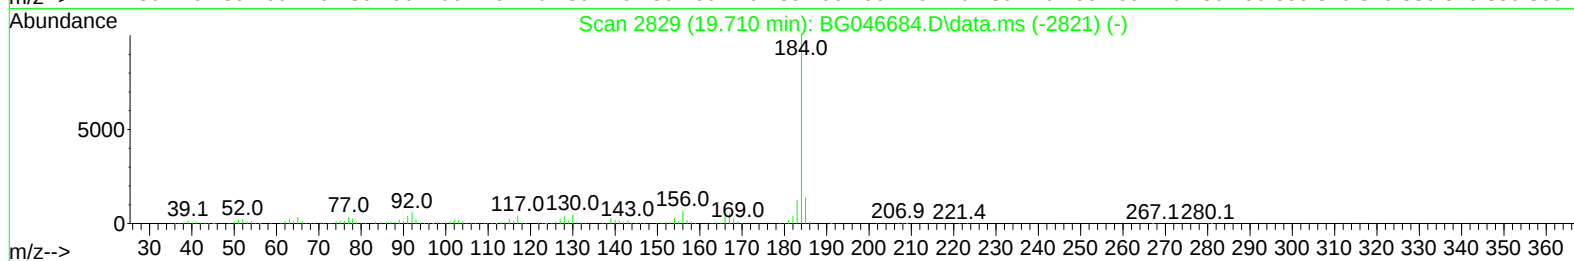
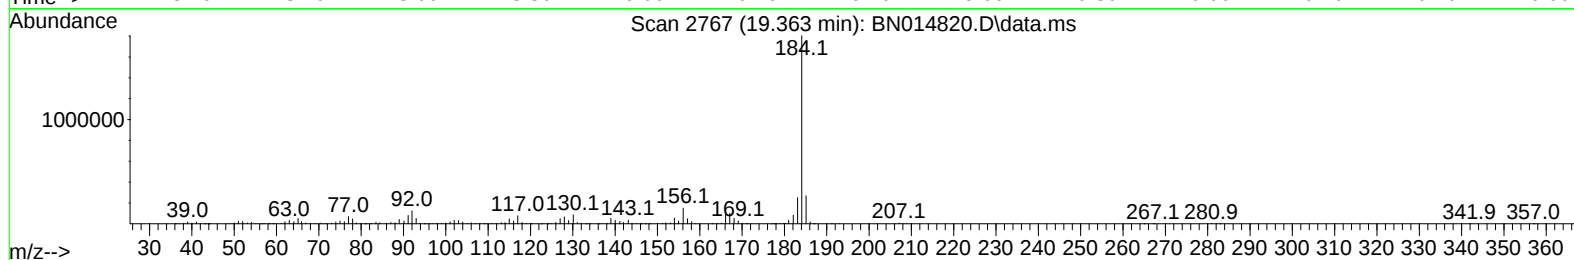


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060221\
 Data File : BN014820.D
 Acq On : 02 Jun 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 11:35:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

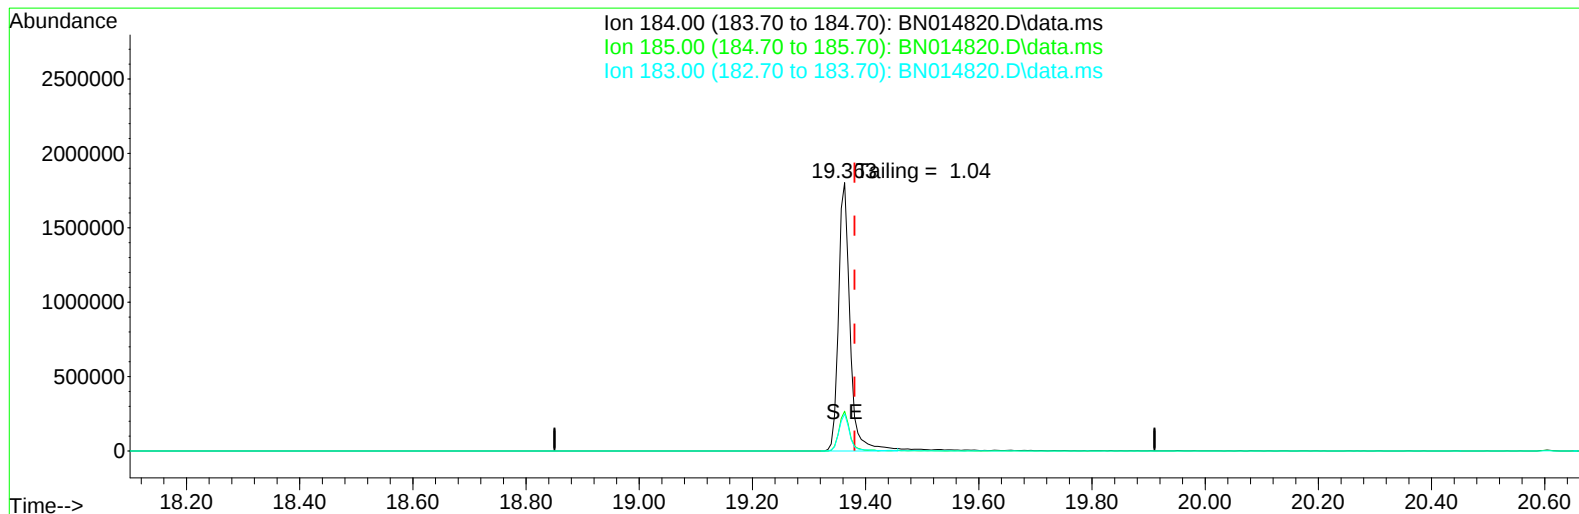




TIC: BN014820.D\data.ms

(77) Benzidine**19.363min (-0.017) 707289.22 ng****response 2550887**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.89
183.00	13.20	13.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060221\
 Data File : BN014820.D
 Acq On : 02 Jun 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 11:35:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

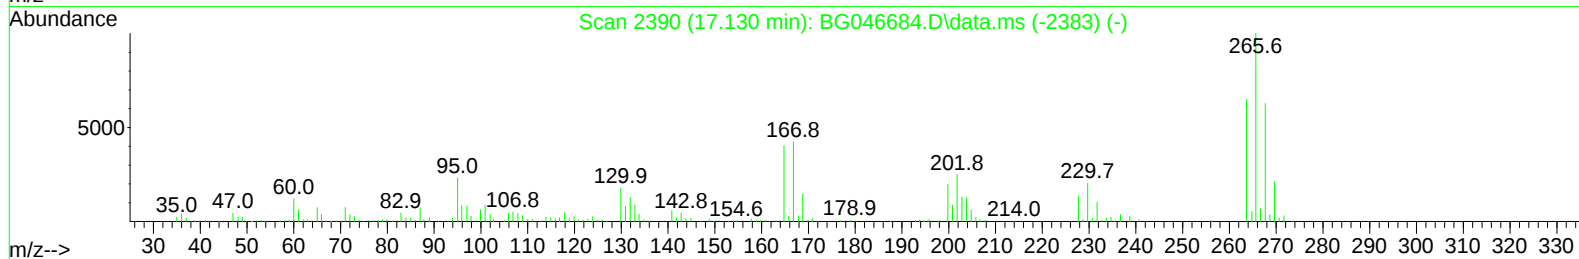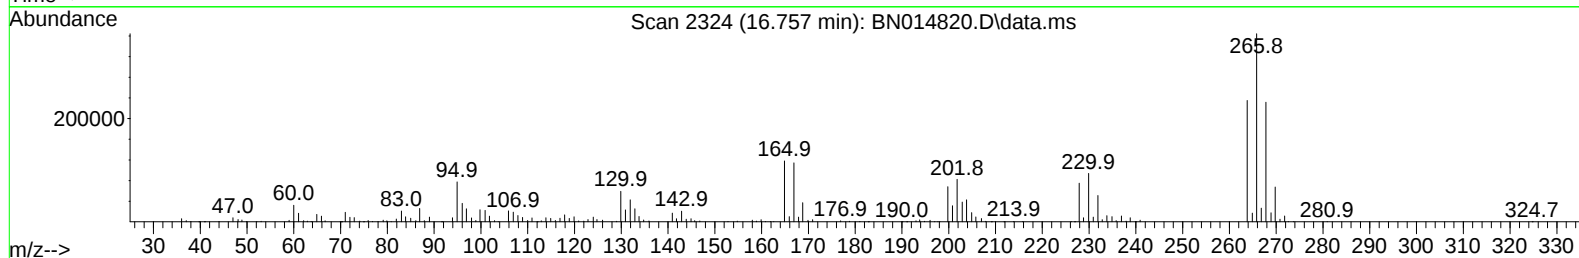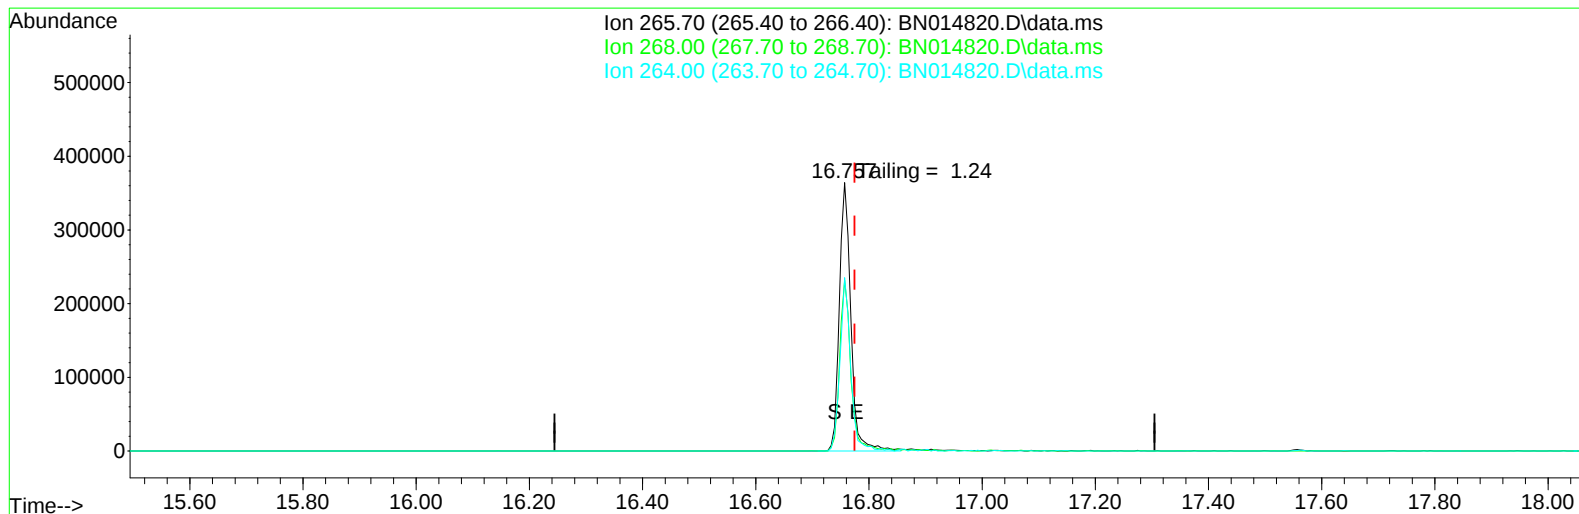

TIC: BN014820.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.017) 18168.64 ng

response 513156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.59
264.00	61.60	64.56
0.00	0.00	0.00