
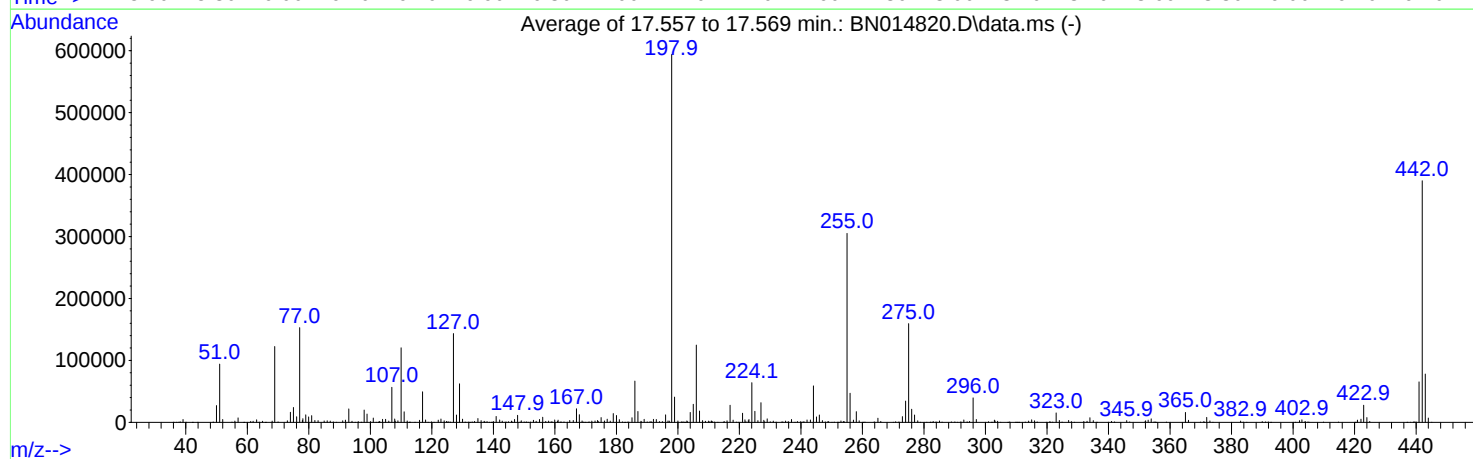


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060221\
 Data File : BN014820.D
 Acq On : 02 Jun 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 01 17:40:45 2021

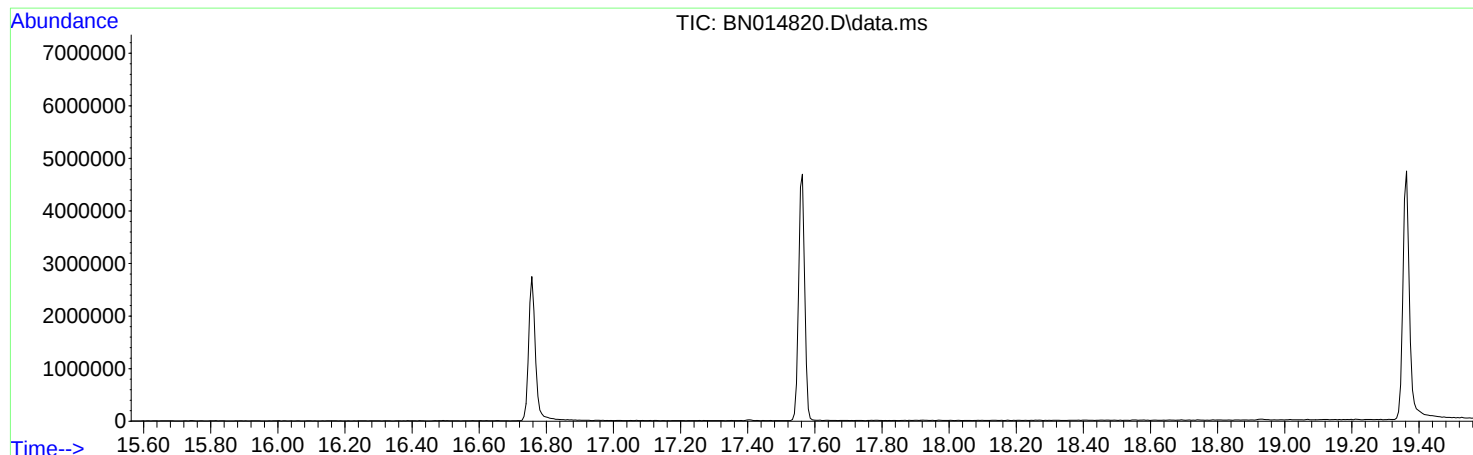




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.8	94117	PASS
68	69	0.00	2	1.7	2131	PASS
69	198	0.00	100	20.6	122421	PASS
70	69	0.00	2	0.6	758	PASS
127	198	10	80	24.1	143368	PASS
197	198	0.00	2	0.4	2382	PASS
198	198	100	100	100.0	593877	PASS
199	198	5	9	6.9	40912	PASS
275	198	10	60	26.8	159360	PASS
365	198	1	100	2.7	16158	PASS
441	198	0.01	100	11.0	65301	PASS
442	442	50	100	100.0	390101	PASS
443	442	15	24	20.0	77944	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060221\
Data File : BN014820.D
Acq On : 02 Jun 2021 10:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 02 11:35:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

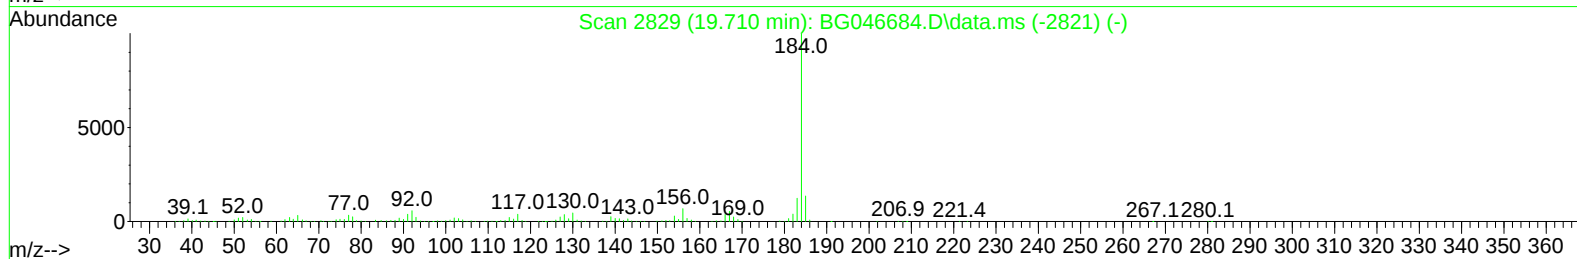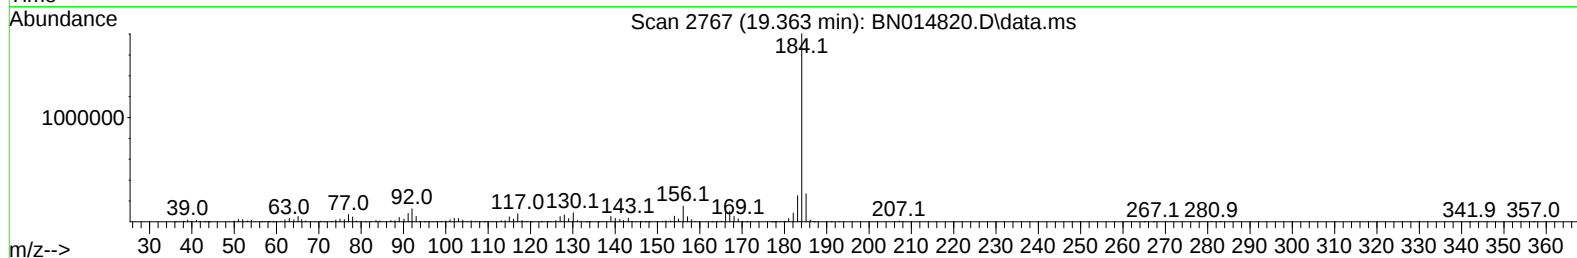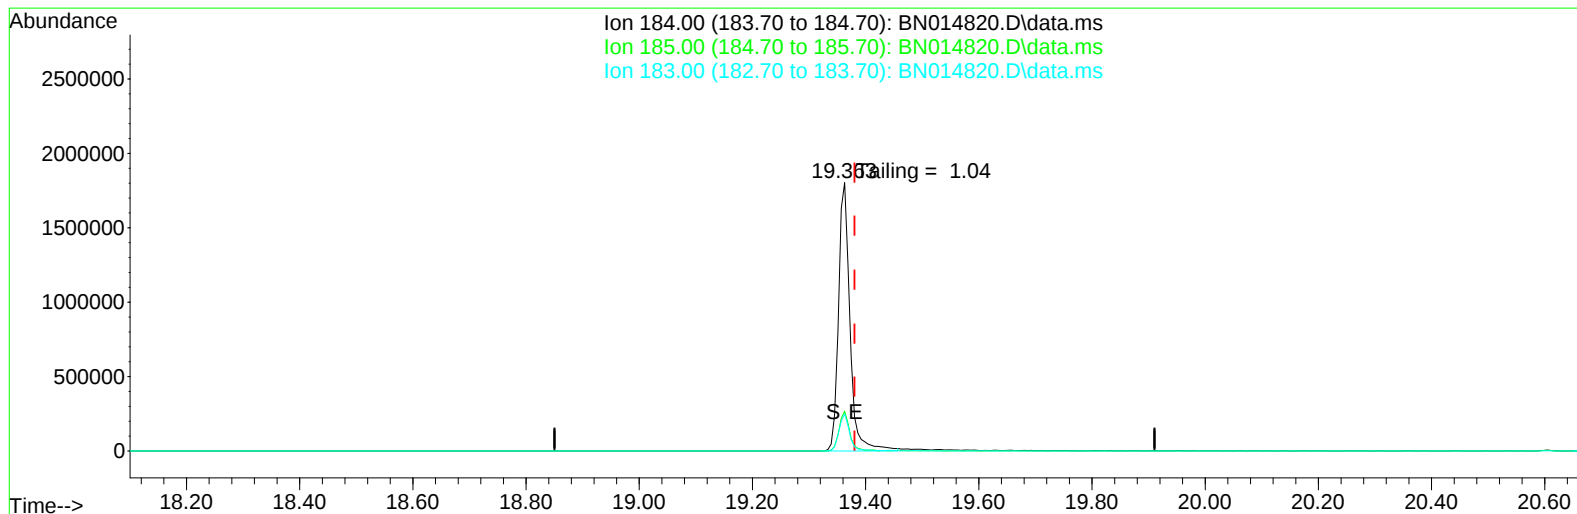

TIC: BN014820.D\data.ms

(77) Benzidine

19.363min (-0.017) 707289.22 ng




response 2550887

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.89
183.00	13.20	13.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060221\
 Data File : BN014820.D
 Acq On : 02 Jun 2021 10:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 02 11:35:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

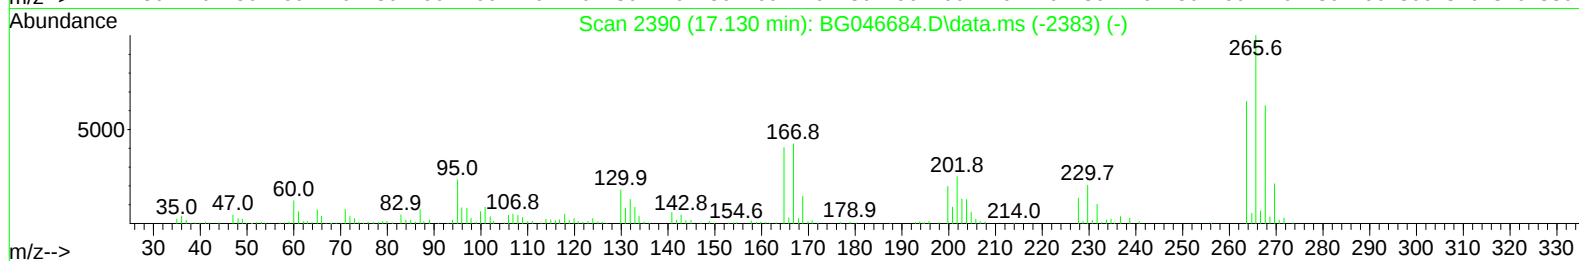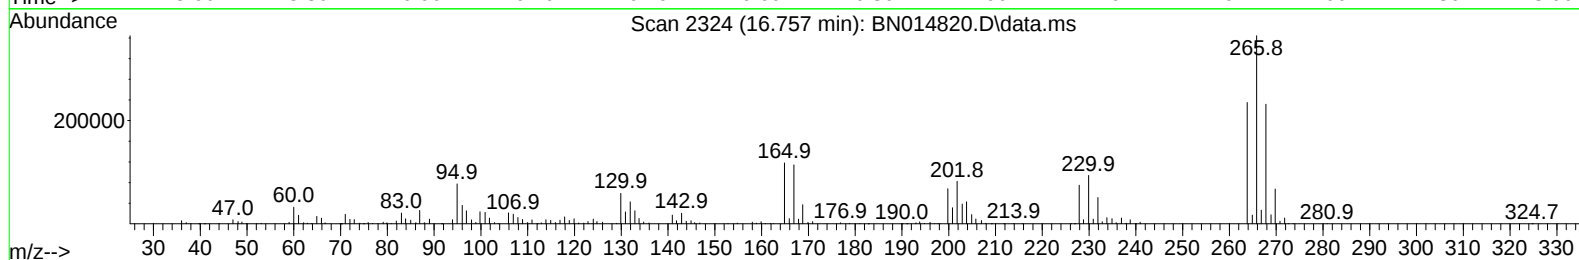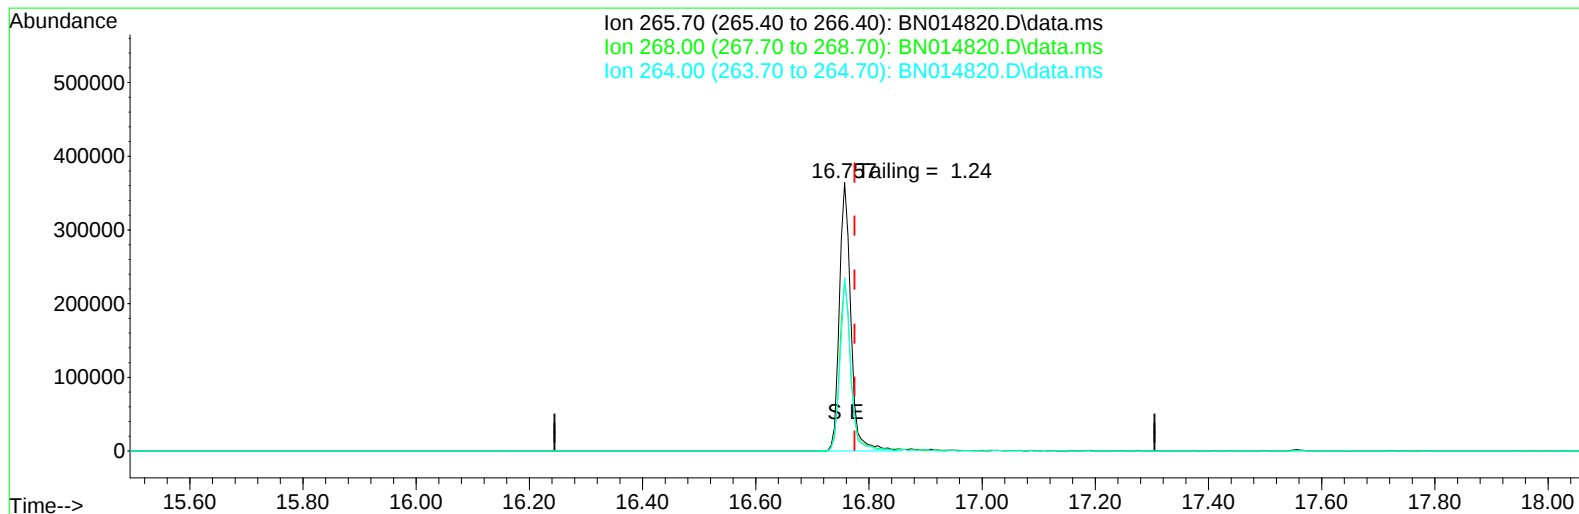

TIC: BN014820.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.017) 18168.64 ng

response 513156

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.59
264.00	61.60	64.56
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/2/2021	BNA_N	<u>BN014820.D</u>
Compound Name	Response	Retention Time
DDT	1674645	20.6
DDD	4408	20.16
DDE	2728	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7136	1681781	0.42

Instrument :
BNA_N
ClientSampleId :
DFTPP