


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060321\
 Data File : BN014826.D
 Acq On : 03 Jun 2021 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 04 05:24:34 2021

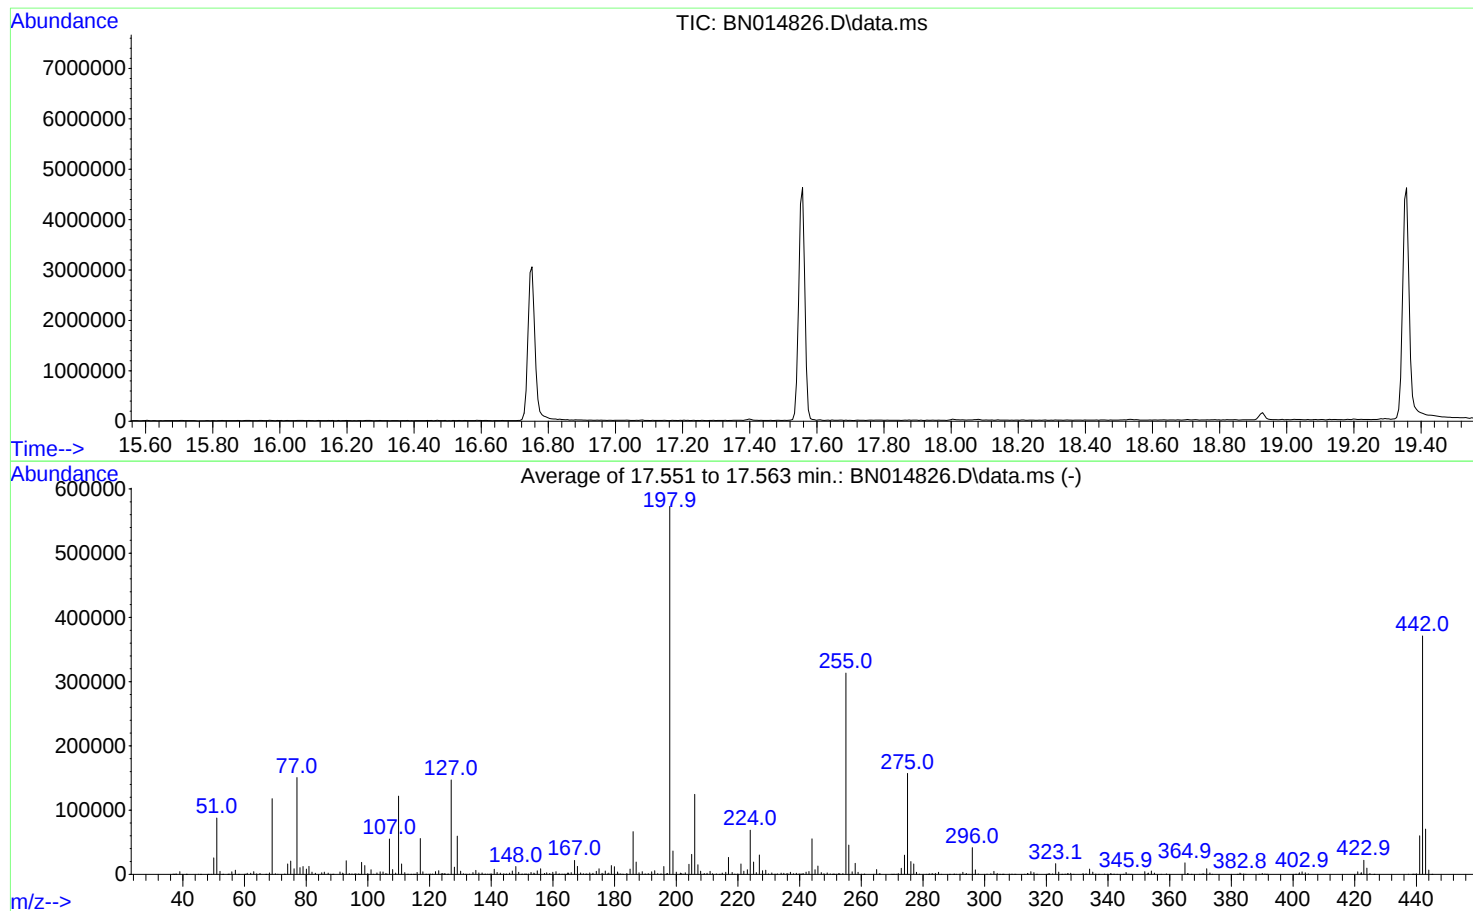




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.3	87664	PASS
68	69	0.00	2	1.9	2184	PASS
69	198	0.00	100	20.6	117912	PASS
70	69	0.00	2	0.9	1027	PASS
127	198	10	80	25.7	147091	PASS
197	198	0.00	2	0.3	1541	PASS
198	198	100	100	100.0	572693	PASS
199	198	5	9	6.3	36291	PASS
275	198	10	60	27.4	157091	PASS
365	198	1	100	3.2	18074	PASS
441	198	0.01	100	10.5	60189	PASS
442	442	50	100	100.0	371072	PASS
443	442	15	24	19.0	70451	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060321\
 Data File : BN014826.D
 Acq On : 03 Jun 2021 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 03 16:04:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

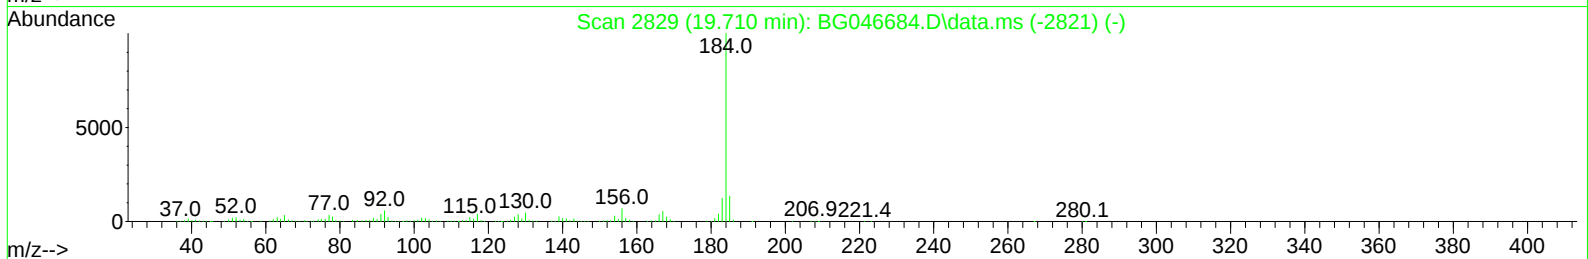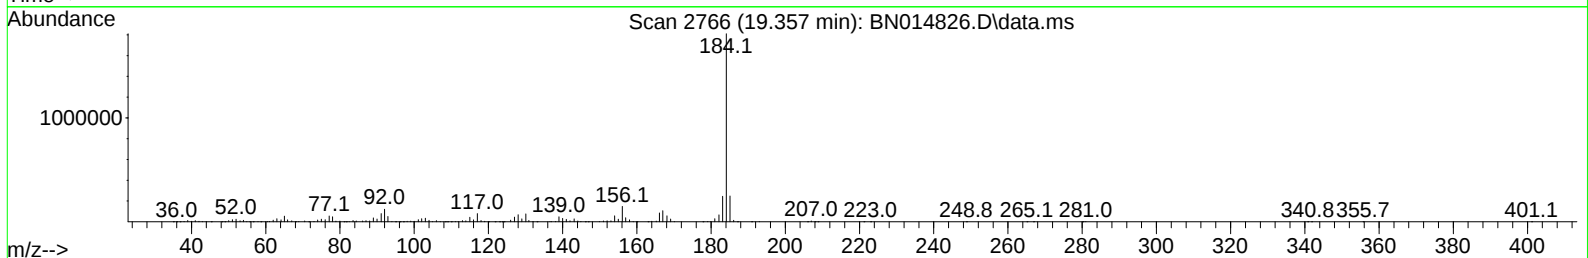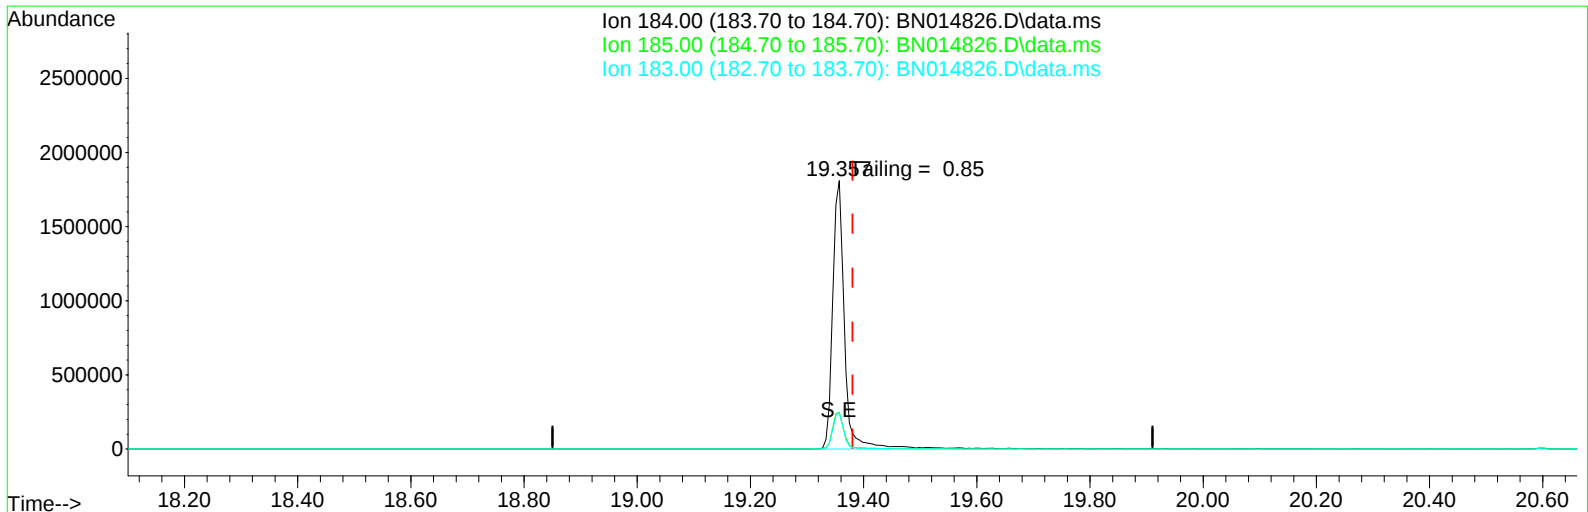

TIC: BN014826.D\data.ms

(77) Benzidine

19.357min (-0.023) 631200.09 ng




response 2587778

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.68
183.00	13.20	13.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060321\
 Data File : BN014826.D
 Acq On : 03 Jun 2021 15:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 03 16:04:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 22 07:55:10 2021
 Response via : Initial Calibration

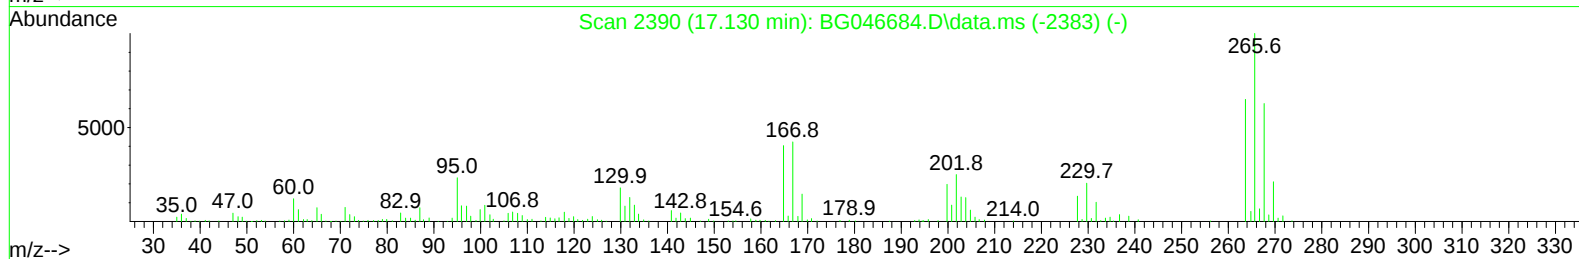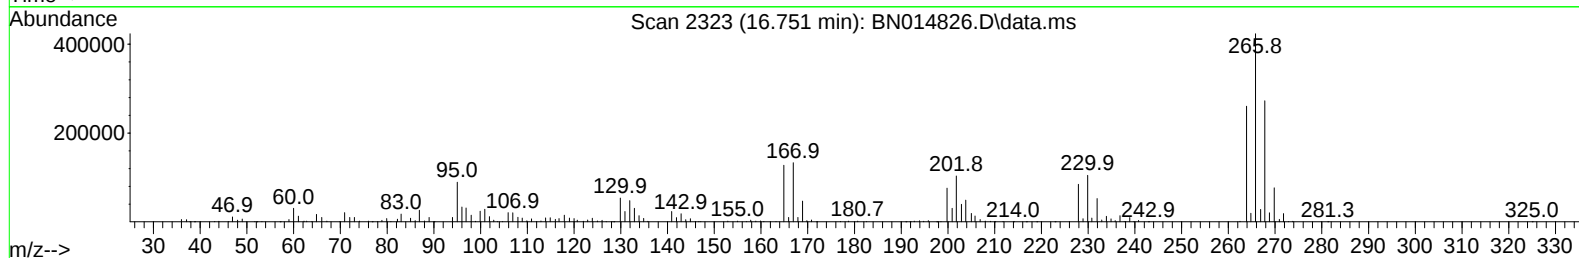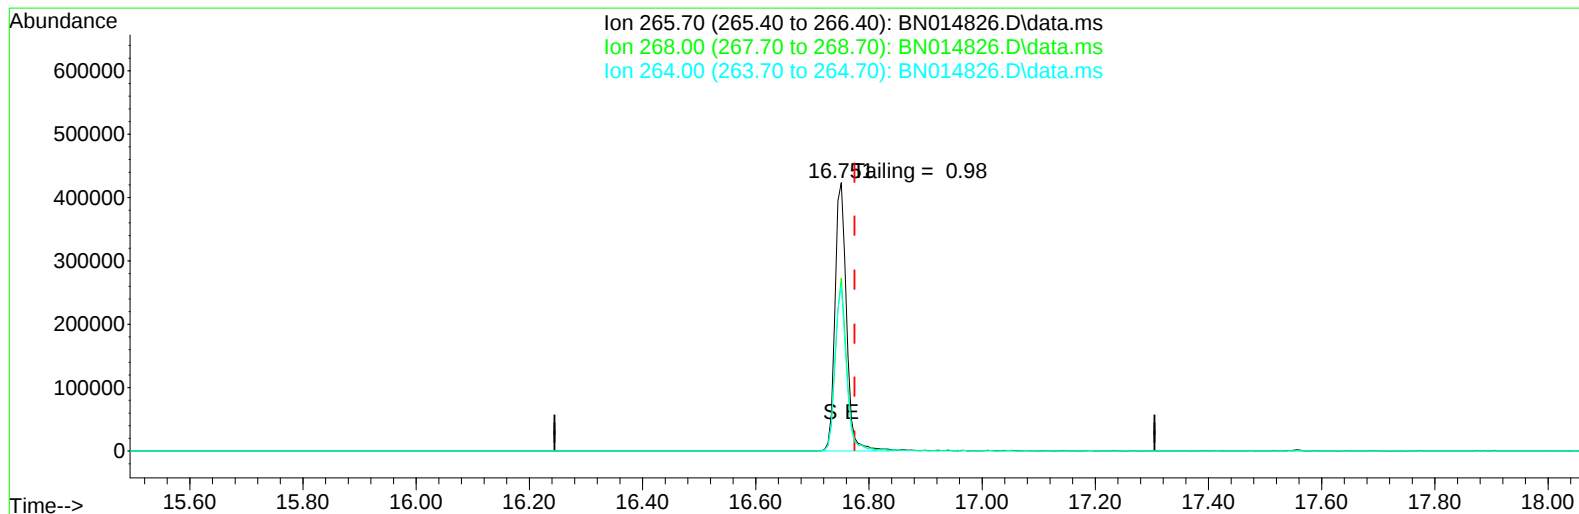

TIC: BN014826.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.023) 22595.53 ng

response 596518

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.37
264.00	61.60	61.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2021	BNA_N	<u>BN014826.D</u>
Compound Name	Response	Retention Time
DDT	1686370	20.59
DDD	1791	20.15
DDE	2469	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4260	1690630	0.25

Instrument :
BNA_N
ClientSampleId :
DFTPP