
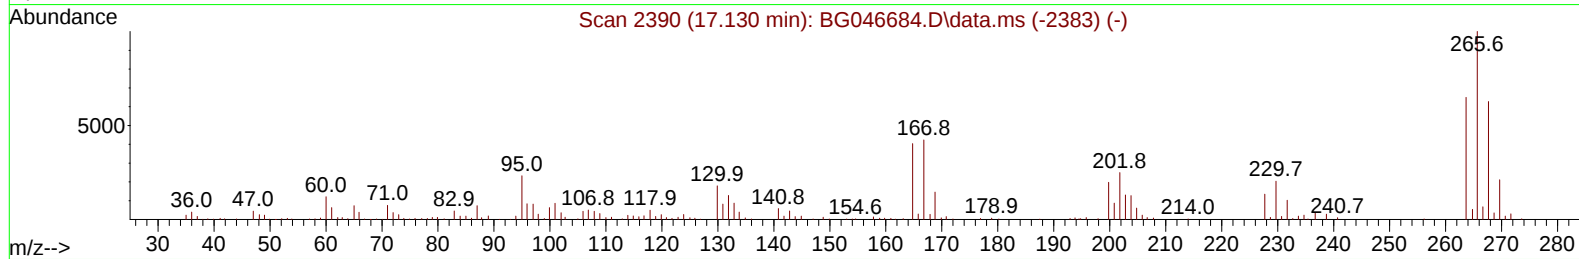
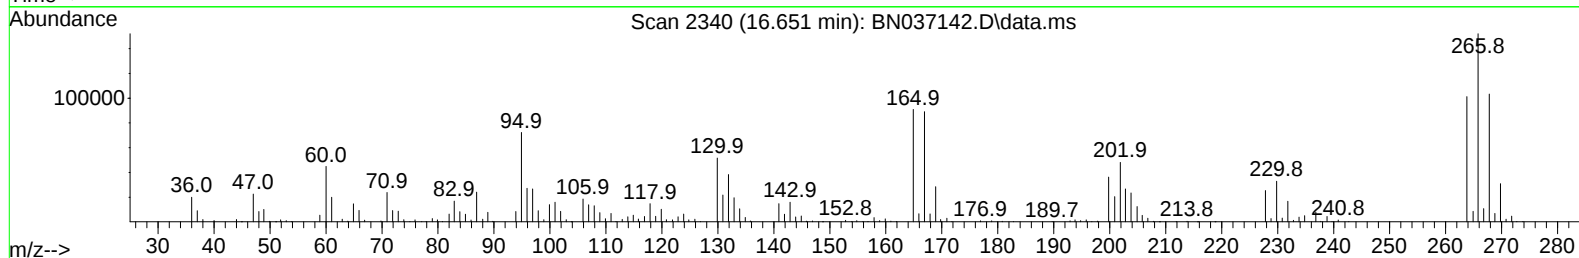


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037142.D
Acq On : 03 Jun 2025 10:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 13:49:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

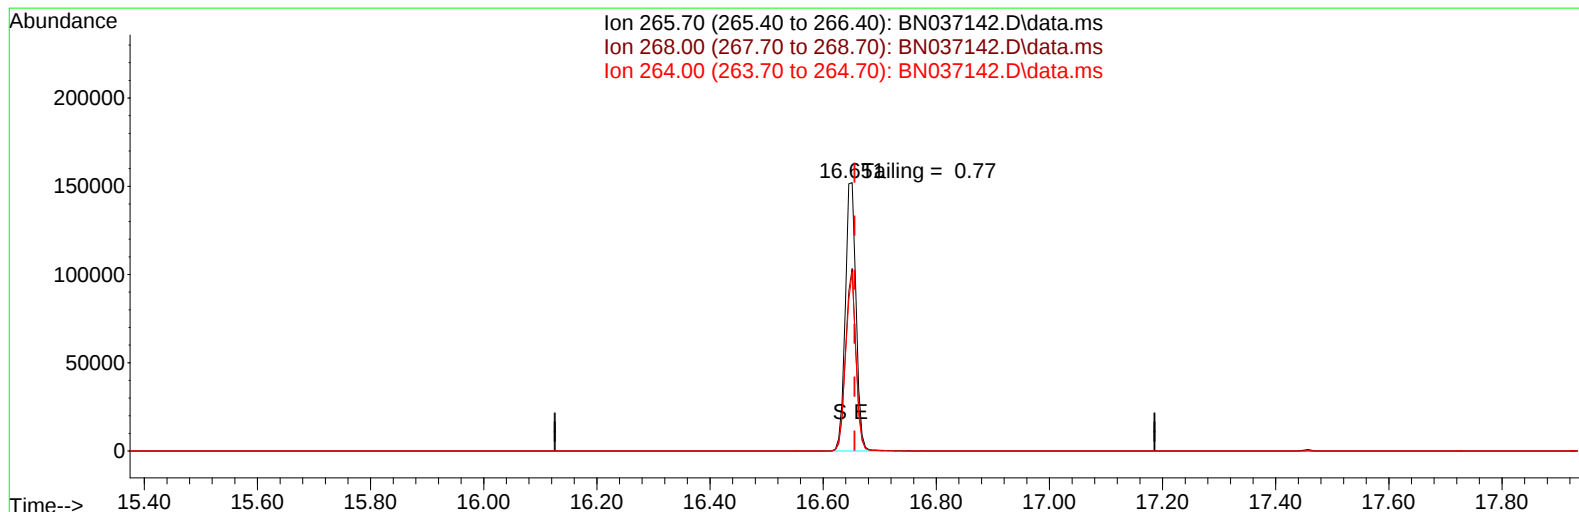

TIC: BN037142.D\data.ms

(70) Pentachlorophenol (C)




16.651min (-0.005) 16176.78 ng

response 200710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.97
264.00	61.60	66.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060325\
Data File : BN037142.D
Acq On : 03 Jun 2025 10:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 13:56:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 27 07:40:28 2025
Response via : Initial Calibration

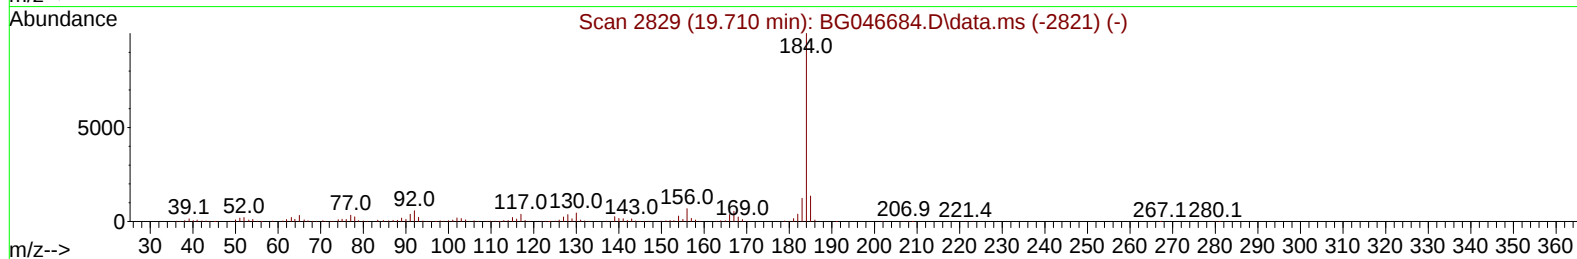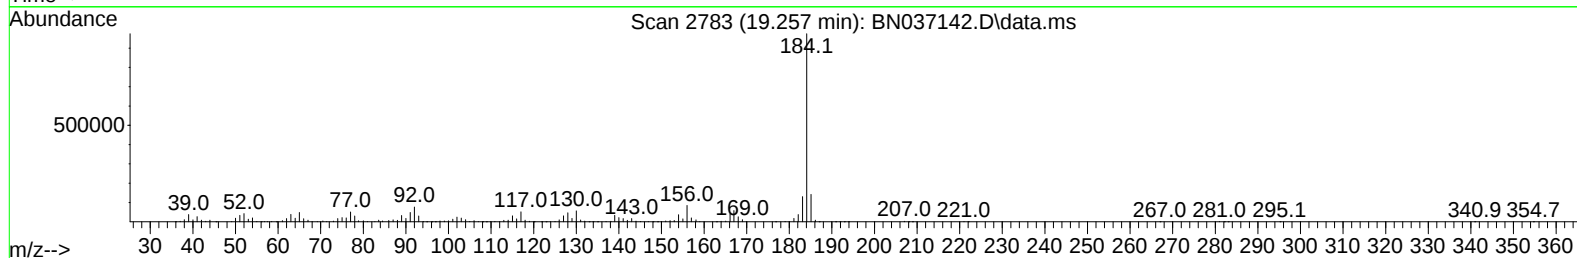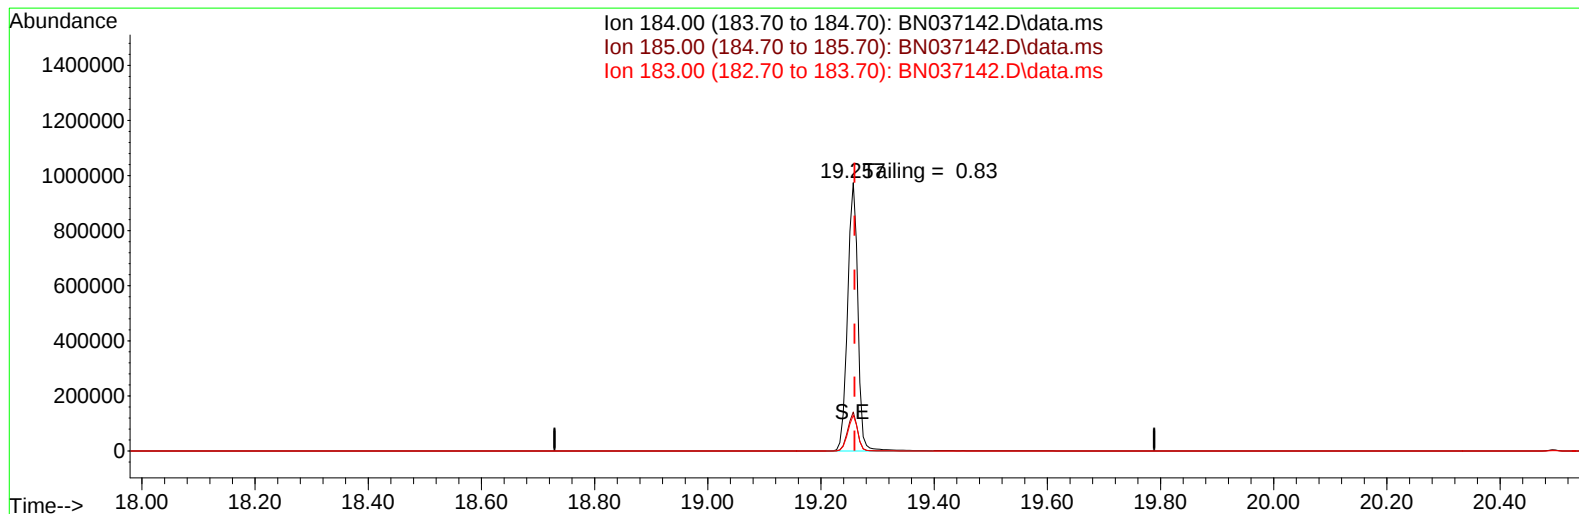

TIC: BN037142.D\data.ms

(77) Benzidine

19.257min (-0.002) 0.00 ng

response 1234162

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	13.40
0.00	0.00	0.00