




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
 Data File : BN010767.D
 Acq On : 04 Jun 2020 18:00
 Operator : CG/JU
 Sample : PB BL-W-02
 Misc : PB BL-W-02
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB BL-W-02

Manual Integrations
 APPROVED

mohammad
 6/5/2020 10:31:04 AM

Quant Time: Jun 04 18:32:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 14:30:28 2020
 Response via : Initial Calibration

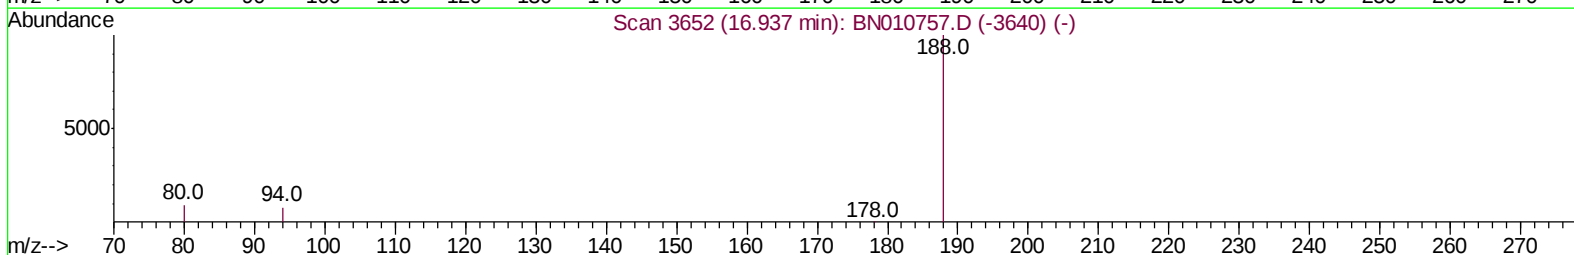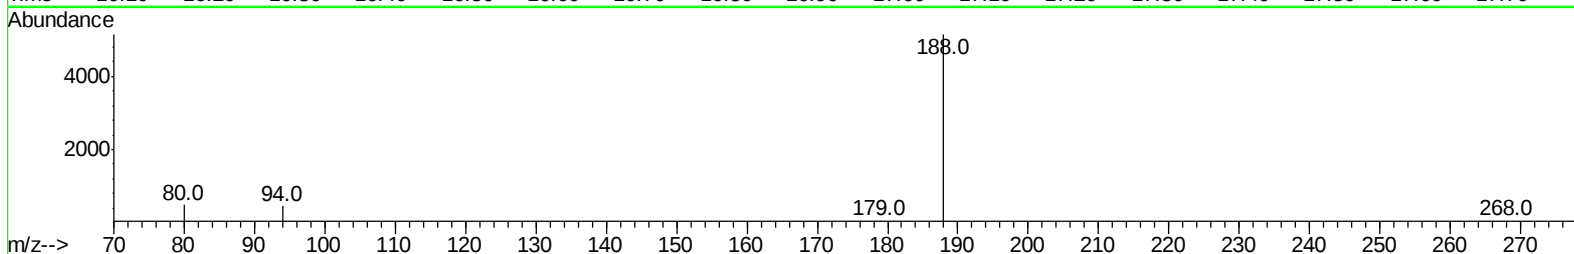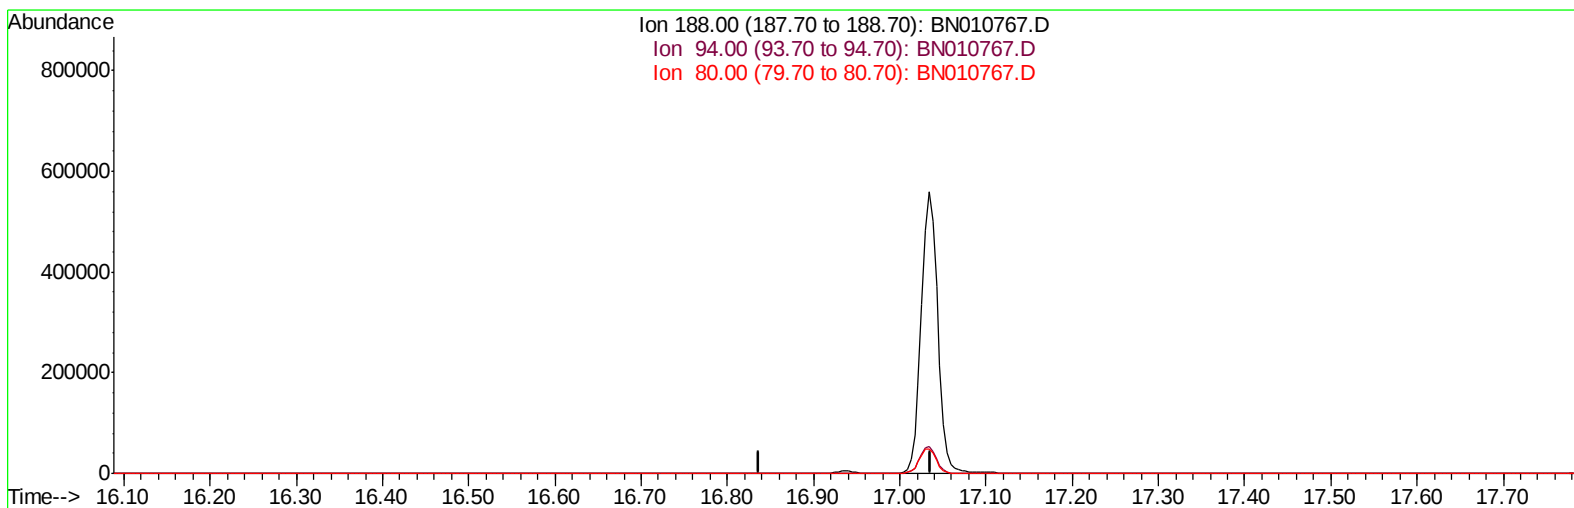

TIC: BN010767.D

(10) Phenanthrene-d10 (I)

16.937min (-16.937) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.70	0.00#
80.00	10.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
 Data File : BN010767.D
 Acq On : 04 Jun 2020 18:00
 Operator : CG/JU
 Sample : PB BL-W-02
 Misc : PB BL-W-02
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB BL-W-02

Manual Integrations
 APPROVED

mohammad
 6/5/2020 10:31:04 AM

Quant Time: Jun 04 18:32:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 14:30:28 2020
 Response via : Initial Calibration

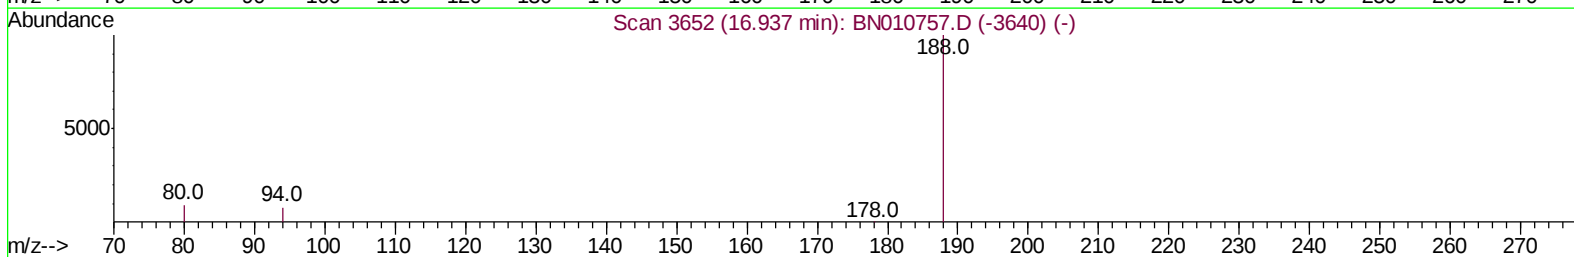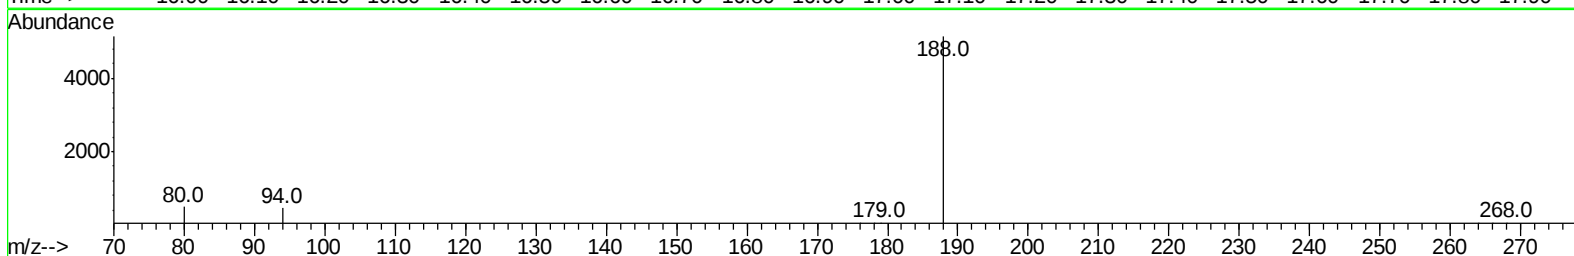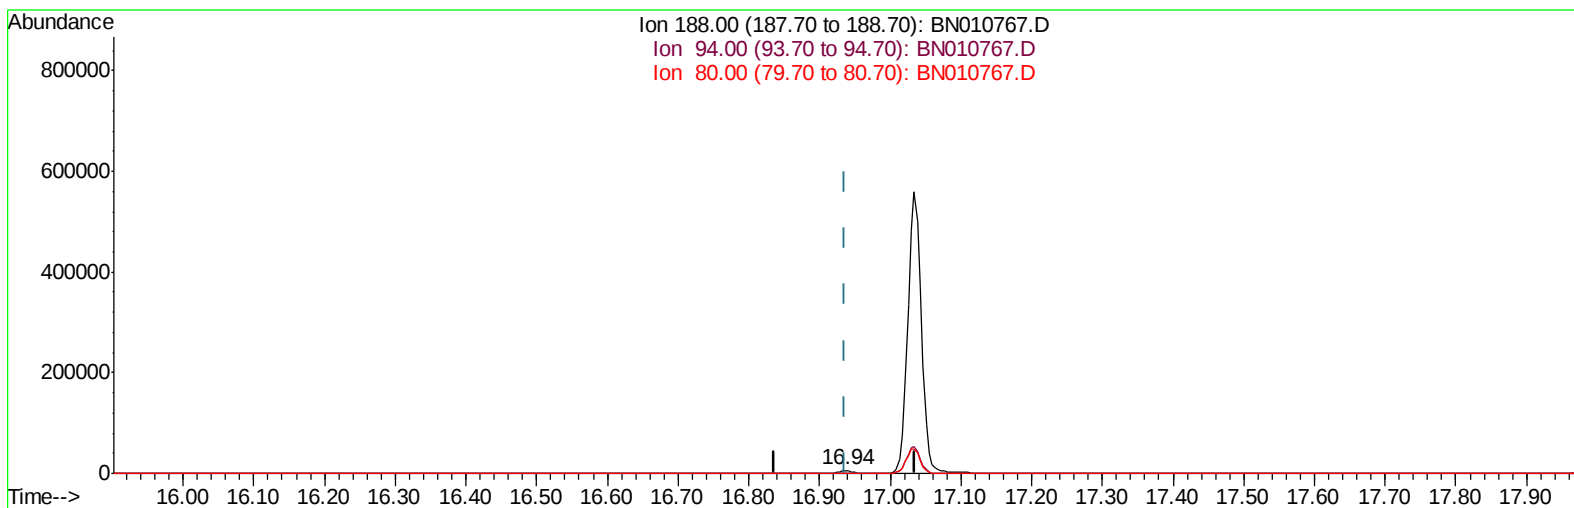

TIC: BN010767.D

(10) Phenanthrene-d10 (I)

16.937min (-0.000) 0.40ng/ul m

response 7138

Ion	Exp%	Act%
188.00	100	100
94.00	9.70	8.92
80.00	10.40	9.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
Data File : BN010767.D
Acq On : 04 Jun 2020 18:00
Operator : CG/JU
Sample : PB BL-W-02
Misc : PB BL-W-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB BL-W-02

Manual Integrations
APPROVED

mohammad
6/5/2020 10:31:04 AM

Quant Time: Jun 04 18:32:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 14:30:28 2020
Response via : Initial Calibration

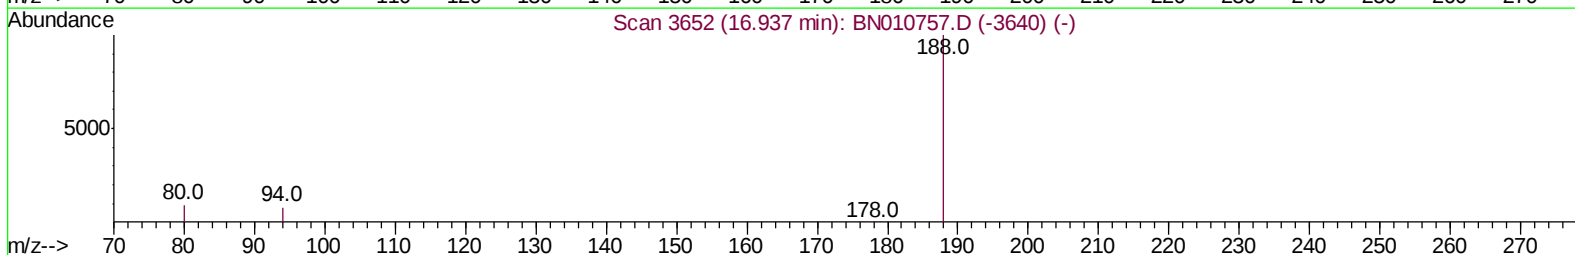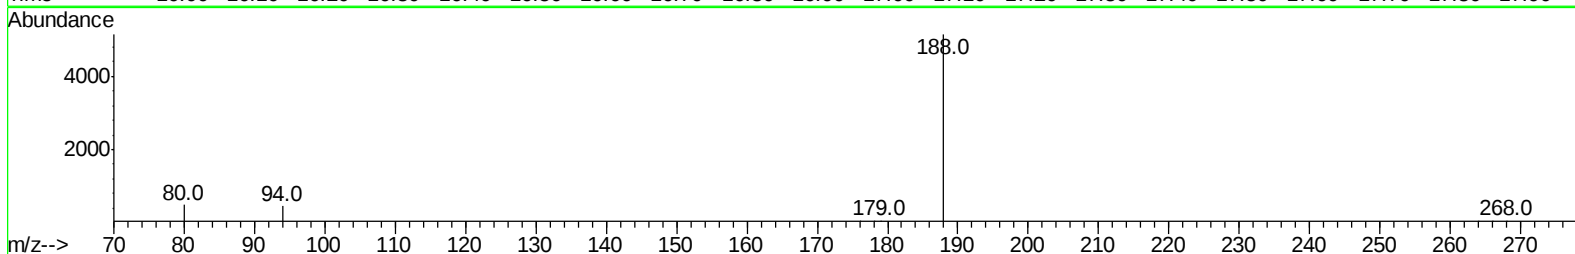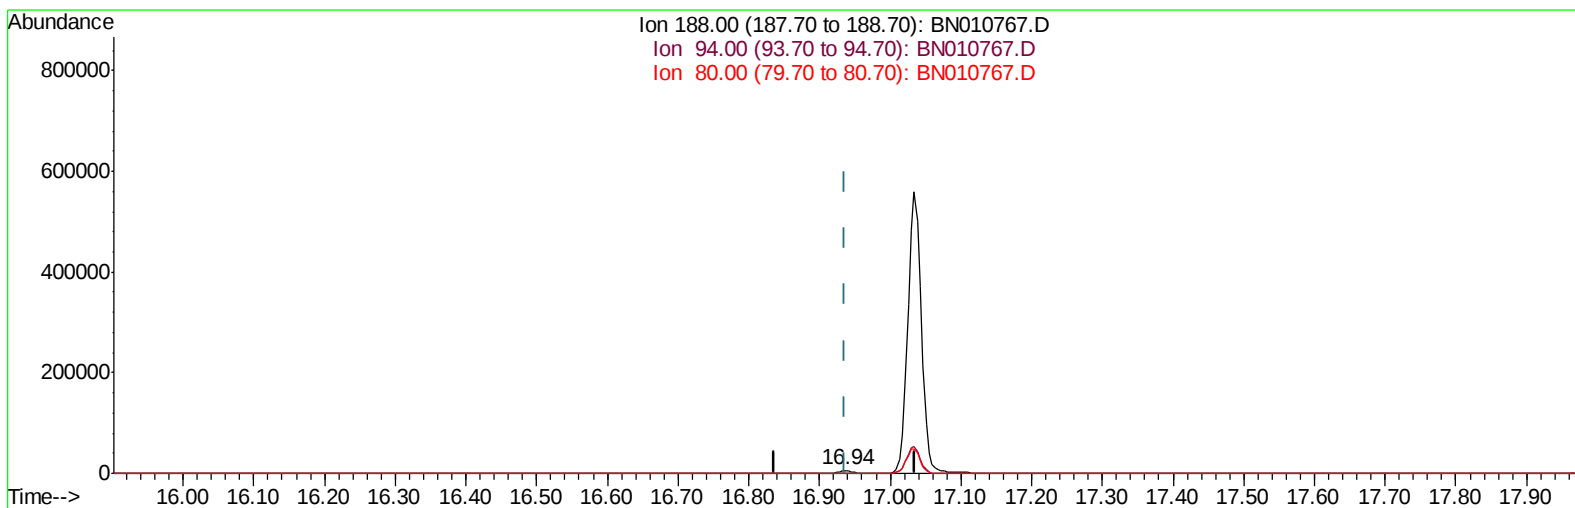

TIC: BN010767.D

(10) Phenanthrene-d10 (I)

16.937min (-0.000) 0.40ng/ul m

response 7138

Ion	Exp%	Act%
188.00	100	100
94.00	9.70	8.92
80.00	10.40	9.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
Data File : BN010767.D
Acq On : 04 Jun 2020 18:00
Operator : CG/JU
Sample : PB BL-W-02
Misc : PB BL-W-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB BL-W-02

Manual Integrations
APPROVED

mohammad
6/5/2020 10:31:04 AM

Quant Time: Jun 04 18:34:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 14:30:28 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1941	0.40	ng/ul	0.00
2) Naphthalene-d8	10.32	136	6350	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	3459	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	7138m	0.40	ng/ul	0.00
16) Chrysene-d12	21.15	240	5575	0.40	ng/ul	0.00
20) Perylene-d12	23.29	264	7185	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.92	152	3904	0.26	ng/ul	0.00
14) Fluoranthene-d10	18.97	212	7659	0.25	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
Data File : BN010767.D
Acq On : 04 Jun 2020 18:00
Operator : CG/JU
Sample : PB BL-W-02
Misc : PB BL-W-02
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB BL-W-02

Manual Integrations
APPROVED

mohammad
6/5/2020 10:31:04 AM

Quant Time: Jun 04 18:34:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 14:30:28 2020
Response via : Initial Calibration

