




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
Data File : BN010771.D
Acq On : 04 Jun 2020 20:25
Operator : CG/JU
Sample : L1955-10
Misc : MDL-W-03
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03

Manual Integrations
APPROVED

mohammad
6/5/2020 10:31:16 AM

Quant Time: Jun 05 02:28:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 02:21:03 2020
Response via : Initial Calibration

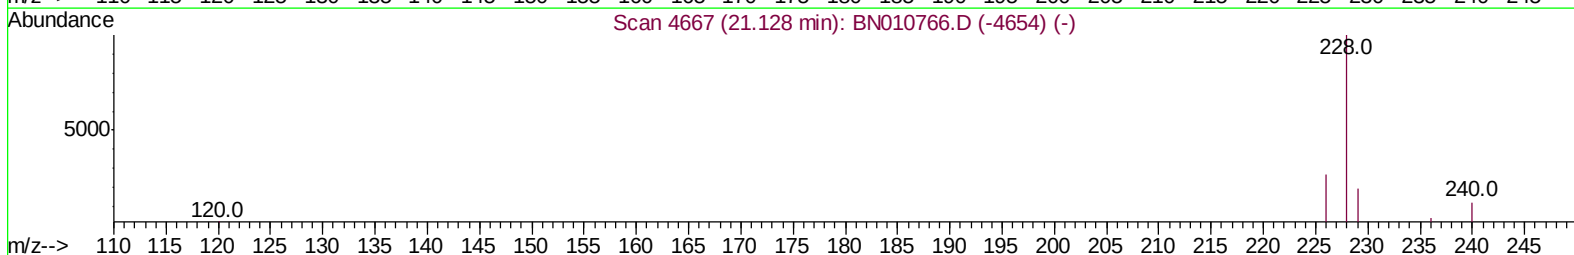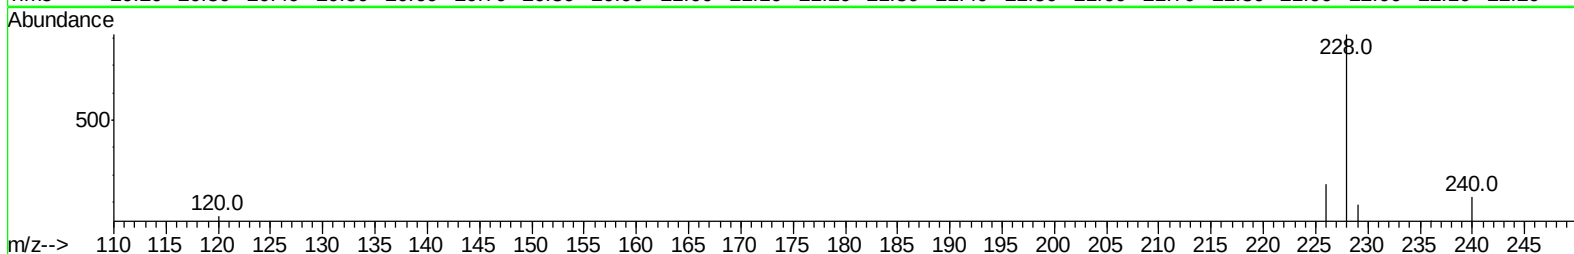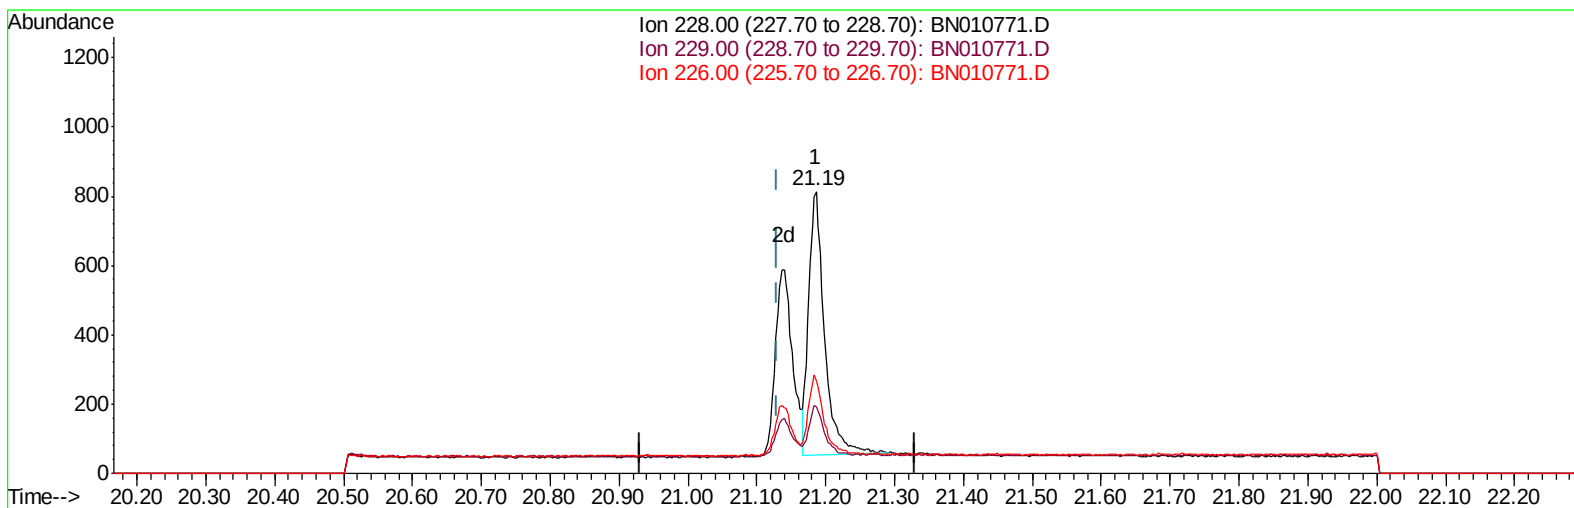

TIC: BN010771.D

(18) Benzo(a)anthracene
21.186min (+0.055) 0.07ng/ul
response 1221

Ion	Exp%	Act%
228.00	100	100
229.00	20.00	23.86
226.00	28.60	32.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060420\
Data File : BN010771.D
Acq On : 04 Jun 2020 20:25
Operator : CG/JU
Sample : L1955-10
Misc : MDL-W-03
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-03

Manual Integrations
APPROVED

mohammad
6/5/2020 10:31:16 AM

Quant Time: Jun 05 02:28:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 02:21:03 2020
Response via : Initial Calibration

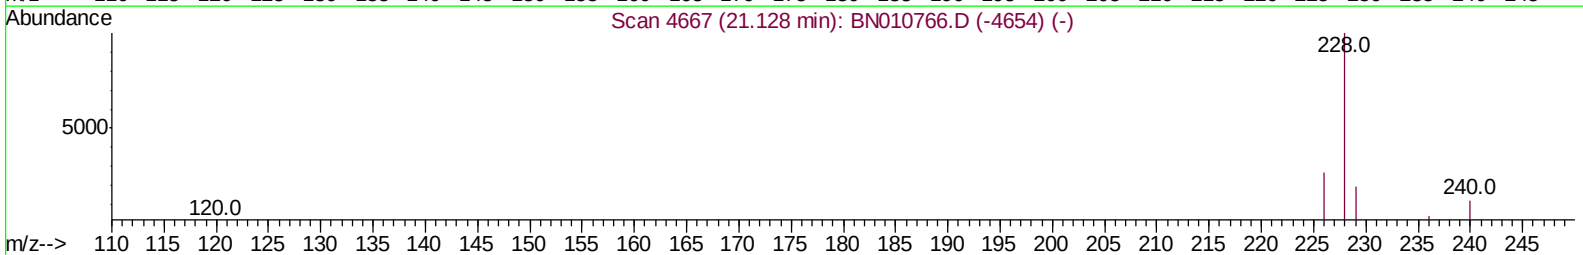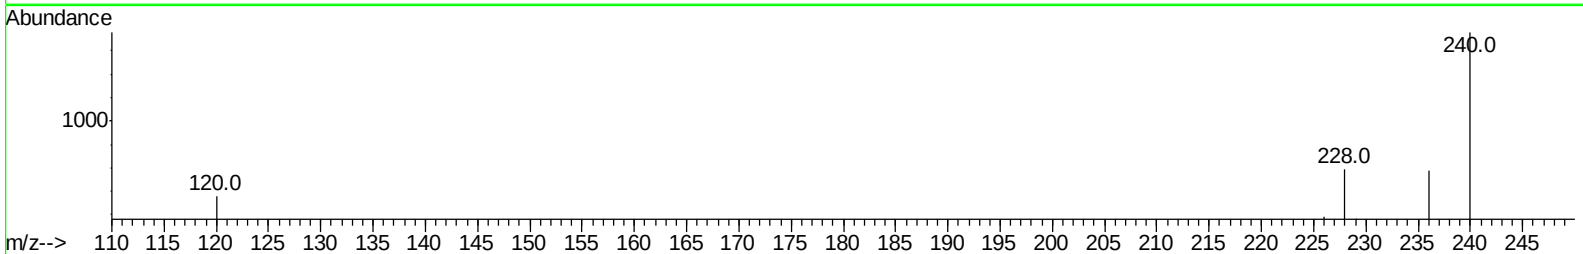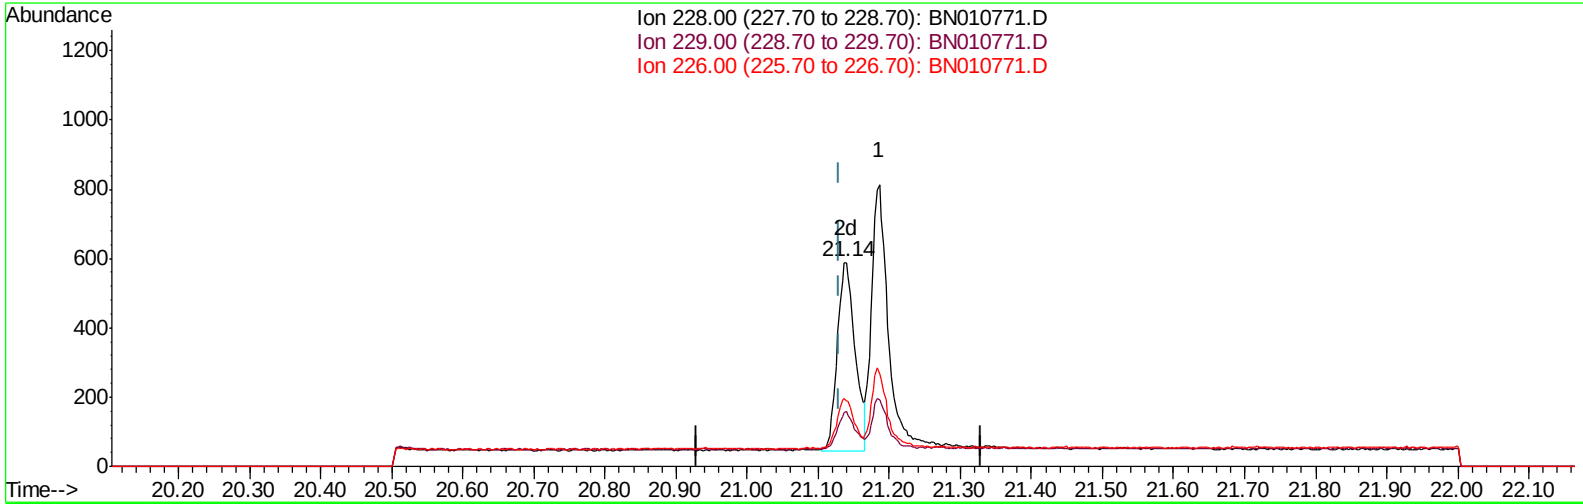

TIC: BN010771.D

(18) Benzo(a)anthracene

21.139min (+0.009) 0.05ng/ul m

response 949

Ion	Exp%	Act%
228.00	100	100
229.00	20.00	27.16#
226.00	28.60	31.75
0.00	0.00	0.00