
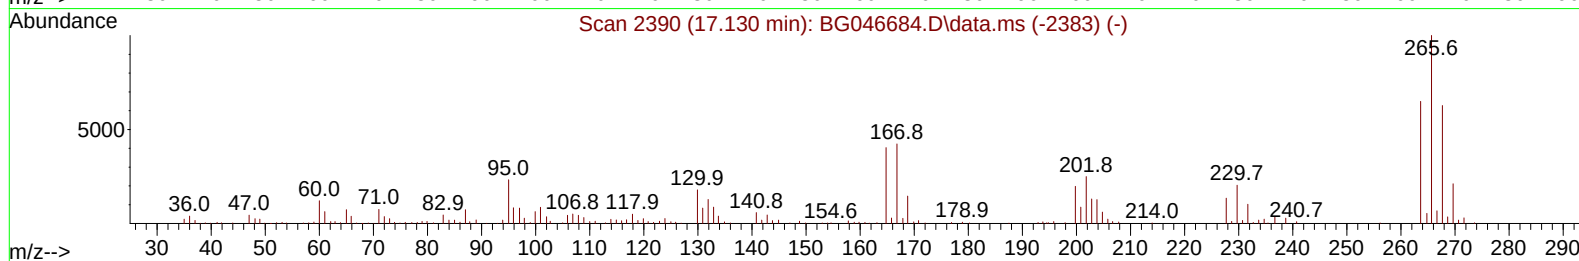
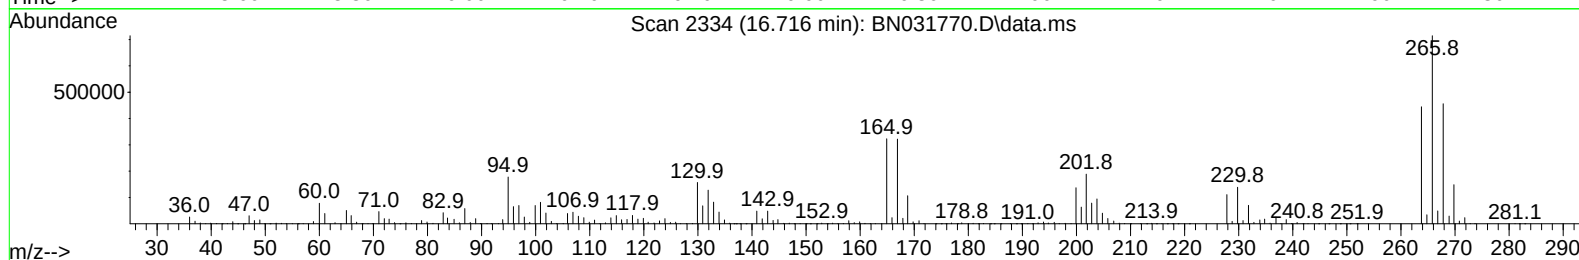


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060424\
Data File : BN031770.D
Acq On : 04 Jun 2024 10:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 12:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

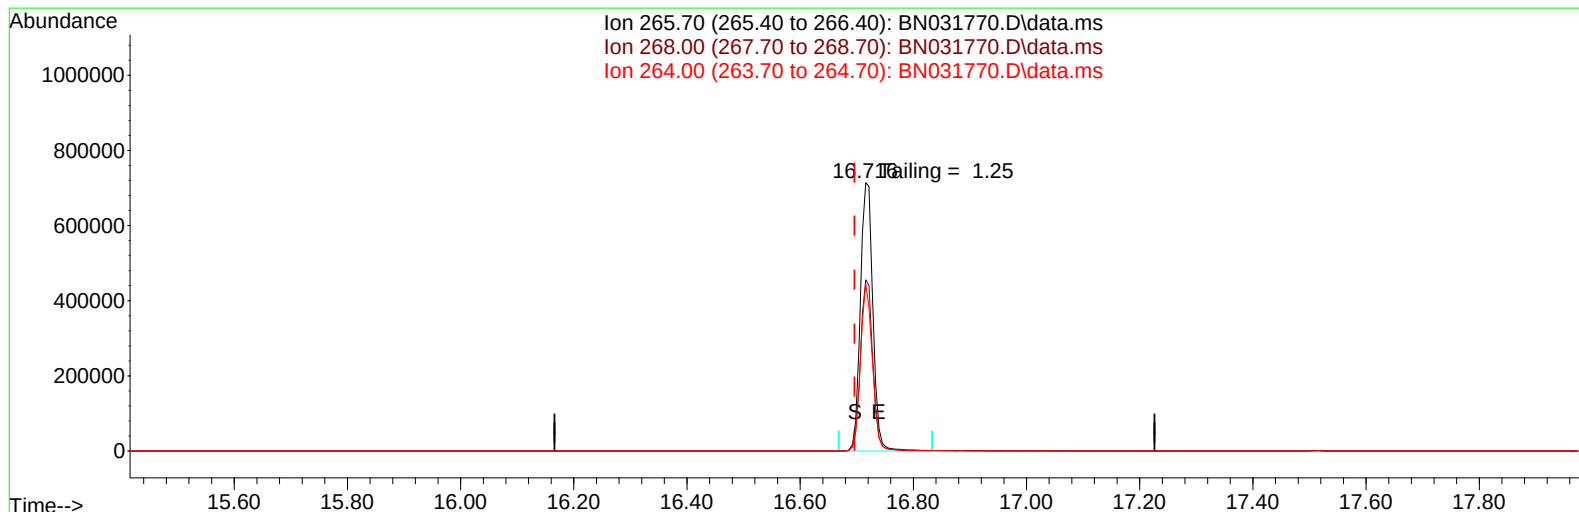

TIC: BN031770.D\data.ms

(70) Pentachlorophenol (C)




16.716min (+ 0.020) 25758.91 ng

response 1099693

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.82
264.00	61.60	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060424\
Data File : BN031770.D
Acq On : 04 Jun 2024 10:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 12:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

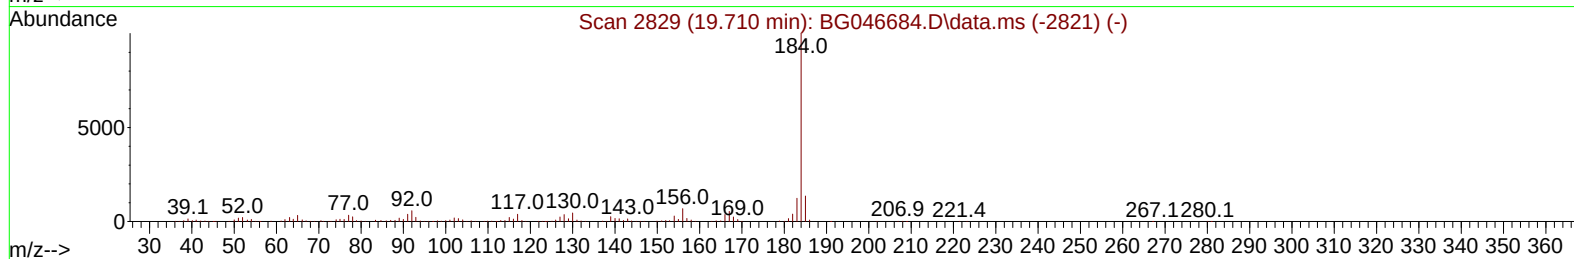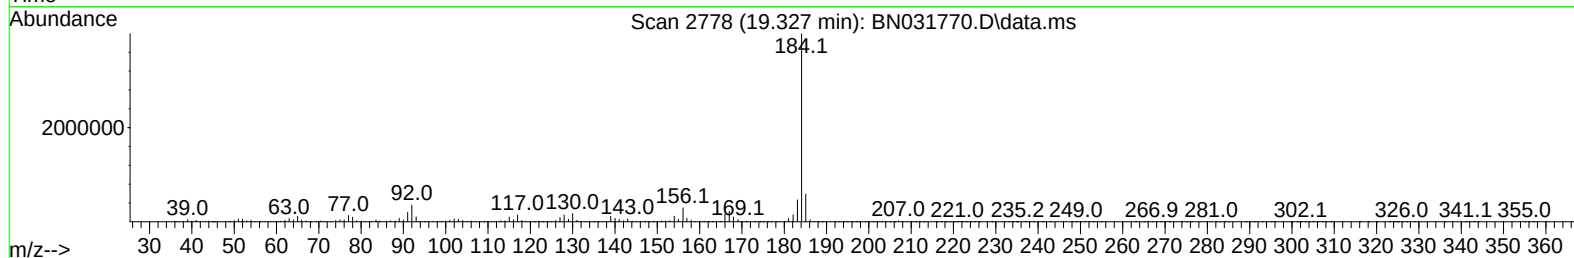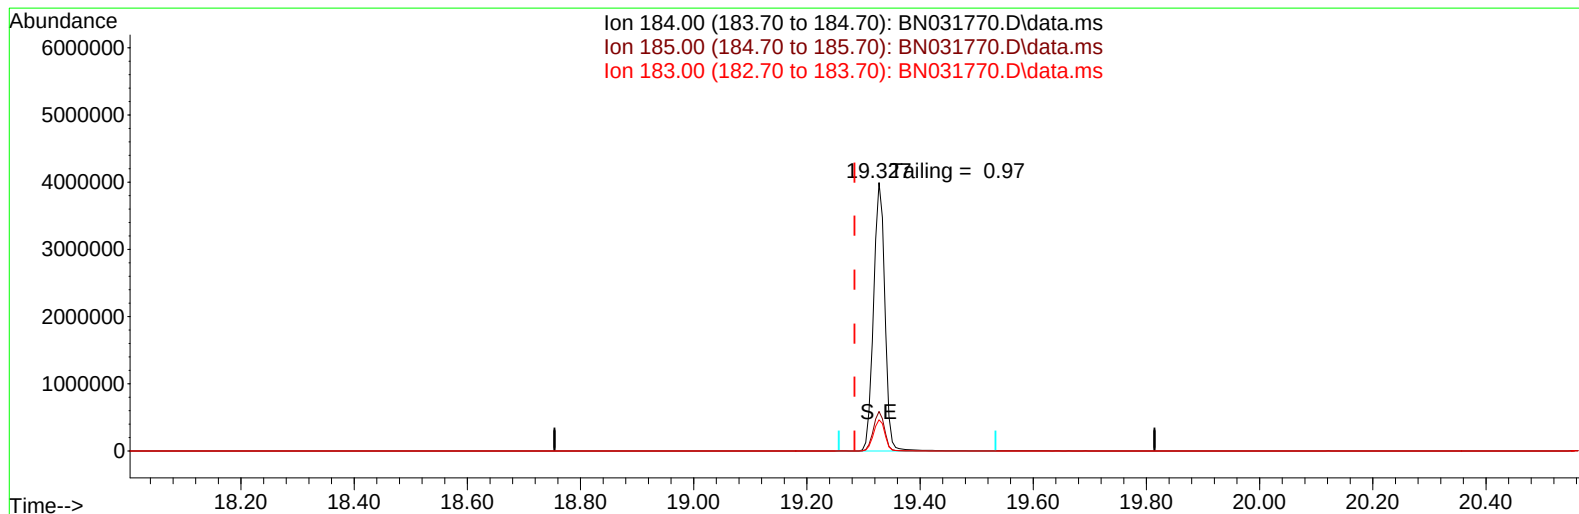

TIC: BN031770.D\data.ms

(77) Benzidine

19.327min (+ 0.043) 281727.19 ng

response 5557981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.75
183.00	13.20	11.63
0.00	0.00	0.00