
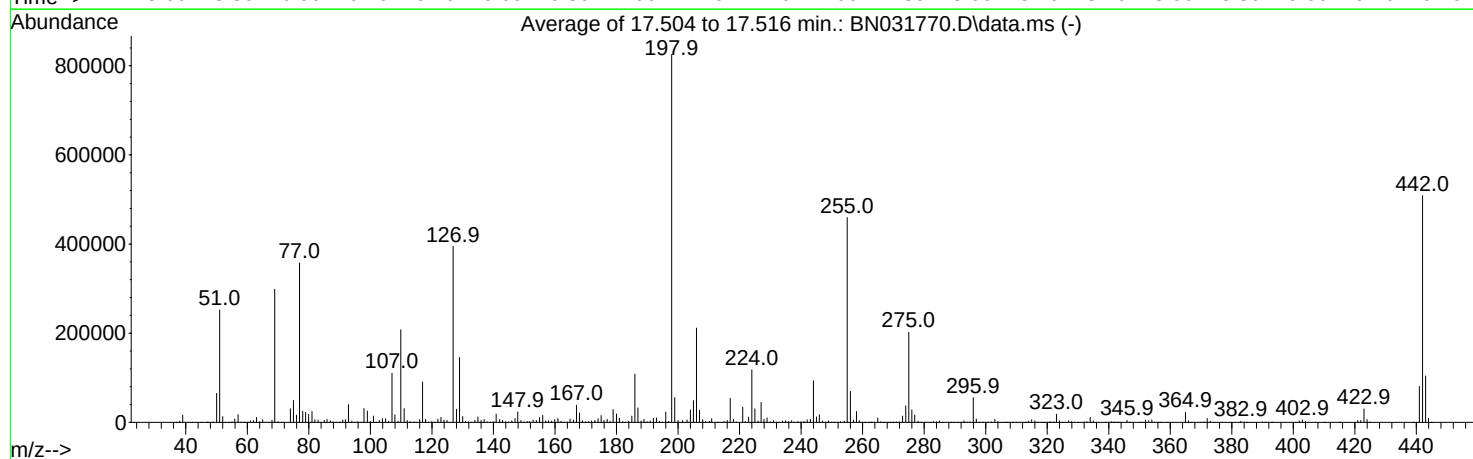


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060424\
Data File : BN031770.D
Acq On : 04 Jun 2024 10:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN050924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 10 02:12:24 2024

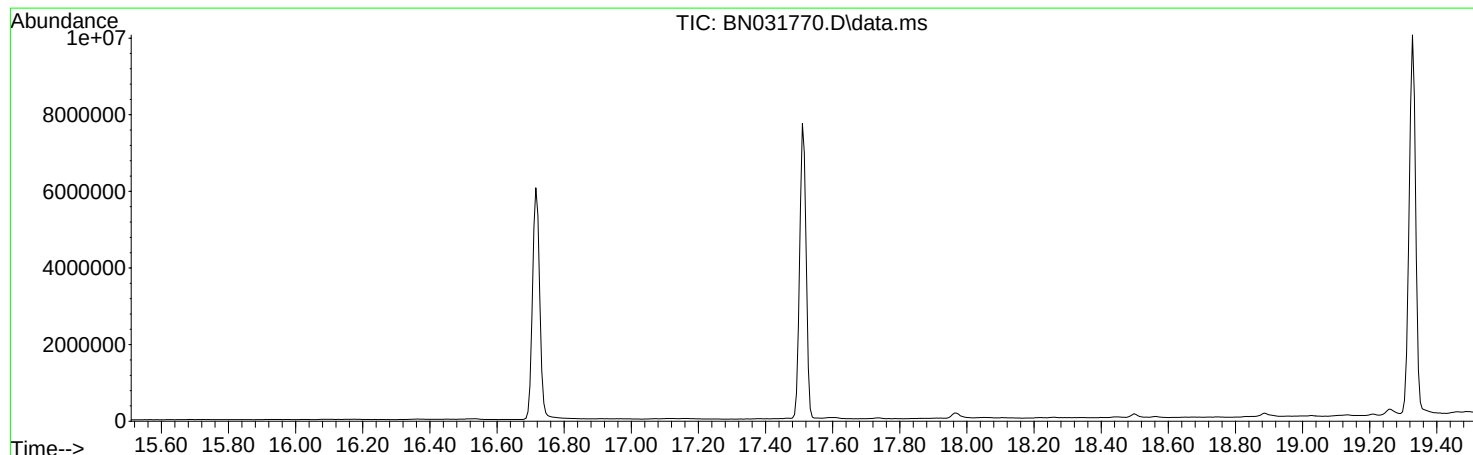




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	252360	PASS
68	69	0.00	2	1.6	4684	PASS
69	198	0.00	100	36.2	298475	PASS
70	69	0.00	2	0.5	1446	PASS
127	198	10	80	47.8	394764	PASS
197	198	0.00	2	0.2	1675	PASS
198	198	100	100	100.0	825216	PASS
199	198	5	9	6.7	55645	PASS
275	198	10	60	24.5	202197	PASS
365	198	1	100	2.7	22574	PASS
441	198	0.01	100	9.8	80896	PASS
442	442	50	100	100.0	508672	PASS
443	442	15	24	20.4	103992	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060424\
Data File : BN031770.D
Acq On : 04 Jun 2024 10:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 12:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

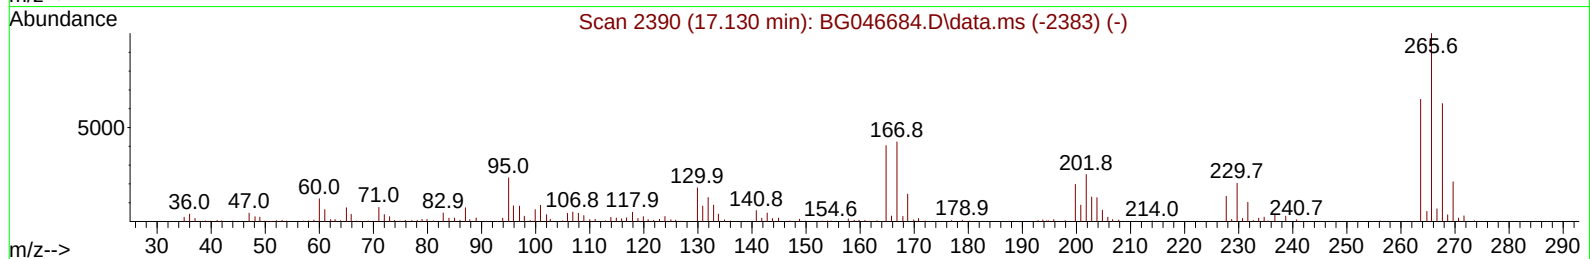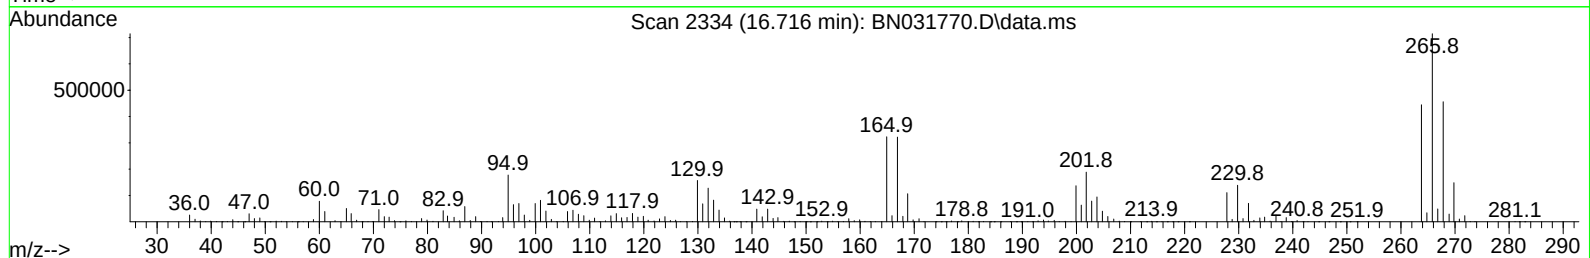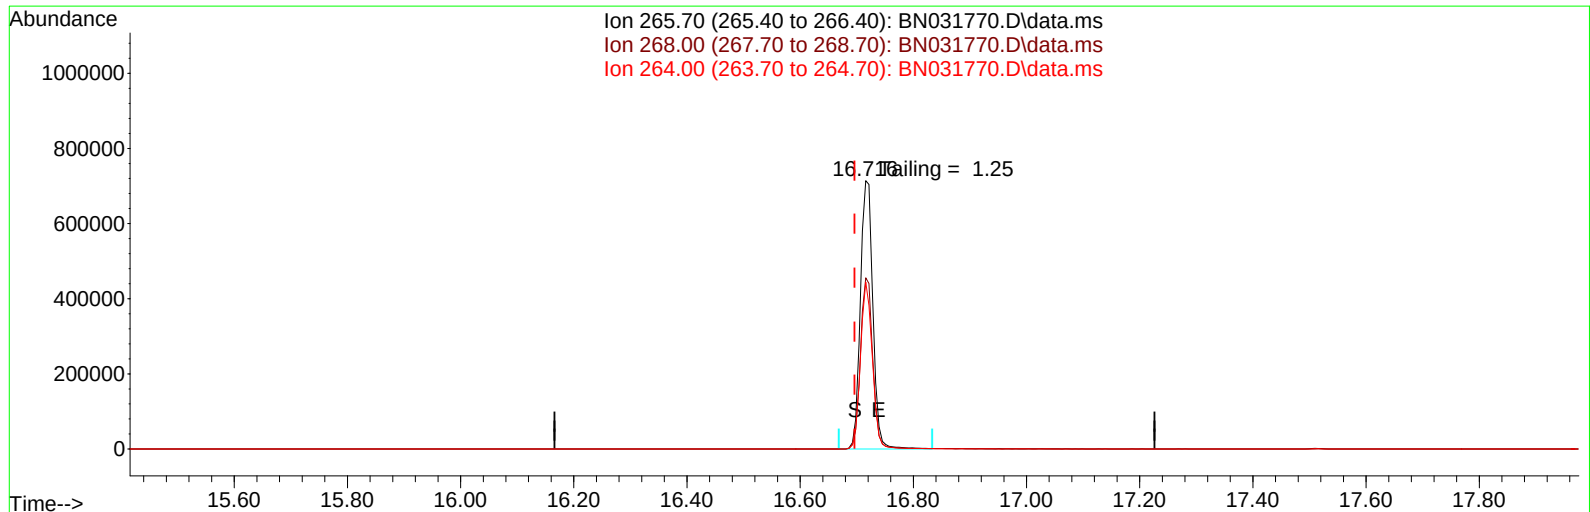

TIC: BN031770.D\data.ms

(70) Pentachlorophenol (C)

16.716min (+ 0.020) 25758.91 ng




response 1099693

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.82
264.00	61.60	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060424\
Data File : BN031770.D
Acq On : 04 Jun 2024 10:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 04 12:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 11 04:09:05 2024
Response via : Initial Calibration

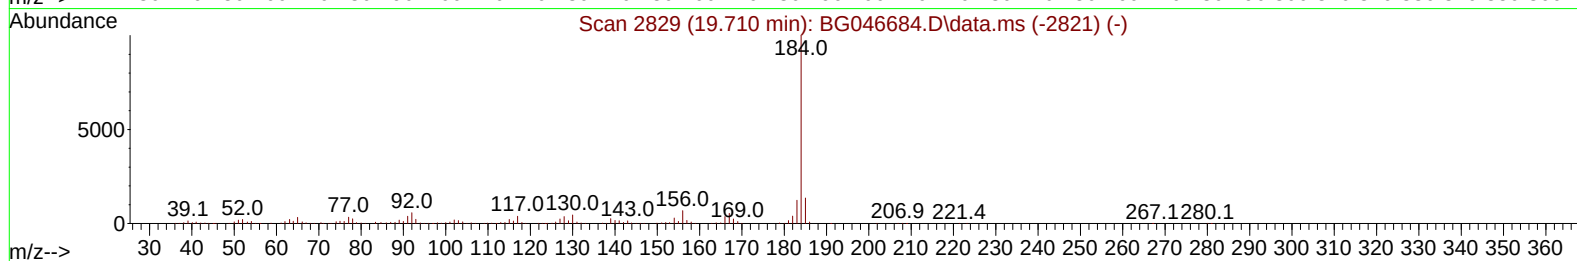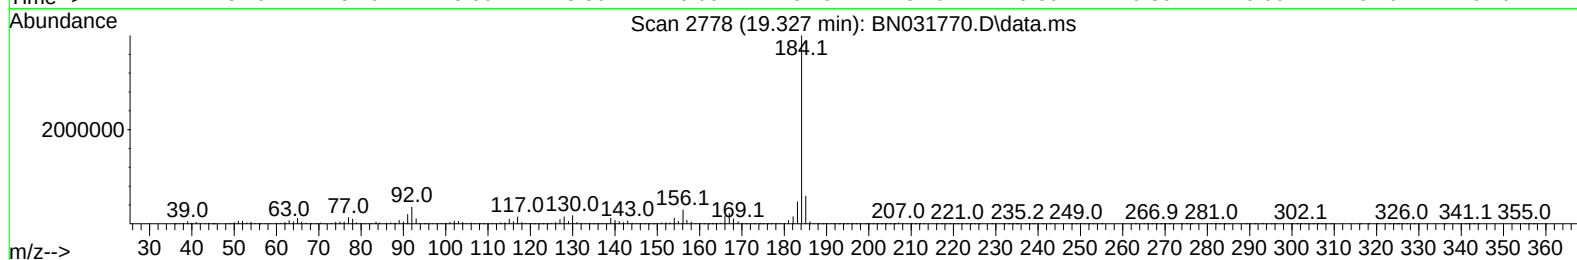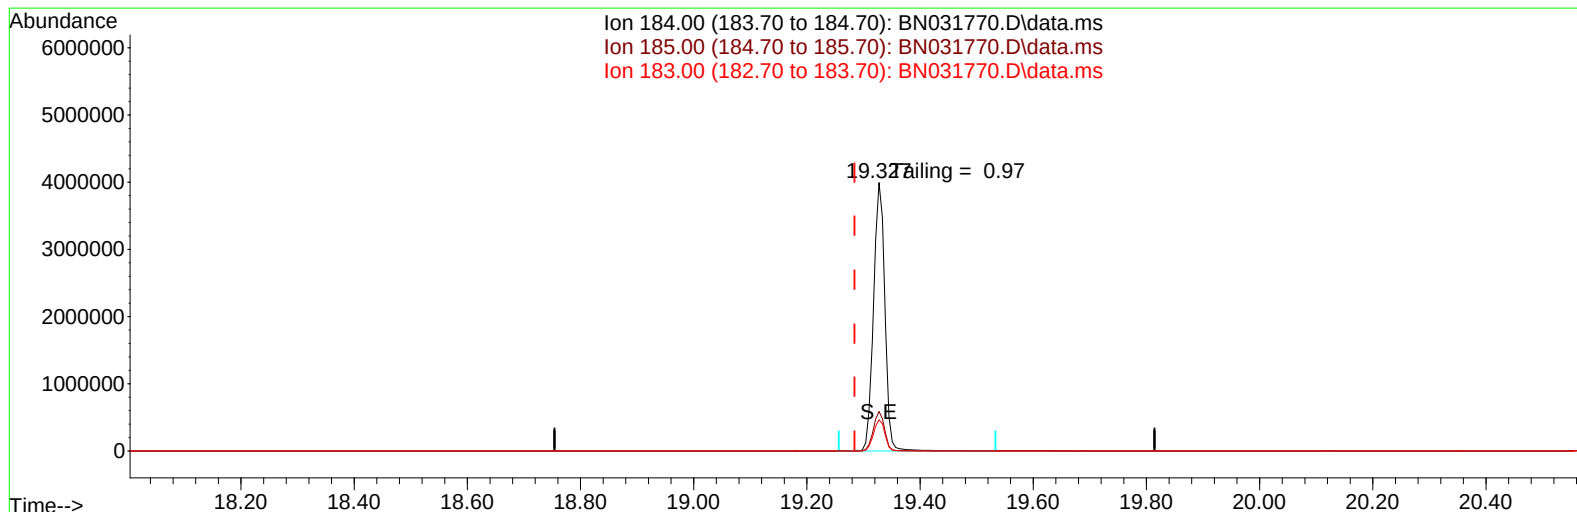

TIC: BN031770.D\data.ms

(77) Benzidine

19.327min (+ 0.043) 281727.19 ng

response 5557981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.75
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2024	BNA_N	<u>BN031770.D</u>
Compound Name	Response	Retention Time
DDT	1852420	20.563
DDD	677176	20.121
DDE	13116	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
690292	2542712	27.15

Instrument :
BNA_N
ClientSampleId :
DFTPP