
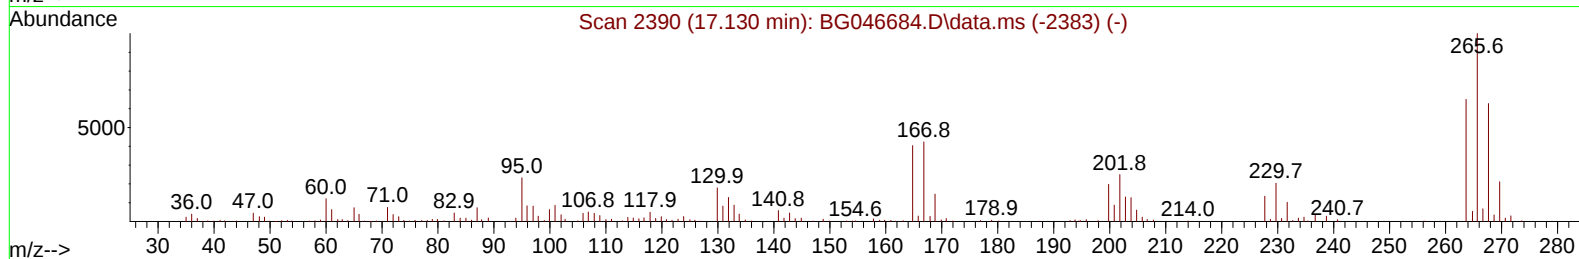
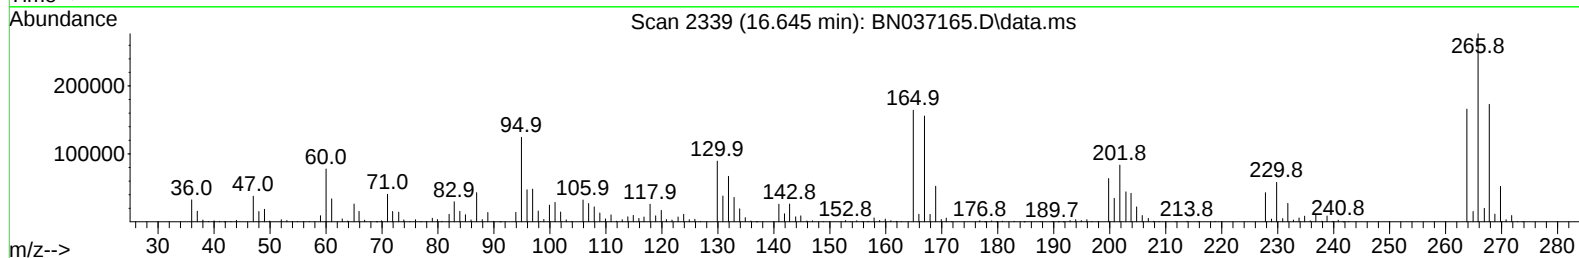


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060425\
Data File : BN037165.D
Acq On : 04 Jun 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 15:38:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

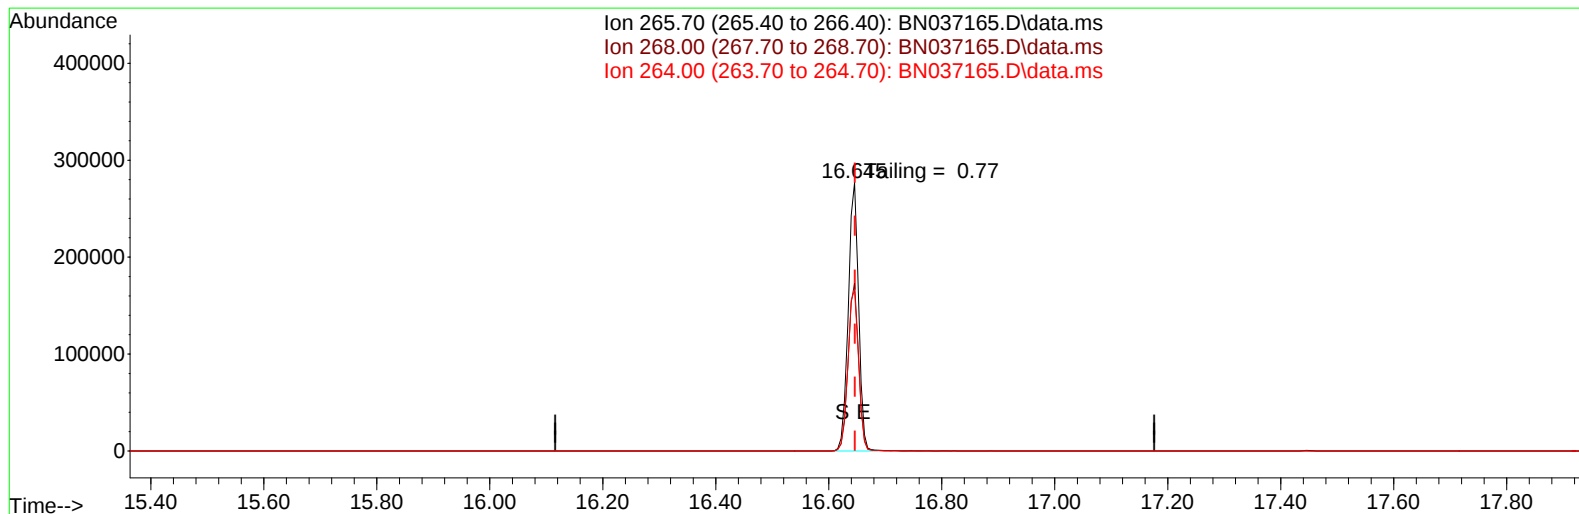

TIC: BN037165.D\data.ms

(70) Pentachlorophenol (C)




16.645min (-0.001) 30128.98 ng

response 352539

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.46
264.00	61.60	59.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060425\
Data File : BN037165.D
Acq On : 04 Jun 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 15:36:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

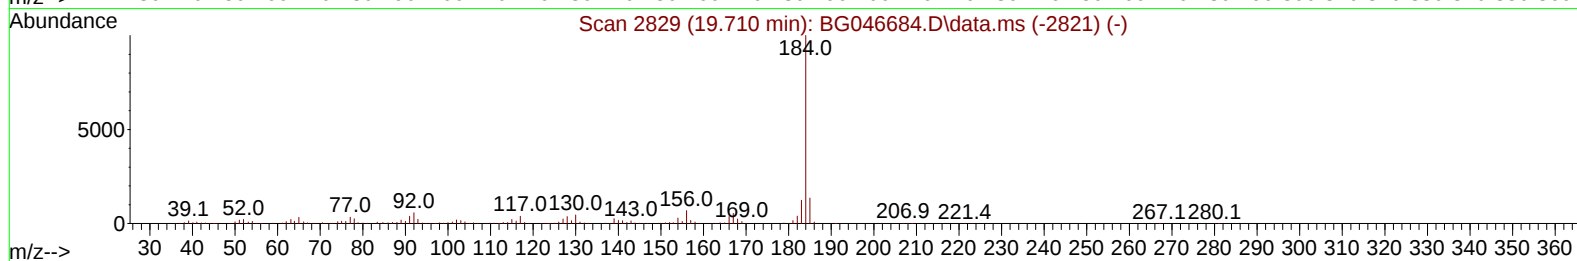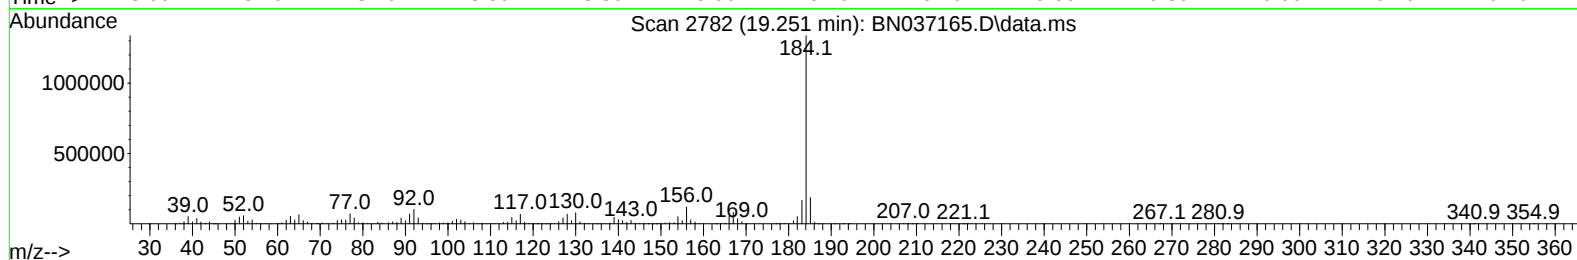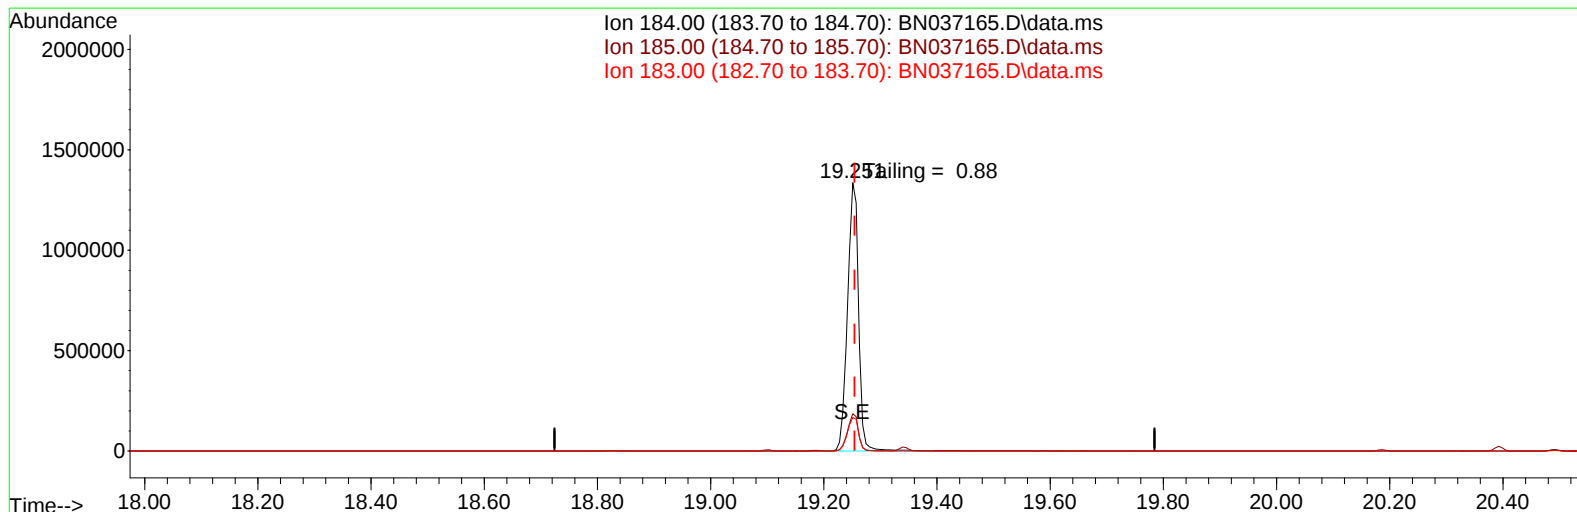

TIC: BN037165.D\data.ms

(77) Benzdine

19.251min (-0.003) 0.00 ng

response 1811758

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.53
0.00	0.00	0.00