




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060520\
 Data File : BN010776.D
 Acq On : 05 Jun 2020 11:43
 Operator : CG/JU
 Sample : PB129250BL
 Misc : PB-SOIL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK50

Manual Integrations
 APPROVED

mohammad
 6/8/2020 12:52:18 PM

Quant Time: Jun 05 12:14:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 10:29:34 2020
 Response via : Initial Calibration

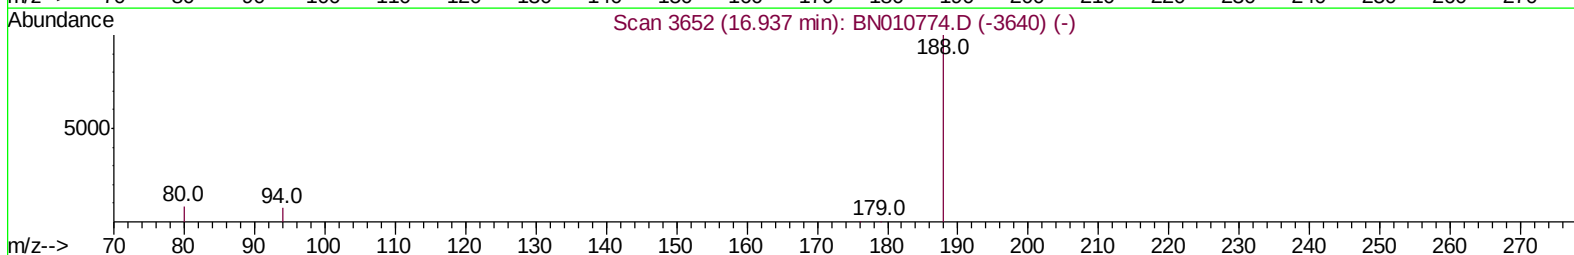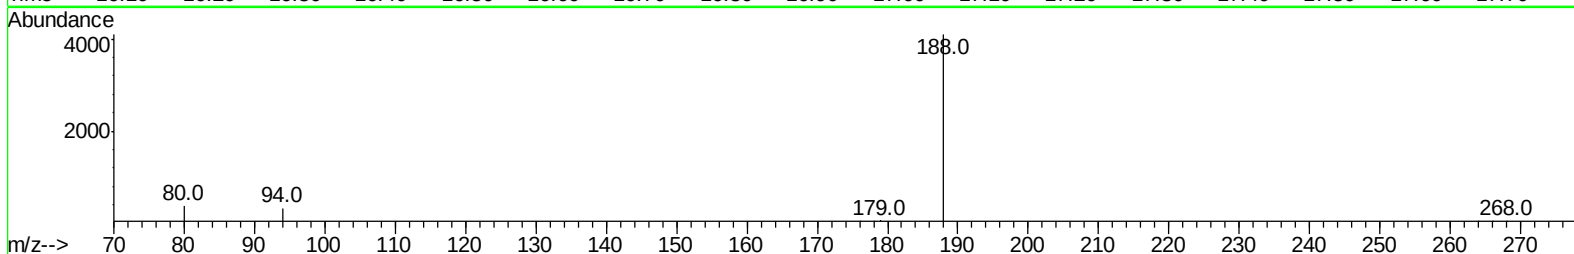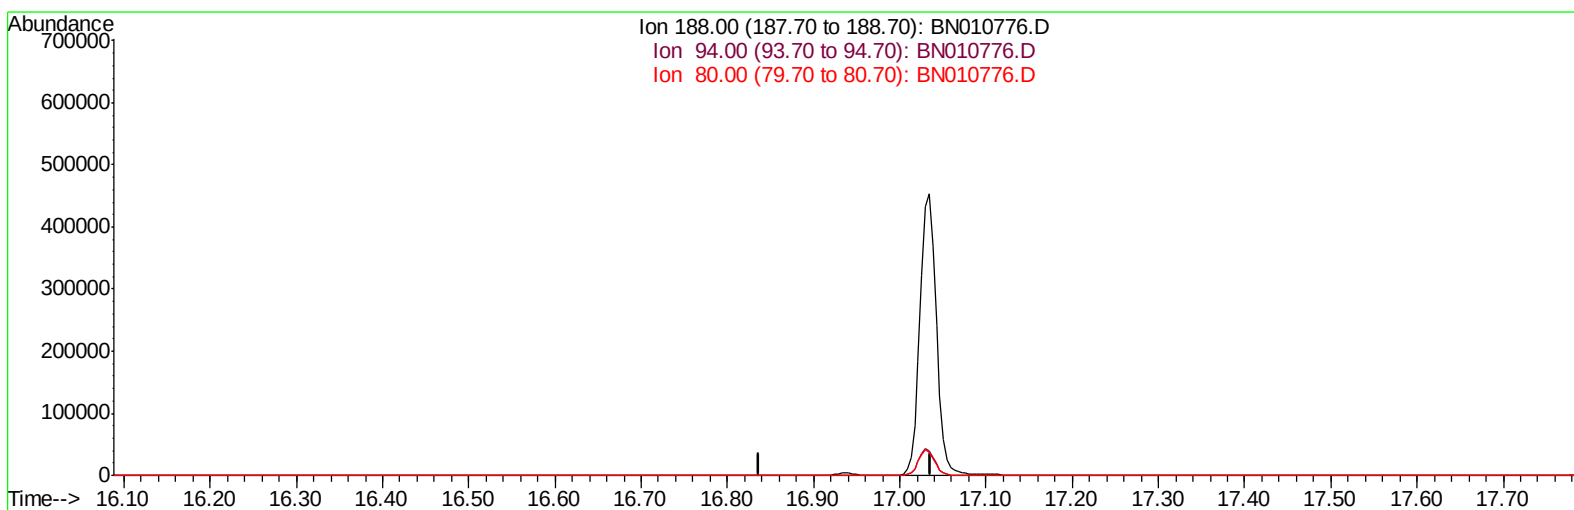

TIC: BN010776.D

(10) Phenanthrene-d10 (I)

16.937min (-16.937) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.70	0.00#
80.00	10.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060520\
 Data File : BN010776.D
 Acq On : 05 Jun 2020 11:43
 Operator : CG/JU
 Sample : PB129250BL
 Misc : PB-SOIL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK50

Manual Integrations
 APPROVED

mohammad
 6/8/2020 12:52:18 PM

Quant Time: Jun 05 12:14:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 10:29:34 2020
 Response via : Initial Calibration

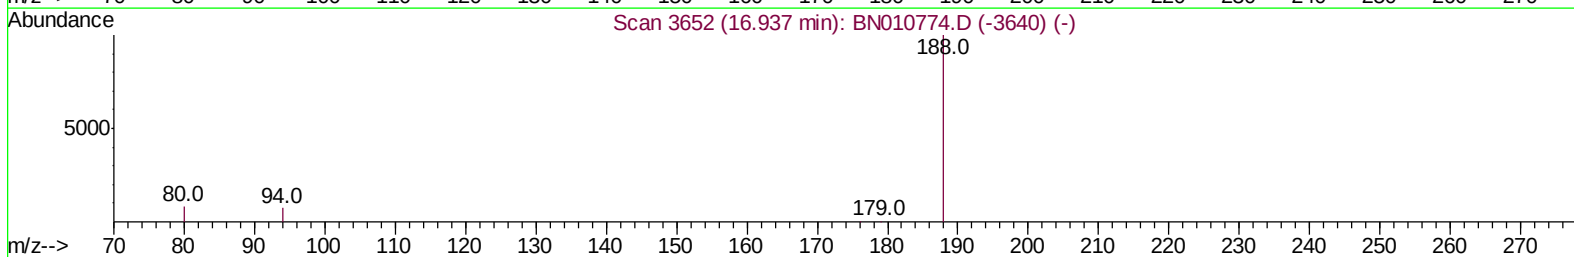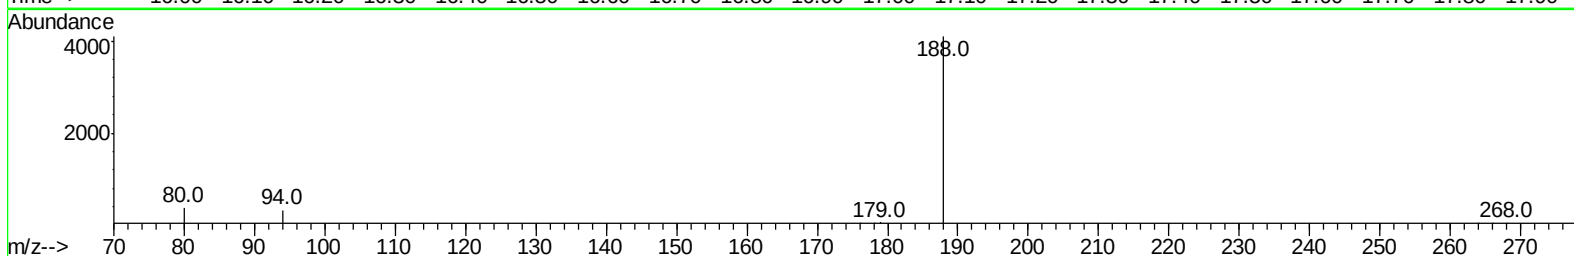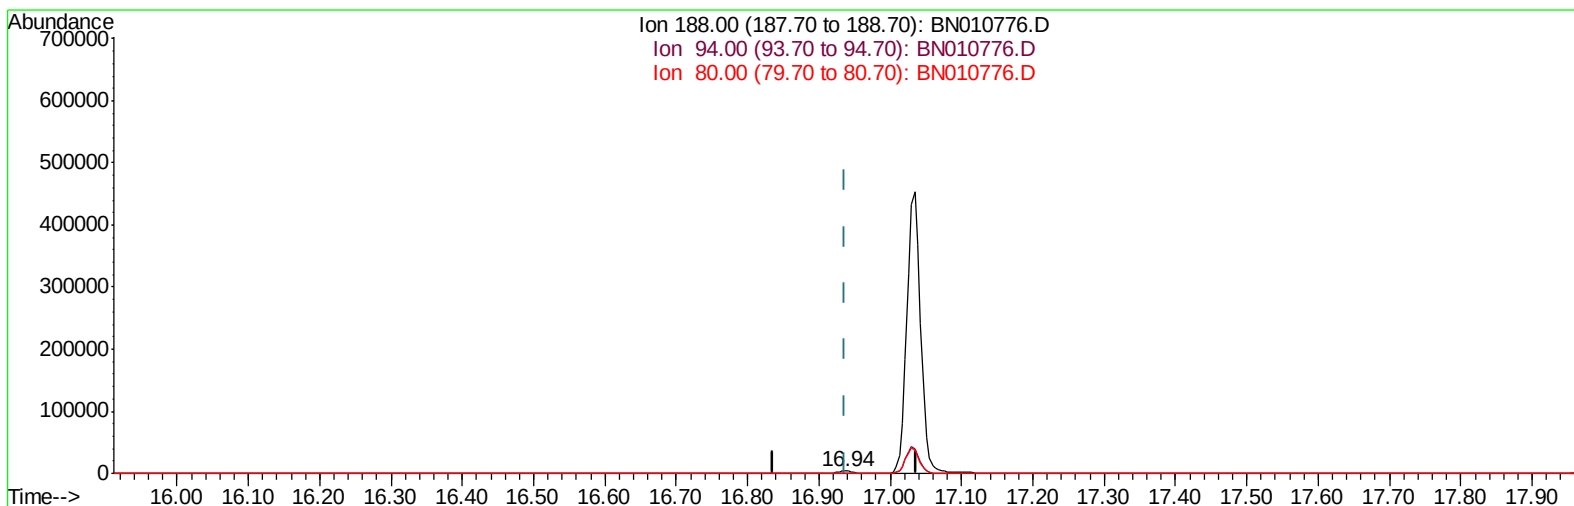

TIC: BN010776.D

(10) Phenanthrene-d10 (I)

16.937min (+0.000) 0.40ng/ul m

response 5696

Ion	Exp%	Act%
188.00	100	100
94.00	9.70	8.10
80.00	10.40	9.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060520\
 Data File : BN010776.D
 Acq On : 05 Jun 2020 11:43
 Operator : CG/JU
 Sample : PB129250BL
 Misc : PB-SOIL-04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK50

Manual Integrations
 APPROVED

mohammad
 6/8/2020 12:52:18 PM

Quant Time: Jun 05 12:16:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 10:29:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	1580	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	5130	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.19	164	2802	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.94	188	5696m	0.40	ng/ul	0.00
16) Chrysene-d12	21.15	240	4330	0.40	ng/ul	0.00
20) Perylene-d12	23.30	264	4803	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.92	152	3158	0.26	ng/ul	0.01
14) Fluoranthene-d10	18.97	212	6033	0.25	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN060520\
Data File : BN010776.D
Acq On : 05 Jun 2020 11:43
Operator : CG/JU
Sample : PB129250BL
Misc : PB-SOIL-04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK50

Manual Integrations
APPROVED

mohammad
6/8/2020 12:52:18 PM

Quant Time: Jun 05 12:16:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN060320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 10:29:34 2020
Response via : Initial Calibration

