


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060620\
 Data File : BN010784.D
 Acq On : 05 Jun 2020 16:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 22:48:49 2020

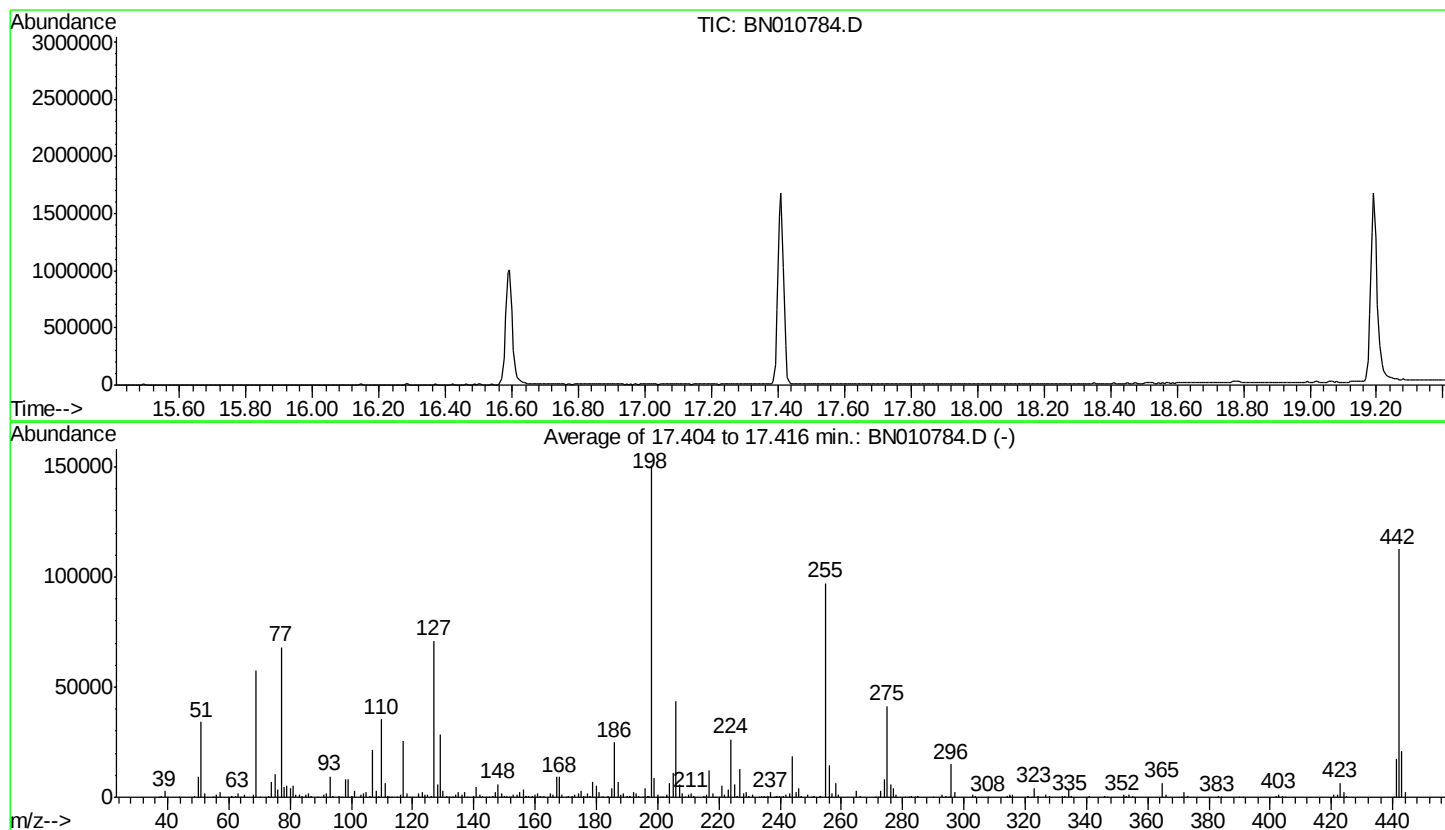

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	34160	PASS
68	69	0.00	2	1.8	1018	PASS
69	198	0.00	100	38.4	57786	PASS
70	69	0.00	2	0.4	231	PASS
127	198	10	80	47.2	71072	PASS
197	198	0.00	2	0.3	453	PASS
198	198	100	100	100.0	150656	PASS
199	198	5	9	5.7	8538	PASS
275	198	10	60	27.5	41496	PASS
365	198	1	100	4.3	6464	PASS
441	198	0.01	100	11.6	17513	PASS
442	198	50	100	74.8	112656	PASS
443	442	15	24	18.8	21224	PASS