

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060622\
 Data File : BN020019.D
 Acq On : 06 Jun 2022 12:45
 Operator : CG/JU
 Sample : SSTD02019
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020219

Quant Time: Jun 06 14:38:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 14:35:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	143889	20.000	ng/u1	0.00
20) Naphthalene-d8	10.616	136	660595	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	428543	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.192	188	913925	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	848425	20.000	ng/u1	0.00
88) Perylene-d12	23.709	264	878257	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	25310	6.638	ng/uL	0.00
4) Pyridine-d5	3.687	84	176480	18.278	ng/u1	0.00
7) Phenol-d5	6.987	99	228674	18.339	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	147904	20.449	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	192383	19.451	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	200647	21.005	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	99476	20.653	ng/u1	0.00
24) 2-Nitrophenol-d4	9.698	143	106530	22.443	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	186718	19.651	ng/u1	0.00
31) 4-Chloroaniline-d4	10.745	131	300445	20.830	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	620424	21.078	ng/u1	0.00
49) Acenaphthylene-d8	14.145	160	734671	18.460	ng/u1	0.00
54) 4-Nitrophenol-d4	14.645	143	123730	21.614	ng/u1	0.00
60) Fluorene-d10	15.439	176	518104	19.940	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	102148	21.893	ng/u1	0.00
73) Anthracene-d10	17.292	188	801275	18.617	ng/u1	0.00
81) Pyrene-d10	19.586	212	915139	18.761	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.562	264	863536	19.234	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.316	88	26227	6.745	ng/uL#	88
5) Pyridine	3.711	79	183067	17.993	ng/u1	93
6) Benzaldehyde	6.963	77	138783	21.716	ng/u1	91
8) Phenol	7.016	94	248557	19.809	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.246	93	196959	20.230	ng/u1	99
12) 2-Chlorophenol	7.387	128	199783	19.890	ng/u1	98
13) 2-Methylphenol	8.263	108	189532	20.401	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.357	45	310020	22.157	ng/u1	97
16) Acetophenone	8.640	105	321742	22.445	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.628	70	165137	24.753	ng/u1	94
18) 4-Methylphenol	8.593	108	214144	21.528	ng/u1	96
19) Hexachloroethane	8.904	117	80097	19.671	ng/u1	91
22) Nitrobenzene	9.016	77	233863	20.594	ng/u1	96
23) Isophorone	9.540	82	464561	22.938	ng/u1	99
25) 2-Nitrophenol	9.728	139	118721	22.149	ng/u1	98
26) 2,4-Dimethylphenol	9.793	107	246775	20.668	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.028	93	279351	20.975	ng/u1	97
29) 2,4-Dichlorophenol	10.263	162	193180	20.279	ng/u1	99
30) Naphthalene	10.663	128	686257	19.397	ng/u1	99
32) 4-Chloroaniline	10.769	127	303041	20.903	ng/u1	97
33) Hexachlorobutadiene	10.957	225	109541	19.167	ng/u1	100
34) Caprolactam	11.516	113	47403	17.595	ng/u1	94
35) 4-Chloro-3-methylphenol	11.898	107	232597	23.068	ng/u1	100
36) 2-Methylnaphthalene	12.275	142	465388	20.439	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060622\
 Data File : BN020019.D
 Acq On : 06 Jun 2022 12:45
 Operator : CG/JU
 Sample : SST02019
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SST020219

Quant Time: Jun 06 14:38:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 14:35:54 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.492	142	469193	20.583	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.651	216	214162	18.011	ng/ul	97
40) Hexachlorocyclopentadiene	12.634	237	127448	17.419	ng/ul	95
41) 2,4,6-Trichlorophenol	12.887	196	152695	20.585	ng/ul	92
42) 2,4,5-Trichlorophenol	12.957	196	168053	20.866	ng/ul	97
43) 1,1'-Biphenyl	13.287	154	632626	18.671	ng/ul	99
44) 2-Chloronaphthalene	13.328	162	484366	18.711	ng/ul	97
45) 2-Nitroaniline	13.528	65	152560	24.559	ng/ul	92
47) Dimethylphthalate	13.910	163	627840	21.479	ng/ul	99
48) 2,6-Dinitrotoluene	14.028	165	124657	24.721	ng/ul	93
50) Acenaphthylene	14.169	152	811044	19.836	ng/ul	100
51) 3-Nitroaniline	14.351	138	136179	26.348	ng/ul	100
52) Acenaphthene	14.516	153	520891	19.466	ng/ul	97
53) 2,4-Dinitrophenol	14.557	184	69783	24.948	ng/ul	91
55) 4-Nitrophenol	14.657	109	104620	22.999	ng/ul	97
56) Dibenzofuran	14.851	168	737558	19.731	ng/ul	99
57) 2,4-Dinitrotoluene	14.810	165	187609	25.586	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.075	232	133379	22.704	ng/ul	90
59) Diethylphthalate	15.275	149	652661	22.701	ng/ul	97
61) Fluorene	15.498	166	580041	19.989	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.492	204	265219	20.214	ng/ul	94
63) 4-Nitroaniline	15.510	138	136926	30.911	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.575	198	107303	22.612	ng/ul	97
67) N-Nitrosodiphenylamine	15.704	169	522661	18.638	ng/ul	99
68) 4-Bromophenyl-phenylether	16.386	248	161045	18.757	ng/ul	92
69) Hexachlorobenzene	16.504	284	174768	18.097	ng/ul#	84
70) Atrazine	16.657	200	183749	20.541	ng/ul	98
71) Pentachlorophenol	16.845	266	111017	18.943	ng/ul	93
72) Phenanthrene	17.233	178	948279	18.567	ng/ul	99
74) Anthracene	17.327	178	960382	18.824	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.251	216	229559	16.294	ng/ul	99
76) Pentachlorobenzene	14.775	250	214244	17.456	ng/ul	96
77) Carbazole	17.592	167	913638	19.698	ng/ul	98
78) Di-n-butylphthalate	18.163	149	1101905	22.209	ng/ul	99
80) Fluoranthene	19.251	202	1089723	18.952	ng/ul	98
82) Pyrene	19.616	202	1120269	18.705	ng/ul	95
83) Butylbenzylphthalate	20.521	149	509501	22.998	ng/ul	94
84) 3,3'-Dichlorobenzidine	21.298	252	358678	21.050	ng/ul#	96
85) Benzo(a)anthracene	21.363	228	1087666	20.016	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.304	149	740212	21.775	ng/ul#	99
87) Chrysene	21.421	228	1027188	19.244	ng/ul	99
89) Di-n-octyl phthalate	22.210	149	1310851	21.802	ng/ul	100
90) Benzo(b)fluoranthene	23.004	252	1081777	19.040	ng/ul#	97
91) Benzo(k)fluoranthene	23.004	252	1081777	20.991	ng/ul	94
93) Benzo(a)pyrene	23.609	252	1059108	19.630	ng/ul	94
94) Indeno(1,2,3-cd)pyrene	26.098	276	1097564	17.751	ng/ul	93
95) Dibenzo(a,h)anthracene	26.121	278	945757	17.889	ng/ul	95
96) Benzo(g,h,i)perylene	26.845	276	932260	17.142	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060622\  
Data File : BN020019.D  
Acq On    : 06 Jun 2022  12:45  
Operator  : CG/JU  
Sample    : SSTD02019  
Misc      :  
ALS Vial  : 4    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
SSTD020219

Quant Time: Jun 06 14:38:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 14:35:54 2022
Response via : Initial Calibration




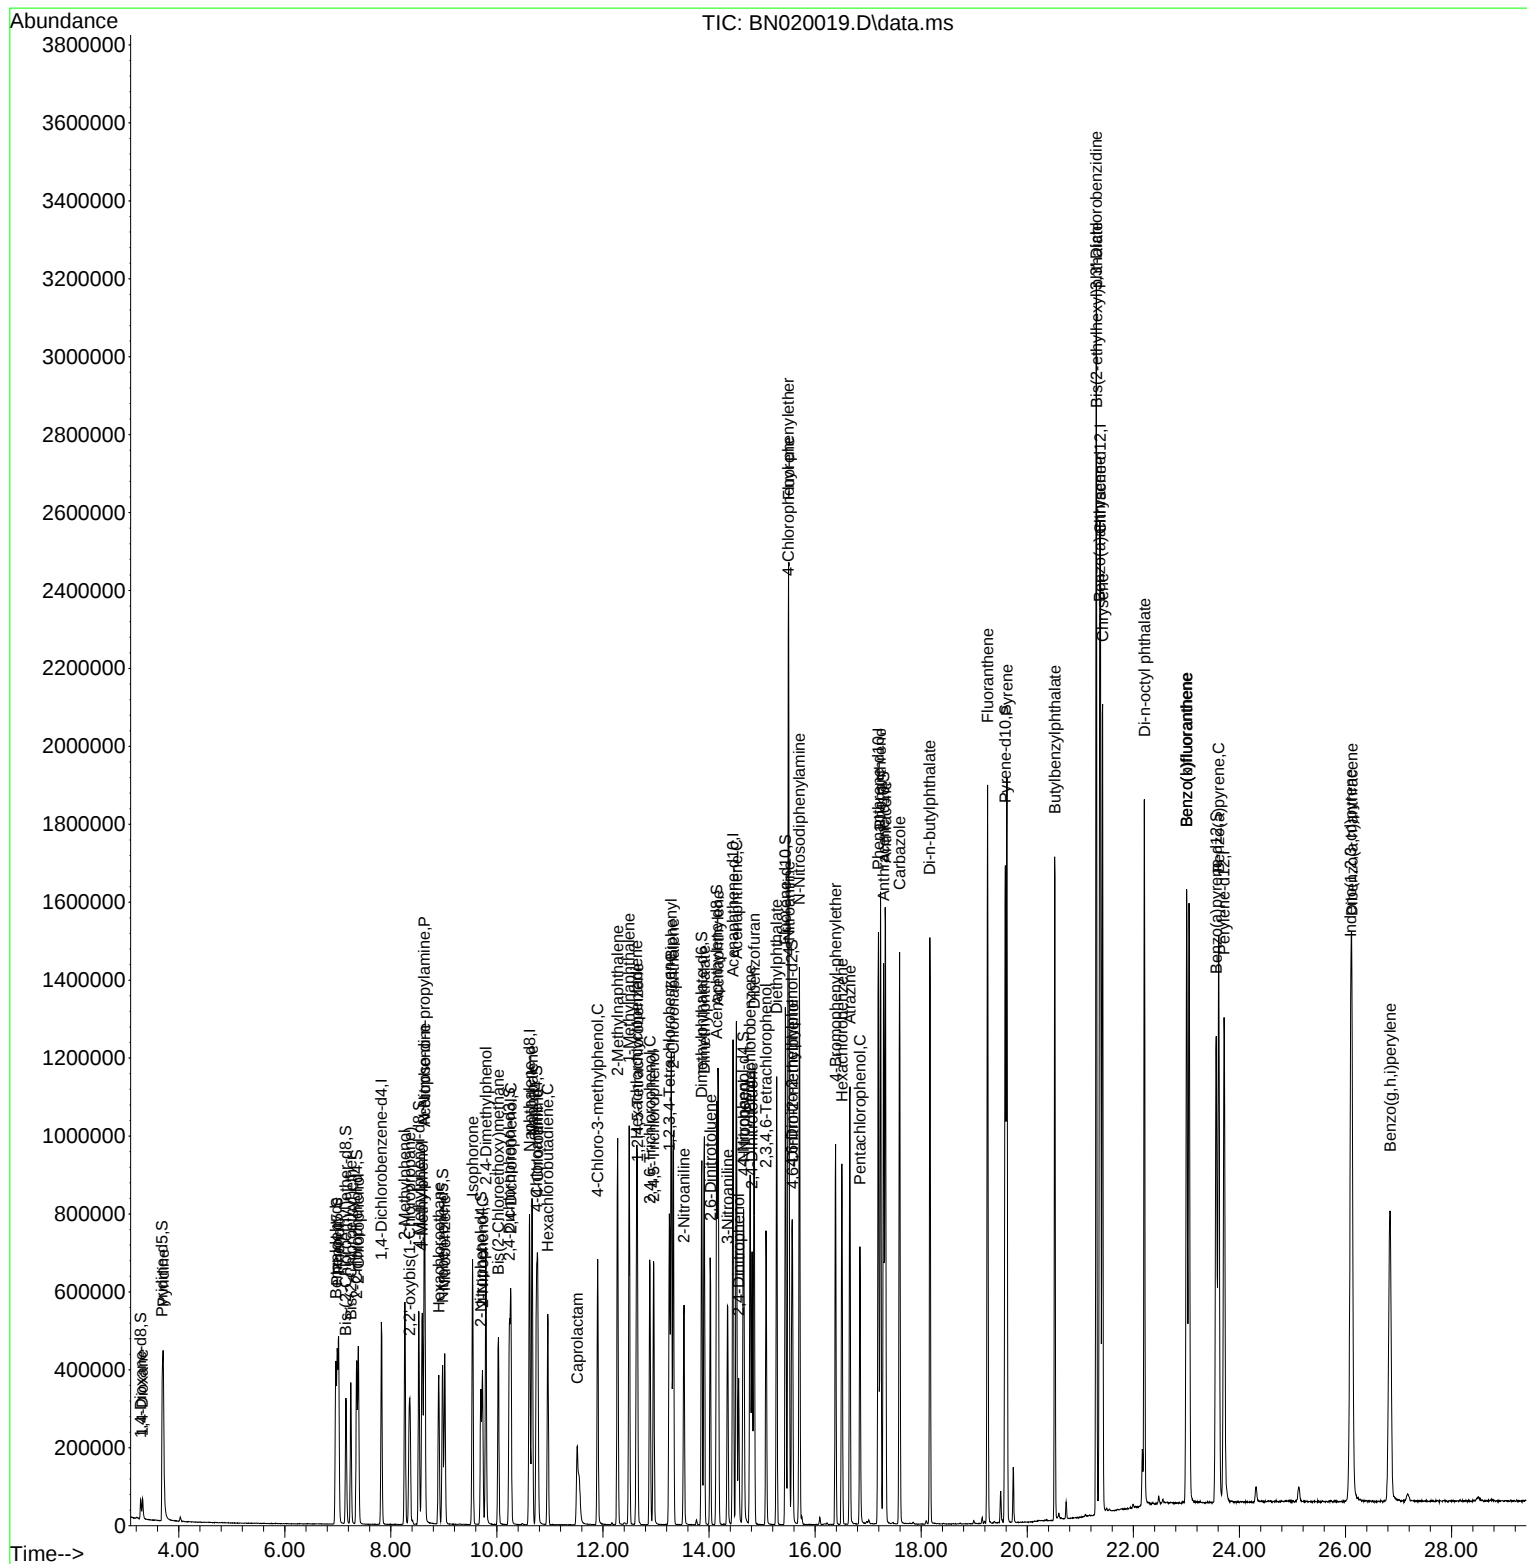




#2
1,4-Dioxane
Concen: 6.745 ng/uL
RT: 3.316 min Scan# 39
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion: 88 Resp: 26227
Ion Ratio Lower Upper
88 100
43 33.9 22.4 33.6#
58 86.4 61.0 91.4

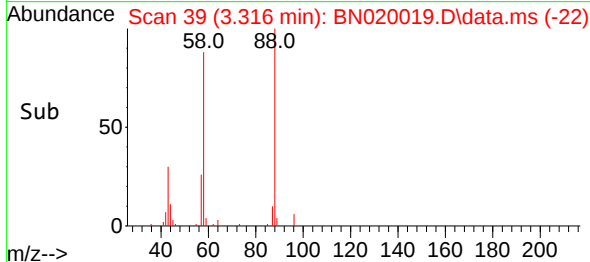

#5
Pyridine
Concen: 17.993 ng/uL
RT: 3.711 min Scan# 106
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 79 Resp: 183067
Ion Ratio Lower Upper
79 100
52 88.5 65.0 97.4
51 42.5 31.6 47.4


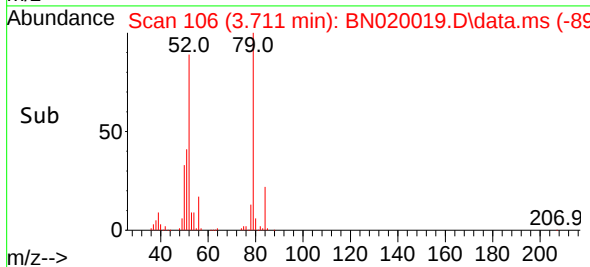

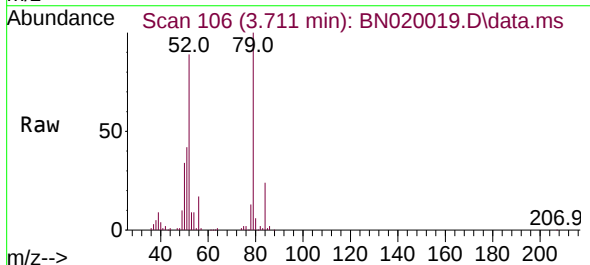




#6
Benzaldehyde
Concen: 21.716 ng/ul
RT: 6.963 min Scan# 659
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion: 77 Resp: 138783
Ion Ratio Lower Upper
77 100
105 103.1 74.7 112.1
106 95.9 70.2 105.4



#8
Phenol
Concen: 19.809 ng/ul
RT: 7.016 min Scan# 668
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 94 Resp: 248557
Ion Ratio Lower Upper
94 100
65 30.1 23.6 35.4
66 38.7 31.2 46.8









#10
 Bis(2-Chloroethyl)ether
 Concen: 20.230 ng/ul
 RT: 7.246 min Scan# 707
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020219

Tgt Ion: 93 Resp: 196959




Ion	Ratio	Lower	Upper
93	100		
63	80.1	63.4	95.0
95	33.3	26.2	39.2

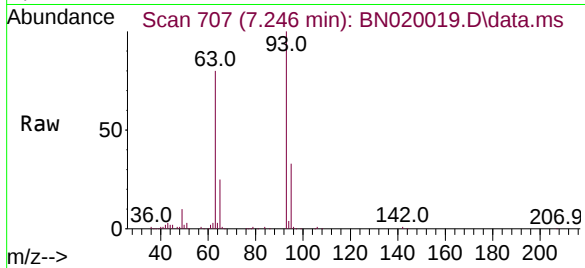


#12
 2-Chlorophenol
 Concen: 19.890 ng/ul
 RT: 7.387 min Scan# 731
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Tgt Ion: 128 Resp: 199783

Ion	Ratio	Lower	Upper
128	100		
64	47.5	38.6	57.8
130	32.8	25.0	37.4




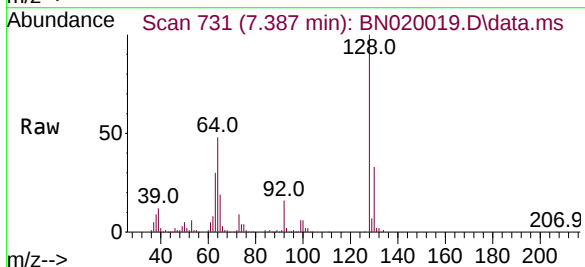




#13
2-Methylphenol
Concen: 20.401 ng/ul
RT: 8.263 min Scan# 880
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:108 Resp: 189532
Ion Ratio Lower Upper
108 100
107 87.3 71.5 107.3

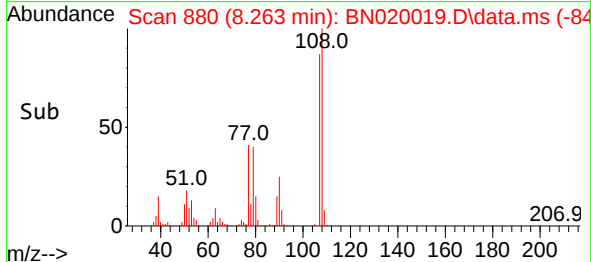

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.157 ng/ul
RT: 8.357 min Scan# 896
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 45 Resp: 310020
Ion Ratio Lower Upper
45 100
77 12.4 10.9 16.3
79 9.8 8.6 13.0




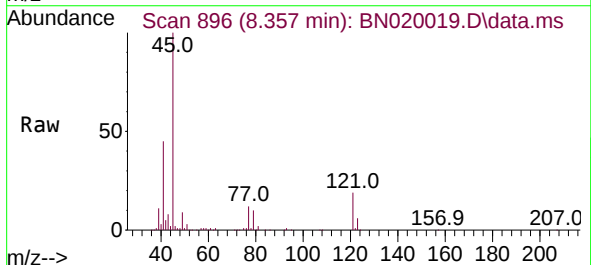




#16
Acetophenone
Concen: 22.445 ng/ul
RT: 8.640 min Scan# 944
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:105 Resp: 321742
Ion Ratio Lower Upper
105 100
77 77.4 63.5 95.3
51 30.6 23.5 35.3

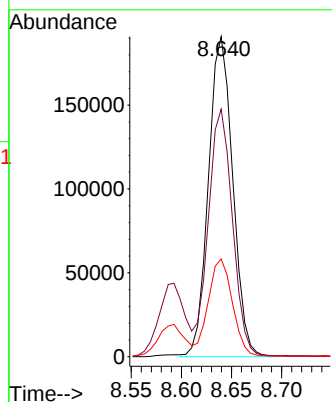

#17
N-Nitroso-di-n-propylamine
Concen: 24.753 ng/ul
RT: 8.628 min Scan# 942
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 70 Resp: 165137
Ion Ratio Lower Upper
70 100
42 65.1 47.8 71.6
101 9.7 7.8 11.6
130 22.2 15.8 23.8









#18
4-Methylphenol
Concen: 21.528 ng/ul
RT: 8.593 min Scan# 911
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:108 Resp: 214144
Ion Ratio Lower Upper
108 100
107 113.9 88.0 132.0

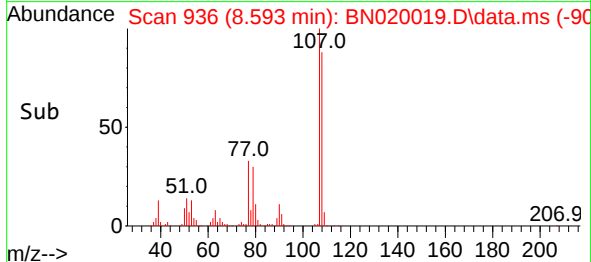

#19
Hexachloroethane
Concen: 19.671 ng/ul
RT: 8.904 min Scan# 989
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:117 Resp: 80097
Ion Ratio Lower Upper
117 100
201 93.0 83.2 124.8
199 57.4 50.2 75.4




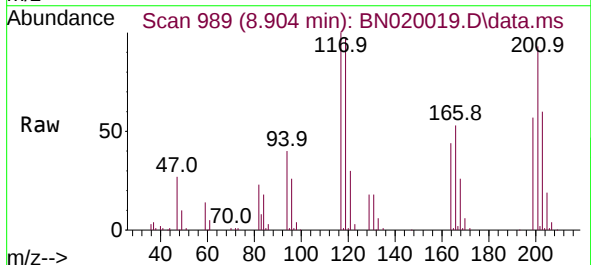


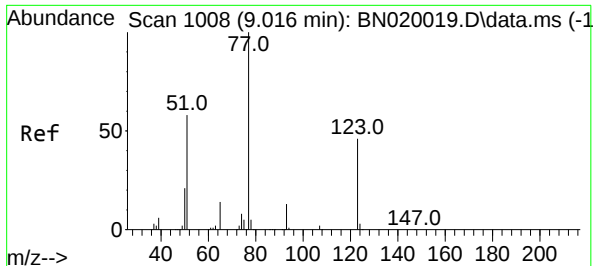

#22
Nitrobenzene
Concen: 20.594 ng/ul
RT: 9.016 min Scan# 1008
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion: 77 Resp: 233863
Ion Ratio Lower Upper
77 100
123 46.1 34.5 51.7
65 14.4 11.1 16.7

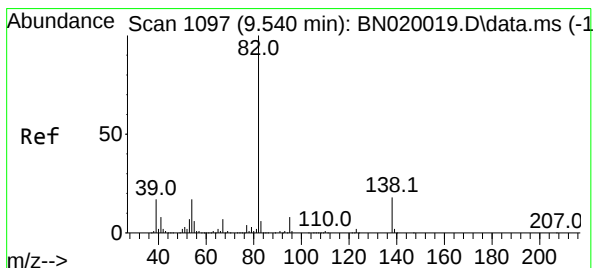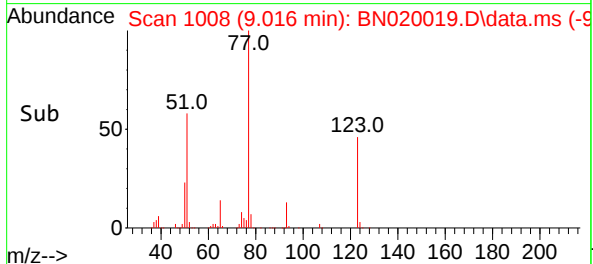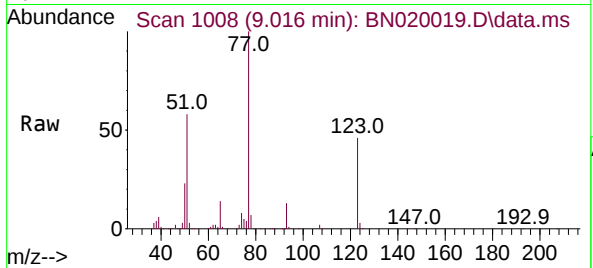

#23
Isophorone
Concen: 22.938 ng/ul
RT: 9.540 min Scan# 1097
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 82 Resp: 464561
Ion Ratio Lower Upper
82 100
95 7.5 5.8 8.8
138 17.9 13.8 20.8

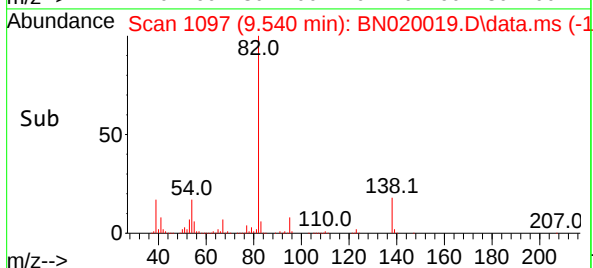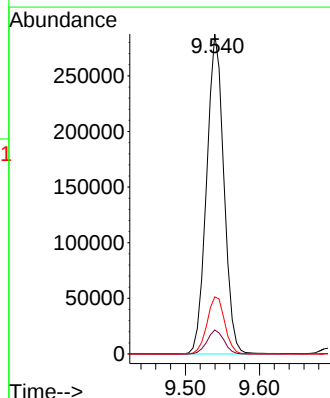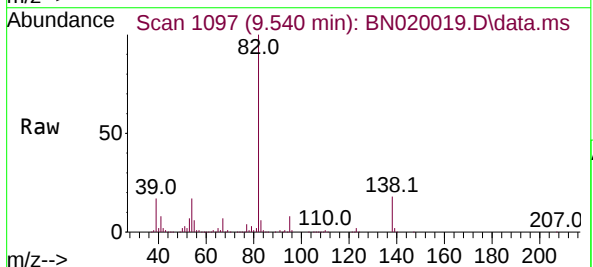



#25

2-Nitrophenol

Concen: 22.149 ng/ul

RT: 9.728 min Scan# 1129

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:139 Resp: 118721

Ion Ratio Lower Upper

139 100

65 52.0 43.7 65.5

109 32.1 25.8 38.6

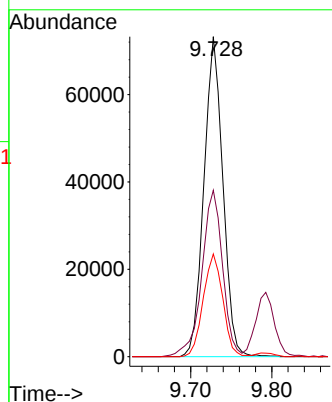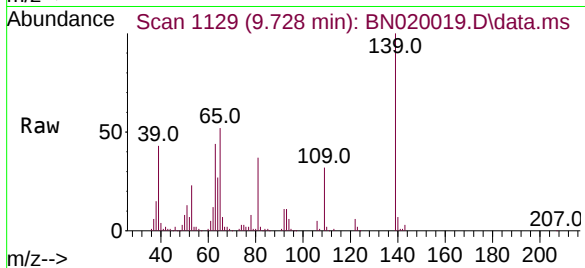

#26

2,4-Dimethylphenol

Concen: 20.668 ng/ul

RT: 9.793 min Scan# 1140

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion:107 Resp: 246775


Ion Ratio Lower Upper

107 100

121 49.5 38.3 57.5

122 82.5 66.3 99.5



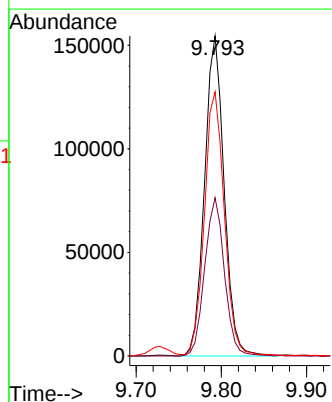
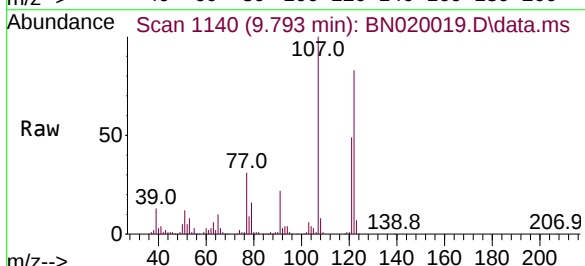




#27
Bis(2-Chloroethoxy)methane
Concen: 20.975 ng/ul
RT: 10.028 min Scan# 1180
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion: 93 Resp: 279351
Ion Ratio Lower Upper
93 100
95 33.4 25.4 38.0
123 12.2 8.3 12.5



#29
2,4-Dichlorophenol
Concen: 20.279 ng/ul
RT: 10.263 min Scan# 1220
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion: 162 Resp: 193180
Ion Ratio Lower Upper
162 100
164 66.9 52.9 79.3
98 37.6 29.8 44.8









#30
Naphthalene
Concen: 19.397 ng/ul
RT: 10.663 min Scan# 1288
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:128 Resp: 686257
Ion Ratio Lower Upper
128 100
129 10.3 8.7 13.1
127 13.0 10.6 16.0

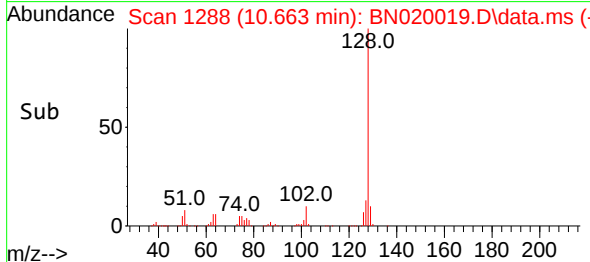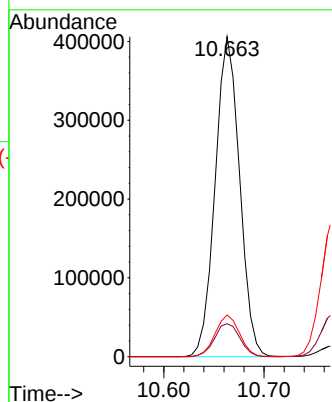

#32
4-Chloroaniline
Concen: 20.903 ng/ul
RT: 10.769 min Scan# 1306
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:127 Resp: 303041
Ion Ratio Lower Upper
127 100
129 30.8 26.1 39.1


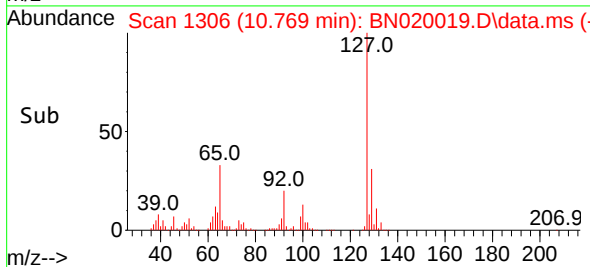

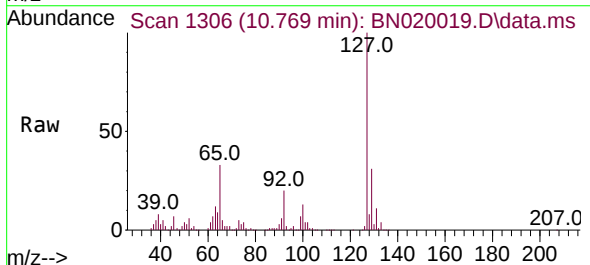




#33
Hexachlorobutadiene
Concen: 19.167 ng/ul
RT: 10.957 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:225 Resp: 109541
Ion Ratio Lower Upper
225 100
223 64.2 51.8 77.6
227 63.1 50.6 76.0

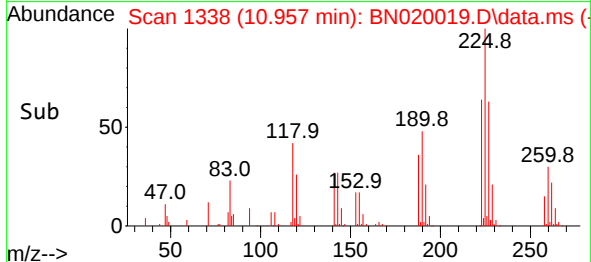

#34
Caprolactam
Concen: 17.595 ng/ul
RT: 11.516 min Scan# 1433
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:113 Resp: 47403
Ion Ratio Lower Upper
113 100
55 176.0 145.5 218.3
56 124.3 106.5 159.7




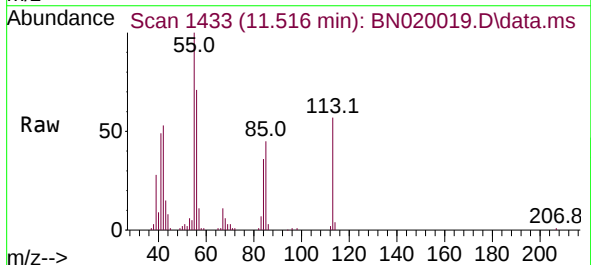




#35
4-Chloro-3-methylphenol
Concen: 23.068 ng/ul
RT: 11.898 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:107 Resp: 232597
Ion Ratio Lower Upper
107 100
144 25.9 20.6 31.0
142 77.9 62.2 93.4

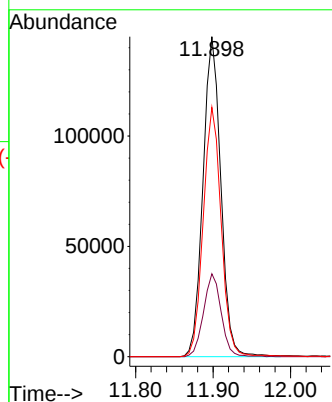

#36
2-Methylnaphthalene
Concen: 20.439 ng/ul
RT: 12.275 min Scan# 1562
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:142 Resp: 465388
Ion Ratio Lower Upper
142 100
141 92.3 70.6 105.8



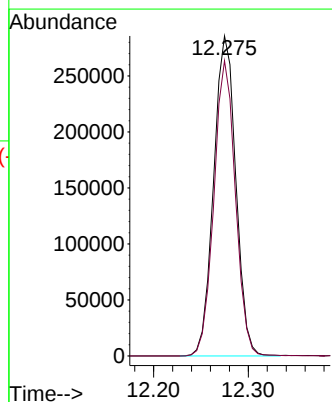





#37
1-Methylnaphthalene
Concen: 20.583 ng/ul
RT: 12.492 min Scan# 1599
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:142 Resp: 469193
Ion Ratio Lower Upper
142 100
141 90.9 70.9 106.3
116 4.1 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 18.011 ng/ul
RT: 12.651 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:216 Resp: 214162
Ion Ratio Lower Upper
216 100
214 75.4 63.4 95.0
179 23.0 17.8 26.8
108 19.2 15.1 22.7




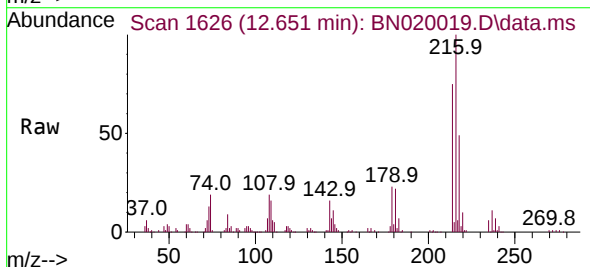




#40
Hexachlorocyclopentadiene
Concen: 17.419 ng/ul
RT: 12.634 min Scan# 1623
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:237 Resp: 127448
Ion Ratio Lower Upper
237 100
235 64.9 48.8 73.2
272 12.0 9.3 13.9

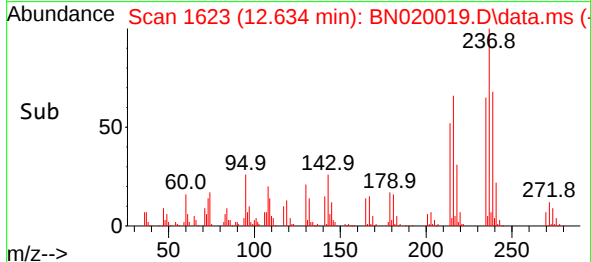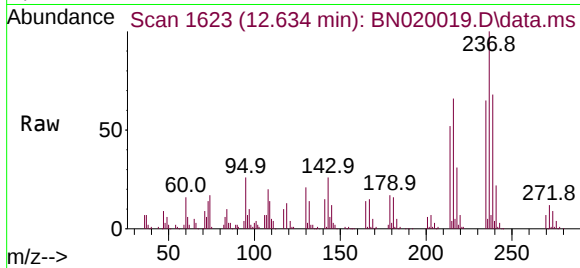

#41
2,4,6-Trichlorophenol
Concen: 20.585 ng/ul
RT: 12.887 min Scan# 1666
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:196 Resp: 152695
Ion Ratio Lower Upper
196 100
198 90.2 79.8 119.8
200 30.5 25.0 37.6




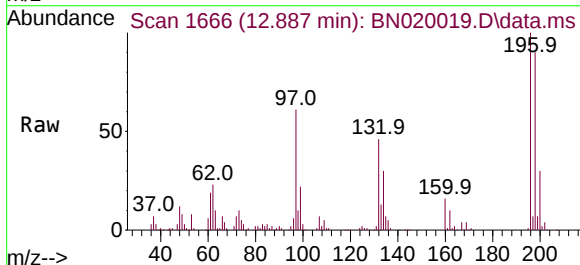




#42
2,4,5-Trichlorophenol
Concen: 20.866 ng/ul
RT: 12.957 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:196 Resp: 168053
Ion Ratio Lower Upper
196 100
198 94.2 77.6 116.4
200 28.7 24.4 36.6



#43
1,1'-Biphenyl
Concen: 18.671 ng/ul
RT: 13.287 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:154 Resp: 632626
Ion Ratio Lower Upper
154 100
153 39.2 31.5 47.3
76 12.3 10.5 15.7

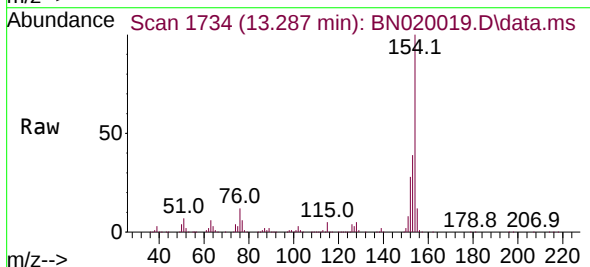

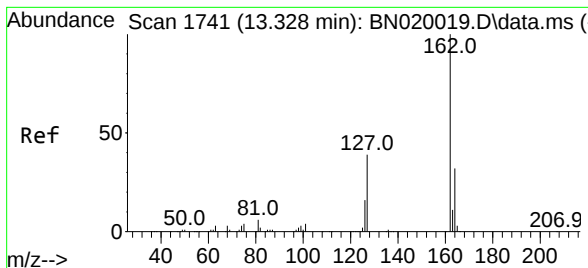

#44

2-Chloronaphthalene

Concen: 18.711 ng/ul

RT: 13.328 min Scan# 1741

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:162 Resp: 484366

Ion Ratio Lower Upper

162 100

164 32.5 25.8 38.6

127 42.8 31.4 47.2

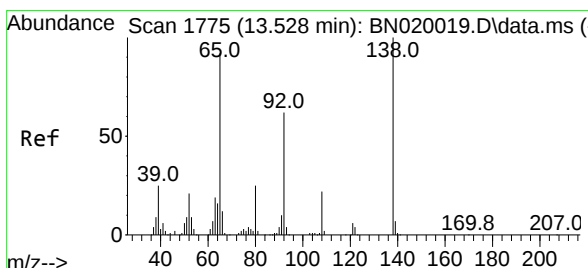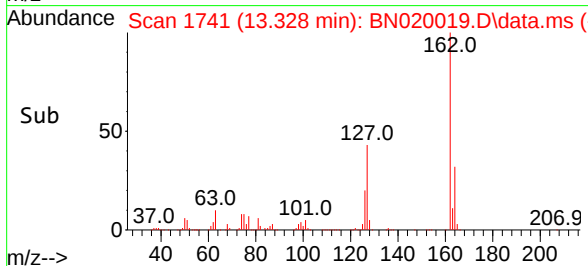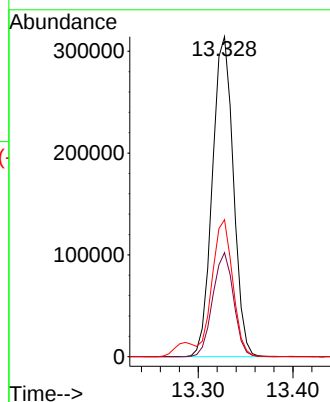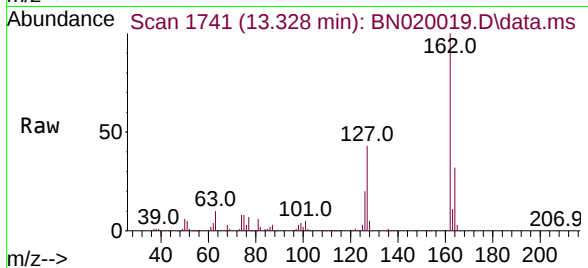

#45

2-Nitroaniline

Concen: 24.559 ng/ul

RT: 13.528 min Scan# 1775

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion: 65 Resp: 152560


Ion Ratio Lower Upper

65 100

92 68.0 54.1 81.1

138 109.2 77.0 115.4


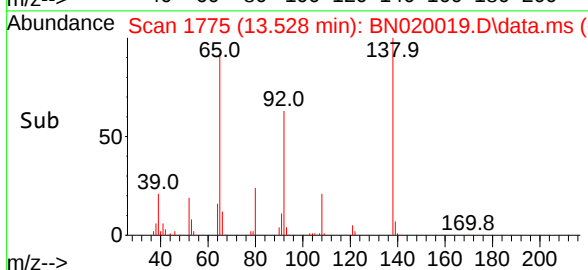

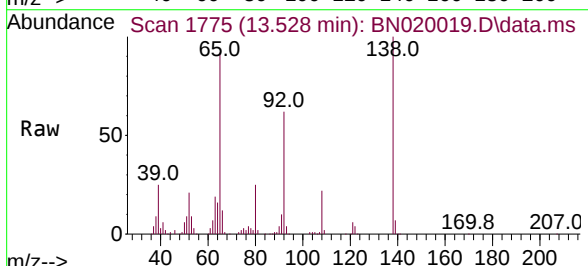




#47
Dimethylphthalate
Concen: 21.479 ng/ul
RT: 13.910 min Scan# 1840
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:163 Resp: 627840
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 10.2 7.7 11.5

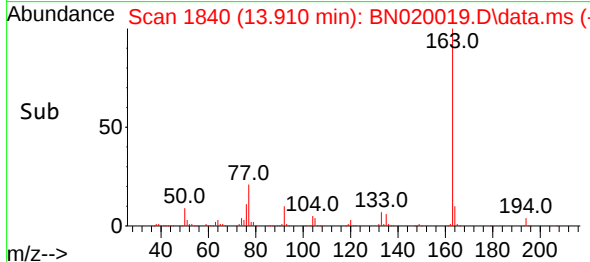

#48
2,6-Dinitrotoluene
Concen: 24.721 ng/ul
RT: 14.028 min Scan# 1860
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:165 Resp: 124657
Ion Ratio Lower Upper
165 100
89 57.3 50.6 75.8
121 20.8 17.9 26.9

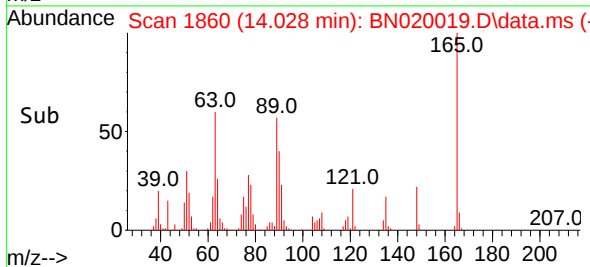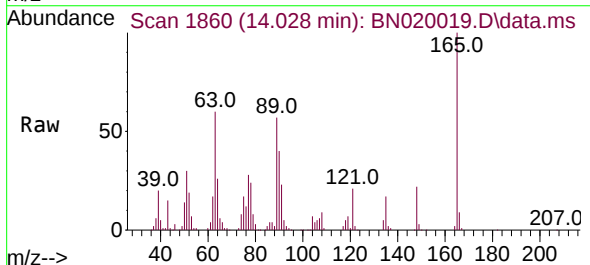



#50

Acenaphthylene

Concen: 19.836 ng/ul

RT: 14.169 min Scan# 1884

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:152 Resp: 811044

Ion Ratio Lower Upper

152 100

151 19.7 16.0 24.0

153 13.4 10.7 16.1



#51

3-Nitroaniline

Concen: 26.348 ng/ul

RT: 14.351 min Scan# 1915

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion:138 Resp: 136179


Ion Ratio Lower Upper

138 100

108 11.7 8.6 12.8

92 116.1 92.9 139.3

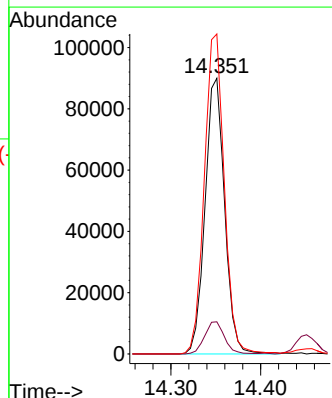



#52

Acenaphthene

Concen: 19.466 ng/ul

RT: 14.516 min Scan# 1943

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:153 Resp: 520891

Ion Ratio Lower Upper

153 100

152 45.2 38.4 57.6

154 89.3 69.7 104.5



#53

2,4-Dinitrophenol

Concen: 24.948 ng/ul

RT: 14.557 min Scan# 1950

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion:184 Resp: 69783


Ion Ratio Lower Upper

184 100

63 78.9 55.9 83.9

154 71.7 53.1 79.7









#55
4-Nitrophenol
Concen: 22.999 ng/ul
RT: 14.657 min Scan# 1967
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:109 Resp: 104620
Ion Ratio Lower Upper
109 100
139 130.3 100.1 150.1
65 132.9 104.6 157.0

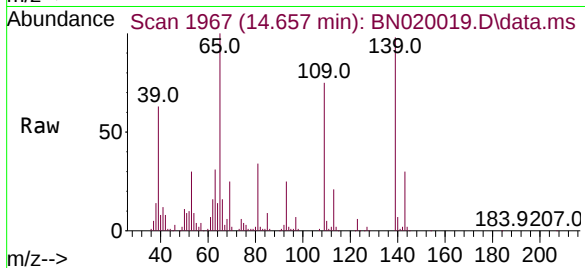

#56
Dibenzofuran
Concen: 19.731 ng/ul
RT: 14.851 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:168 Resp: 737558
Ion Ratio Lower Upper
168 100
139 39.5 31.1 46.7


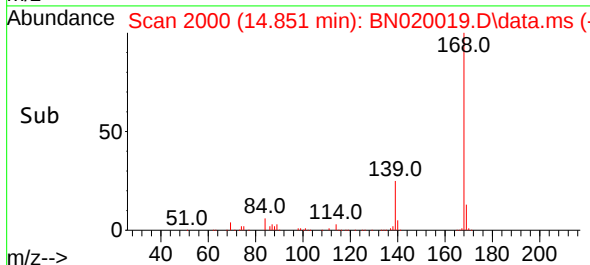

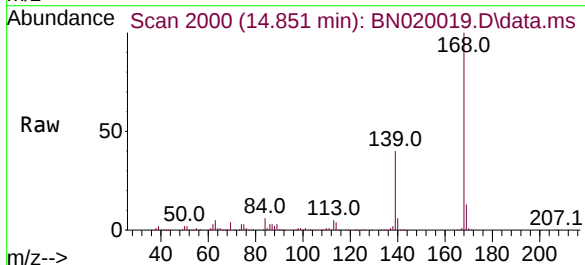




#57
2,4-Dinitrotoluene
Concen: 25.586 ng/ul
RT: 14.810 min Scan# 1993
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:165 Resp: 187609
Ion Ratio Lower Upper
165 100
63 48.7 36.3 54.5
182 2.8 2.3 3.5

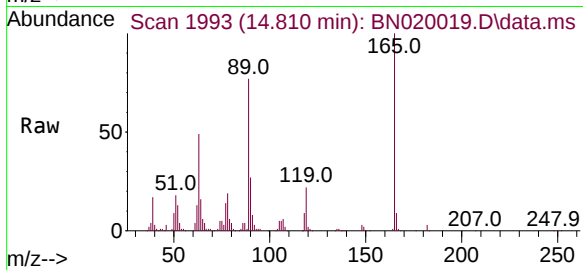

#58
2,3,4,6-Tetrachlorophenol
Concen: 22.704 ng/ul
RT: 15.075 min Scan# 2038
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:232 Resp: 133379
Ion Ratio Lower Upper
232 100
131 55.7 38.5 57.7
130 2.5 2.2 3.2
166 36.7 25.8 38.8




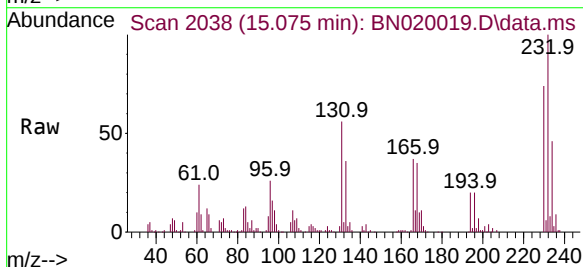




#59
Diethylphthalate
Concen: 22.701 ng/ul
RT: 15.275 min Scan# 2072
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:149 Resp: 652661
Ion Ratio Lower Upper
149 100
177 20.2 17.8 26.8
150 12.5 10.5 15.7

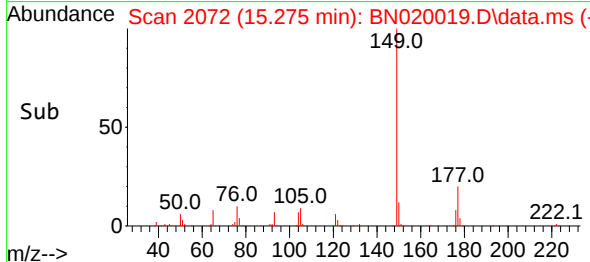

#61
Fluorene
Concen: 19.989 ng/ul
RT: 15.498 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:166 Resp: 580041
Ion Ratio Lower Upper
166 100
165 102.1 77.7 116.5
167 13.7 11.1 16.7


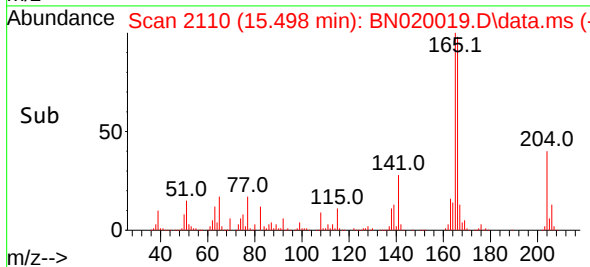

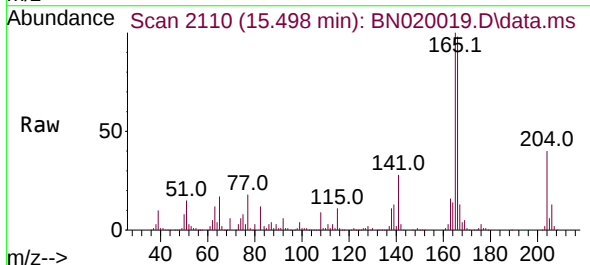




#62
4-Chlorophenyl-phenylether
Concen: 20.214 ng/ul
RT: 15.492 min Scan# 2109
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:204 Resp: 265219
Ion Ratio Lower Upper
204 100
206 32.5 26.7 40.1
141 69.2 50.2 75.2

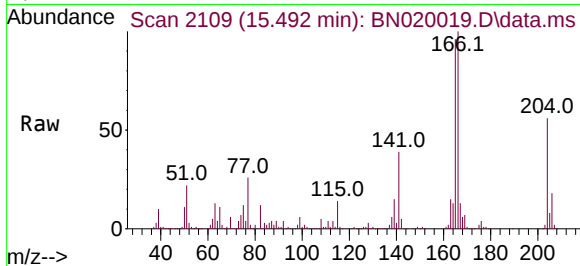

#63
4-Nitroaniline
Concen: 30.911 ng/ul
RT: 15.510 min Scan# 2112
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:138 Resp: 136926
Ion Ratio Lower Upper
138 100
92 51.1 41.0 61.6
108 81.6 65.3 97.9




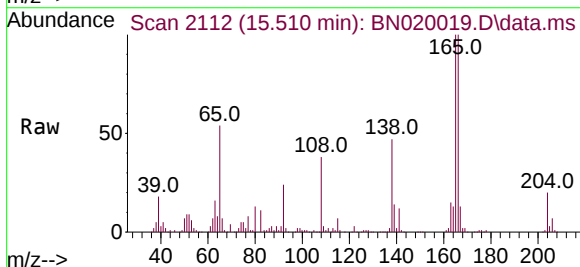




#66
 4,6-Dinitro-2-methylphenol
 Concen: 22.612 ng/ul
 RT: 15.575 min Scan# 2123
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45




Instrument :
 BNA_N
 ClientSampleId :
 SST020219


Tgt Ion:198 Resp: 107303
 Ion Ratio Lower Upper
 198 100
 182 3.9 3.0 4.4
 77 26.8 20.1 30.1



#67
 N-Nitrosodiphenylamine
 Concen: 18.638 ng/ul
 RT: 15.704 min Scan# 2145
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Tgt Ion:169 Resp: 522661
 Ion Ratio Lower Upper
 169 100
 168 65.2 52.4 78.6
 167 36.0 27.5 41.3









#68
4-Bromophenyl-phenylether
Concen: 18.757 ng/ul
RT: 16.386 min Scan# 2261
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:248 Resp: 161045
Ion Ratio Lower Upper
248 100
250 94.7 77.8 116.8
141 90.5 62.6 93.8

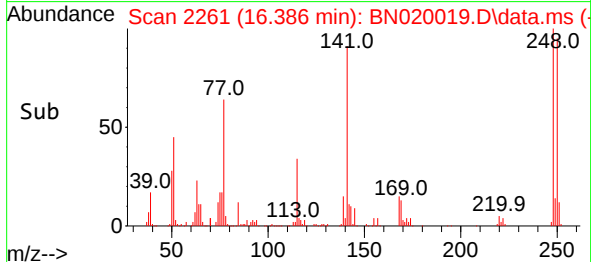

#69
Hexachlorobenzene
Concen: 18.097 ng/ul
RT: 16.504 min Scan# 2281
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:284 Resp: 174768
Ion Ratio Lower Upper
284 100
142 47.9 27.8 41.8#
249 37.4 25.7 38.5




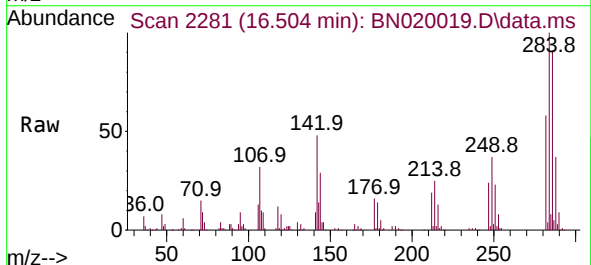




#70
Atrazine
Concen: 20.541 ng/ul
RT: 16.657 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:200 Resp: 183749
Ion Ratio Lower Upper
200 100
173 28.5 20.5 30.7
215 49.0 38.9 58.3

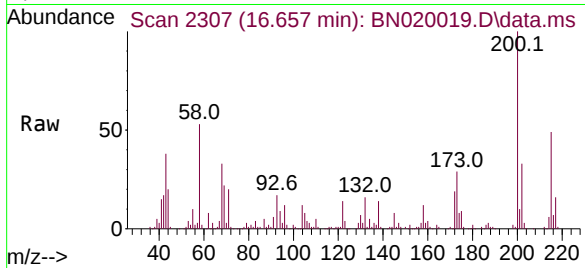

#71
Pentachlorophenol
Concen: 18.943 ng/ul
RT: 16.845 min Scan# 2339
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:266 Resp: 111017
Ion Ratio Lower Upper
266 100
264 56.1 50.2 75.2
268 56.9 49.3 73.9




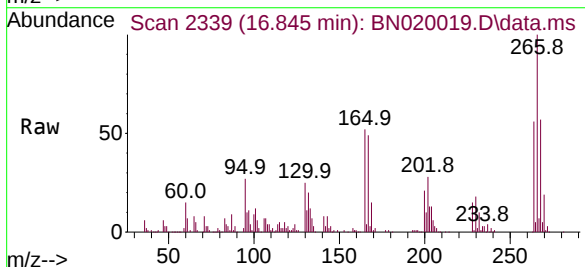




#72
Phenanthrene
Concen: 18.567 ng/ul
RT: 17.233 min Scan# 2405
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:178 Resp: 948279
Ion Ratio Lower Upper
178 100
179 15.5 12.2 18.4
176 19.3 15.2 22.8



#74
Anthracene
Concen: 18.824 ng/ul
RT: 17.327 min Scan# 2421
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:178 Resp: 960382
Ion Ratio Lower Upper
178 100
179 14.6 13.0 19.4
176 17.9 15.5 23.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 16.294 ng/uL
RT: 13.251 min Scan# 1728
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:216 Resp: 229559
Ion Ratio Lower Upper
216 100
214 77.7 63.2 94.8
218 48.3 37.9 56.9



#76
Pentachlorobenzene
Concen: 17.456 ng/uL
RT: 14.775 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:250 Resp: 214244
Ion Ratio Lower Upper
250 100
248 63.1 53.0 79.4
252 64.3 53.4 80.2




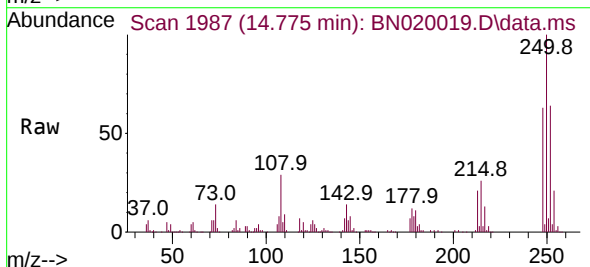




#77
 Carbazole
 Concen: 19.698 ng/ul
 RT: 17.592 min Scan# 2466
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45




Instrument :
 BNA_N
 ClientSampleId :
 SSTD020219


Tgt Ion:167 Resp: 913638
 Ion Ratio Lower Upper
 167 100
 166 21.2 16.1 24.1
 139 13.2 10.2 15.2

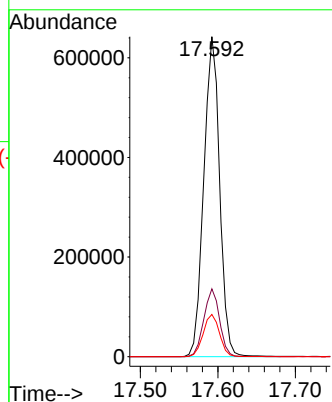

#78
 Di-n-butylphthalate
 Concen: 22.209 ng/ul
 RT: 18.163 min Scan# 2563
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Tgt Ion:149 Resp: 1101905
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.1 10.7
 104 5.3 4.1 6.1









#80
Fluoranthene
Concen: 18.952 ng/u1
RT: 19.251 min Scan# 2748
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:202 Resp: 1089723
Ion Ratio Lower Upper
202 100
101 11.5 8.9 13.3
100 9.2 6.7 10.1



#82
Pyrene
Concen: 18.705 ng/u1
RT: 19.616 min Scan# 2810
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:202 Resp: 1120269
Ion Ratio Lower Upper
202 100
101 14.1 9.7 14.5
100 11.4 8.0 12.0





#83

Butylbenzylphthalate

Concen: 22.998 ng/ul

RT: 20.521 min Scan# 2964

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:149 Resp: 509501

Ion Ratio Lower Upper

149 100

91 68.0 58.8 88.2

206 19.6 18.1 27.1



#84

3,3'-Dichlorobenzidine

Concen: 21.050 ng/ul

RT: 21.298 min Scan# 3096

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion:252 Resp: 358678


Ion Ratio Lower Upper

252 100

254 60.8 50.8 76.2

126 13.1 8.2 12.4









#85
Benzo(a)anthracene
Concen: 20.016 ng/ul
RT: 21.363 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:228 Resp: 1087666
Ion Ratio Lower Upper
228 100
229 18.3 16.3 24.5
226 26.1 23.2 34.8

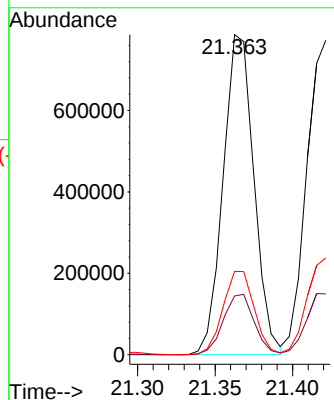

#86
Bis(2-ethylhexyl)phthalate
Concen: 21.775 ng/ul
RT: 21.304 min Scan# 3097
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:149 Resp: 740212
Ion Ratio Lower Upper
149 100
167 27.9 22.5 33.7
279 3.4 3.5 5.3#

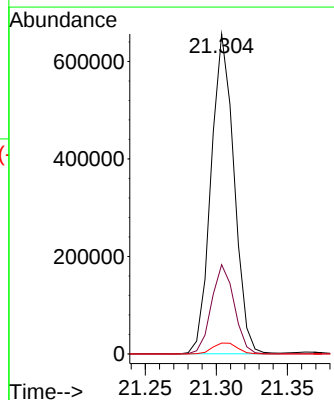



#87

Chrysene

Concen: 19.244 ng/ul

RT: 21.421 min Scan# 3117

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:228 Resp: 1027188

Ion Ratio Lower Upper

228 100

226 30.8 24.2 36.2

229 19.3 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 21.802 ng/ul




RT: 22.210 min Scan# 3251


Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Tgt Ion:149 Resp: 1310851









#90
Benzo(b)fluoranthene
Concen: 19.040 ng/ul
RT: 23.004 min Scan# 3386
Delta R.T. 0.000 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45




Instrument :
BNA_N
ClientSampleId :
SSTD020219


Tgt Ion:252 Resp: 1081777
Ion Ratio Lower Upper
252 100
253 19.9 16.5 24.7
125 12.0 7.8 11.8#

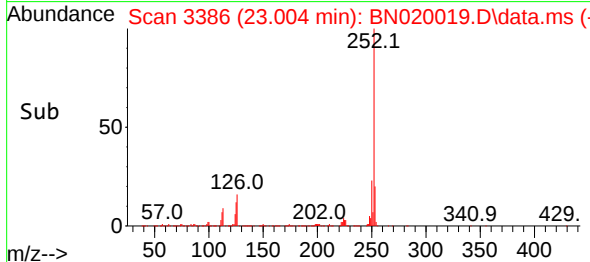

#91
Benzo(k)fluoranthene
Concen: 20.991 ng/ul
RT: 23.004 min Scan# 3386
Delta R.T. -0.047 min
Lab File: BN020019.D
Acq: 06 Jun 2022 12:45

Tgt Ion:252 Resp: 1081777
Ion Ratio Lower Upper
252 100
253 19.9 18.2 27.4
125 12.0 8.2 12.4

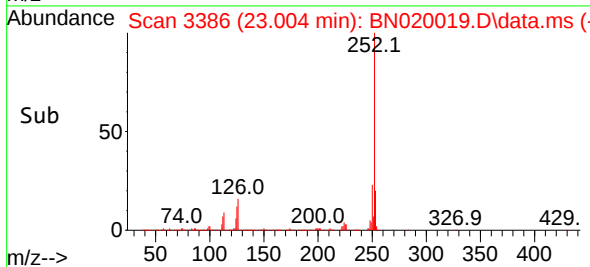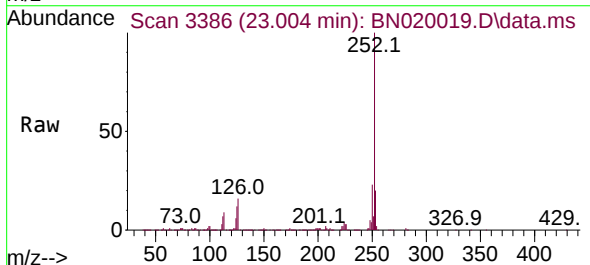



#93

Benzo(a)pyrene

Concen: 19.630 ng/ul

RT: 23.609 min Scan# 3489

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45

Instrument :

BNA_N

ClientSampleId :

SSTD020219





Tgt Ion:252 Resp: 1059108

Ion Ratio Lower Upper

252 100

253 20.2 18.7 28.1

125 13.1 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 17.751 ng/ul

RT: 26.098 min Scan# 3912

Delta R.T. 0.000 min

Lab File: BN020019.D

Acq: 06 Jun 2022 12:45




Tgt Ion:276 Resp: 1097564


Ion Ratio Lower Upper

276 100

138 28.4 19.5 29.3

277 23.3 21.4 32.0









#95
 Dibenzo(a,h)anthracene
 Concen: 17.889 ng/ul
 RT: 26.121 min Scan# 3916
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Instrument :
 BNA_N
 ClientSampleId :
 SSTD020219

Tgt Ion:278 Resp: 945757
 Ion Ratio Lower Upper
 278 100
 139 20.6 13.8 20.8
 279 24.6 18.3 27.5

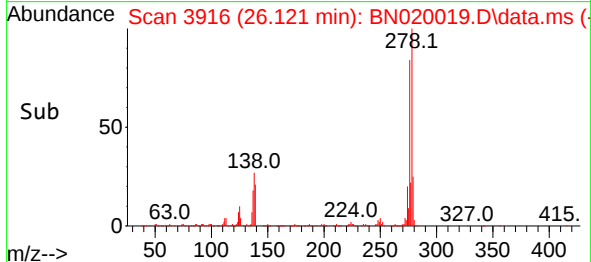

#96
 Benzo(g,h,i)perylene
 Concen: 17.142 ng/ul
 RT: 26.845 min Scan# 4039
 Delta R.T. 0.000 min
 Lab File: BN020019.D
 Acq: 06 Jun 2022 12:45

Tgt Ion:276 Resp: 932260
 Ion Ratio Lower Upper
 276 100
 138 26.7 17.0 25.6#
 277 23.4 17.8 26.6

