

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060622\
 Data File : BN020020.D
 Acq On : 06 Jun 2022 13:21
 Operator : CG/JU
 Sample : SSTD04020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD040220

Quant Time: Jun 06 14:38:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 14:35:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	137022	20.000	ng/u1	0.00
20) Naphthalene-d8	10.616	136	620760	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	391296	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.192	188	818571	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	734708	20.000	ng/u1	0.00
88) Perylene-d12	23.722	264	752046	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	52696	14.513	ng/uL	0.00
4) Pyridine-d5	3.687	84	368405	40.068	ng/u1	0.00
7) Phenol-d5	6.993	99	488439	41.135	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.158	67	302984	43.990	ng/u1	0.00
11) 2-Chlorophenol-d4	7.358	132	407078	43.220	ng/u1	0.00
15) 4-Methylphenol-d8	8.534	113	429629	47.231	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	214467	47.385	ng/u1	0.00
24) 2-Nitrophenol-d4	9.699	143	234406	52.553	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	398720	44.657	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	617202	45.537	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1234610	45.937	ng/u1	0.00
49) Acenaphthylene-d8	14.146	160	1444844	39.760	ng/u1	0.00
54) 4-Nitrophenol-d4	14.651	143	252965	48.396	ng/u1	0.00
60) Fluorene-d10	15.446	176	1009667	42.557	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.563	200	210577	50.391	ng/u1	0.00
73) Anthracene-d10	17.292	188	1507902	39.116	ng/u1	0.00
81) Pyrene-d10	19.586	212	1719325	40.703	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.569	264	1588509	41.320	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	55578	15.009	ng/uL	95
5) Pyridine	3.705	79	390433	40.298	ng/u1	92
6) Benzaldehyde	6.964	77	268542	44.125	ng/u1	92
8) Phenol	7.017	94	519364	43.466	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.246	93	407001	43.900	ng/u1	96
12) 2-Chlorophenol	7.387	128	419703	43.879	ng/u1	98
13) 2-Methylphenol	8.264	108	404611	45.734	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.358	45	644015	48.334	ng/u1	98
16) Acetophenone	8.640	105	645340	47.276	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.634	70	335418	52.797	ng/u1	93
18) 4-Methylphenol	8.599	108	447034	47.193	ng/u1	98
19) Hexachloroethane	8.905	117	167599	43.223	ng/u1	89
22) Nitrobenzene	9.016	77	481867	45.156	ng/u1	97
23) Isophorone	9.546	82	972093	51.077	ng/u1	99
25) 2-Nitrophenol	9.728	139	253728	50.375	ng/u1	97
26) 2,4-Dimethylphenol	9.793	107	502450	44.781	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.028	93	577193	46.120	ng/u1	98
29) 2,4-Dichlorophenol	10.263	162	402312	44.942	ng/u1	98
30) Naphthalene	10.663	128	1364584	41.046	ng/u1	100
32) 4-Chloroaniline	10.769	127	612918	44.991	ng/u1	97
33) Hexachlorobutadiene	10.963	225	220537	41.065	ng/u1	98
34) Caprolactam	11.528	113	86938	34.340	ng/u1	97
35) 4-Chloro-3-methylphenol	11.899	107	483894	51.071	ng/u1	99
36) 2-Methylnaphthalene	12.275	142	942957	44.071	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060622\
 Data File : BN020020.D
 Acq On : 06 Jun 2022 13:21
 Operator : CG/JU
 Sample : SST04020
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SST040220

Quant Time: Jun 06 14:38:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 14:35:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.499	142	944656	44.101	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.652	216	442149	40.723	ng/ul	96
40) Hexachlorocyclopentadiene	12.634	237	273533	40.944	ng/ul	100
41) 2,4,6-Trichlorophenol	12.887	196	316808	46.775	ng/ul	90
42) 2,4,5-Trichlorophenol	12.957	196	346571	47.127	ng/ul	96
43) 1,1'-Biphenyl	13.287	154	1260392	40.740	ng/ul	99
44) 2-Chloronaphthalene	13.328	162	951011	40.234	ng/ul	97
45) 2-Nitroaniline	13.528	65	322745	56.900	ng/ul	95
47) Dimethylphthalate	13.910	163	1236009	46.310	ng/ul	98
48) 2,6-Dinitrotoluene	14.028	165	263219	57.169	ng/ul	97
50) Acenaphthylene	14.175	152	1557374	41.715	ng/ul	98
51) 3-Nitroaniline	14.351	138	270746	57.370	ng/ul	98
52) Acenaphthene	14.516	153	1020707	41.774	ng/ul	99
53) 2,4-Dinitrophenol	14.557	184	161625	63.283	ng/ul	97
55) 4-Nitrophenol	14.663	109	213450	51.391	ng/ul	99
56) Dibenzofuran	14.851	168	1410655	41.330	ng/ul	95
57) 2,4-Dinitrotoluene	14.816	165	373956	55.855	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.081	232	265142	49.430	ng/ul	93
59) Diethylphthalate	15.281	149	1276261	48.617	ng/ul	98
61) Fluorene	15.498	166	1091231	41.185	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.493	204	496842	41.473	ng/ul	90
63) 4-Nitroaniline	15.516	138	260516	64.409	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.581	198	214986	50.581	ng/ul	95
67) N-Nitrosodiphenylamine	15.710	169	1006676	40.080	ng/ul	98
68) 4-Bromophenyl-phenylether	16.387	248	305735	39.758	ng/ul	90
69) Hexachlorobenzene	16.504	284	346428	40.051	ng/ul#	91
70) Atrazine	16.663	200	367035	45.810	ng/ul	98
71) Pentachlorophenol	16.845	266	228296	43.492	ng/ul	97
72) Phenanthrene	17.234	178	1798868	39.324	ng/ul	100
74) Anthracene	17.328	178	1806605	39.535	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.257	216	468842	37.155	ng/ul	98
76) Pentachlorobenzene	14.775	250	413983	37.660	ng/ul	97
77) Carbazole	17.592	167	1751557	42.163	ng/ul	98
78) Di-n-butylphthalate	18.169	149	2196192	49.421	ng/ul	100
80) Fluoranthene	19.251	202	2059191	41.356	ng/ul	96
82) Pyrene	19.616	202	2050448	39.534	ng/ul#	93
83) Butylbenzylphthalate	20.522	149	1027451	53.555	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.304	252	656936	44.522	ng/ul#	99
85) Benzo(a)anthracene	21.369	228	1941288	41.254	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.310	149	1414845	48.064	ng/ul	100
87) Chrysene	21.422	228	1916933	41.472	ng/ul	98
89) Di-n-octyl phthalate	22.210	149	2616492	50.821	ng/ul	100
90) Benzo(b)fluoranthene	23.016	252	2002717	41.165	ng/ul	96
91) Benzo(k)fluoranthene	23.057	252	1930728	43.751	ng/ul	96
93) Benzo(a)pyrene	23.622	252	1947447	42.152	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	26.121	276	1963726	37.090	ng/ul#	90
95) Dibenzo(a,h)anthracene	26.133	278	1684560	37.210	ng/ul	97
96) Benzo(g,h,i)perylene	26.851	276	1684922	36.181	ng/ul#	93





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 15.009 ng/uL
RT: 3.317 min Scan# 39
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion: 88 Resp: 55578
Ion Ratio Lower Upper
88 100
43 32.4 22.4 33.6
58 79.8 61.0 91.4



#5
Pyridine
Concen: 40.298 ng/uL
RT: 3.705 min Scan# 105
Delta R.T. -0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion: 79 Resp: 390433
Ion Ratio Lower Upper
79 100
52 90.1 65.0 97.4
51 41.4 31.6 47.4









#6
Benzaldehyde
Concen: 44.125 ng/ul
RT: 6.964 min Scan# 659
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion: 77 Resp: 268542
Ion Ratio Lower Upper
77 100
105 100.1 74.7 112.1
106 95.6 70.2 105.4



#8
Phenol
Concen: 43.466 ng/ul
RT: 7.017 min Scan# 668
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion: 94 Resp: 519364
Ion Ratio Lower Upper
94 100
65 29.6 23.6 35.4
66 39.8 31.2 46.8









#10
 Bis(2-Chloroethyl)ether
 Concen: 43.900 ng/ul
 RT: 7.246 min Scan# 707
 Delta R.T. 0.000 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21

Instrument :
 BNA_N
 ClientSampleId :
 SST040220

Tgt Ion: 93 Resp: 407001




Ion	Ratio	Lower	Upper
93	100		
63	83.6	63.4	95.0
95	33.4	26.2	39.2




#12
 2-Chlorophenol
 Concen: 43.879 ng/ul
 RT: 7.387 min Scan# 731
 Delta R.T. 0.000 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21

Tgt Ion: 128 Resp: 419703

Ion	Ratio	Lower	Upper
128	100		
64	47.9	38.6	57.8
130	33.1	25.0	37.4









#13
2-Methylphenol
Concen: 45.734 ng/ul
RT: 8.264 min Scan# 880
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:108 Resp: 404611
Ion Ratio Lower Upper
108 100
107 91.2 71.5 107.3



#14
2,2'-oxybis(1-Chloropropane)
Concen: 48.334 ng/ul
RT: 8.358 min Scan# 896
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion: 45 Resp: 644015
Ion Ratio Lower Upper
45 100
77 12.4 10.9 16.3
79 10.2 8.6 13.0









#16
Acetophenone
Concen: 47.276 ng/ul
RT: 8.640 min Scan# 944
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:105 Resp: 645340
Ion Ratio Lower Upper
105 100
77 78.2 63.5 95.3
51 30.0 23.5 35.3



#17
N-Nitroso-di-n-propylamine
Concen: 52.797 ng/ul
RT: 8.634 min Scan# 943
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion: 70 Resp: 335418
Ion Ratio Lower Upper
70 100
42 66.9 47.8 71.6
101 9.8 7.8 11.6
130 21.6 15.8 23.8









#18
4-Methylphenol
Concen: 47.193 ng/ul
RT: 8.599 min Scan# 911
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:108 Resp: 447034
Ion Ratio Lower Upper
108 100
107 111.9 88.0 132.0



#19
Hexachloroethane
Concen: 43.223 ng/ul
RT: 8.905 min Scan# 989
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:117 Resp: 167599
Ion Ratio Lower Upper
117 100
201 91.4 83.2 124.8
199 56.5 50.2 75.4





#22

Nitrobenzene

Concen: 45.156 ng/ul

RT: 9.016 min Scan# 1008

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion: 77 Resp: 481867

Ion Ratio Lower Upper

77 100

123 45.2 34.5 51.7

65 14.6 11.1 16.7



#23

Isophorone

Concen: 51.077 ng/ul

RT: 9.546 min Scan# 1098

Delta R.T. 0.006 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion: 82 Resp: 972093


Ion Ratio Lower Upper

82 100

95 7.6 5.8 8.8

138 17.6 13.8 20.8





#25

2-Nitrophenol

Concen: 50.375 ng/ul

RT: 9.728 min Scan# 1129

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:139 Resp: 253728

Ion Ratio Lower Upper

139 100

65 52.4 43.7 65.5

109 30.9 25.8 38.6



#26

2,4-Dimethylphenol

Concen: 44.781 ng/ul

RT: 9.793 min Scan# 1140

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion:107 Resp: 502450


Ion Ratio Lower Upper

107 100

121 50.1 38.3 57.5

122 84.5 66.3 99.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 46.120 ng/ul
 RT: 10.028 min Scan# 1180
 Delta R.T. 0.000 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21




Instrument :
 BNA_N
 ClientSampleId :
 SST040220


Tgt Ion: 93 Resp: 577193
 Ion Ratio Lower Upper
 93 100
 95 32.3 25.4 38.0
 123 11.6 8.3 12.5



#29
 2,4-Dichlorophenol
 Concen: 44.942 ng/ul
 RT: 10.263 min Scan# 1220
 Delta R.T. 0.000 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21

Tgt Ion: 162 Resp: 402312
 Ion Ratio Lower Upper
 162 100
 164 67.5 52.9 79.3
 98 38.4 29.8 44.8









#30
Naphthalene
Concen: 41.046 ng/ul
RT: 10.663 min Scan# 1288
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:128 Resp: 1364584
Ion Ratio Lower Upper
128 100
129 10.9 8.7 13.1
127 13.2 10.6 16.0



#32
4-Chloroaniline
Concen: 44.991 ng/ul
RT: 10.769 min Scan# 1306
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:127 Resp: 612918
Ion Ratio Lower Upper
127 100
129 31.1 26.1 39.1





#33

Hexachlorobutadiene

Concen: 41.065 ng/uI

RT: 10.963 min Scan# 11

Delta R.T. 0.006 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:225 Resp: 220537

Ion Ratio Lower Upper

225 100

223 64.3 51.8 77.6

227 59.8 50.6 76.0



#34

Caprolactam

Concen: 34.340 ng/uI

RT: 11.528 min Scan# 1435

Delta R.T. 0.012 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion:113 Resp: 86938


Ion Ratio Lower Upper

113 100

55 180.3 145.5 218.3

56 138.3 106.5 159.7









#35
4-Chloro-3-methylphenol
Concen: 51.071 ng/ul
RT: 11.899 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:107 Resp: 483894
Ion Ratio Lower Upper
107 100
144 24.9 20.6 31.0
142 77.0 62.2 93.4



#36
2-Methylnaphthalene
Concen: 44.071 ng/ul
RT: 12.275 min Scan# 1562
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:142 Resp: 942957
Ion Ratio Lower Upper
142 100
141 87.0 70.6 105.8









#37
1-Methylnaphthalene
Concen: 44.101 ng/ul
RT: 12.499 min Scan# 1
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:142 Resp: 944656
Ion Ratio Lower Upper
142 100
141 93.6 70.9 106.3
116 4.0 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 40.723 ng/ul
RT: 12.652 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:216 Resp: 442149
Ion Ratio Lower Upper
216 100
214 73.7 63.4 95.0
179 22.3 17.8 26.8
108 19.5 15.1 22.7









#40
Hexachlorocyclopentadiene
Concen: 40.944 ng/ul
RT: 12.634 min Scan# 1623
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:237 Resp: 273533
Ion Ratio Lower Upper
237 100
235 60.8 48.8 73.2
272 11.5 9.3 13.9



#41
2,4,6-Trichlorophenol
Concen: 46.775 ng/ul
RT: 12.887 min Scan# 1666
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:196 Resp: 316808
Ion Ratio Lower Upper
196 100
198 88.5 79.8 119.8
200 28.0 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 47.127 ng/ul
RT: 12.957 min Scan# 1678
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:196 Resp: 346571
Ion Ratio Lower Upper
196 100
198 92.4 77.6 116.4
200 29.2 24.4 36.6



#43
1,1'-Biphenyl
Concen: 40.740 ng/ul
RT: 13.287 min Scan# 1734
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:154 Resp: 1260392
Ion Ratio Lower Upper
154 100
153 40.3 31.5 47.3
76 12.7 10.5 15.7





#44

2-Chloronaphthalene

Concen: 40.234 ng/ul

RT: 13.328 min Scan# 1741

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:162 Resp: 951011

Ion Ratio Lower Upper

162 100

164 32.5 25.8 38.6

127 42.1 31.4 47.2

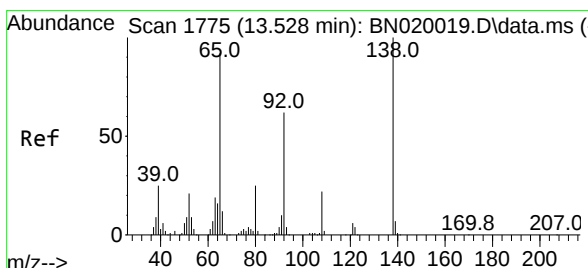

#45

2-Nitroaniline

Concen: 56.900 ng/ul

RT: 13.528 min Scan# 1775

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion: 65 Resp: 322745


Ion Ratio Lower Upper

65 100

92 66.2 54.1 81.1

138 103.8 77.0 115.4









#47
Dimethylphthalate
Concen: 46.310 ng/ul
RT: 13.910 min Scan# 1840
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:163 Resp: 1236009
Ion Ratio Lower Upper
163 100
194 4.0 3.4 5.0
164 10.4 7.7 11.5



#48
2,6-Dinitrotoluene
Concen: 57.169 ng/ul
RT: 14.028 min Scan# 1860
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:165 Resp: 263219
Ion Ratio Lower Upper
165 100
89 60.6 50.6 75.8
121 21.8 17.9 26.9









#50
Acenaphthylene
Concen: 41.715 ng/ul
RT: 14.175 min Scan# 1885
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:152 Resp: 1557374
Ion Ratio Lower Upper
152 100
151 21.2 16.0 24.0
153 13.2 10.7 16.1



#51
3-Nitroaniline
Concen: 57.370 ng/ul
RT: 14.351 min Scan# 1915
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:138 Resp: 270746
Ion Ratio Lower Upper
138 100
108 11.6 8.6 12.8
92 118.8 92.9 139.3





#52

Acenaphthene

Concen: 41.774 ng/ul

RT: 14.516 min Scan# 1943

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:153 Resp: 1020707

Ion Ratio Lower Upper

153 100

152 45.8 38.4 57.6

154 87.5 69.7 104.5



#53

2,4-Dinitrophenol

Concen: 63.283 ng/ul

RT: 14.557 min Scan# 1950

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion:184 Resp: 161625


Ion Ratio Lower Upper

184 100

63 74.1 55.9 83.9

154 67.2 53.1 79.7









#55
4-Nitrophenol
Concen: 51.391 ng/ul
RT: 14.663 min Scan# 1967
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:109 Resp: 213450
Ion Ratio Lower Upper
109 100
139 127.4 100.1 150.1
65 129.9 104.6 157.0



#56
Dibenzofuran
Concen: 41.330 ng/ul
RT: 14.851 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:168 Resp: 1410655
Ion Ratio Lower Upper
168 100
139 41.7 31.1 46.7









#57
2,4-Dinitrotoluene
Concen: 55.855 ng/ul
RT: 14.816 min Scan# 1994
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:165 Resp: 373956
Ion Ratio Lower Upper
165 100
63 50.7 36.3 54.5
182 2.8 2.3 3.5



#58
2,3,4,6-Tetrachlorophenol
Concen: 49.430 ng/ul
RT: 15.081 min Scan# 2039
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:232 Resp: 265142
Ion Ratio Lower Upper
232 100
131 53.5 38.5 57.7
130 2.9 2.2 3.2
166 35.4 25.8 38.8









#59
Diethylphthalate
Concen: 48.617 ng/ul
RT: 15.281 min Scan# 2072
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:149 Resp: 1276261
Ion Ratio Lower Upper
149 100
177 21.4 17.8 26.8
150 12.1 10.5 15.7



#61
Fluorene
Concen: 41.185 ng/ul
RT: 15.498 min Scan# 2110
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:166 Resp: 1091231
Ion Ratio Lower Upper
166 100
165 96.3 77.7 116.5
167 13.1 11.1 16.7









#62
4-Chlorophenyl-phenylether
Concen: 41.473 ng/ul
RT: 15.493 min Scan# 2109
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:204 Resp: 496842
Ion Ratio Lower Upper
204 100
206 32.8 26.7 40.1
141 74.1 50.2 75.2



#63
4-Nitroaniline
Concen: 64.409 ng/ul
RT: 15.516 min Scan# 2113
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:138 Resp: 260516
Ion Ratio Lower Upper
138 100
92 51.0 41.0 61.6
108 83.4 65.3 97.9









#66
 4,6-Dinitro-2-methylphenol
 Concen: 50.581 ng/ul
 RT: 15.581 min Scan# 2123
 Delta R.T. 0.006 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21




Instrument :
 BNA_N
 ClientSampleId :
 SST040220


Tgt Ion:198 Resp: 214986
 Ion Ratio Lower Upper
 198 100
 182 3.8 3.0 4.4
 77 28.1 20.1 30.1



#67
 N-Nitrosodiphenylamine
 Concen: 40.080 ng/ul
 RT: 15.710 min Scan# 2146
 Delta R.T. 0.006 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21

Tgt Ion:169 Resp: 1006676
 Ion Ratio Lower Upper
 169 100
 168 64.4 52.4 78.6
 167 35.7 27.5 41.3









#68
4-Bromophenyl-phenylether
Concen: 39.758 ng/ul
RT: 16.387 min Scan# 2261
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:248 Resp: 305735
Ion Ratio Lower Upper
248 100
250 101.5 77.8 116.8
141 93.7 62.6 93.8



#69
Hexachlorobenzene
Concen: 40.051 ng/ul
RT: 16.504 min Scan# 2281
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:284 Resp: 346428
Ion Ratio Lower Upper
284 100
142 44.4 27.8 41.8#
249 33.1 25.7 38.5









#70
Atrazine
Concen: 45.810 ng/ul
RT: 16.663 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:200 Resp: 367035
Ion Ratio Lower Upper
200 100
173 26.5 20.5 30.7
215 46.7 38.9 58.3



#71
Pentachlorophenol
Concen: 43.492 ng/ul
RT: 16.845 min Scan# 2339
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:266 Resp: 228296
Ion Ratio Lower Upper
266 100
264 63.6 50.2 75.2
268 65.3 49.3 73.9





#72

Phenanthrene

Concen: 39.324 ng/u1

RT: 17.234 min Scan# 2405

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:178 Resp: 1798868

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4

176 19.1 15.2 22.8



#74

Anthracene

Concen: 39.535 ng/u1

RT: 17.328 min Scan# 2421

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion:178 Resp: 1806605


Ion Ratio Lower Upper

178 100

179 16.0 13.0 19.4

176 18.6 15.5 23.3









#75
1,2,3,4-Tetrachlorobenzene
Concen: 37.155 ng/uL
RT: 13.257 min Scan# 1729
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:216 Resp: 468842
Ion Ratio Lower Upper
216 100
214 76.9 63.2 94.8
218 45.8 37.9 56.9



#76
Pentachlorobenzene
Concen: 37.660 ng/uL
RT: 14.775 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:250 Resp: 413983
Ion Ratio Lower Upper
250 100
248 64.1 53.0 79.4
252 63.9 53.4 80.2









#77
 Carbazole
 Concen: 42.163 ng/ul
 RT: 17.592 min Scan# 2466
 Delta R.T. 0.000 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21




Instrument :
 BNA_N
 ClientSampleId :
 SST040220


Tgt Ion:167 Resp: 1751557
 Ion Ratio Lower Upper
 167 100
 166 21.0 16.1 24.1
 139 13.3 10.2 15.2



#78
 Di-n-butylphthalate
 Concen: 49.421 ng/ul
 RT: 18.169 min Scan# 2564
 Delta R.T. 0.006 min
 Lab File: BN020020.D
 Acq: 06 Jun 2022 13:21

Tgt Ion:149 Resp: 2196192
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.1 10.7
 104 5.1 4.1 6.1









#80
Fluoranthene
Concen: 41.356 ng/u1
RT: 19.251 min Scan# 2748
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:202 Resp: 2059191
Ion Ratio Lower Upper
202 100
101 12.7 8.9 13.3
100 9.7 6.7 10.1



#82
Pyrene
Concen: 39.534 ng/u1
RT: 19.616 min Scan# 2810
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:202 Resp: 2050448
Ion Ratio Lower Upper
202 100
101 15.1 9.7 14.5#
100 12.2 8.0 12.0#









#83
Butylbenzylphthalate
Concen: 53.555 ng/ul
RT: 20.522 min Scan# 2964
Delta R.T. 0.000 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:149 Resp: 1027451
Ion Ratio Lower Upper
149 100
91 71.4 58.8 88.2
206 18.8 18.1 27.1



#84
3,3'-Dichlorobenzidine
Concen: 44.522 ng/ul
RT: 21.304 min Scan# 3097
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:252 Resp: 656936
Ion Ratio Lower Upper
252 100
254 63.1 50.8 76.2
126 13.0 8.2 12.4#









#85
Benzo(a)anthracene
Concen: 41.254 ng/ul
RT: 21.369 min Scan# 3107
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:228 Resp: 1941288
Ion Ratio Lower Upper
228 100
229 19.9 16.3 24.5
226 28.3 23.2 34.8



#86
Bis(2-ethylhexyl)phthalate
Concen: 48.064 ng/ul
RT: 21.310 min Scan# 3098
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:149 Resp: 1414845
Ion Ratio Lower Upper
149 100
167 28.0 22.5 33.7
279 4.0 3.5 5.3





#87

Chrysene

Concen: 41.472 ng/ul

RT: 21.422 min Scan# 3117

Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:228 Resp: 1916933

Ion Ratio Lower Upper

228 100

226 29.5 24.2 36.2

229 18.8 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 50.821 ng/ul




RT: 22.210 min Scan# 3251


Delta R.T. 0.000 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Tgt Ion:149 Resp: 2616492









#90
Benzo(b)fluoranthene
Concen: 41.165 ng/ul
RT: 23.016 min Scan# 3388
Delta R.T. 0.012 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21




Instrument :
BNA_N
ClientSampleId :
SSTD040220


Tgt Ion:252 Resp: 2002717
Ion Ratio Lower Upper
252 100
253 22.0 16.5 24.7
125 11.7 7.8 11.8



#91
Benzo(k)fluoranthene
Concen: 43.751 ng/ul
RT: 23.057 min Scan# 3395
Delta R.T. 0.006 min
Lab File: BN020020.D
Acq: 06 Jun 2022 13:21

Tgt Ion:252 Resp: 1930728
Ion Ratio Lower Upper
252 100
253 21.2 18.2 27.4
125 11.8 8.2 12.4





#93

Benzo(a)pyrene

Concen: 42.152 ng/ul

RT: 23.622 min Scan# 3489

Delta R.T. 0.012 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:252 Resp: 1947447

Ion Ratio Lower Upper

252 100

253 20.9 18.7 28.1

125 12.3 9.2 13.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 37.090 ng/ul

RT: 26.121 min Scan# 3916

Delta R.T. 0.024 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21




Tgt Ion:276 Resp: 1963726


Ion Ratio Lower Upper

276 100

138 33.1 19.5 29.3#

277 24.9 21.4 32.0





#95

Dibenzo(a,h)anthracene

Concen: 37.210 ng/ul

RT: 26.133 min Scan# 3916

Delta R.T. 0.012 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Instrument :

BNA_N

ClientSampleId :

SSTD040220





Tgt Ion:278 Resp: 1684560

Ion Ratio Lower Upper

278 100

139 20.0 13.8 20.8

279 22.7 18.3 27.5



#96

Benzo(g,h,i)perylene

Concen: 36.181 ng/ul

RT: 26.851 min Scan# 4040

Delta R.T. 0.006 min

Lab File: BN020020.D

Acq: 06 Jun 2022 13:21

Tgt Ion:276 Resp: 1684922

Ion Ratio Lower Upper

276 100

138 26.0 17.0 25.6#

277 23.9 17.8 26.6

