

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060624\
 Data File : BN031814.D
 Acq On : 06 Jun 2024 11:56
 Operator : MA/JU
 Sample : PB161173BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK173

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031814.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	29	34	40	rBV	112701	147494	2.09%	0.171%
2	3.587	99	102	122	rBV	1449583	2101504	29.73%	2.435%
3	3.911	152	157	163	rVB	19348	33630	0.48%	0.039%
4	6.675	625	627	633	rVB7	4910	8411	0.12%	0.010%
5	6.846	648	656	670	rVB	1639916	2641127	37.36%	3.060%
6	7.010	673	684	694	rBV	1379214	2199587	31.12%	2.548%
7	7.205	710	717	727	rBV	1692238	2726314	38.57%	3.158%
8	7.669	788	796	808	rVB	1264908	2006043	28.38%	2.324%
9	8.375	908	916	930	rBV	2101737	3352529	47.43%	3.884%
10	8.828	983	993	1003	rBV	1550565	2578535	36.48%	2.987%
11	9.546	1107	1115	1127	rBV	1215667	2071556	29.31%	2.400%
12	10.075	1197	1205	1224	rBV	1836187	3215534	45.49%	3.725%
13	10.451	1261	1269	1278	rBV	1710418	2885275	40.82%	3.343%
14	10.593	1285	1293	1310	rBV	1959365	3437829	48.63%	3.983%
15	12.046	1534	1540	1547	rBV2	32464	62098	0.88%	0.072%
16	13.281	1746	1750	1755	rBV5	7148	10063	0.14%	0.012%
17	13.728	1819	1826	1836	rBV	3063929	4477133	63.34%	5.187%
18	14.004	1866	1873	1885	rBV	3682204	5639490	79.78%	6.533%
19	14.316	1918	1926	1935	rBV	2445138	3688517	52.18%	4.273%
20	14.416	1939	1943	1949	rVB8	5394	10740	0.15%	0.012%
21	14.522	1953	1961	1981	rBV	1331901	2178763	30.82%	2.524%
22	14.734	1993	1997	2003	rVB8	7178	14758	0.21%	0.017%
23	15.310	2088	2095	2106	rBV	4642907	6552135	92.69%	7.590%
24	15.434	2110	2116	2130	rVV	1178828	1727177	24.43%	2.001%
25	15.551	2131	2136	2143	rVB3	25848	42564	0.60%	0.049%
26	16.098	2224	2229	2233	rBV7	5307	8562	0.12%	0.010%
27	16.739	2335	2338	2342	rVB5	5898	7924	0.11%	0.009%
28	16.851	2353	2357	2361	rVB2	6815	8656	0.12%	0.010%
29	17.063	2386	2393	2402	rBV	2792319	3948797	55.86%	4.575%
30	17.163	2403	2410	2420	rBV	4799414	6813657	96.39%	7.893%
31	17.963	2541	2546	2561	rBV	148340	334702	4.74%	0.388%
32	19.022	2722	2726	2735	rBV3	59733	99110	1.40%	0.115%
33	19.098	2735	2739	2743	rBV	60672	94338	1.33%	0.109%
34	19.251	2761	2765	2773	rBV2	85391	174037	2.46%	0.202%
35	19.463	2795	2801	2808	rBV	5175838	7068638	100.00%	8.189%
36	21.298	3108	3113	3119	rVB2	2476488	3509440	49.65%	4.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060624\
Data File : BN031814.D
Acq On : 06 Jun 2024 11:56
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	24.033	3569	3578	3589	rVB2	2761834	6693954	94.70%	7.755%
38	24.239	3605	3613	3624	rVB2	1433929	3749625	53.05%	4.344%




Sum of corrected areas: 86320246

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060624\
Data File : BN031814.D
Acq On : 06 Jun 2024 11:56
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

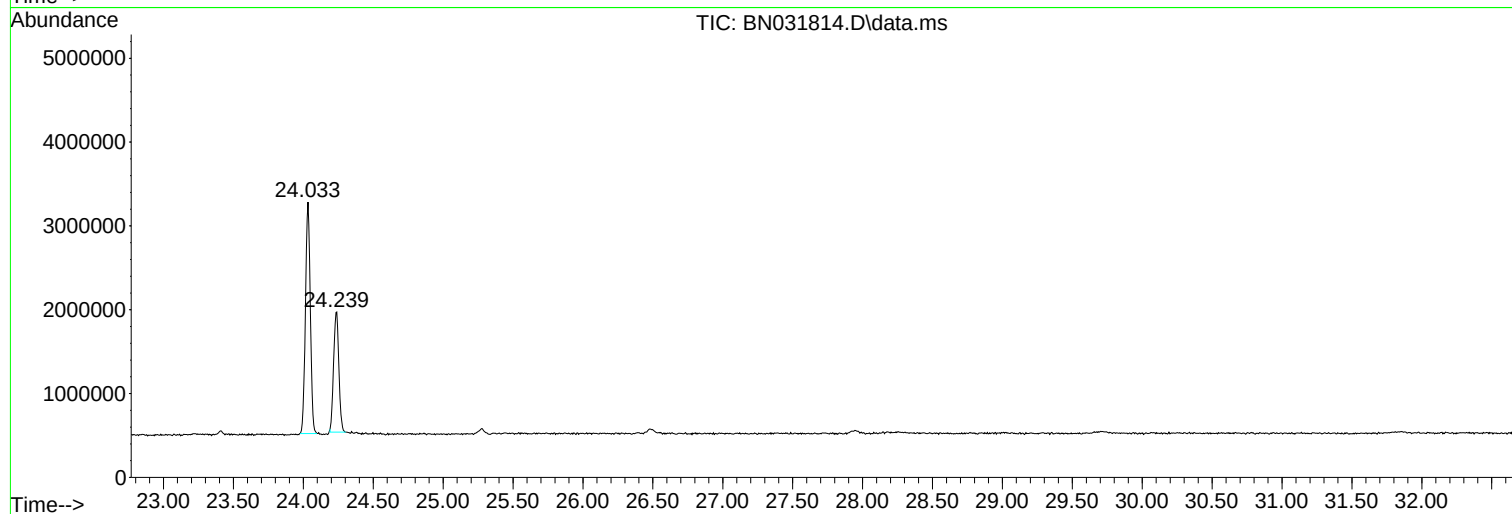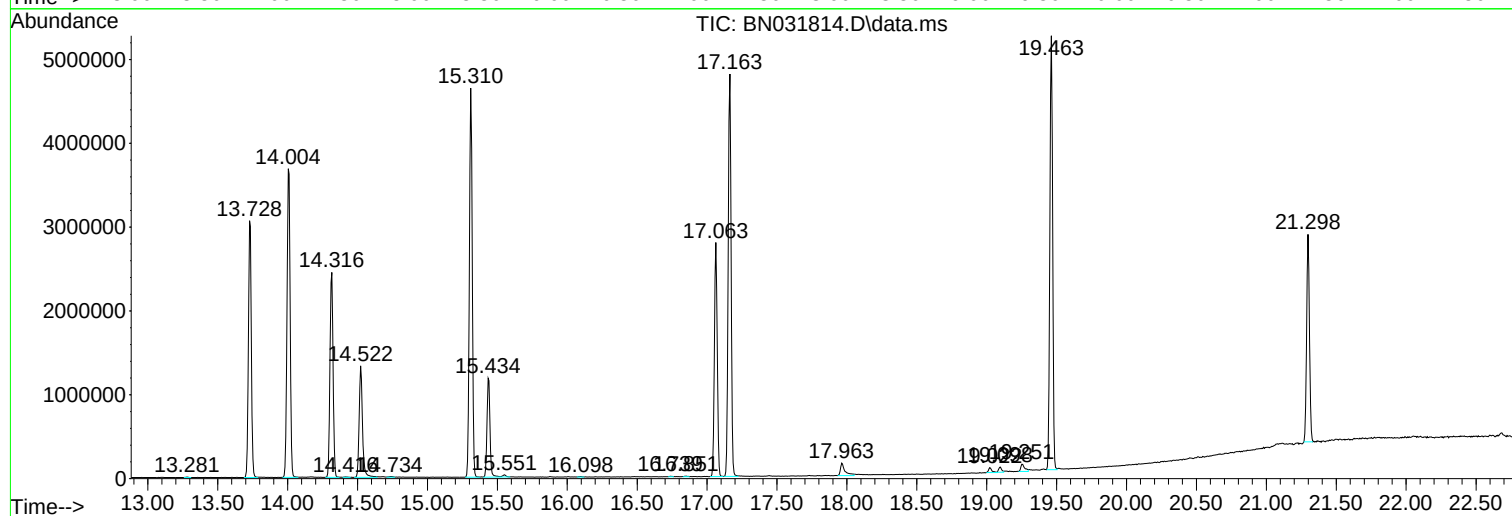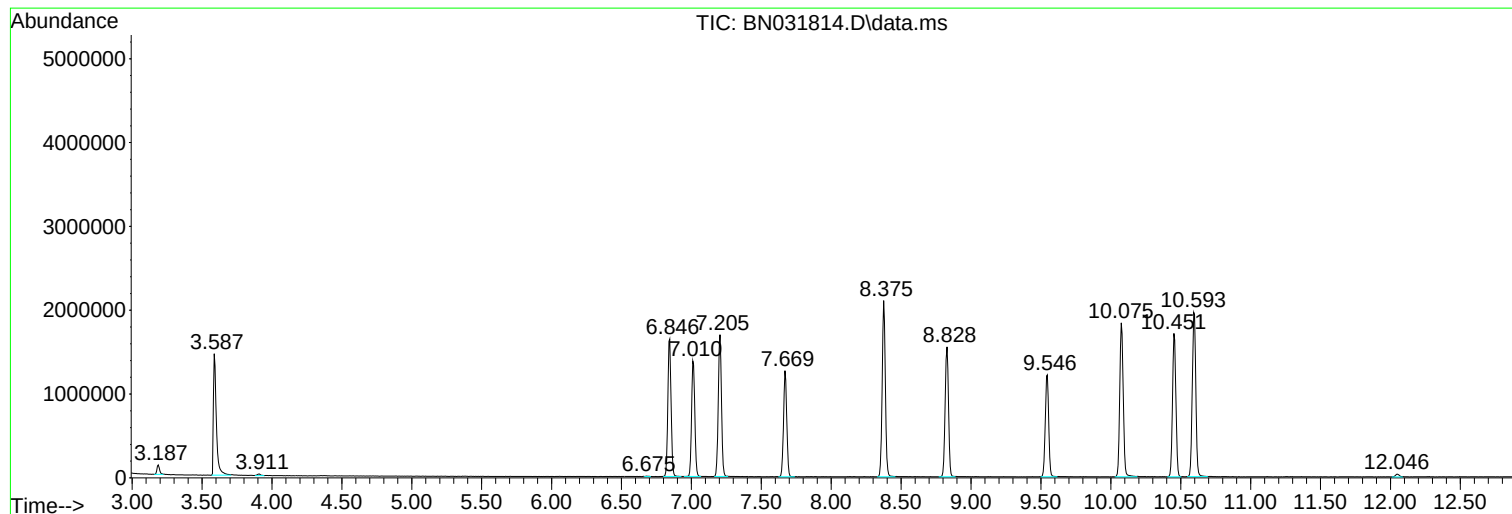

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060624\
Data File : BN031814.D
Acq On : 06 Jun 2024 11:56
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060624\
Data File : BN031814.D
Acq On : 06 Jun 2024 11:56
Operator : MA/JU
Sample : PB161173BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK173

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc