


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060820\
 Data File : BN010799.D
 Acq On : 08 Jun 2020 08:01
 Operator : CG/JU
 Sample : DFTPP66
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP66

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN060320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 10:24:50 2020

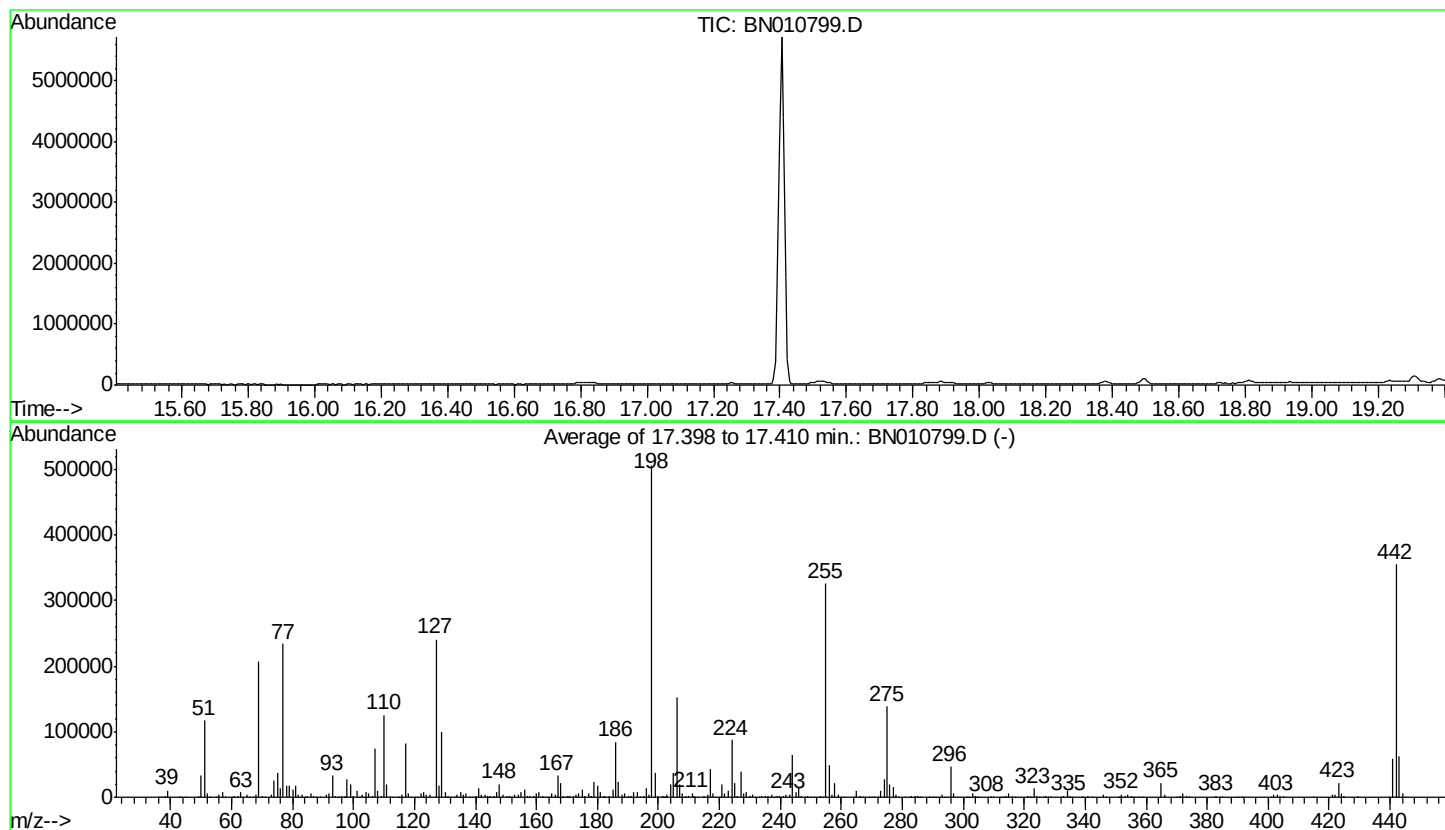

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	116416	PASS
68	69	0.00	2	1.9	3920	PASS
69	198	0.00	100	41.0	207274	PASS
70	69	0.00	2	0.7	1382	PASS
127	198	10	80	47.7	240917	PASS
197	198	0.00	2	0.8	4152	PASS
198	198	100	100	100.0	505578	PASS
199	198	5	9	7.2	36261	PASS
275	198	10	60	27.4	138386	PASS
365	198	1	100	4.4	22374	PASS
441	198	0.01	100	11.4	57704	PASS
442	198	50	100	70.2	355029	PASS
443	442	15	24	17.9	63485	PASS