
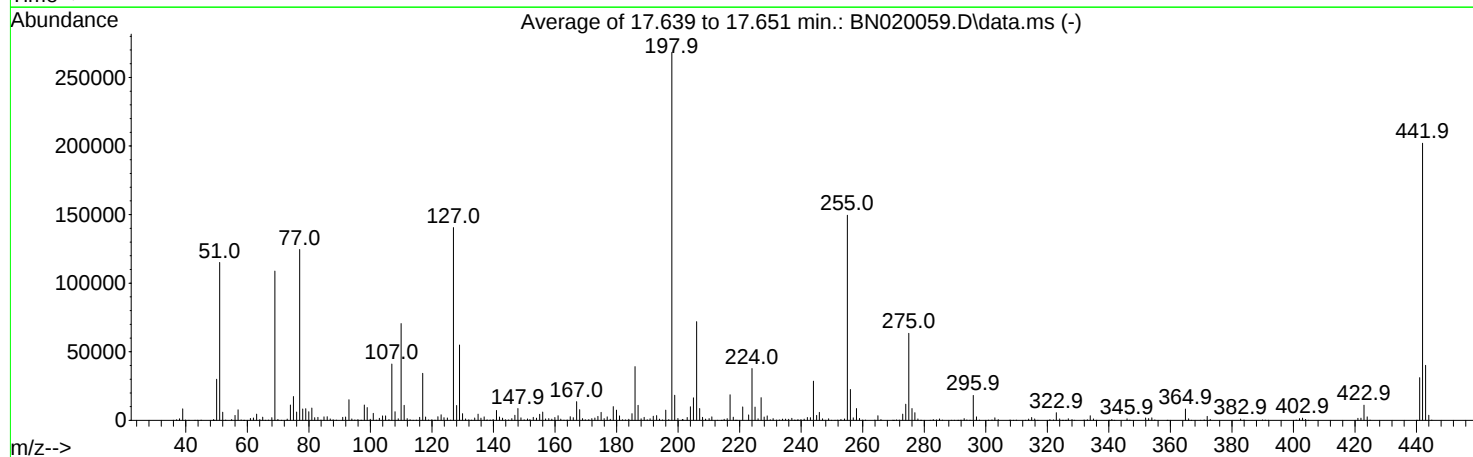


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060822\
 Data File : BN020059.D
 Acq On : 08 Jun 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN051322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 09 01:49:56 2022

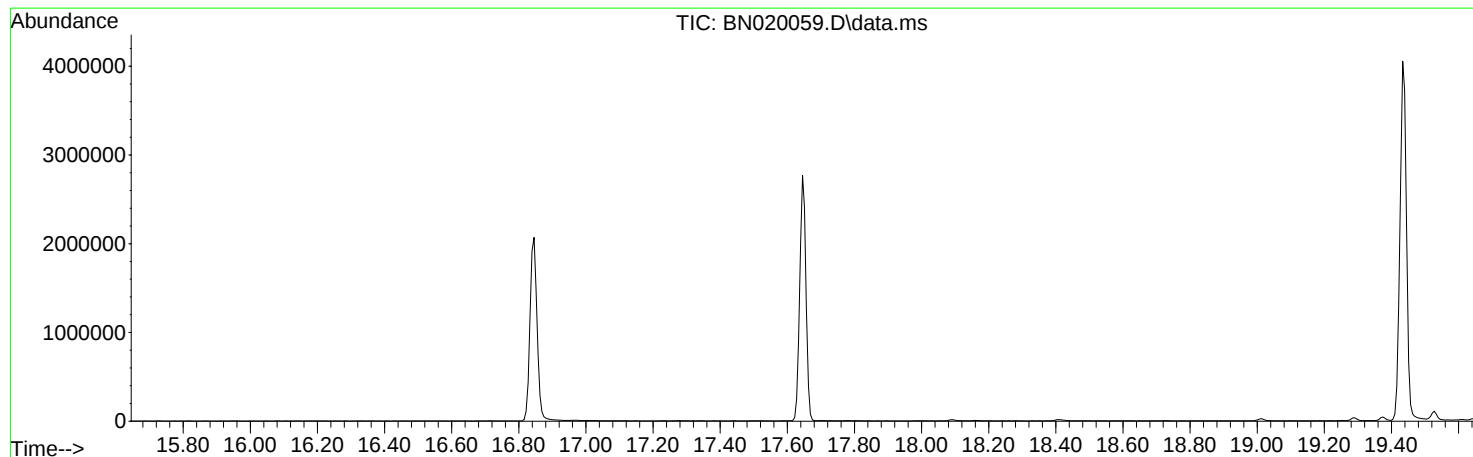




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	115088	PASS
68	69	0.00	2	1.9	2041	PASS
69	198	0.00	100	40.6	108821	PASS
70	69	0.00	2	0.6	665	PASS
127	198	10	80	52.4	140528	PASS
197	198	0.00	2	0.2	567	PASS
198	198	100	100	100.0	268181	PASS
199	198	5	9	6.8	18338	PASS
275	198	10	60	23.7	63456	PASS
365	198	1	100	3.1	8348	PASS
441	198	0.01	100	11.6	31131	PASS
442	442	50	100	100.0	202093	PASS
443	442	15	24	19.8	40085	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060822\
Data File : BN020059.D
Acq On : 08 Jun 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 04:41:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 09 04:41:15 2022
Response via : Initial Calibration

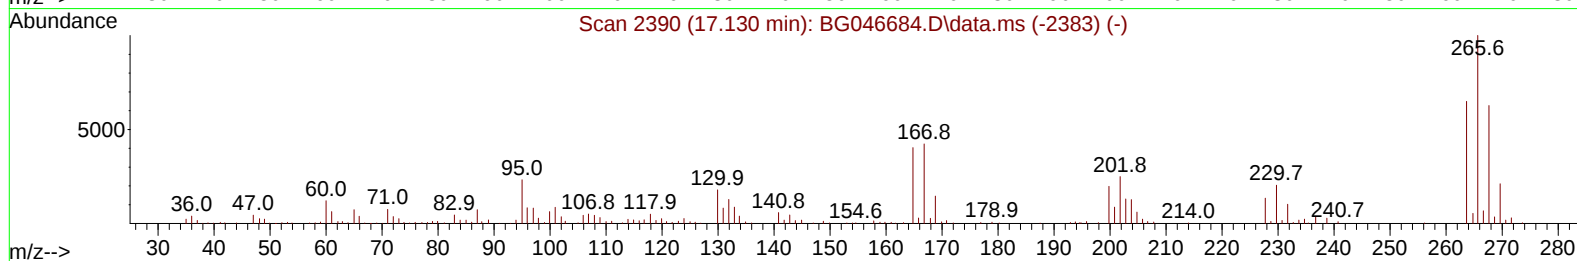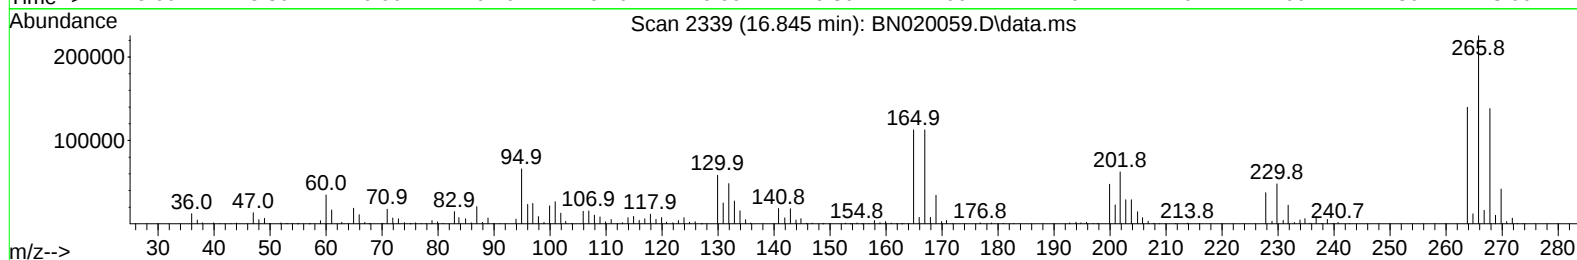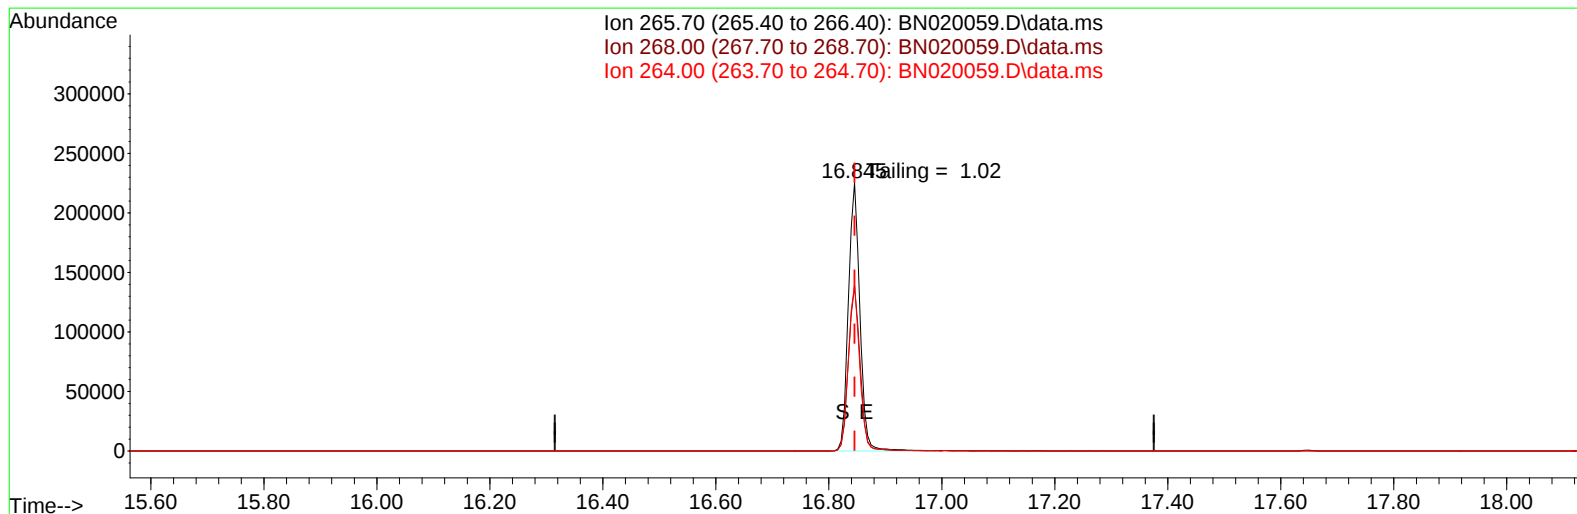

TIC: BN020059.D\data.ms

(70) Pentachlorophenol (C)

16.845min (0.000) 22953.46 ng




response 319736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.34
264.00	61.60	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060822\
Data File : BN020059.D
Acq On : 08 Jun 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 04:41:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 09 04:41:15 2022
Response via : Initial Calibration

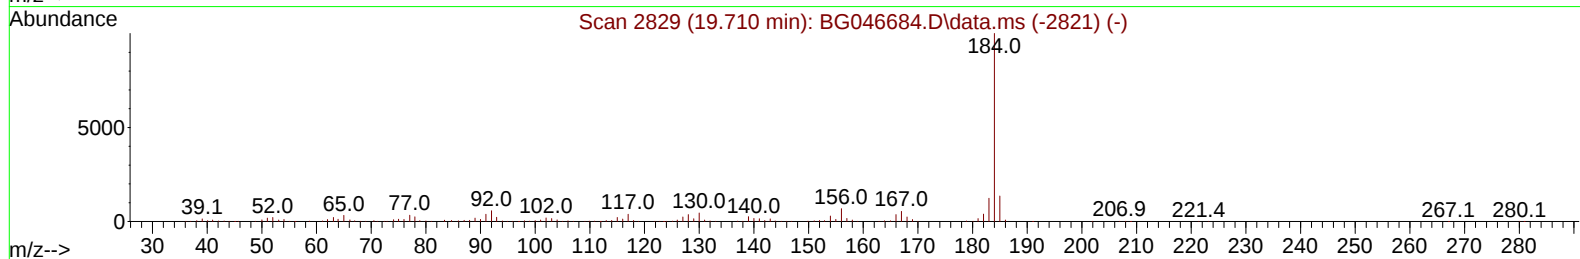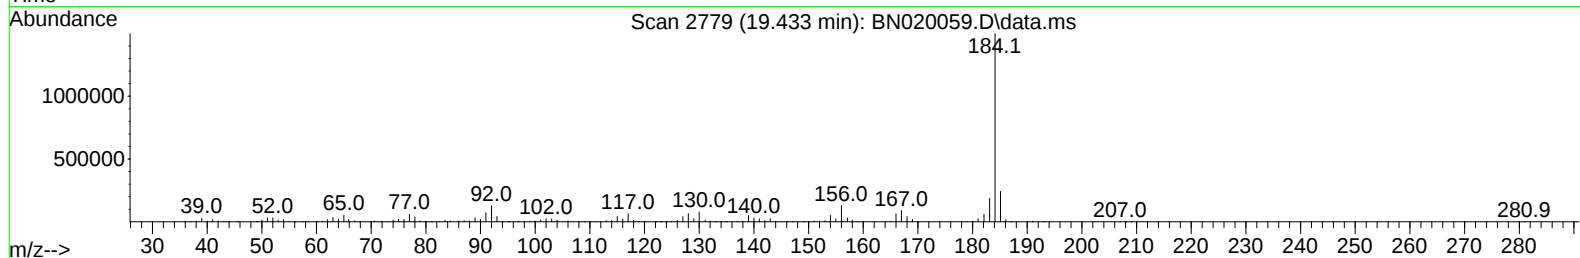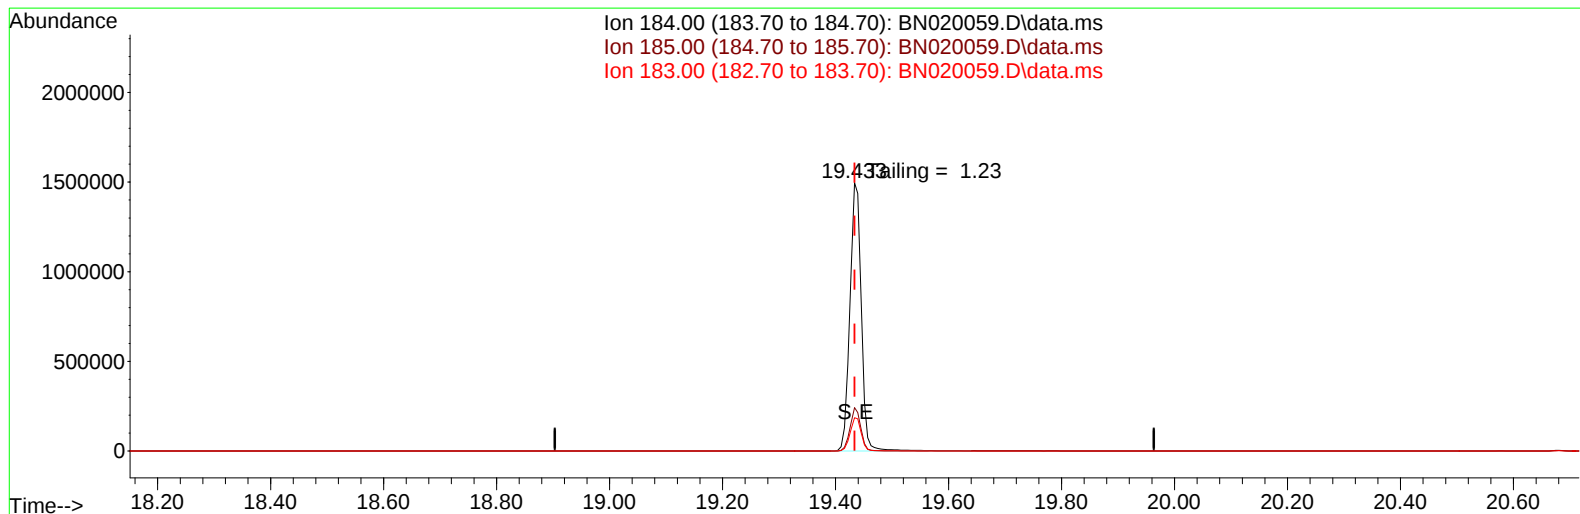

TIC: BN020059.D\data.ms

(77) Benzidine

19.433min (0.000) 0.00 ng

response 2102596

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.17
183.00	13.20	12.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/8/2022	BNA_N	<u>BN020059.D</u>
Compound Name	Response	Retention Time
DDT	965662	20.68
DDD	40769	20.239
DDE	784	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
41553	1007215	4.13

Instrument :
BNA_N
ClientSampleId :
DFTPP