


# n-Nitrosodimethylamine

Response Ratio

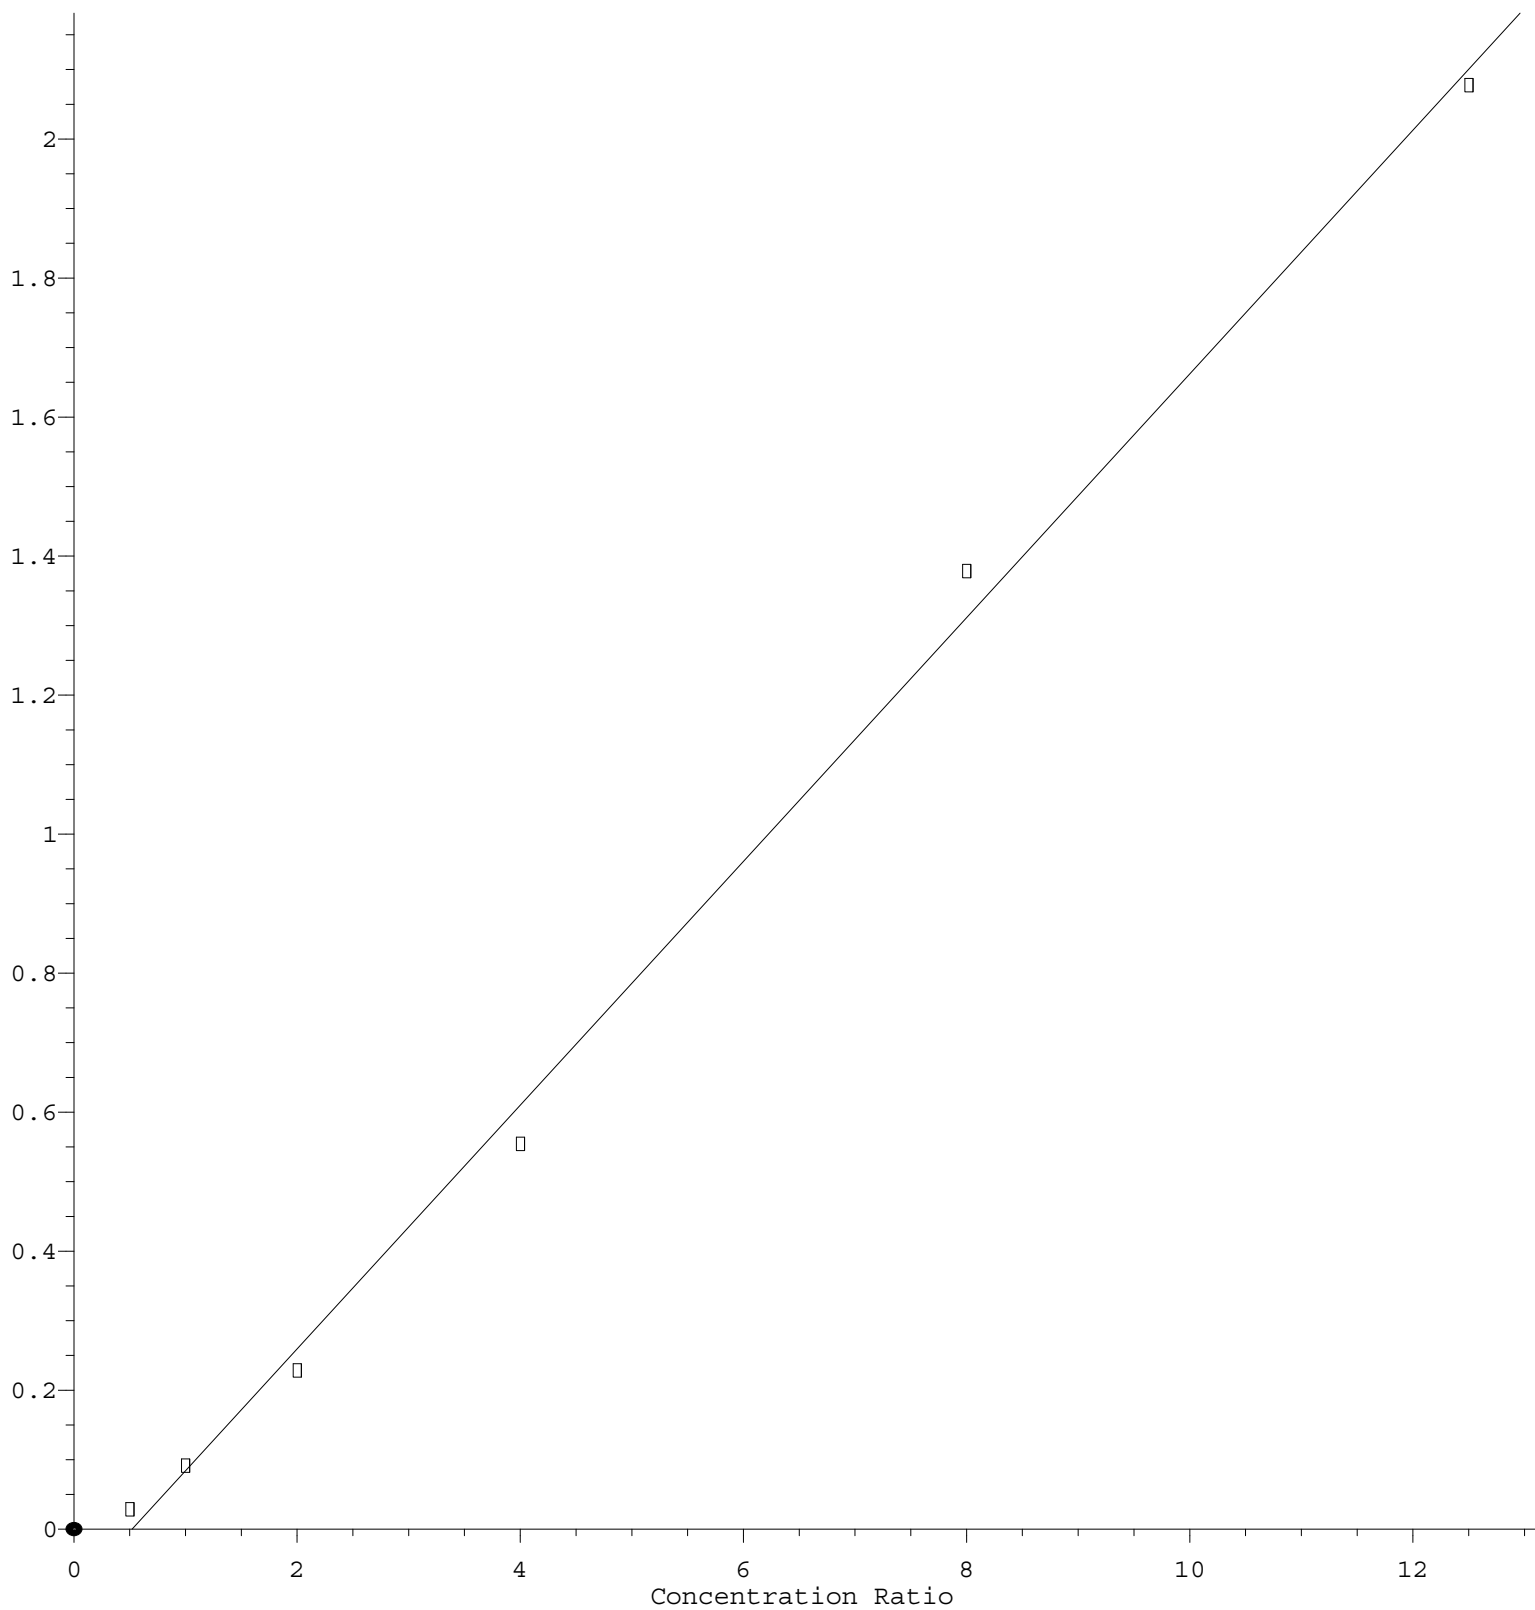


$$\text{Response} = 1.753\text{e-}001 * \text{Amt} - 9.190\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.997022 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN060921.M

Calibration Table Last Updated: Wed Jun 09 16:35:36 2021


# 4,6-Dinitro-2-methylphenol

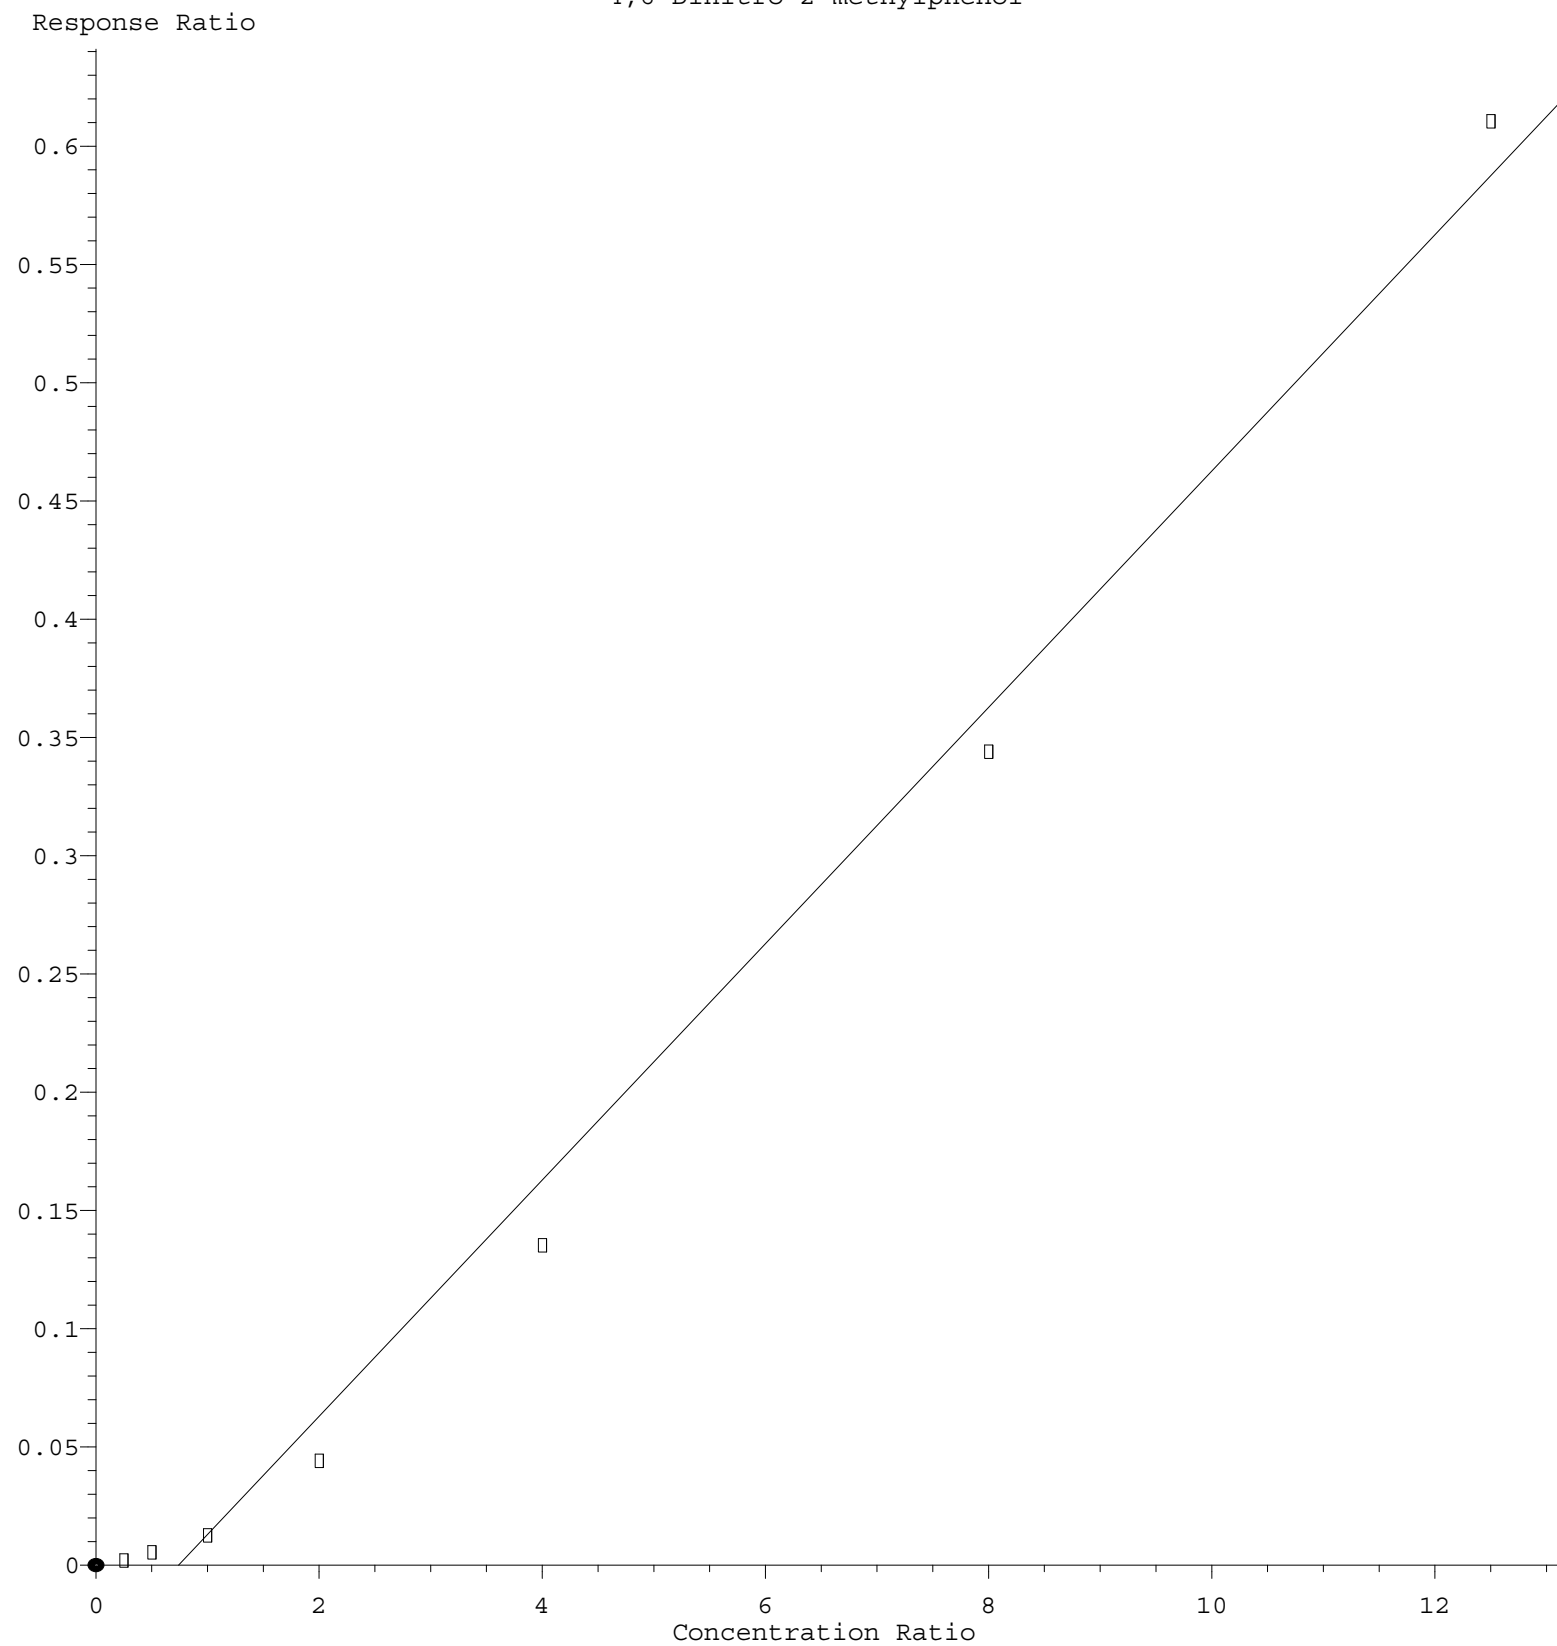

Response =  $4.995 \times 10^{-2} \times \text{Amt} - 3.678 \times 10^{-2}$   
 Coef of Det ( $r^2$ ) = 0.990672    Curve Fit: Linear  
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN060921.M  
 Calibration Table Last Updated: Wed Jun 09 16:35:36 2021

# Pentachlorophenol

Response Ratio

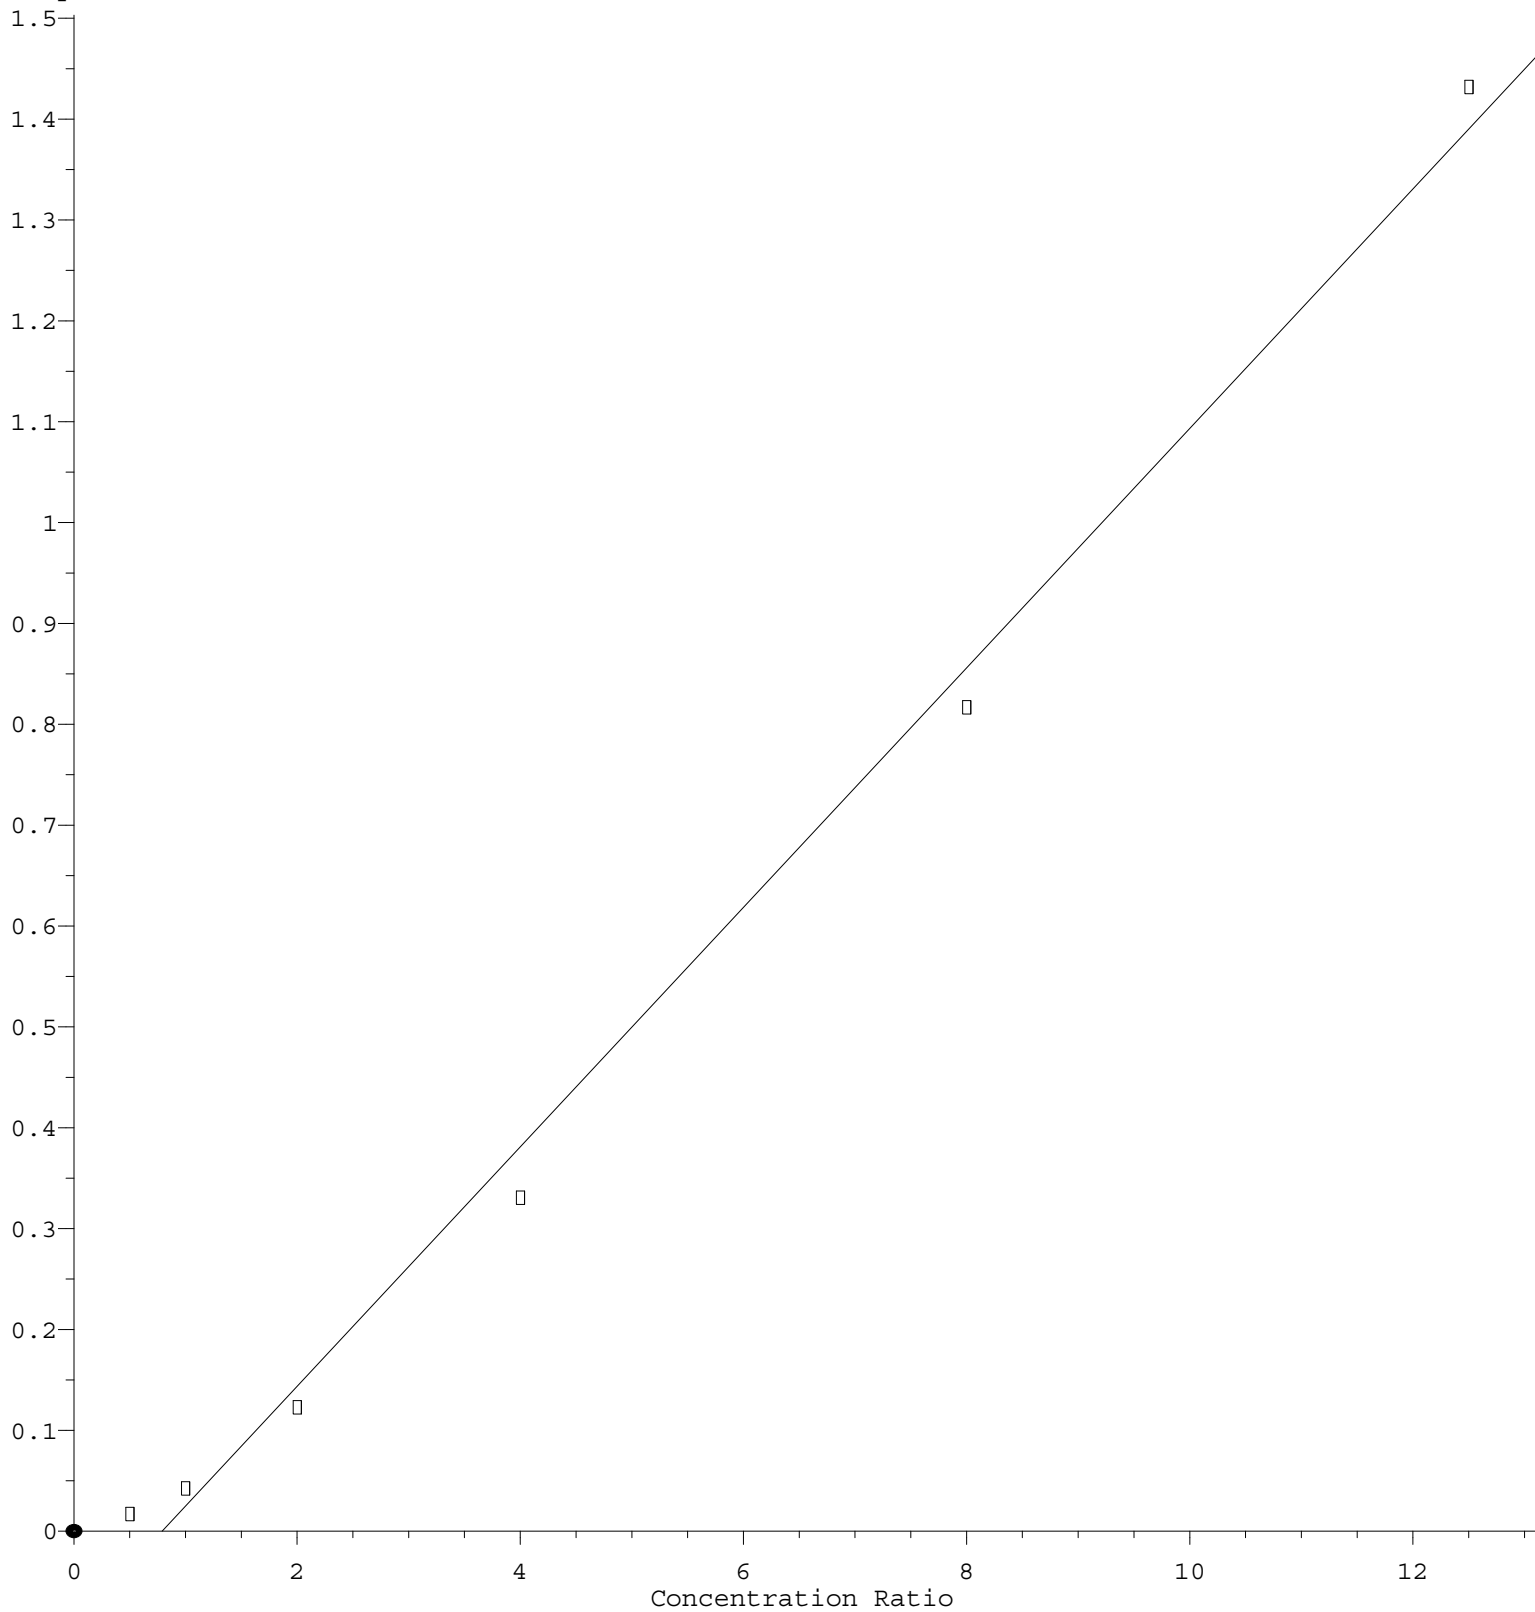

$$\text{Response} = 1.188\text{e-}001 * \text{Amt} - 9.406\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.994146 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN060921.M

Calibration Table Last Updated: Wed Jun 09 16:35:36 2021

# Indeno (1,2,3-cd)pyrene

Response Ratio

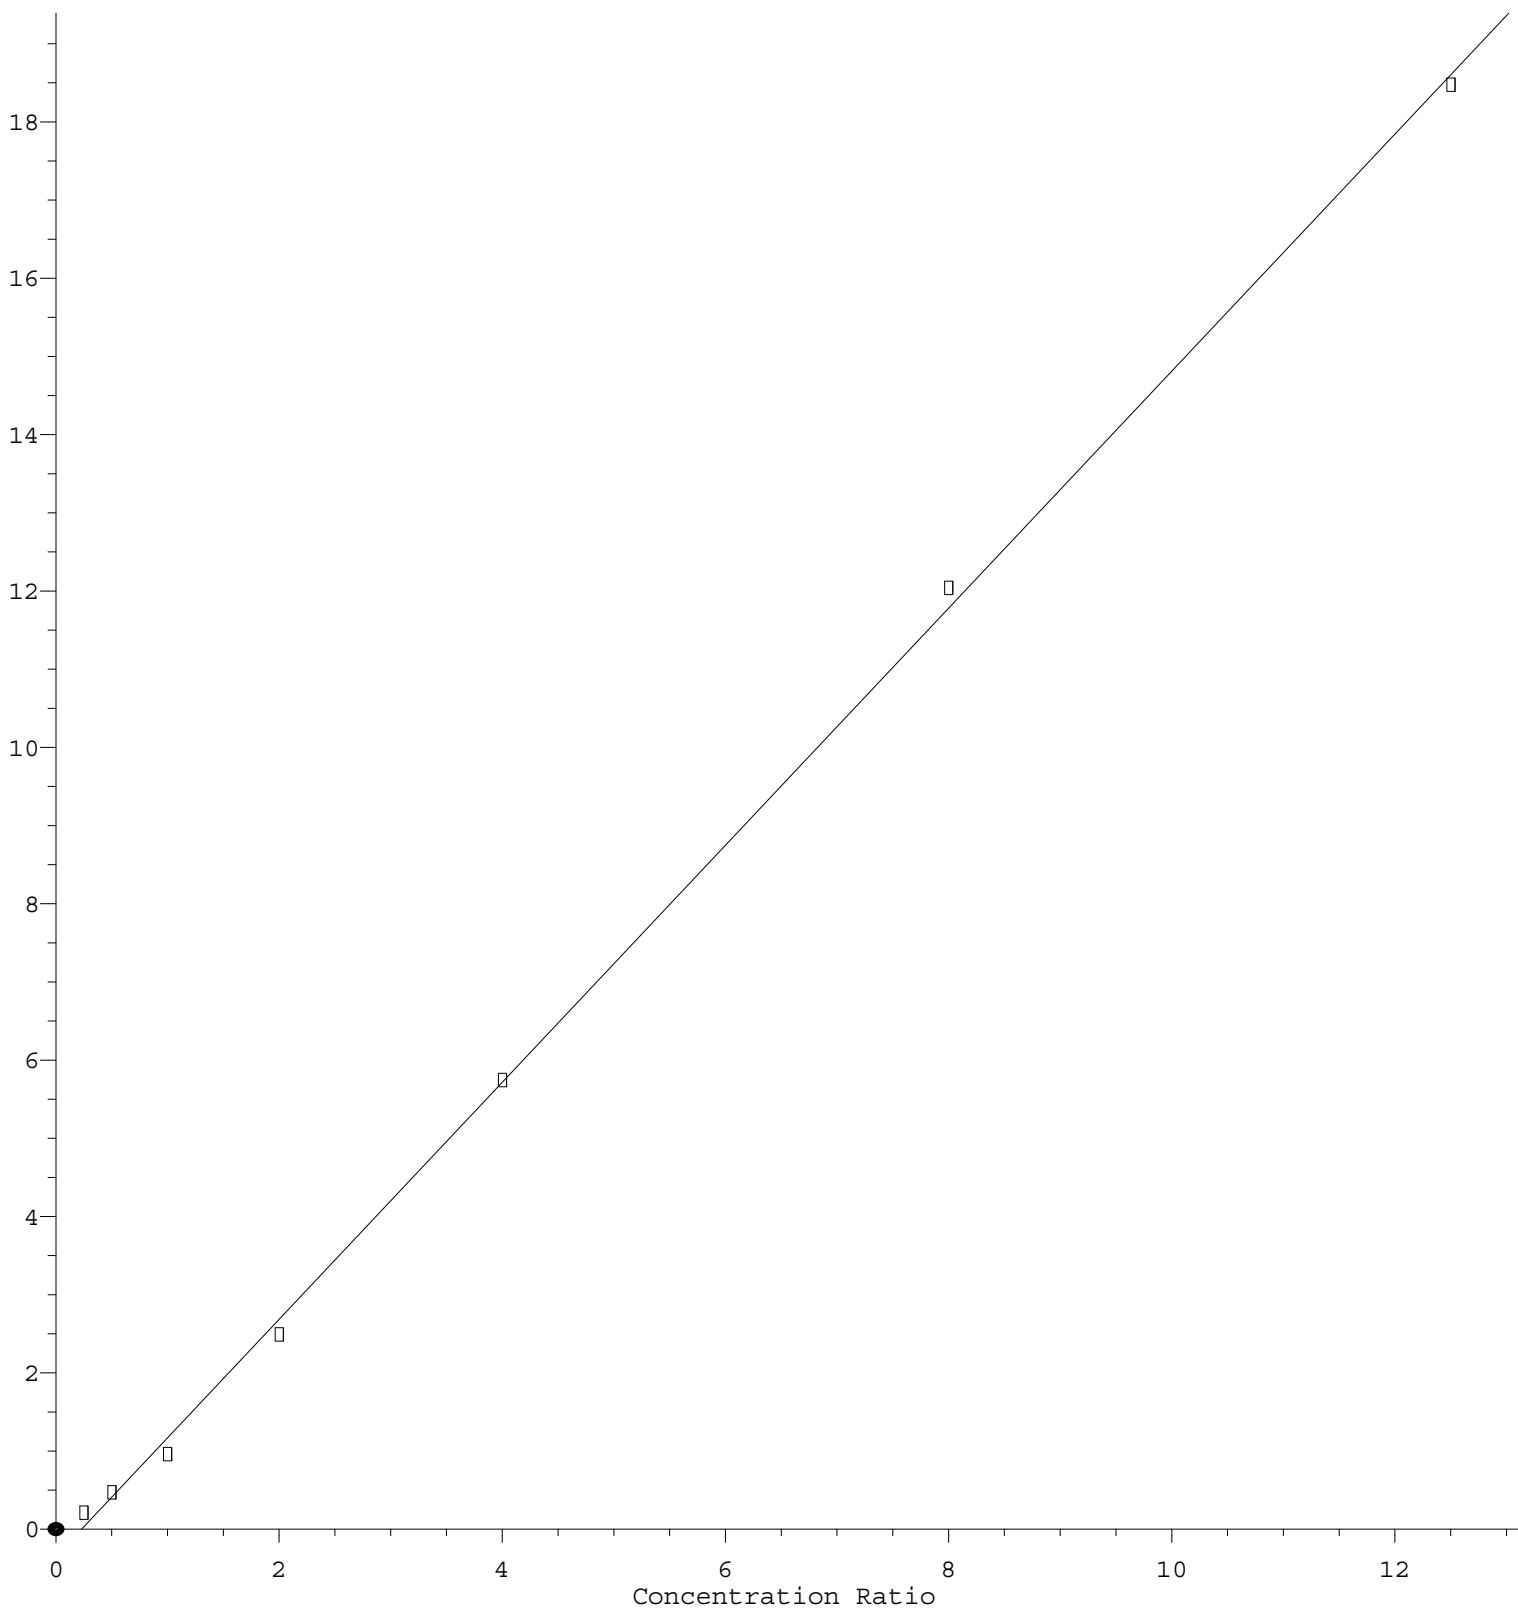

$$\text{Response} = 1.517\text{e}+000 * \text{Amt} - 3.509\text{e}-001$$


Coef of Det ( $r^2$ ) = 0.999314 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN060921.M

Calibration Table Last Updated: Wed Jun 09 16:35:36 2021

# Dibenzo (a,h) anthracene

Response Ratio

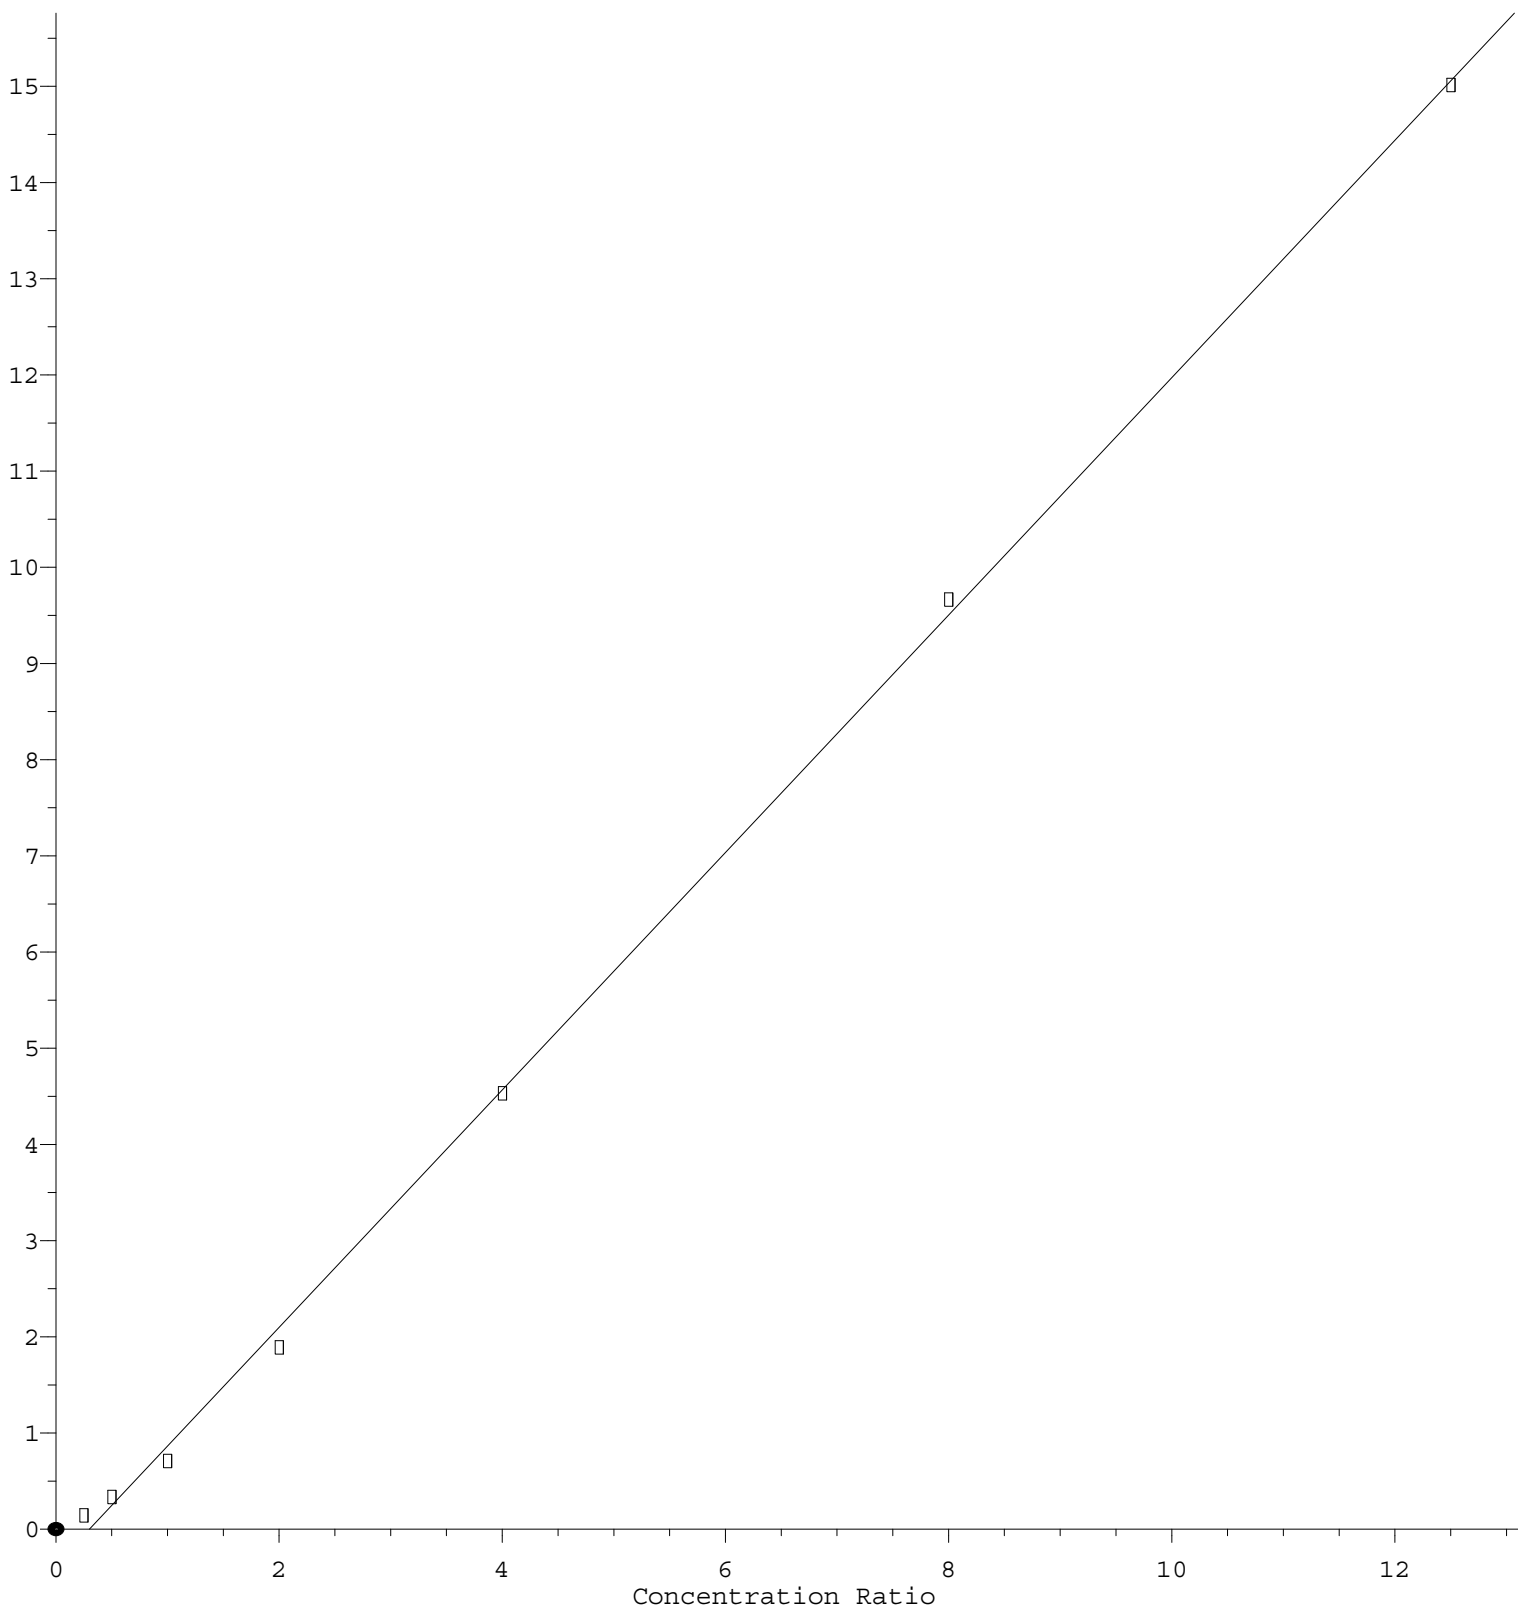

$$\text{Response} = 1.235\text{e}+000 * \text{Amt} - 3.715\text{e}-001$$

Coef of Det ( $r^2$ ) = 0.999246 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN060921.M

Calibration Table Last Updated: Wed Jun 09 16:35:36 2021