

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060921\
 Data File : BN014854.D
 Acq On : 09 Jun 2021 15:49
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN060921

Quant Time: Jun 09 16:37:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 09 16:35:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.717	152	2463	0.400	ng	0.00
7) Naphthalene-d8	10.496	136	9973	0.400	ng	# 0.01
13) Acenaphthene-d10	14.346	164	6558	0.400	ng	0.00
19) Phenanthrene-d10	17.103	188	13852	0.400	ng	# 0.01
29) Chrysene-d12	21.313	240	16454	0.400	ng	# 0.01
35) Perylene-d12	23.571	264	15547	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.329	112	2559	0.385	ng	0.00
5) Phenol-d6	6.887	99	2995	0.387	ng	0.00
8) Nitrobenzene-d5	8.861	82	2824	0.343	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	6821	0.363	ng	0.00
14) 2,4,6-Tribromophenol	15.855	330	989	0.359	ng	0.01
15) 2-Fluorobiphenyl	12.975	172	9461	0.382	ng	0.01
27) Fluoranthene-d10	19.143	212	16725	0.350	ng	0.00
31) Terphenyl-d14	19.749	244	15153	0.372	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.282	88	234	0.327	ng	94
3) n-Nitrosodimethylamine	3.706	42	224	0.417	ng	# 96
6) bis(2-Chloroethyl)ether	7.154	93	2184	0.372	ng	99
9) Naphthalene	10.534	128	10332	0.378	ng	100
10) Hexachlorobutadiene	10.838	225	2936	0.369	ng	# 97
12) 2-Methylnaphthalene	12.159	142	7202	0.375	ng	99
16) Acenaphthylene	14.066	152	10142	0.371	ng	100
17) Acenaphthene	14.409	154	6903	0.373	ng	99
18) Fluorene	15.399	166	8929	0.377	ng	99
20) 4,6-Dinitro-2-methylph...	15.487	198	176	0.396	ng	97
21) 4-Bromophenyl-phenylether	16.300	248	3608	0.366	ng	# 89
22) Hexachlorobenzene	16.410	284	4209	0.376	ng	99
23) Atrazine	16.568	200	1920	0.359	ng	97
24) Pentachlorophenol	16.763	266	581	0.458	ng	96
25) Phenanthrene	17.140	178	14817	0.376	ng	100
26) Anthracene	17.237	178	12533	0.360	ng	100
28) Fluoranthene	19.173	202	18465	0.371	ng	100
30) Pyrene	19.535	202	18389	0.375	ng	100
32) Benzo(a)anthracene	21.292	228	17234	0.368	ng	98
33) Chrysene	21.345	228	19938	0.363	ng	99
34) Bis(2-ethylhexyl)phtha...	21.228	149	4837	0.335	ng	100
36) Indeno(1,2,3-cd)pyrene	25.850	276	15311	0.352	ng	99
37) Benzo(b)fluoranthene	22.890	252	17422	0.351	ng	100
38) Benzo(k)fluoranthene	22.934	252	22489	0.381	ng	99
39) Benzo(a)pyrene	23.471	252	17390	0.370	ng	99
40) Dibenzo(a,h)anthracene	25.861	278	11435	0.359	ng	98
41) Benzo(g,h,i)perylene	26.538	276	15576	0.345	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060921\
Data File : BN014854.D
Acq On : 09 Jun 2021 15:49
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ICVBN060921

Quant Time: Jun 09 16:37:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 09 16:35:36 2021
Response via : Initial Calibration




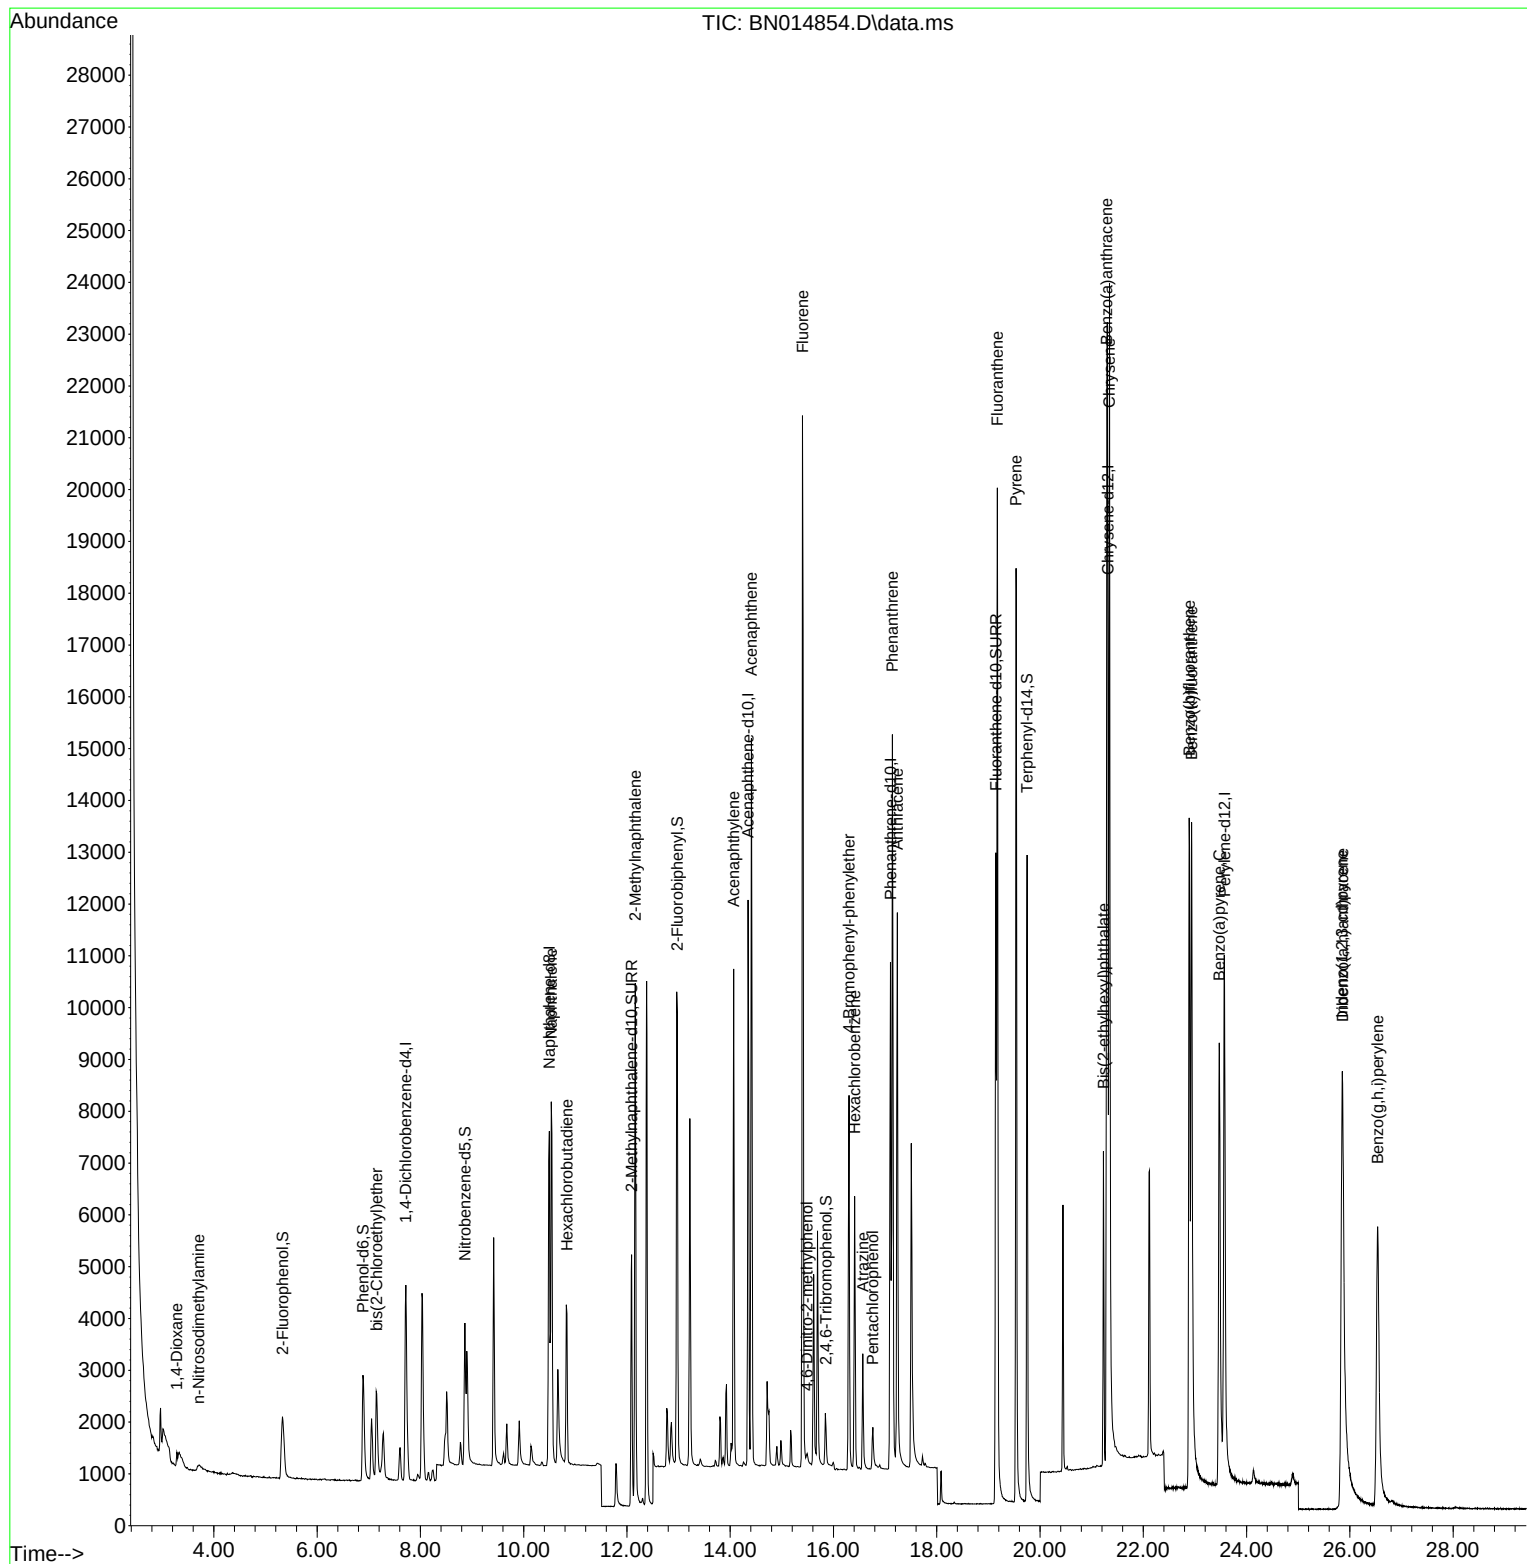


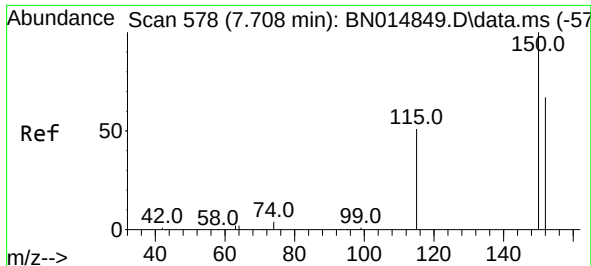

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.717 min Scan# 579
 Delta R.T. 0.009 min
 Lab File: BN014854.D
 Acq: 09 Jun 2021 15:49




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN060921


Tgt Ion: 152 Resp: 2463
 Ion Ratio Lower Upper
 152 100
 150 148.4 119.0 178.6
 115 73.8 62.2 93.4

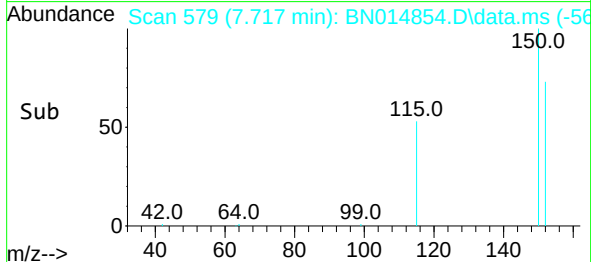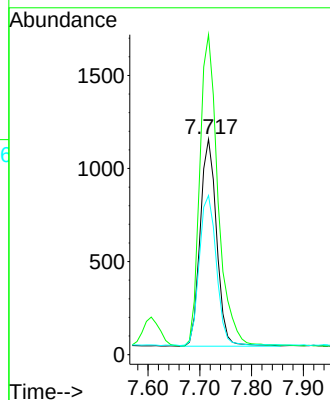

#2
 1,4-Dioxane
 Concen: 0.327 ng
 RT: 3.282 min Scan# 98
 Delta R.T. -0.000 min
 Lab File: BN014854.D
 Acq: 09 Jun 2021 15:49

Tgt Ion: 88 Resp: 234
 Ion Ratio Lower Upper
 88 100
 43 15.0 12.9 19.3
 58 52.1 38.1 57.1


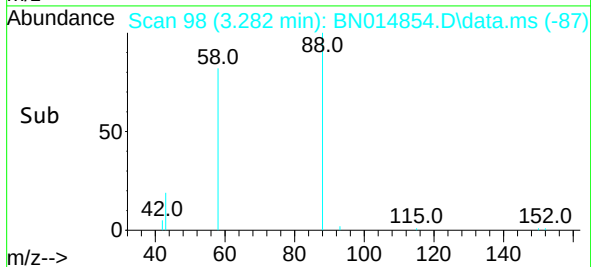
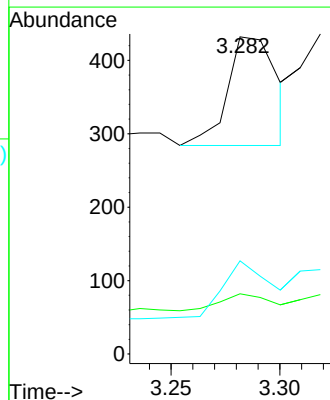
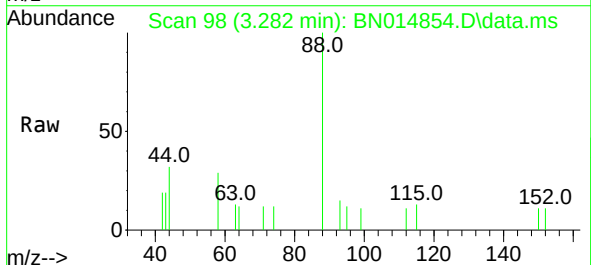


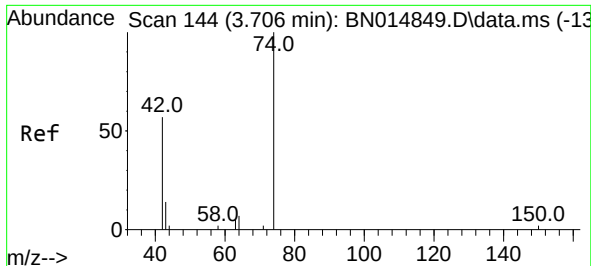

#3
n-Nitrosodimethylamine
Concen: 0.417 ng
RT: 3.706 min Scan# 144
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion: 42 Resp: 224
Ion Ratio Lower Upper
42 100
74 192.0 149.5 224.3
44 7.6 4.2 6.2#

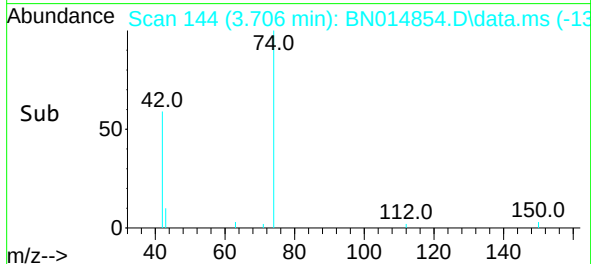

#4
2-Fluorophenol
Concen: 0.385 ng
RT: 5.329 min Scan# 320
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion: 112 Resp: 2559
Ion Ratio Lower Upper
112 100
64 47.6 39.0 58.6
63 25.6 20.6 30.8


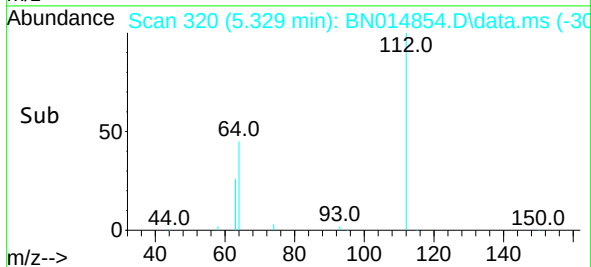

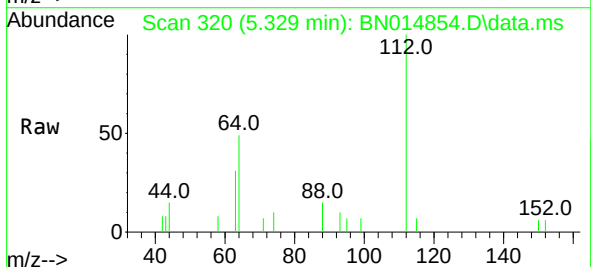


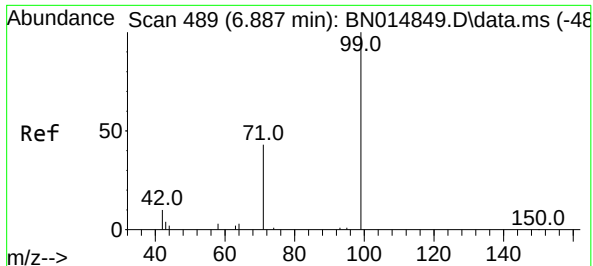

#5
Phenol-d6
Concen: 0.387 ng
RT: 6.887 min Scan# 489
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:	99	Resp:	2995
Ion	Ratio	Lower	Upper
99	100		
42	11.3	8.9	13.3
71	42.4	35.6	53.4

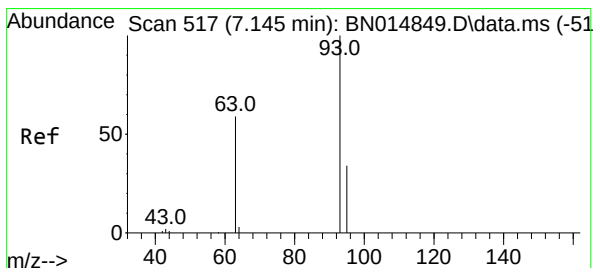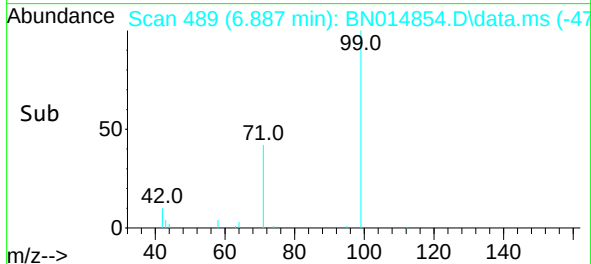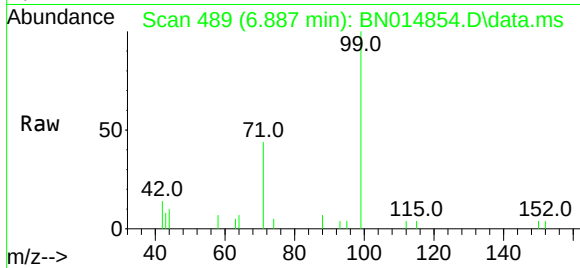

#6
bis(2-Chloroethyl)ether
Concen: 0.372 ng
RT: 7.154 min Scan# 518
Delta R.T. 0.009 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:	93	Resp:	2184
Ion	Ratio	Lower	Upper
93	100		
63	59.3	46.6	70.0
95	35.1	28.6	42.8


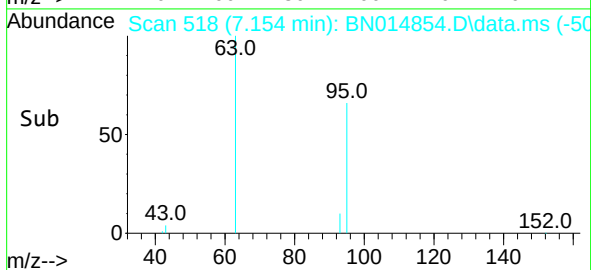

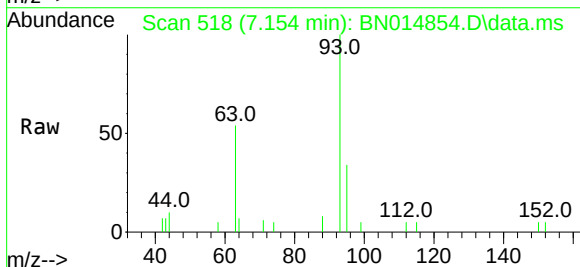


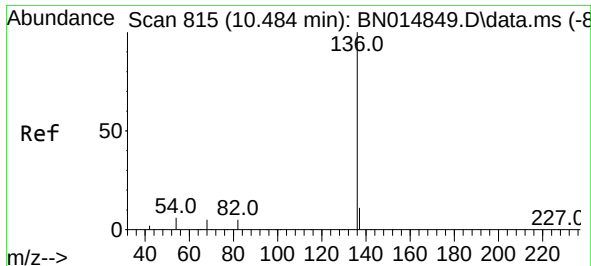

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.496 min Scan# 816
Delta R.T. 0.013 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:	136	Resp:	9973
Ion Ratio	Lower	Upper	
136	100		
137	11.6	9.8	14.8
54	4.4	5.4	8.2#
68	3.8	4.9	7.3#

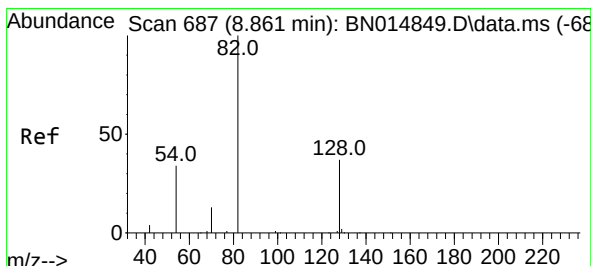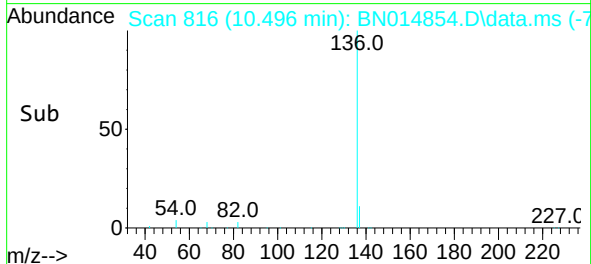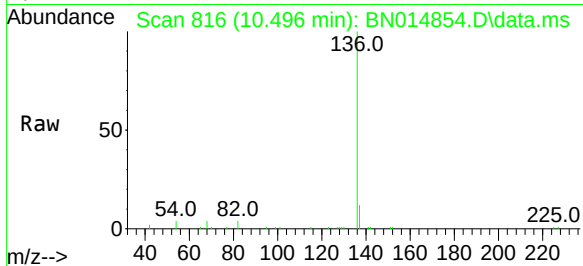

#8
Nitrobenzene-d5
Concen: 0.343 ng
RT: 8.861 min Scan# 687
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:	82	Resp:	2824
Ion Ratio	Lower	Upper	
82	100		
128	36.4	31.6	47.4
54	38.2	29.0	43.4


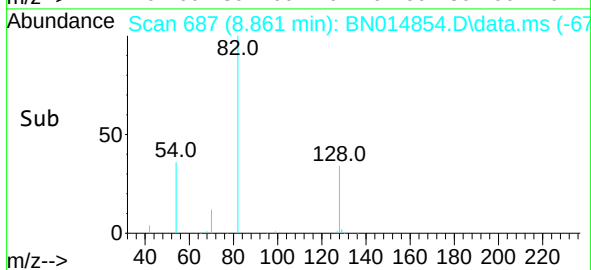

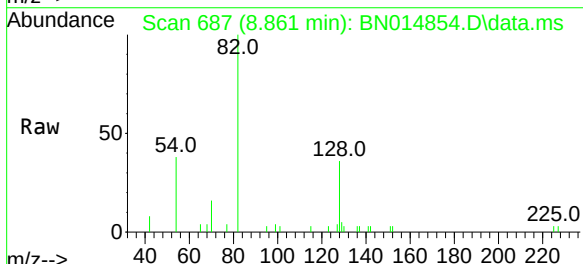


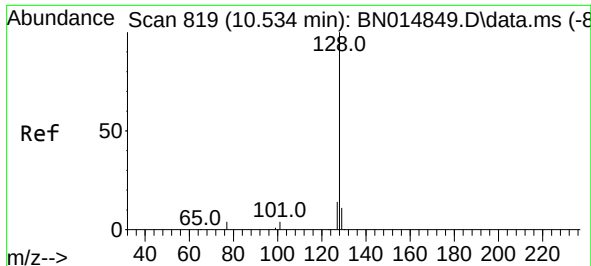

#9
Naphthalene
Concen: 0.378 ng
RT: 10.534 min Scan# 819
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:128 Resp: 10332
Ion Ratio Lower Upper
128 100
129 11.3 9.1 13.7
127 14.6 11.8 17.6

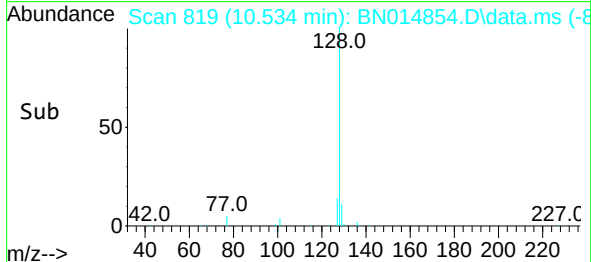

#10
Hexachlorobutadiene
Concen: 0.369 ng
RT: 10.838 min Scan# 843
Delta R.T. 0.013 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:225 Resp: 2936
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 65.4 50.2 75.2


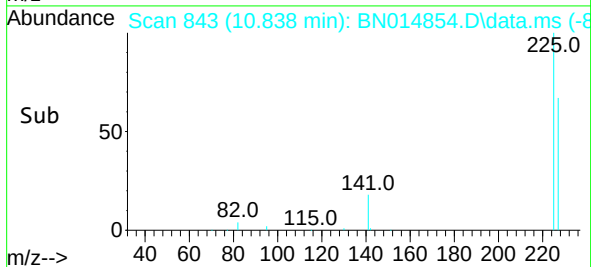

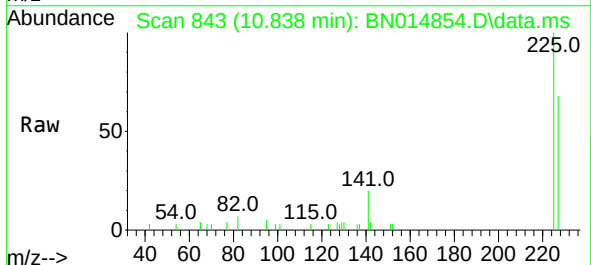


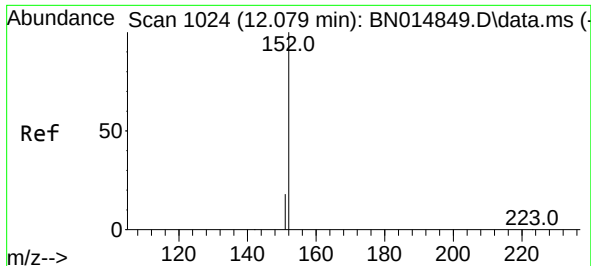

#11
2-Methylnaphthalene-d10
Concen: 0.363 ng
RT: 12.088 min Scan# 1026
Delta R.T. 0.009 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:152 Resp: 6821
Ion Ratio Lower Upper
152 100
151 21.0 16.7 25.1

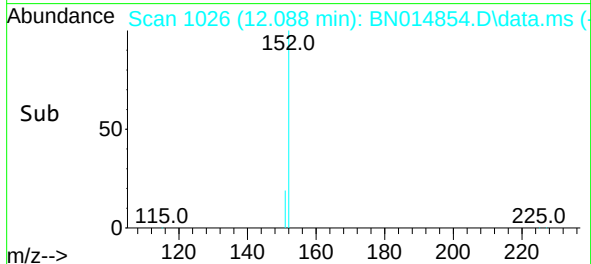

#12
2-Methylnaphthalene
Concen: 0.375 ng
RT: 12.159 min Scan# 1042
Delta R.T. 0.004 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:142 Resp: 7202
Ion Ratio Lower Upper
142 100
141 90.1 72.3 108.5
115 49.9 40.7 61.1




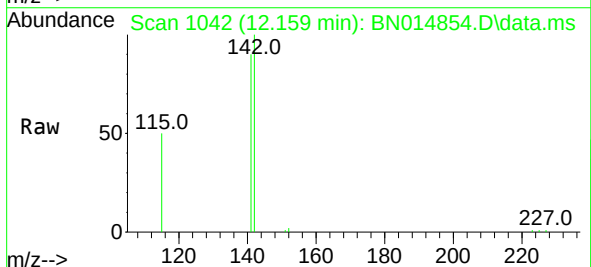


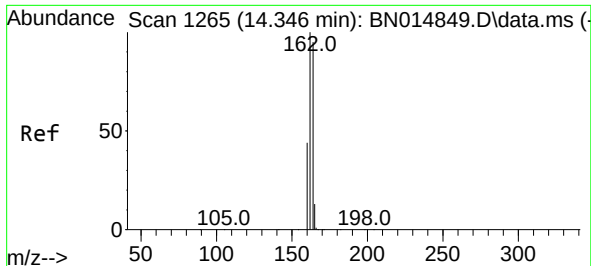

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.346 min Scan# 1265
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:164 Resp: 6558
Ion Ratio Lower Upper
164 100
162 105.3 83.8 125.6
160 48.3 37.4 56.0

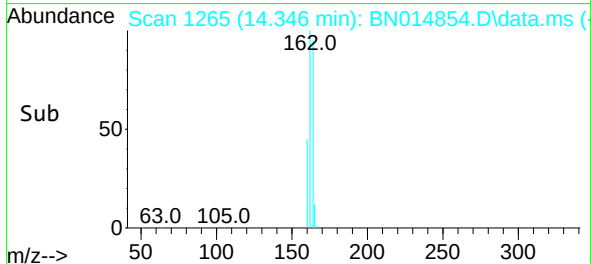

#14
2,4,6-Tribromophenol
Concen: 0.359 ng
RT: 15.855 min Scan# 1384
Delta R.T. 0.012 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:330 Resp: 989
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 28.4 22.4 33.6


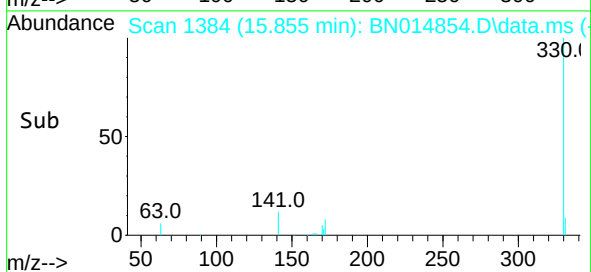

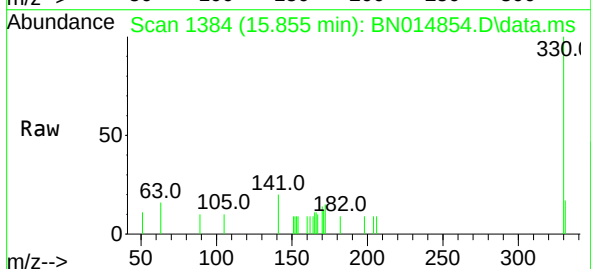


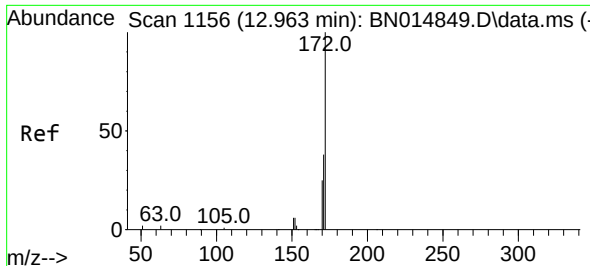

#15
2-Fluorobiphenyl
Concen: 0.382 ng
RT: 12.975 min Scan# 1157
Delta R.T. 0.013 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:	172	Resp:	9461
Ion Ratio	Lower	Upper	
172	100		
171	36.7	30.6	45.8
170	23.2	20.2	30.4

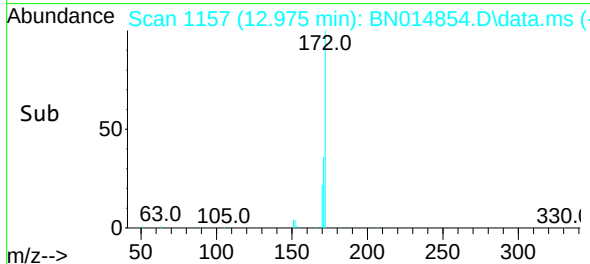

#16
Acenaphthylene
Concen: 0.371 ng
RT: 14.066 min Scan# 1243
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:	152	Resp:	10142
Ion Ratio	Lower	Upper	
152	100		
151	21.0	16.7	25.1
153	12.9	10.5	15.7


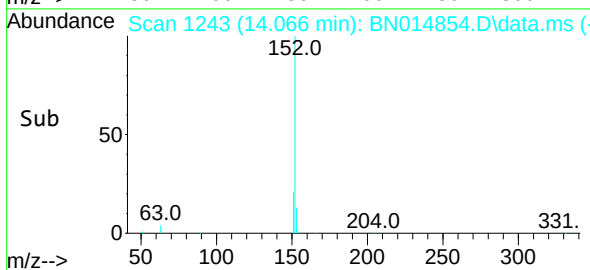

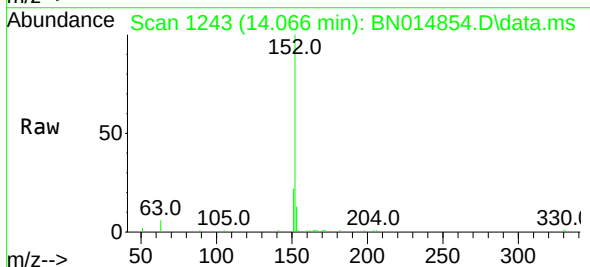


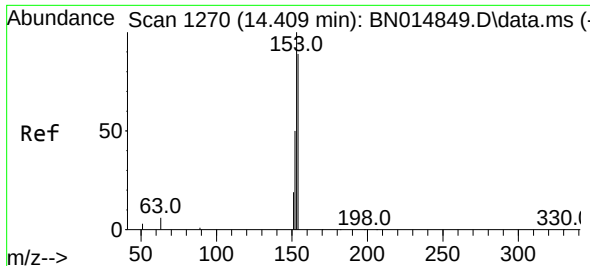

#17
Acenaphthene
Concen: 0.373 ng
RT: 14.409 min Scan# 1270
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:154 Resp: 6903
Ion Ratio Lower Upper
154 100
153 115.4 90.9 136.3
152 57.1 45.8 68.8

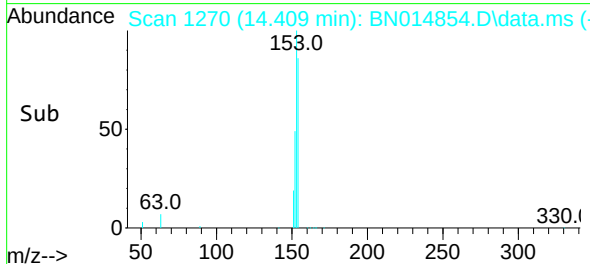

#18
Fluorene
Concen: 0.377 ng
RT: 15.399 min Scan# 1348
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:166 Resp: 8929
Ion Ratio Lower Upper
166 100
165 98.5 79.2 118.8
167 14.2 10.7 16.1


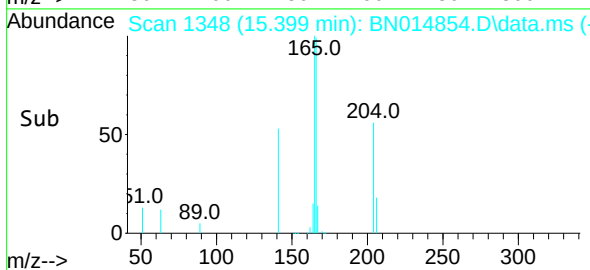

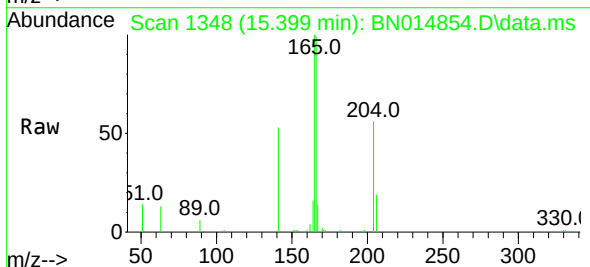




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.103 min Scan# 1486
Delta R.T. 0.012 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:188 Resp: 13852
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.2 9.0 13.4#

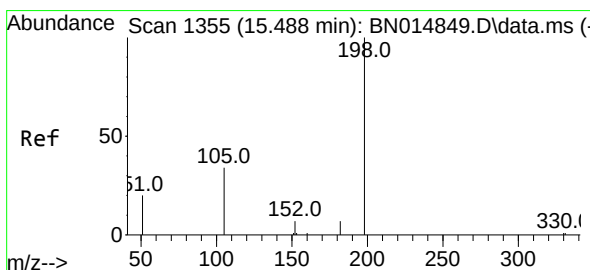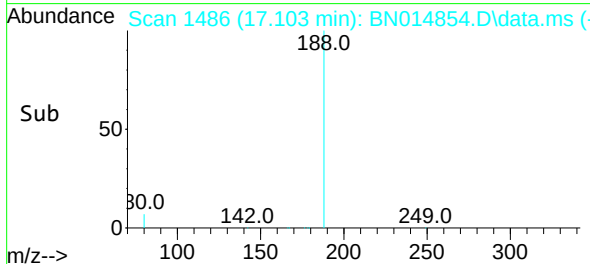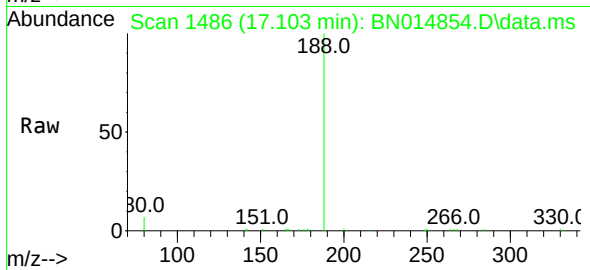

#20
4,6-Dinitro-2-methylphenol
Concen: 0.396 ng
RT: 15.487 min Scan# 1355
Delta R.T. -0.001 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:198 Resp: 176
Ion Ratio Lower Upper
198 100
182 44.7 34.5 51.7
77 0.0 0.0 0.0


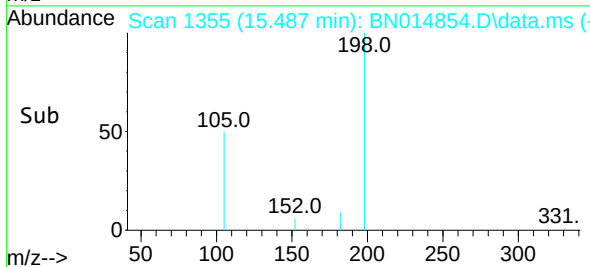

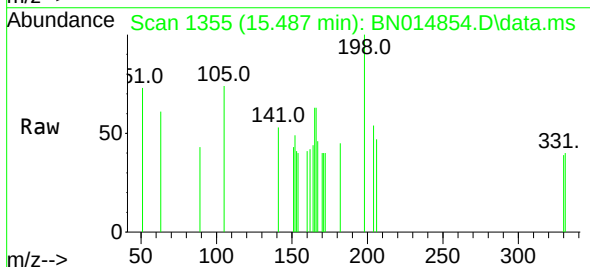


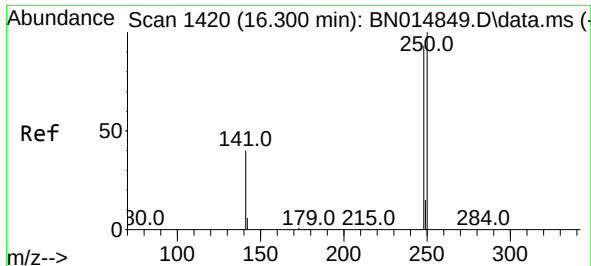

#21
4-Bromophenyl-phenylether
Concen: 0.366 ng
RT: 16.300 min Scan# 1420
Delta R.T. 0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:248 Resp: 3608
Ion Ratio Lower Upper
248 100
250 99.1 86.2 129.4
141 57.1 36.2 54.2#

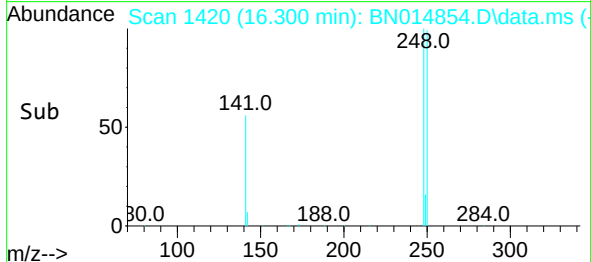

#22
Hexachlorobenzene
Concen: 0.376 ng
RT: 16.410 min Scan# 1429
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:284 Resp: 4209
Ion Ratio Lower Upper
284 100
142 27.7 22.2 33.2
249 32.2 26.6 39.8

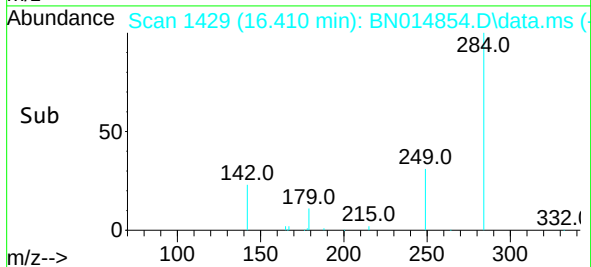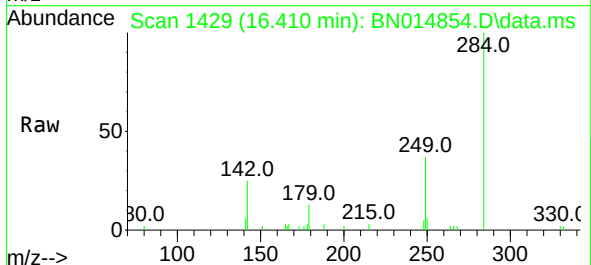

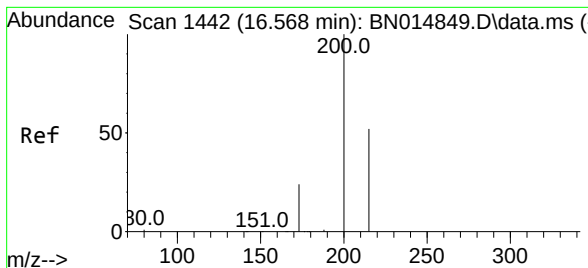

#23

Atrazine

Concen: 0.359 ng

RT: 16.568 min Scan# 1442

Delta R.T. -0.000 min

Lab File: BN014854.D

Acq: 09 Jun 2021 15:49





Tgt Ion:	200	Resp:	1920
Ion Ratio	Lower	Upper	
200	100		
173	27.7	21.7	32.5
215	50.9	43.1	64.7

Instrument :

BNA_N

ClientSampleId :

ICVBN060921

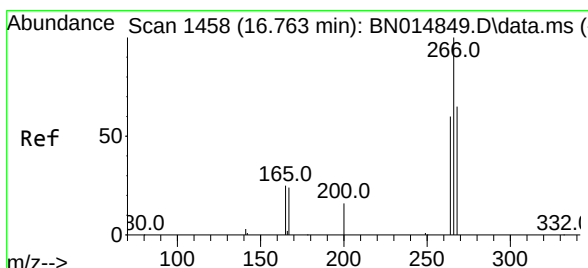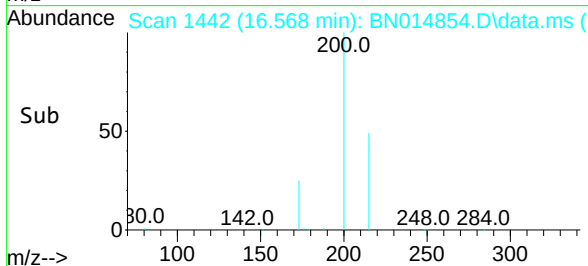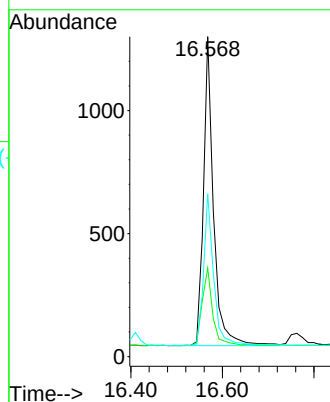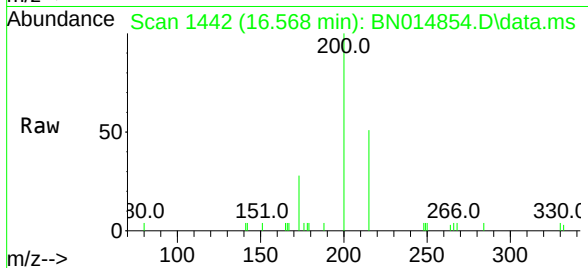

#24

Pentachlorophenol

Concen: 0.458 ng




RT: 16.763 min Scan# 1458


Delta R.T. -0.000 min

Lab File: BN014854.D

Acq: 09 Jun 2021 15:49

Tgt Ion:	266	Resp:	581
Ion Ratio	Lower	Upper	
266	100		
264	64.7	51.0	76.4
268	68.5	50.6	76.0


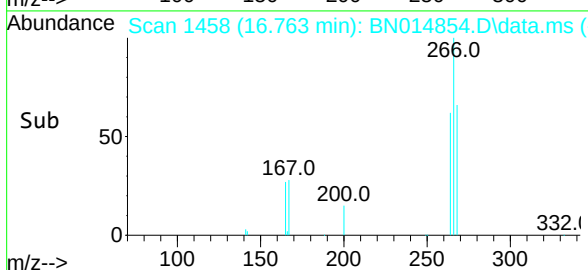
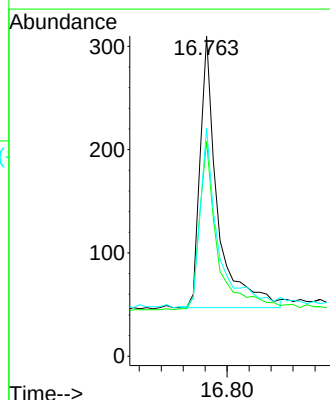
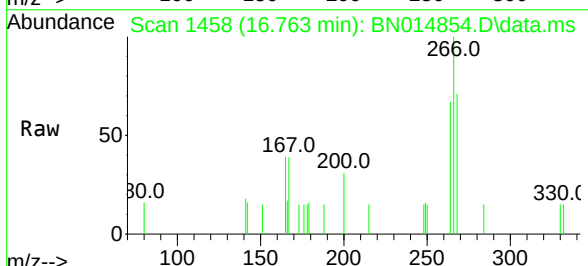


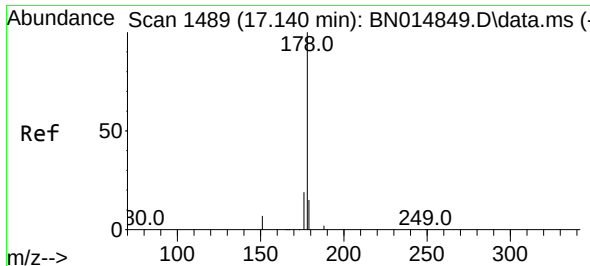

#25
Phenanthrene
Concen: 0.376 ng
RT: 17.140 min Scan# 1489
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:178 Resp: 14817
Ion Ratio Lower Upper
178 100
176 19.3 15.6 23.4
179 15.3 12.1 18.1

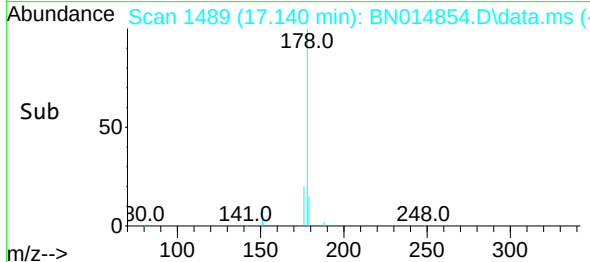

#26
Anthracene
Concen: 0.360 ng
RT: 17.237 min Scan# 1497
Delta R.T. 0.012 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:178 Resp: 12533
Ion Ratio Lower Upper
178 100
176 19.0 15.1 22.7
179 15.4 12.2 18.2


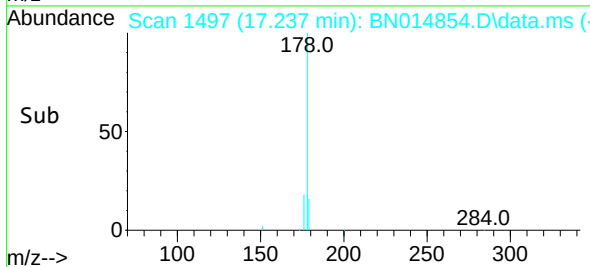

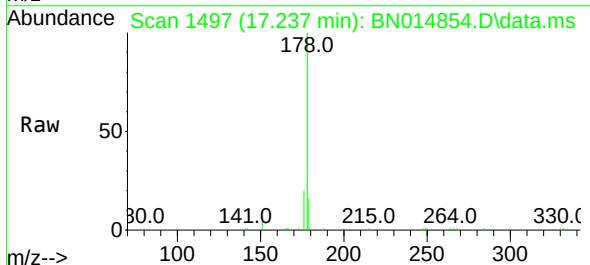




#27
Fluoranthene-d10
Concen: 0.350 ng
RT: 19.143 min Scan# 1788
Delta R.T. 0.005 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:212 Resp: 16725
Ion Ratio Lower Upper
212 100
106 9.1 7.0 10.6
104 5.2 4.1 6.1

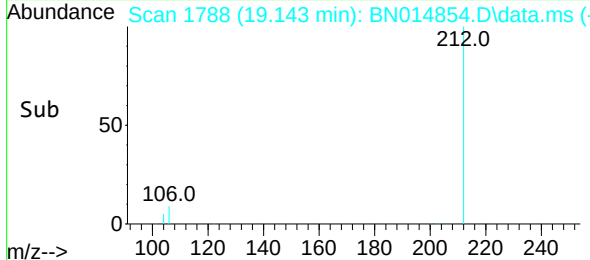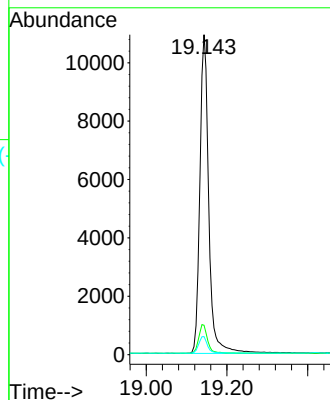

#28
Fluoranthene
Concen: 0.371 ng
RT: 19.173 min Scan# 1794
Delta R.T. 0.005 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:202 Resp: 18465
Ion Ratio Lower Upper
202 100
101 8.4 6.6 10.0
203 17.3 13.9 20.9


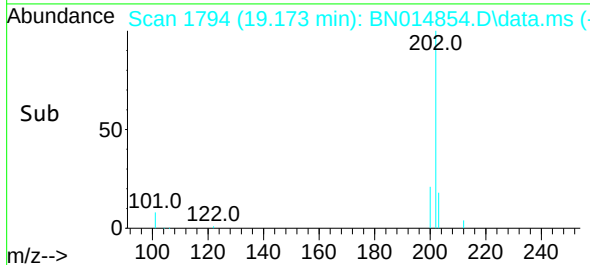
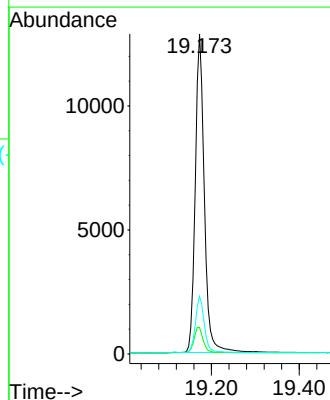
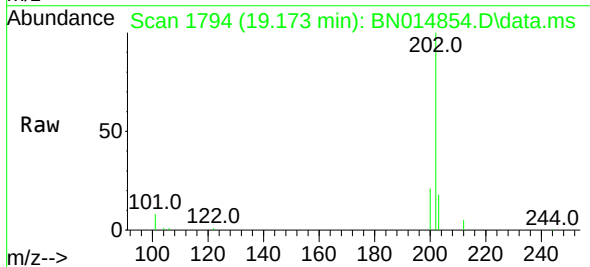


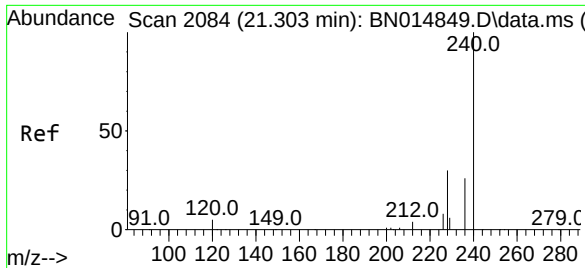

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.313 min Scan# 2085
Delta R.T. 0.010 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:240 Resp: 16454
Ion Ratio Lower Upper
240 100
120 4.2 4.2 6.4#
236 25.9 21.4 32.2

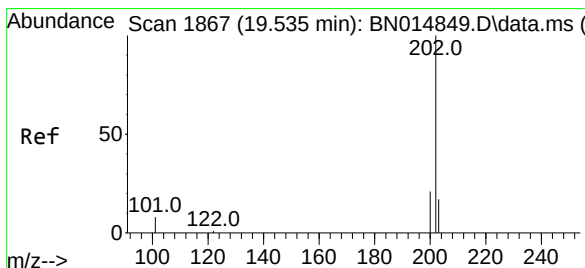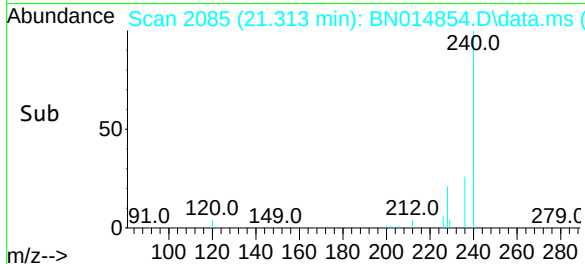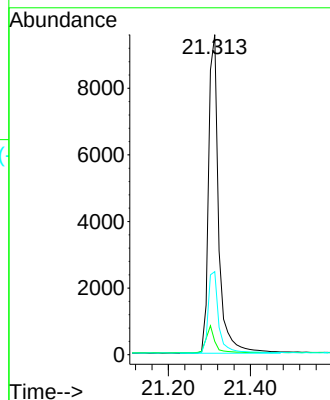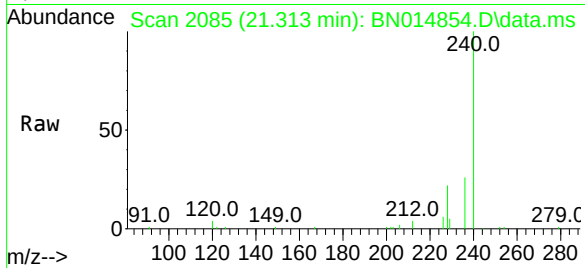

#30
Pyrene
Concen: 0.375 ng
RT: 19.535 min Scan# 1867
Delta R.T. -0.000 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49


Tgt Ion:202 Resp: 18389
Ion Ratio Lower Upper
202 100
200 21.1 16.9 25.3
203 17.6 13.9 20.9

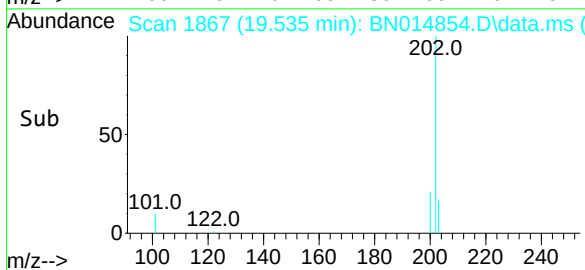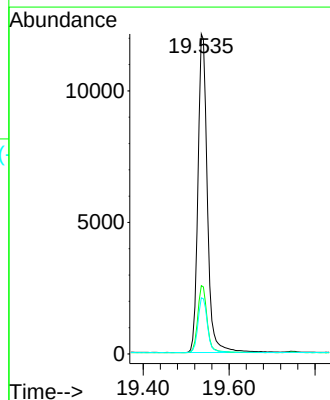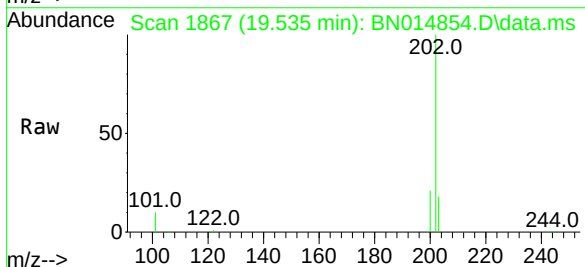






#31
Terphenyl-d14
Concen: 0.372 ng
RT: 19.749 min Scan# 1910
Delta R.T. 0.005 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Instrument :
BNA_N
ClientSampleId :
ICVBN060921



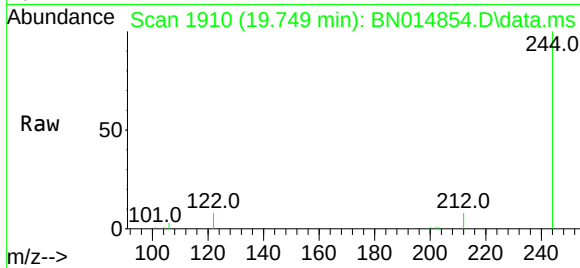



Tgt Ion:244 Resp: 15153
Ion Ratio Lower Upper
244 100
212 7.9 6.3 9.5
122 7.6 6.2 9.2

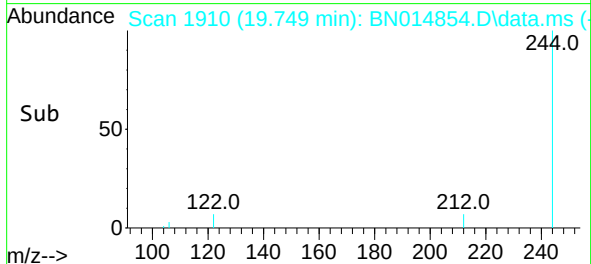

#32
Benzo(a)anthracene
Concen: 0.368 ng
RT: 21.292 min Scan# 2083
Delta R.T. 0.010 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:228 Resp: 17234
Ion Ratio Lower Upper
228 100
226 27.5 23.0 34.6
229 19.5 15.7 23.5

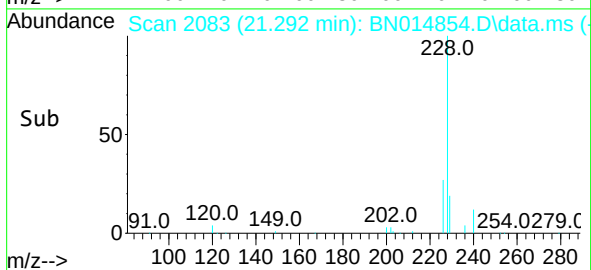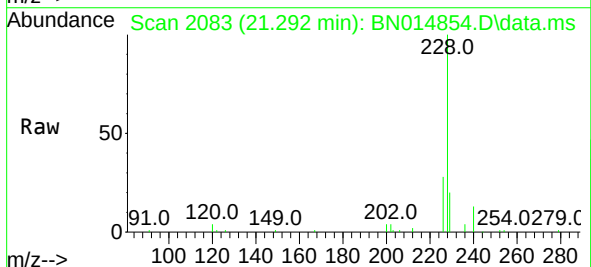

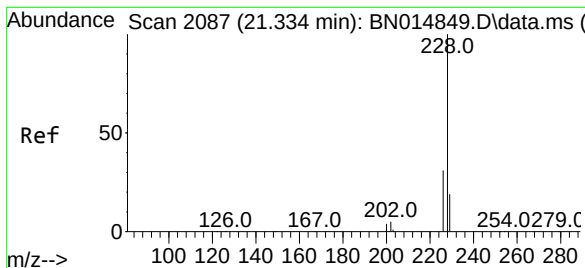

#33

Chrysene

Concen: 0.363 ng

RT: 21.345 min Scan# 2088

Delta R.T. 0.010 min

Lab File: BN014854.D

Acq: 09 Jun 2021 15:49





Tgt Ion:228 Resp: 19938

Ion Ratio Lower Upper

228 100

226 30.2 25.0 37.6

229 19.8 15.9 23.9

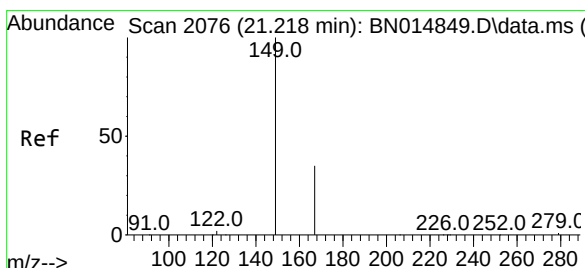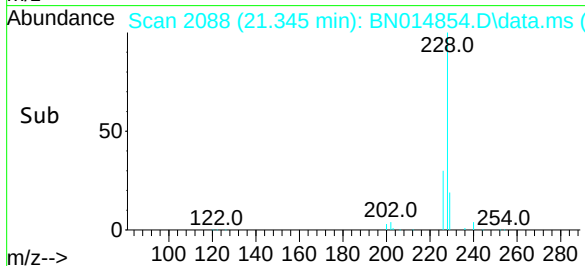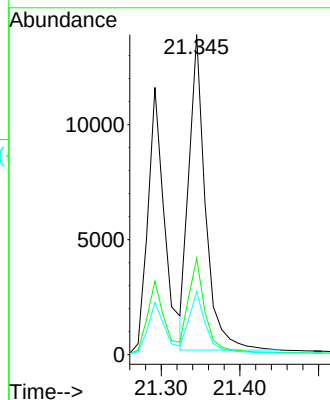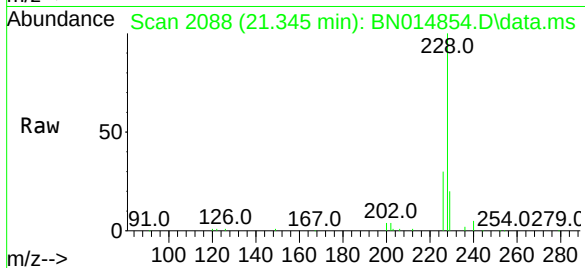

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.335 ng

RT: 21.228 min Scan# 2077

Delta R.T. 0.010 min

Lab File: BN014854.D

Acq: 09 Jun 2021 15:49




Tgt Ion:149 Resp: 4837


Ion Ratio Lower Upper

149 100

167 36.1 28.9 43.3


279 6.4 4.9 7.3

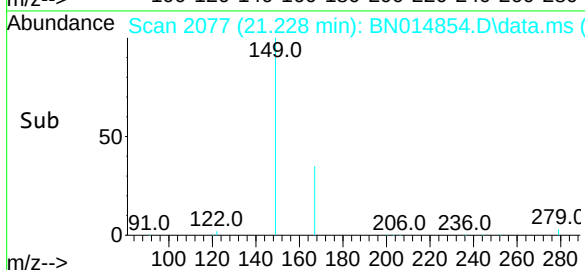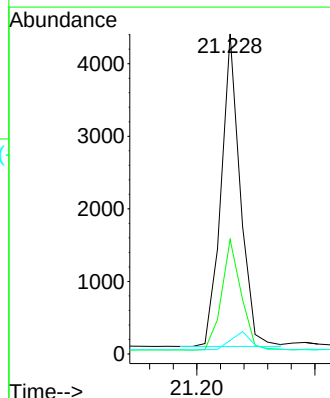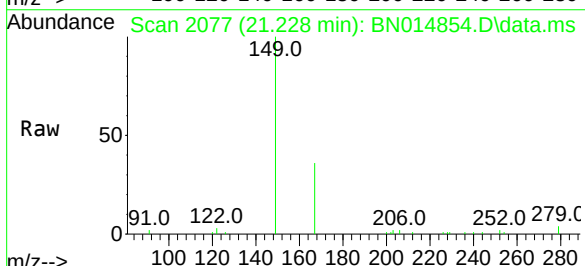






#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.571 min Scan# 2528
 Delta R.T. 0.010 min
 Lab File: BN014854.D
 Acq: 09 Jun 2021 15:49

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN060921

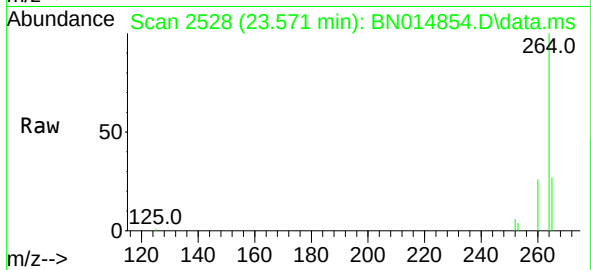

Tgt Ion:264 Resp: 15547




Ion	Ratio	Lower	Upper
264	100		
260	25.6	20.6	31.0
265	26.7	21.4	32.2

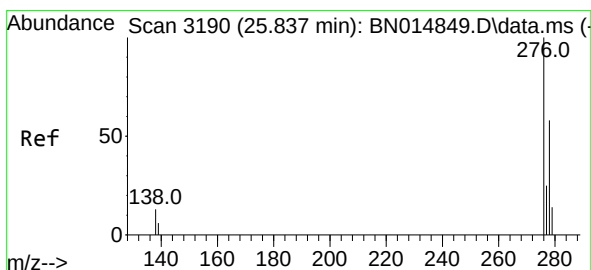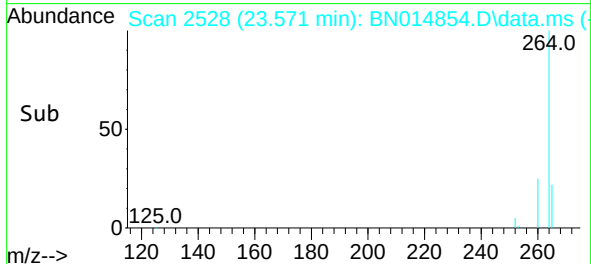


#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.352 ng
 RT: 25.850 min Scan# 3194
 Delta R.T. 0.013 min
 Lab File: BN014854.D
 Acq: 09 Jun 2021 15:49

Tgt Ion:276 Resp: 15311

Ion	Ratio	Lower	Upper
276	100		
138	13.1	10.0	15.0
277	25.8	20.4	30.6


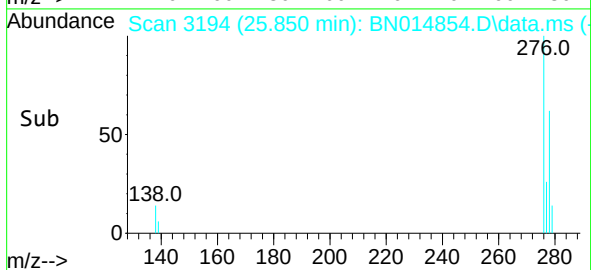

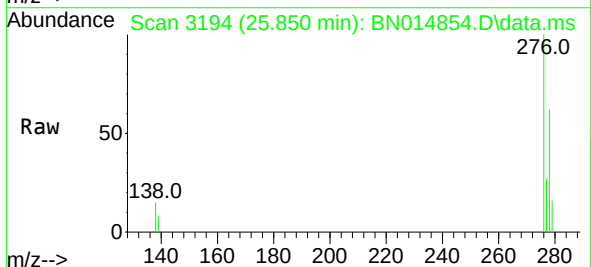


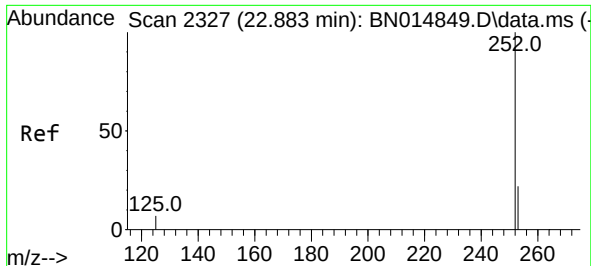

#37
Benzo(b)fluoranthene
Concen: 0.351 ng
RT: 22.890 min Scan# 2329
Delta R.T. 0.007 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:252 Resp: 17422
Ion Ratio Lower Upper
252 100
253 23.2 18.5 27.7
125 7.3 5.8 8.6

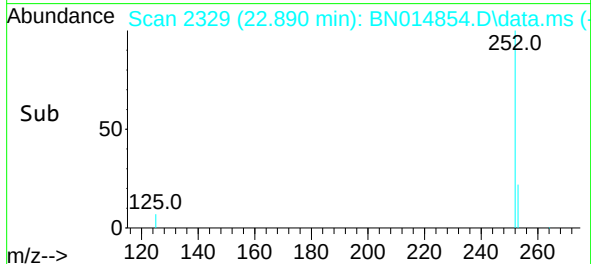

#38
Benzo(k)fluoranthene
Concen: 0.381 ng
RT: 22.934 min Scan# 2342
Delta R.T. 0.007 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:252 Resp: 22489
Ion Ratio Lower Upper
252 100
253 23.3 19.1 28.7
125 6.7 5.4 8.0


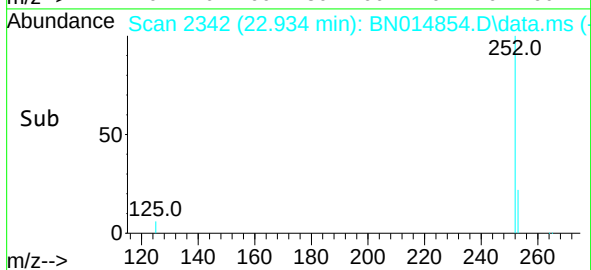

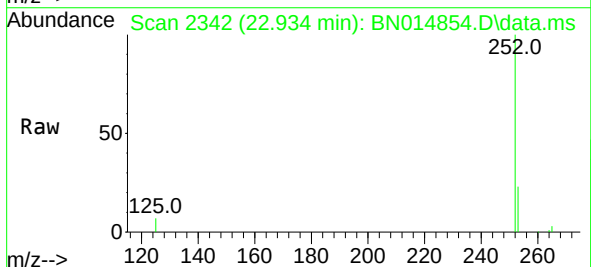




#39
Benzo(a)pyrene
Concen: 0.370 ng
RT: 23.471 min Scan# 2499
Delta R.T. 0.010 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49




Instrument :
BNA_N
ClientSampleId :
ICVBN060921


Tgt Ion:252	Resp:	17390
Ion Ratio	Lower	Upper
252	100	
253	24.7	19.4 29.2
125	9.8	7.4 11.2

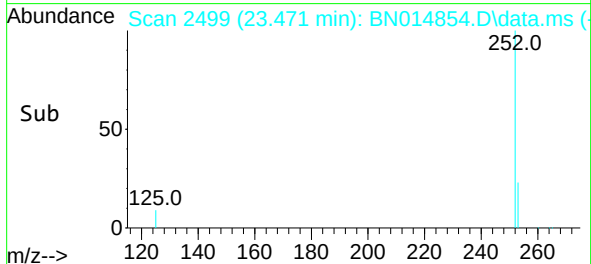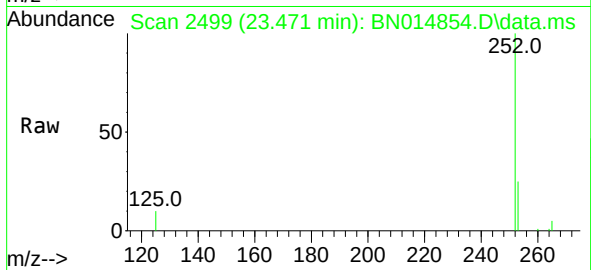

#40
Dibenzo(a,h)anthracene
Concen: 0.359 ng
RT: 25.861 min Scan# 3197
Delta R.T. 0.010 min
Lab File: BN014854.D
Acq: 09 Jun 2021 15:49

Tgt Ion:278	Resp:	11435
Ion Ratio	Lower	Upper
278	100	
139	11.7	9.0 13.4
279	25.3	21.0 31.4

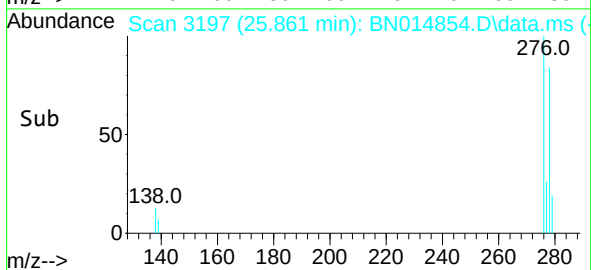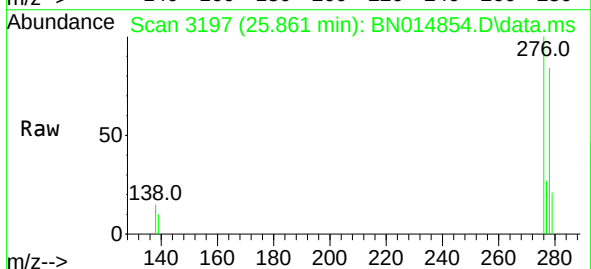

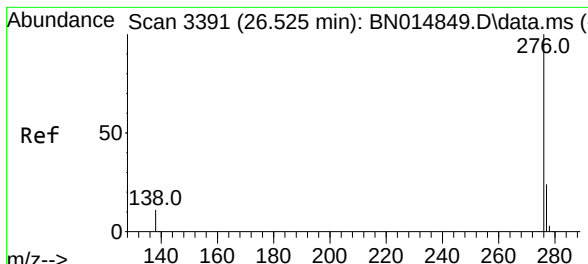

#41
 Benzo(g,h,i)perylene
 Concen: 0.345 ng
 RT: 26.538 min Scan# 3395
 Delta R.T. 0.014 min
 Lab File: BN014854.D
 Acq: 09 Jun 2021 15:49

Instrument :
 BNA_N
ClientSampleId :
 ICVBN060921

Tgt Ion:	276	Resp:	15576
Ion Ratio	Lower	Upper	
276	100		
277	24.6	19.7	29.5
138	12.7	9.8	14.6

