
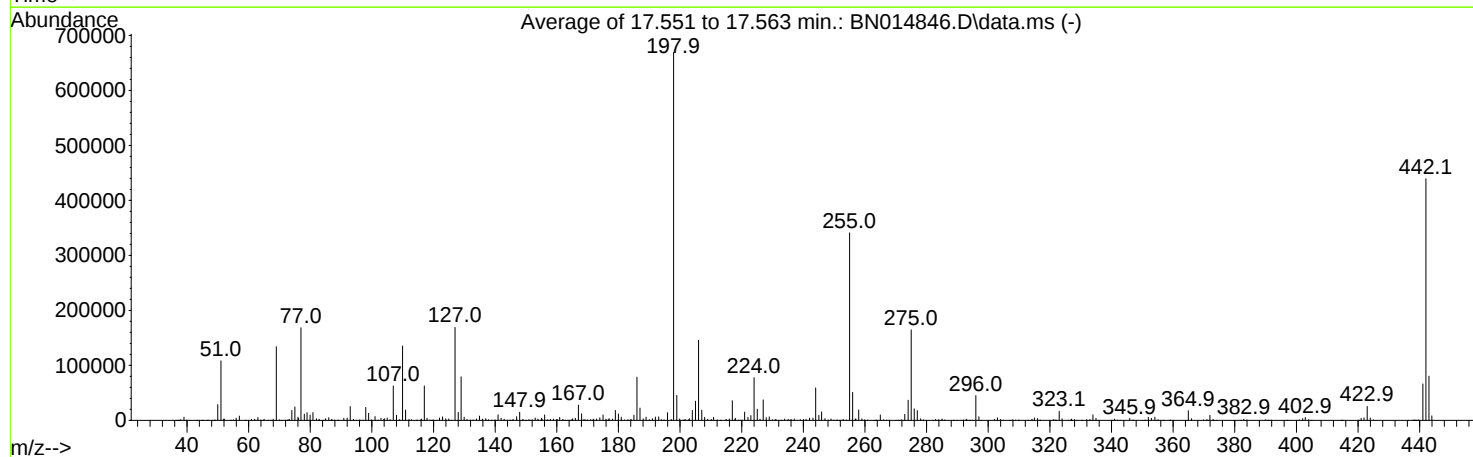


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060921\
 Data File : BN014846.D
 Acq On : 09 Jun 2021 10:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN060921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 09 16:35:36 2021

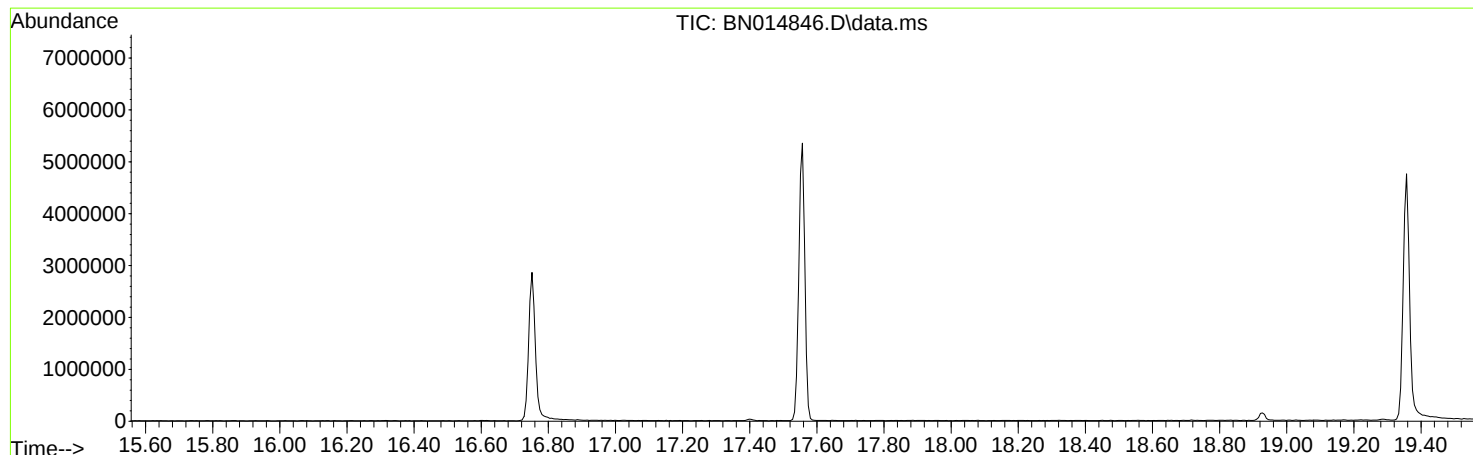

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	16.2	108187	PASS
68	69	0.00	2	1.4	1930	PASS
69	198	0.00	100	20.0	133763	PASS
70	69	0.00	2	0.7	888	PASS
127	198	10	80	25.3	169136	PASS
197	198	0.00	2	0.3	1769	PASS
198	198	100	100	100.0	668971	PASS
199	198	5	9	6.8	45320	PASS
275	198	10	60	24.6	164741	PASS
365	198	1	100	2.6	17495	PASS
441	198	0.01	100	9.9	66325	PASS
442	442	50	100	100.0	439296	PASS
443	442	15	24	18.3	80448	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/9/2021	BNA_N	<u>BN014846.D</u>
Compound Name	Response	Retention Time
DDT	1568202	20.598
DDD	16270	20.157
DDE	4774	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21044	1589246	1.32

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060921\
Data File : BN014846.D
Acq On : 09 Jun 2021 10:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 16:13:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

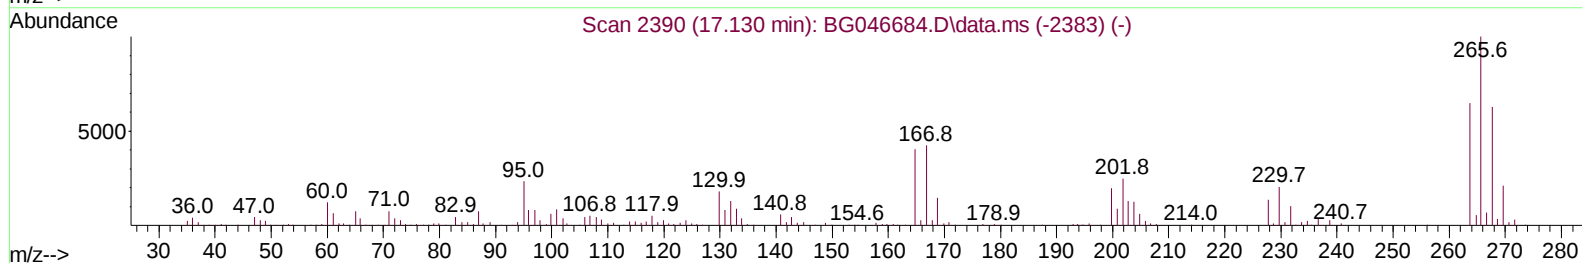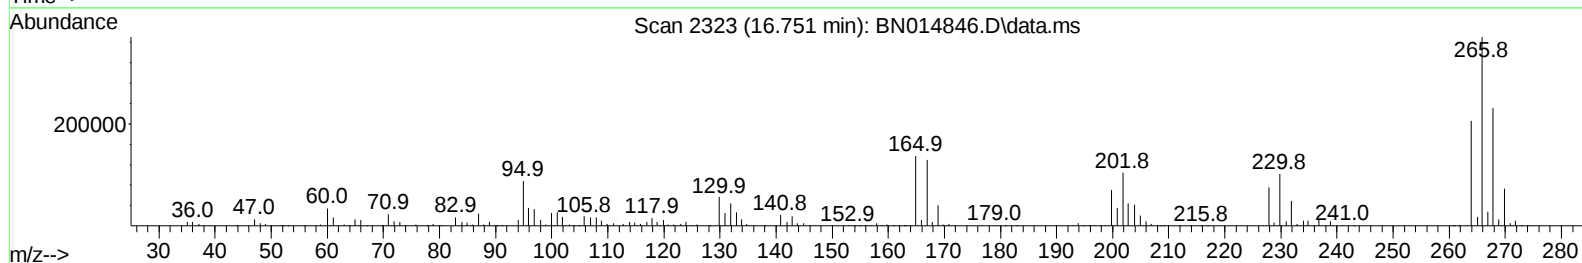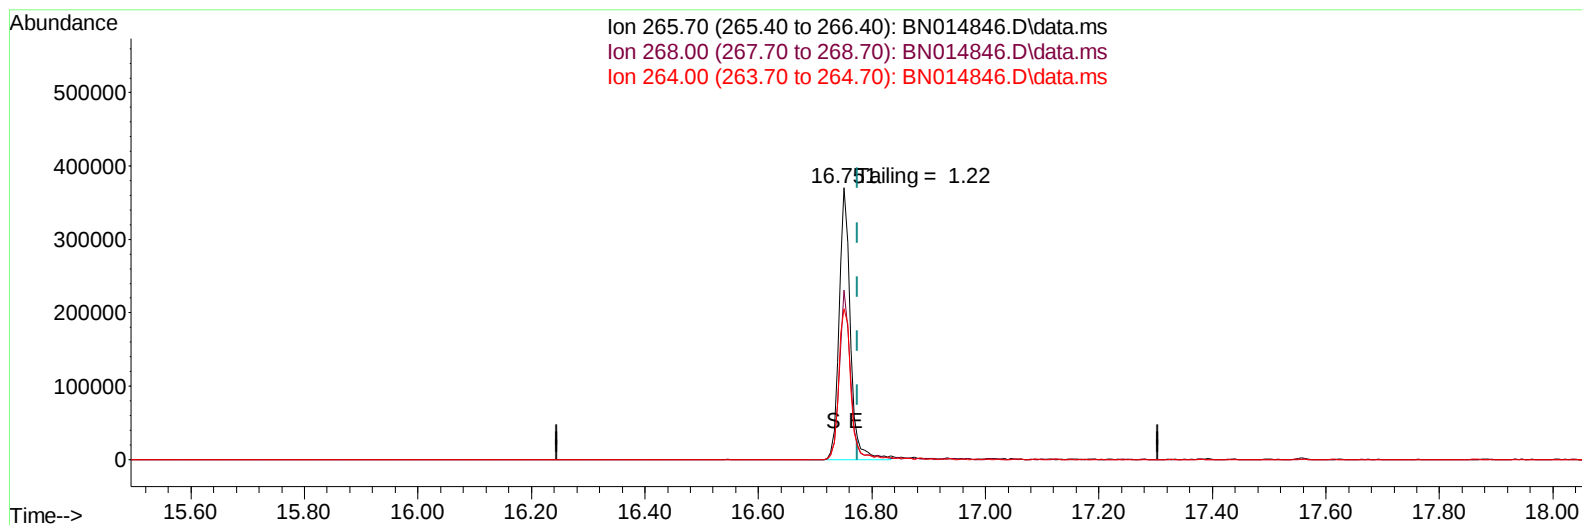

TIC: BN014846.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.023) 16056.50 ng




response 497729

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.27
264.00	61.60	55.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060921\
Data File : BN014846.D
Acq On : 09 Jun 2021 10:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 09 16:13:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 22 07:55:10 2021
Response via : Initial Calibration

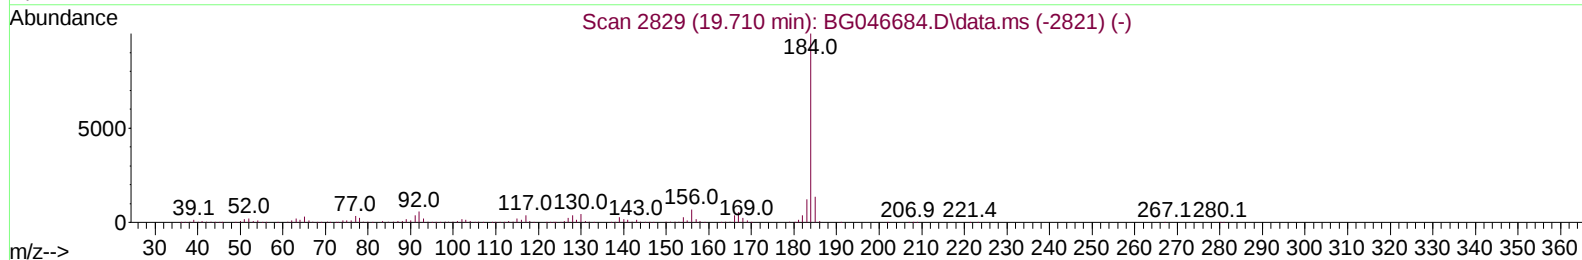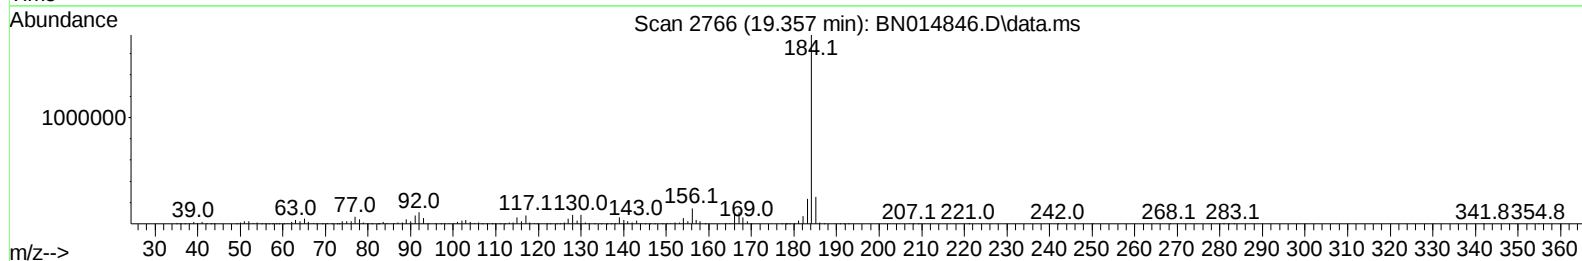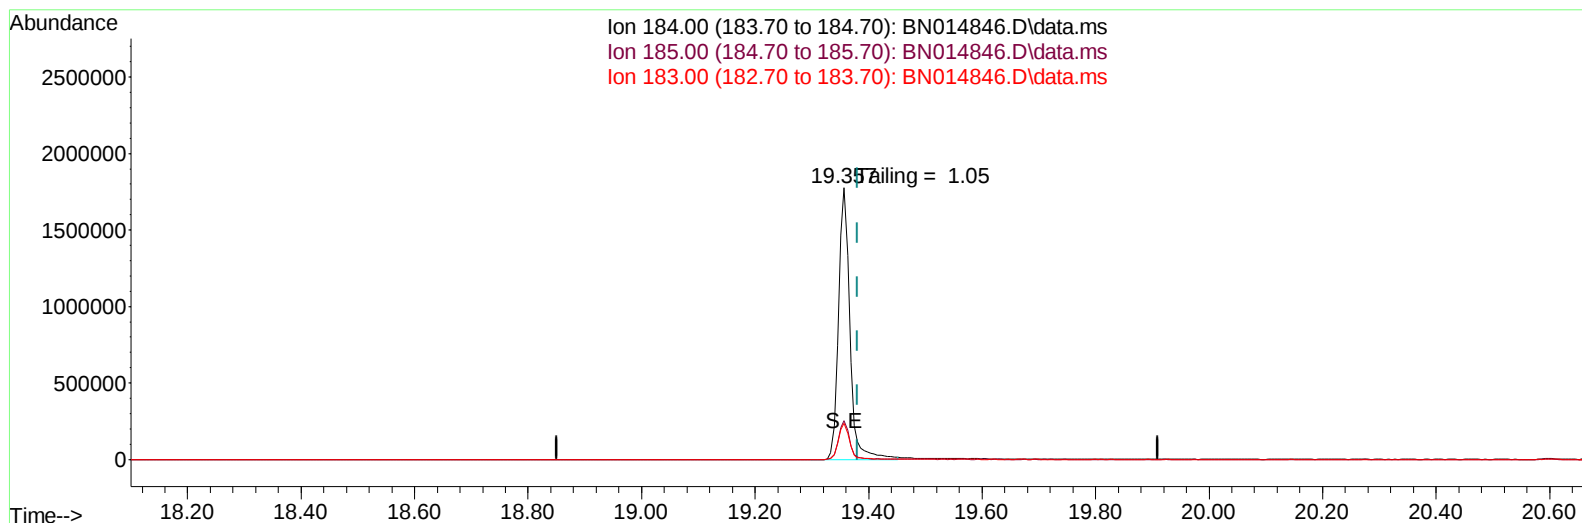

TIC: BN014846.D\data.ms

(77) Benzidine

19.357min (-0.023) 0.00 ng

response 2484208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.37
183.00	13.20	13.33
0.00	0.00	0.00