

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020075.D
 Acq On : 09 Jun 2022 11:44
 Operator : CG/JU
 Sample : N3212-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A54

Quant Time: Jun 10 01:04:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	138165	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	645792	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	429962	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	910287	20.000	ng/u1	0.00
79) Chrysene-d12	21.375	240	867746	20.000	ng/u1	0.00
88) Perylene-d12	23.704	264	791208	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	16130	5.056	ng/uL	0.00
4) Pyridine-d5	3.693	84	97742	11.210	ng/u1	0.00
7) Phenol-d5	6.987	99	73565	6.435	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	213977	29.956	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	198811	21.402	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	144142	14.573	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	145439	29.603	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	137410	26.354	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	223171	24.518	ng/u1	0.00
31) 4-Chloroaniline-d4	10.740	131	406304	27.564	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	1031215	32.962	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1112611	30.667	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	35306	5.632	ng/u1	0.00
60) Fluorene-d10	15.440	176	862489	33.316	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	117105	22.209	ng/u1	0.00
73) Anthracene-d10	17.287	188	1438926	36.220	ng/u1	0.00
81) Pyrene-d10	19.580	212	1666465	35.425	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.563	264	1440404	37.208	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.317	88	16951	5.034	ng/uL 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020075.D
Acq On : 09 Jun 2022 11:44
Operator : CG/JU
Sample : N3212-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A54

Quant Time: Jun 10 01:04:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

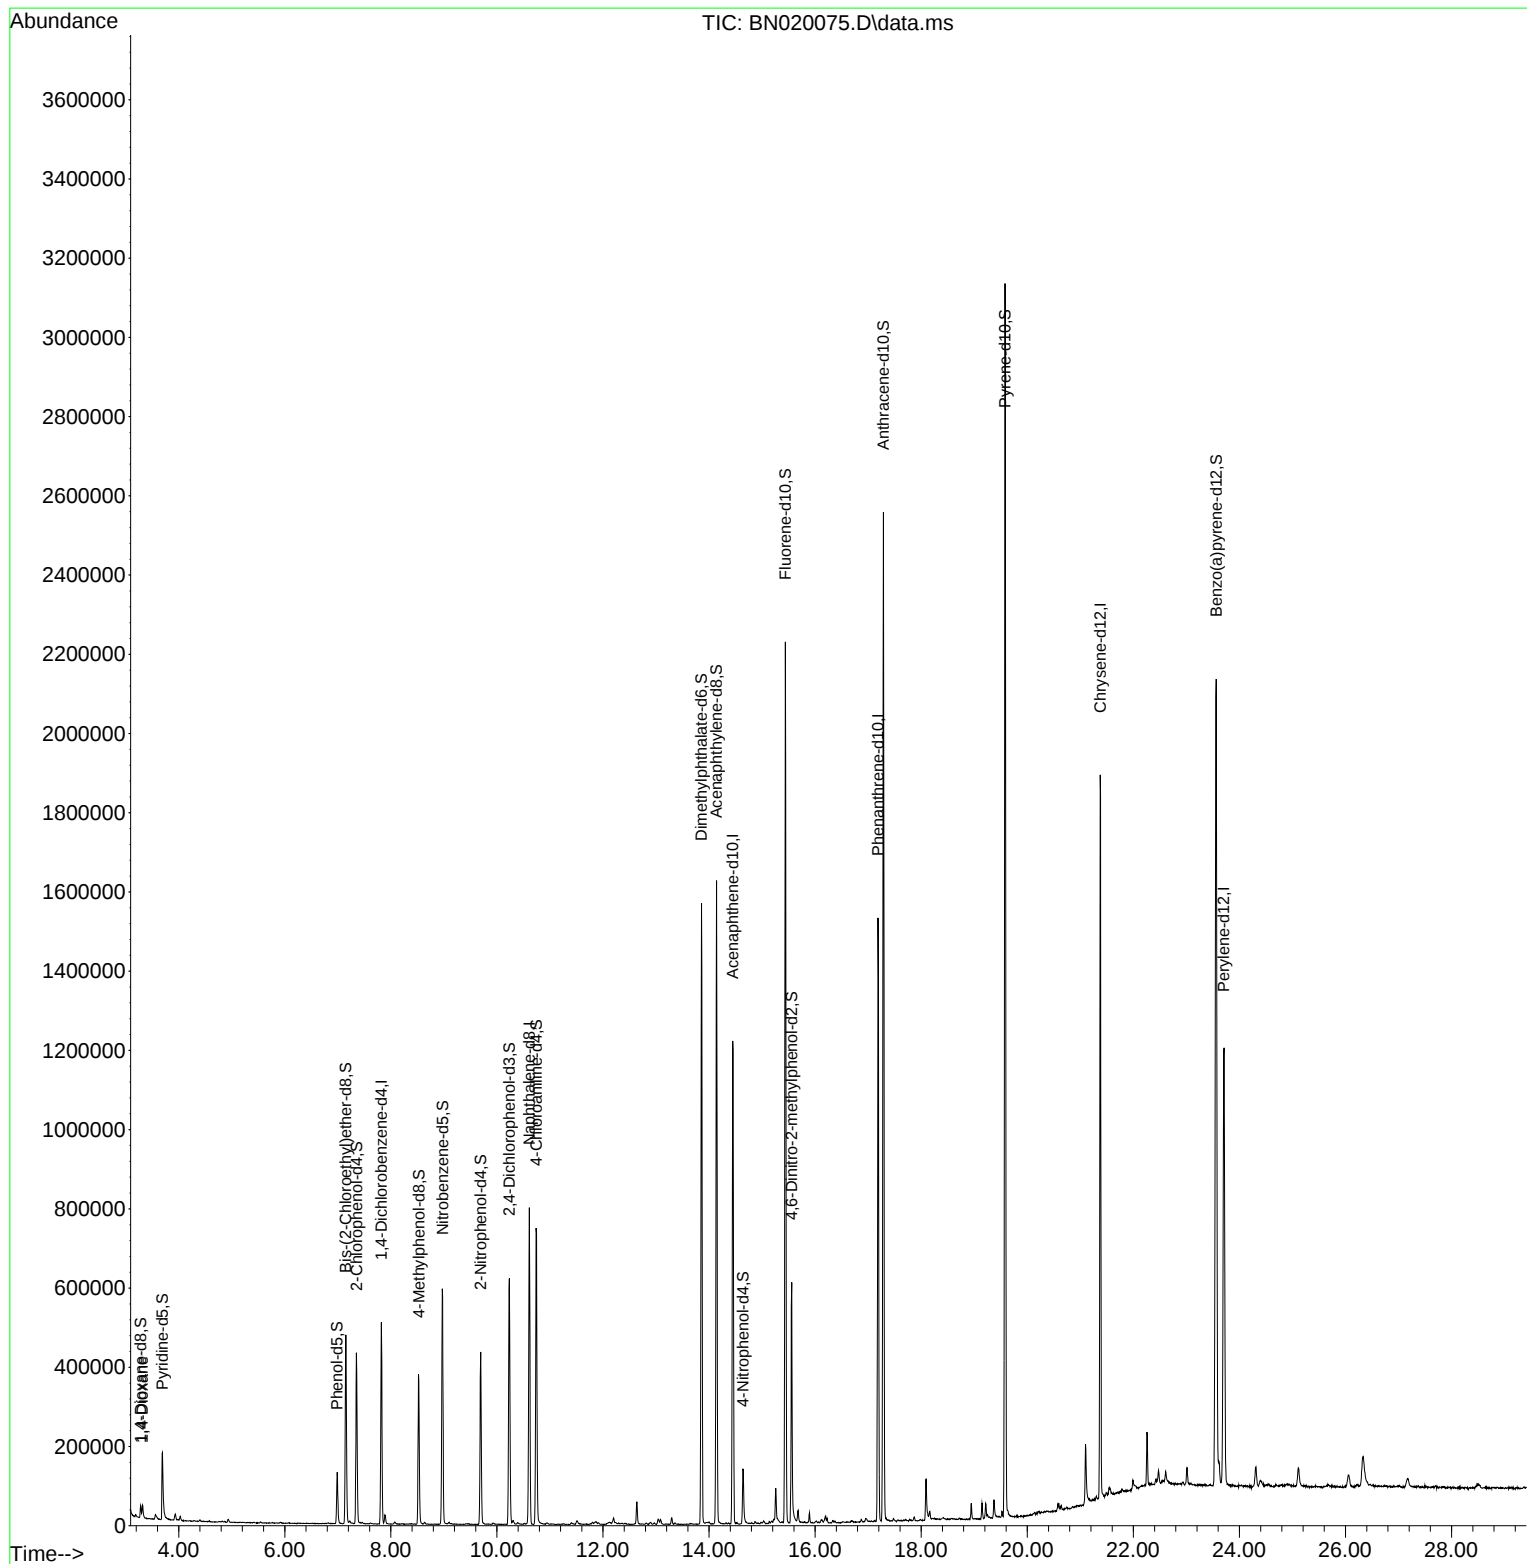

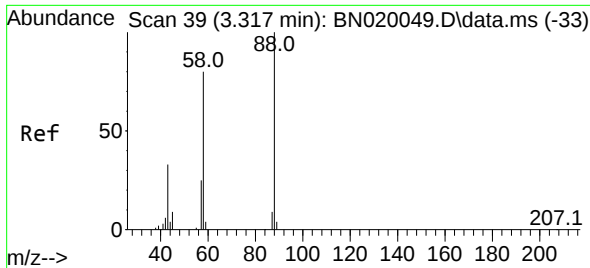

#2
 1,4-Dioxane
 Concen: 5.034 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020075.D
 Acq: 09 Jun 2022 11:44

Instrument :
 BNA_N
 ClientSampleId :
 F5A54

Tgt Ion:	88	Resp:	16951
Ion	Ratio	Lower	Upper
88	100		
43	32.2	22.4	33.6
58	80.5	61.0	91.4

