

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020076.D
 Acq On : 09 Jun 2022 12:21
 Operator : CG/JU
 Sample : N3212-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A53

Quant Time: Jun 10 01:04:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	154214	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	720191	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	462936	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.186	188	943341	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	843756	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	750861	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	17091	4.800	ng/uL	0.00
4) Pyridine-d5	3.693	84	114080	11.723	ng/u1	0.00
7) Phenol-d5	6.987	99	113444	8.890	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	255908	32.098	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	291540	28.118	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	230676	20.894	ng/u1	0.00
21) Nitrobenzene-d5	8.975	128	181944	33.207	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	191318	32.902	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	351311	34.608	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	276650	16.829	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1298806	38.559	ng/u1	0.00
49) Acenaphthylene-d8	14.139	160	1407890	36.041	ng/u1	0.00
54) 4-Nitrophenol-d4	14.663	143	62868	9.314	ng/u1	0.02
60) Fluorene-d10	15.439	176	1034824	37.126	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	180764	33.080	ng/u1	0.00
73) Anthracene-d10	17.292	188	1605895	39.007	ng/u1	0.00
81) Pyrene-d10	19.586	212	1789520	39.122	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.562	264	1458631	39.704	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.316	88	115783	30.804	ng/uL	93
14) 2,2'-oxybis(1-Chloropr...	8.351	45	31427	1.884	ng/u1#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020076.D
Acq On : 09 Jun 2022 12:21
Operator : CG/JU
Sample : N3212-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A53

Quant Time: Jun 10 01:04:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration




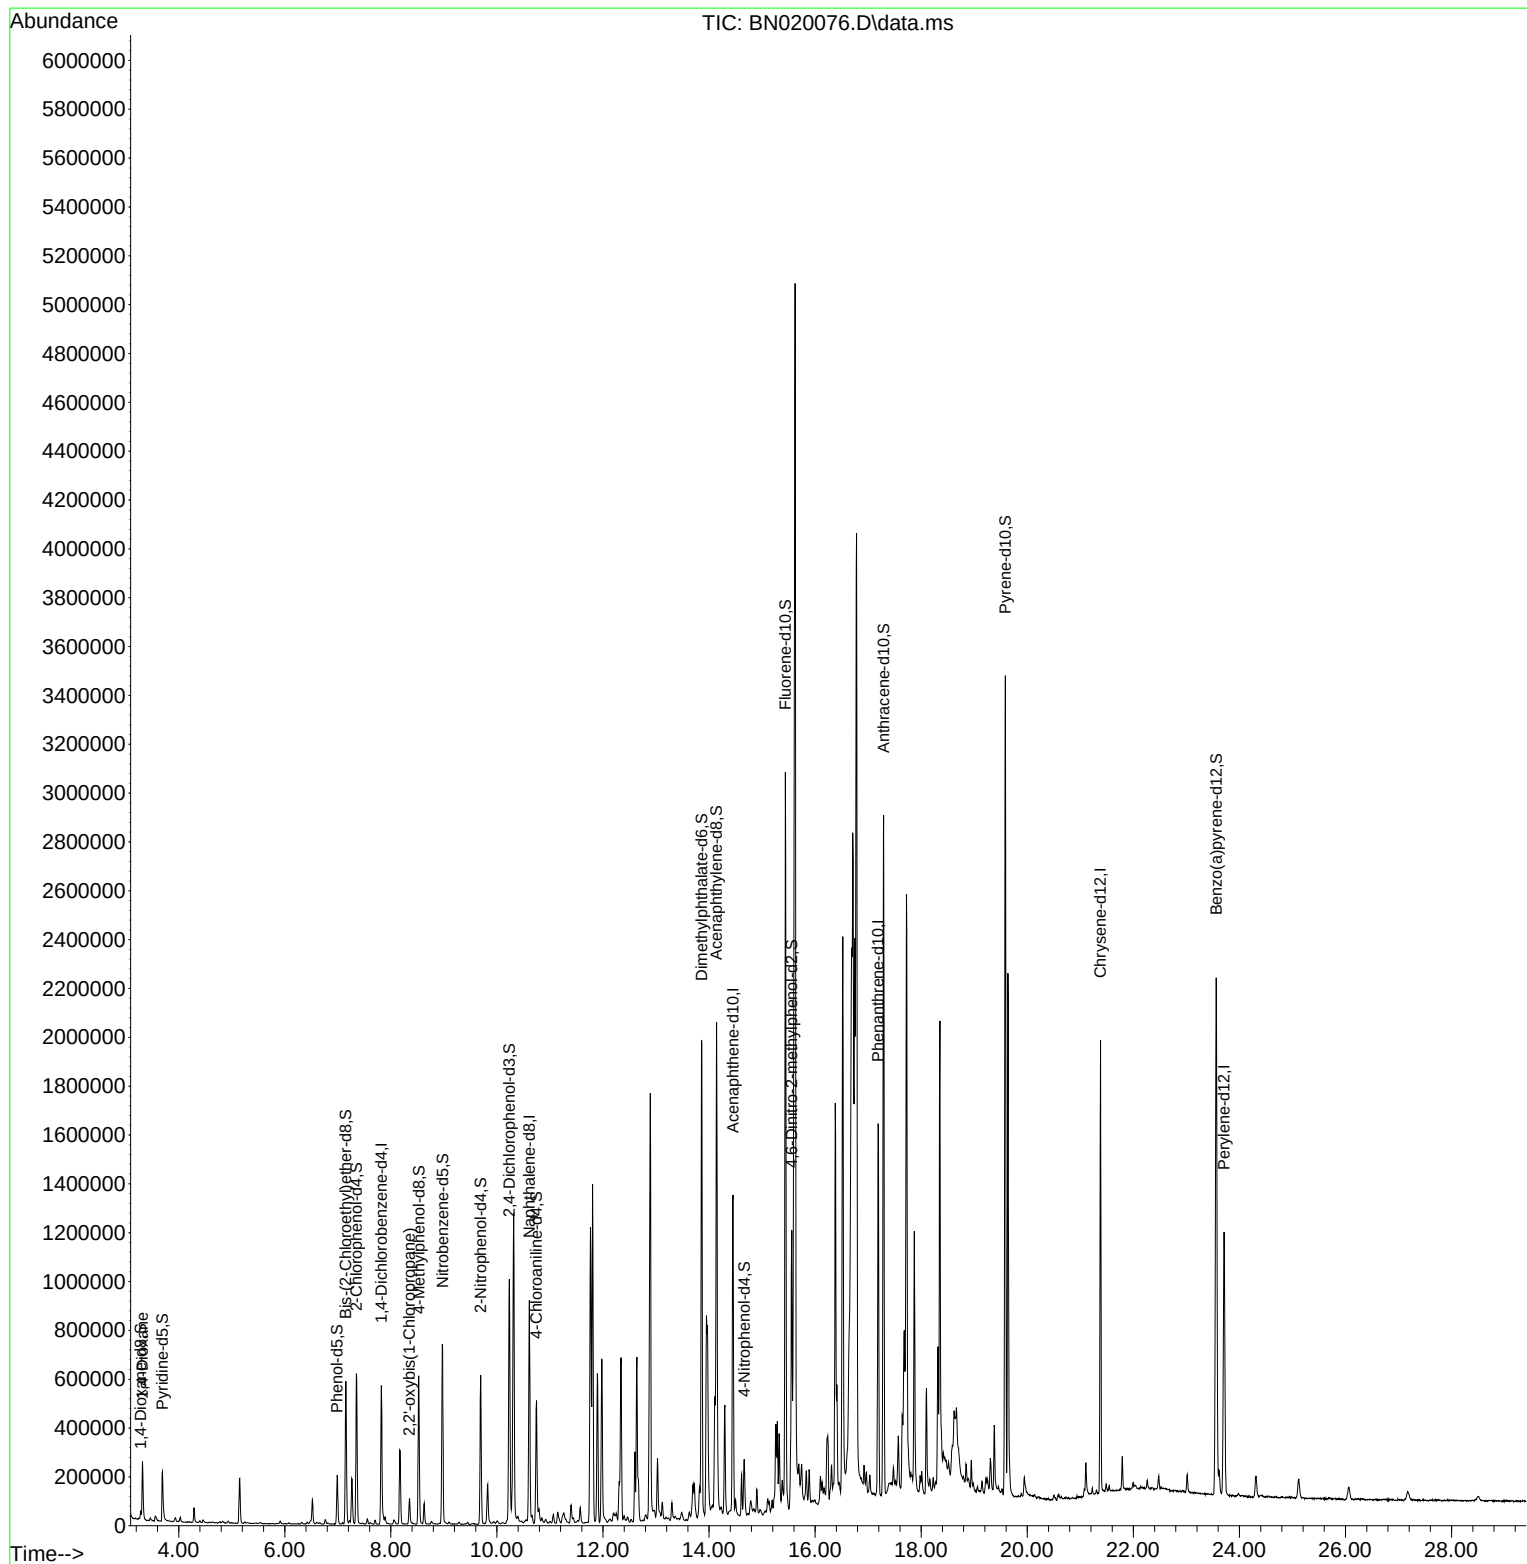


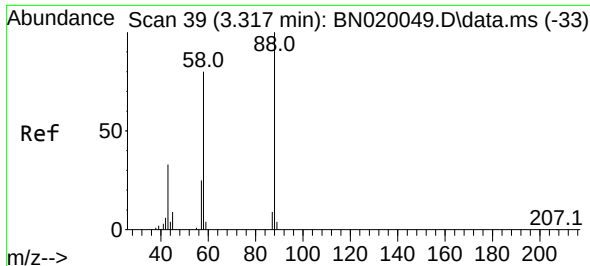

#2
 1,4-Dioxane
 Concen: 30.804 ng/uL
 RT: 3.316 min Scan# 39
 Delta R.T. 0.000 min
 Lab File: BN020076.D
 Acq: 09 Jun 2022 12:21

Instrument :
 BNA_N
 ClientSampleId :
 F5A53

Tgt Ion: 88 Resp: 115783
 Ion Ratio Lower Upper
 88 100
 43 32.4 22.4 33.6
 58 82.2 61.0 91.4

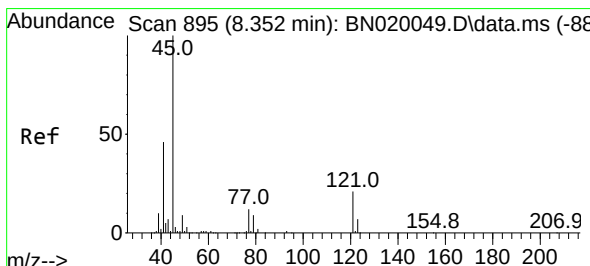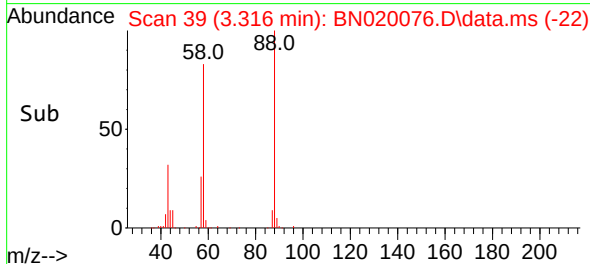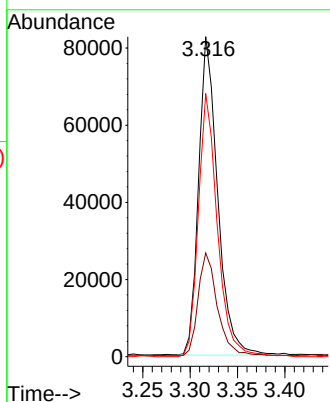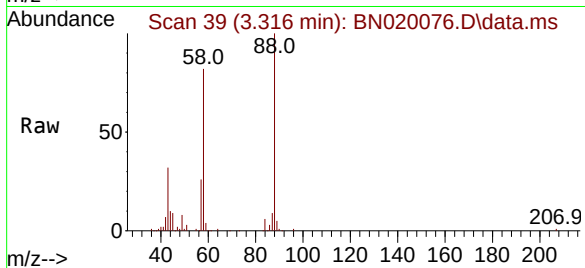

#14
 2,2'-oxybis(1-Chloropropane)
 Concen: 1.884 ng/uL
 RT: 8.351 min Scan# 895
 Delta R.T. -0.006 min
 Lab File: BN020076.D
 Acq: 09 Jun 2022 12:21

Tgt Ion: 45 Resp: 31427
 Ion Ratio Lower Upper
 45 100
 77 0.0 10.9 16.3#
 79 0.0 8.6 13.0#

