

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020078.D
 Acq On : 09 Jun 2022 13:34
 Operator : CG/JU
 Sample : N3212-09DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A56DL

Quant Time: Jun 10 01:05:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	170281	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	801149	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.445	164	525463	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.187	188	1082775	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	1021057	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	933424	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	4540	1.155	ng/uL	0.00
4) Pyridine-d5	3.699	84	25956	2.415	ng/u1	0.01
7) Phenol-d5	6.993	99	23238	1.649	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	55181	6.268	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	58372	5.099	ng/u1	0.00
15) 4-Methylphenol-d8	8.522	113	47213	3.873	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	35328	5.796	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	34815	5.382	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	69167	6.125	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	81510	4.457	ng/u1	0.00
46) Dimethylphthalate-d6	13.857	166	283074	7.404	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	304312	6.863	ng/u1	0.00
54) 4-Nitrophenol-d4	14.651	143	10807	1.411	ng/u1	0.00
60) Fluorene-d10	15.440	176	238026	7.523	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.551	200	23083	3.680	ng/u1	-0.01
73) Anthracene-d10	17.287	188	367062	7.768	ng/u1	0.00
81) Pyrene-d10	19.581	212	426519	7.705	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.563	264	341106	7.469	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.317	88	67730	16.319 ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020078.D
Acq On : 09 Jun 2022 13:34
Operator : CG/JU
Sample : N3212-09DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A56DL


Quant Time: Jun 10 01:05:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

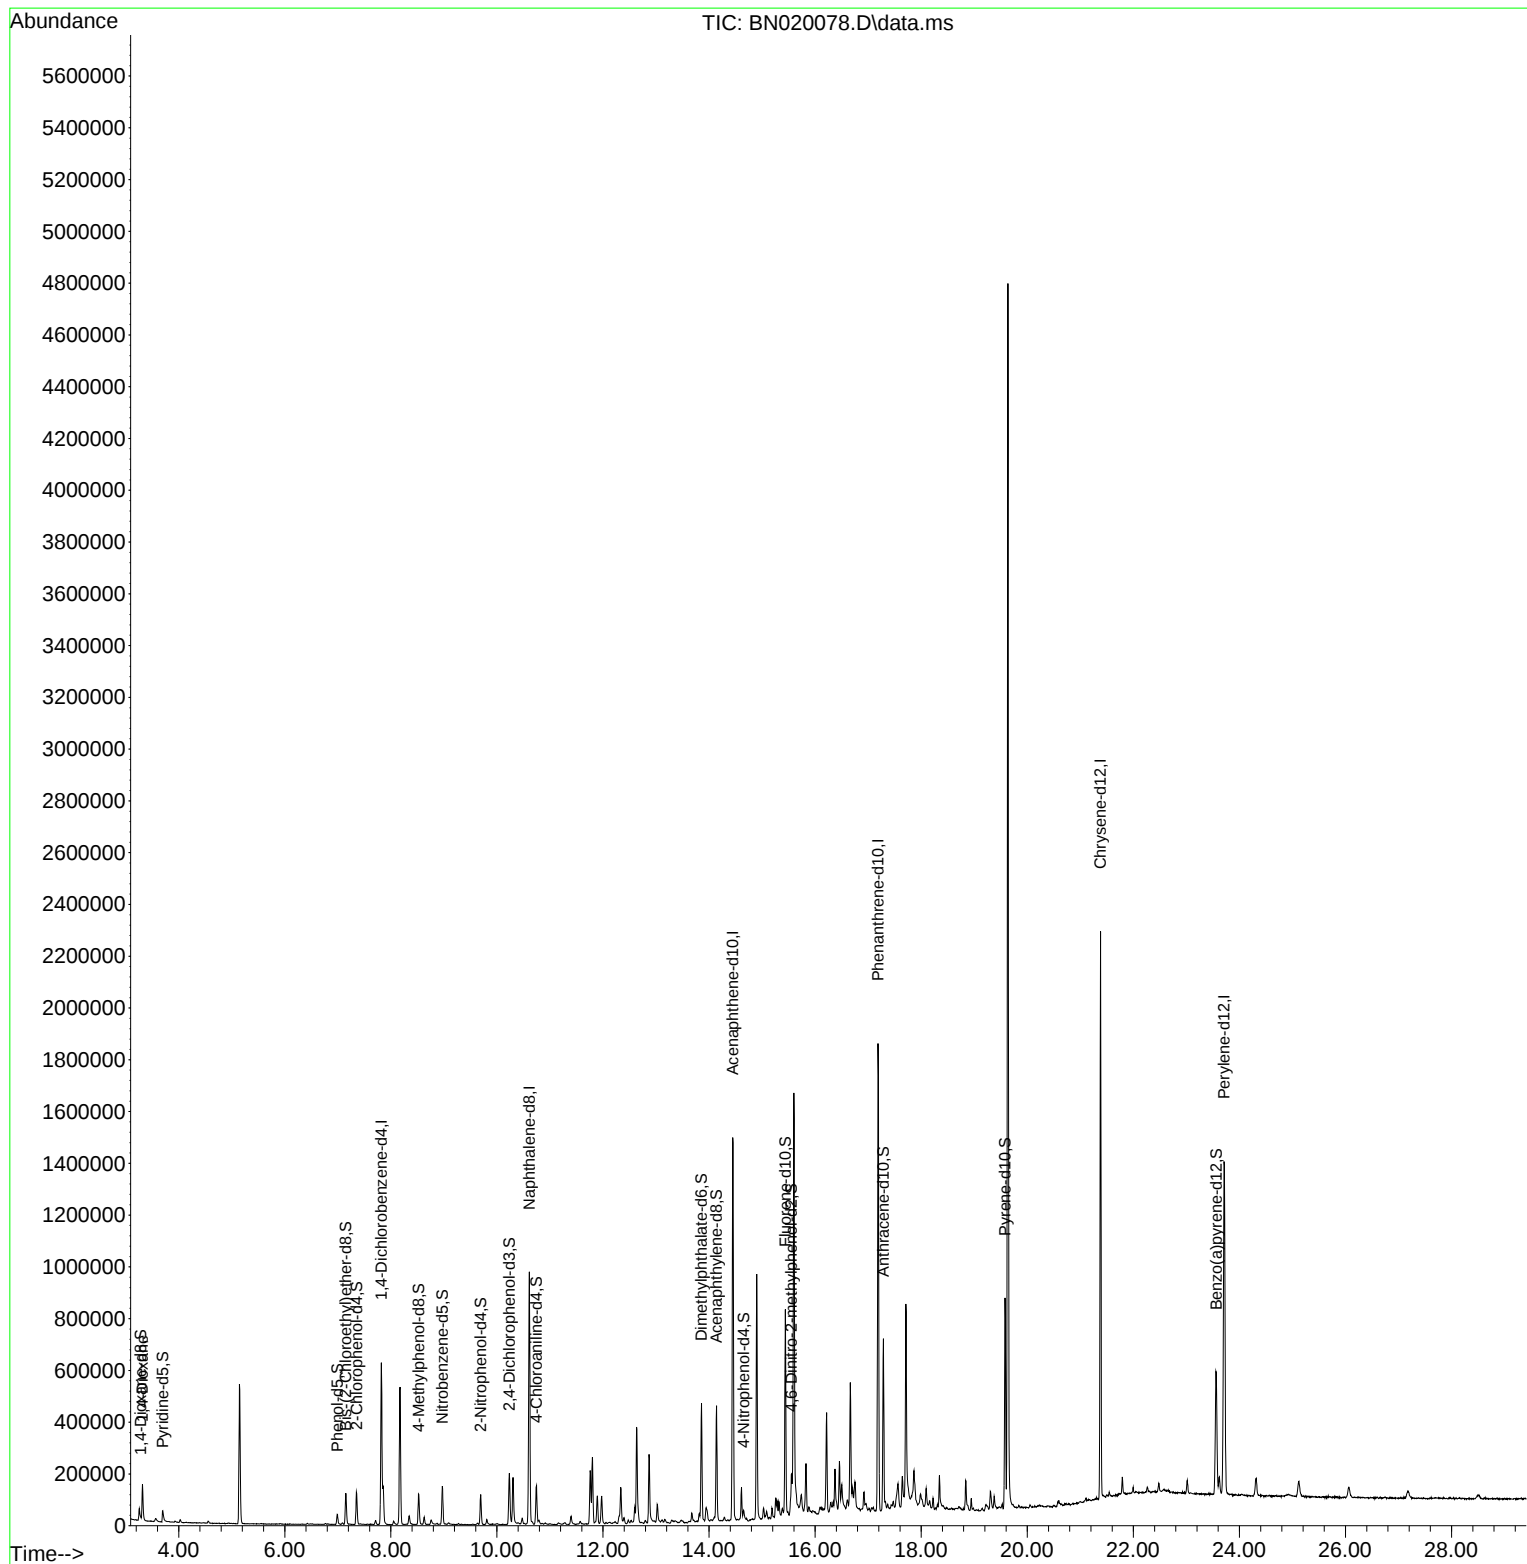

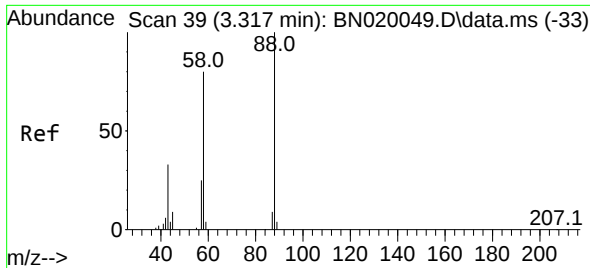

#2
 1,4-Dioxane
 Concen: 16.319 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020078.D
 Acq: 09 Jun 2022 13:34

Instrument :
 BNA_N
 ClientSampleId :
 F5A56DL

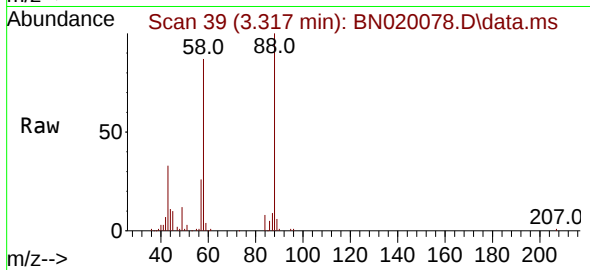

Tgt Ion:	88	Resp:	67730
Ion	Ratio	Lower	Upper
88	100		
43	32.7	22.4	33.6
58	86.8	61.0	91.4

