




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020072.D
Acq On : 09 Jun 2022 09:55
Operator : CG/JU
Sample : N3212-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A57

Manual IntegrationsAPPROVED

Quant Time: Jun 10 01:04:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

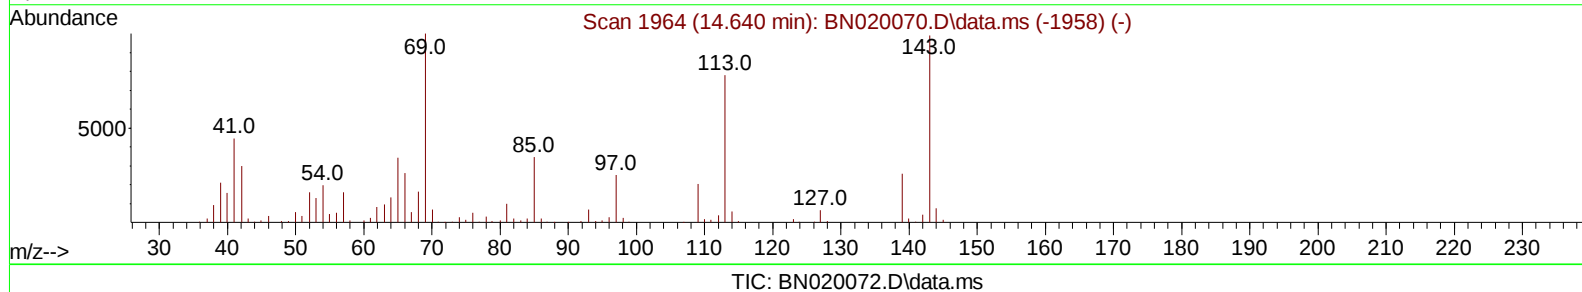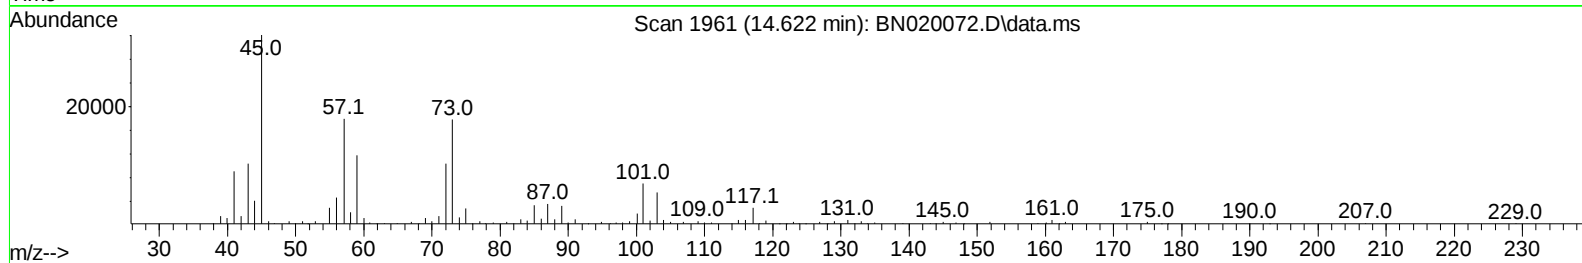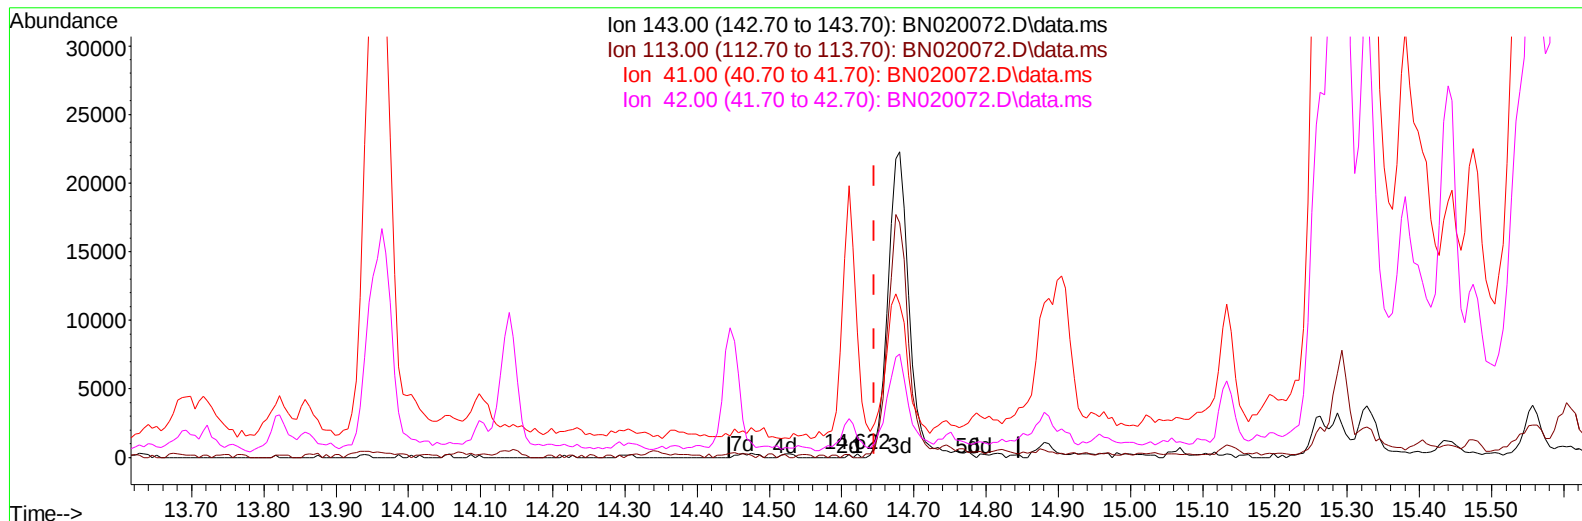

(54) 4-Nitrophenol-d4 (S)

14.622min (-0.023) 0.02 ng/u1

response 99

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	0.00#
41.00	39.70	3222.34#
42.00	27.00	510.64#




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020072.D
Acq On : 09 Jun 2022 09:55
Operator : CG/JU
Sample : N3212-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A57

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

Quant Time: Jun 10 01:04:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

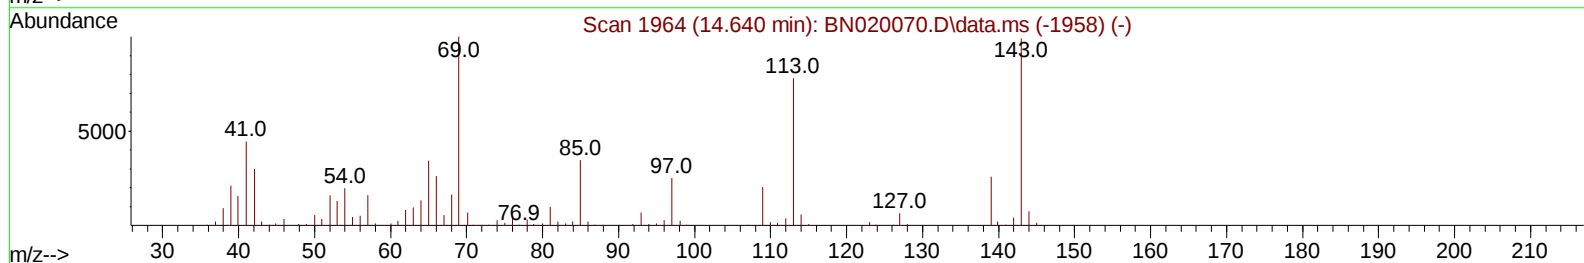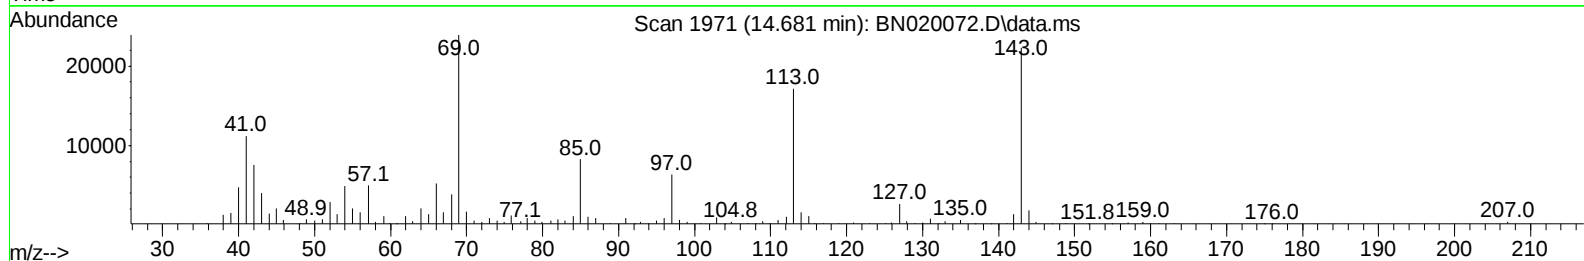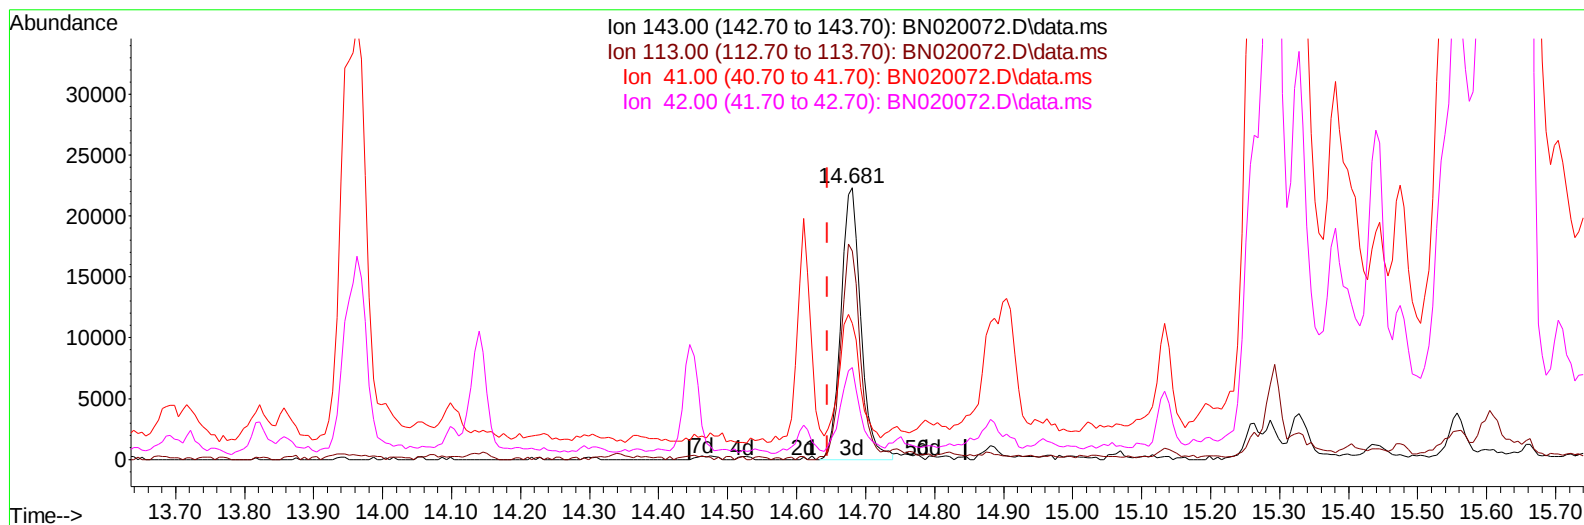

TIC: BN020072.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (+ 0.035) 7.64 ng/ul m

response 44772

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.20	76.69
41.00	39.70	50.14#
42.00	27.00	33.83#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020072.D
 Acq On : 09 Jun 2022 09:55
 Operator : CG/JU
 Sample : N3212-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A57

Manual IntegrationsAPPROVED

Quant Time: Jun 10 01:04:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/10/2022
 Supervised By :mohammad ahmed 06/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	135620	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	635540	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.445	164	401692	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.192	188	825051	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	777306	20.000	ng/ul	0.00
88) Perylene-d12	23.704	264	755060	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	14623	4.670	ng/uL	0.00
4) Pyridine-d5	3.687	84	92593	10.819	ng/ul	0.00
7) Phenol-d5	6.987	99	85105	7.584	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	219581	31.318	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	245659	26.941	ng/ul	0.00
15) 4-Methylphenol-d8	8.522	113	180318	18.572	ng/ul	0.00
21) Nitrobenzene-d5	8.969	128	150301	31.086	ng/ul	0.00
24) 2-Nitrophenol-d4	9.693	143	161706	31.514	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	289936	32.366	ng/ul	0.00
31) 4-Chloroaniline-d4	10.746	131	322975	22.264	ng/ul	0.00
46) Dimethylphthalate-d6	13.857	166	1049480	35.907	ng/ul	0.00
49) Acenaphthylene-d8	14.139	160	1157503	34.149	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	44772m	7.644	ng/ul	0.04
60) Fluorene-d10	15.439	176	833097	34.445	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	156069	32.656	ng/ul	0.00
73) Anthracene-d10	17.286	188	1345278	37.361	ng/ul	0.00
81) Pyrene-d10	19.586	212	1489769	35.353	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	1378233	37.307	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.316	88	133679	40.441	ng/uL	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020072.D
Acq On : 09 Jun 2022 09:55
Operator : CG/JU
Sample : N3212-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A57

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/10/2022
Supervised By :mohammad ahmed 06/10/2022

Quant Time: Jun 10 01:04:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

