

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020074.D
 Acq On : 09 Jun 2022 11:08
 Operator : CG/JU
 Sample : N3212-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A56

Quant Time: Jun 10 01:04:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 06 15:14:59 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	155663	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	712555	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.451	164	448863	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.192	188	901833	20.000	ng/u1	0.00
79) Chrysene-d12	21.380	240	851621	20.000	ng/u1	0.00
88) Perylene-d12	23.710	264	747569	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	19449	5.412	ng/uL	0.00
4) Pyridine-d5	3.687	84	140477	14.301	ng/u1	0.00
7) Phenol-d5	6.987	99	122081	9.478	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	263901	32.792	ng/u1	0.00
11) 2-Chlorophenol-d4	7.352	132	299347	28.602	ng/u1	0.00
15) 4-Methylphenol-d8	8.528	113	240522	21.583	ng/u1	0.00
21) Nitrobenzene-d5	8.969	128	185550	34.228	ng/u1	0.00
24) 2-Nitrophenol-d4	9.693	143	198620	34.524	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.234	165	345980	34.448	ng/u1	0.00
31) 4-Chloroaniline-d4	10.746	131	338377	20.805	ng/u1	0.00
46) Dimethylphthalate-d6	13.863	166	1255240	38.434	ng/u1	0.00
49) Acenaphthylene-d8	14.140	160	1396769	36.878	ng/u1	0.00
54) 4-Nitrophenol-d4	14.669	143	63822	9.752	ng/u1	0.02
60) Fluorene-d10	15.440	176	985089	36.449	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.557	200	179010	34.267	ng/u1	0.00
73) Anthracene-d10	17.292	188	1535865	39.023	ng/u1	0.00
81) Pyrene-d10	19.586	212	1719232	37.239	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.563	264	1451288	39.678	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.317	88	317242	83.615	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020074.D
Acq On : 09 Jun 2022 11:08
Operator : CG/JU
Sample : N3212-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A56

Quant Time: Jun 10 01:04:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 06 15:14:59 2022
Response via : Initial Calibration

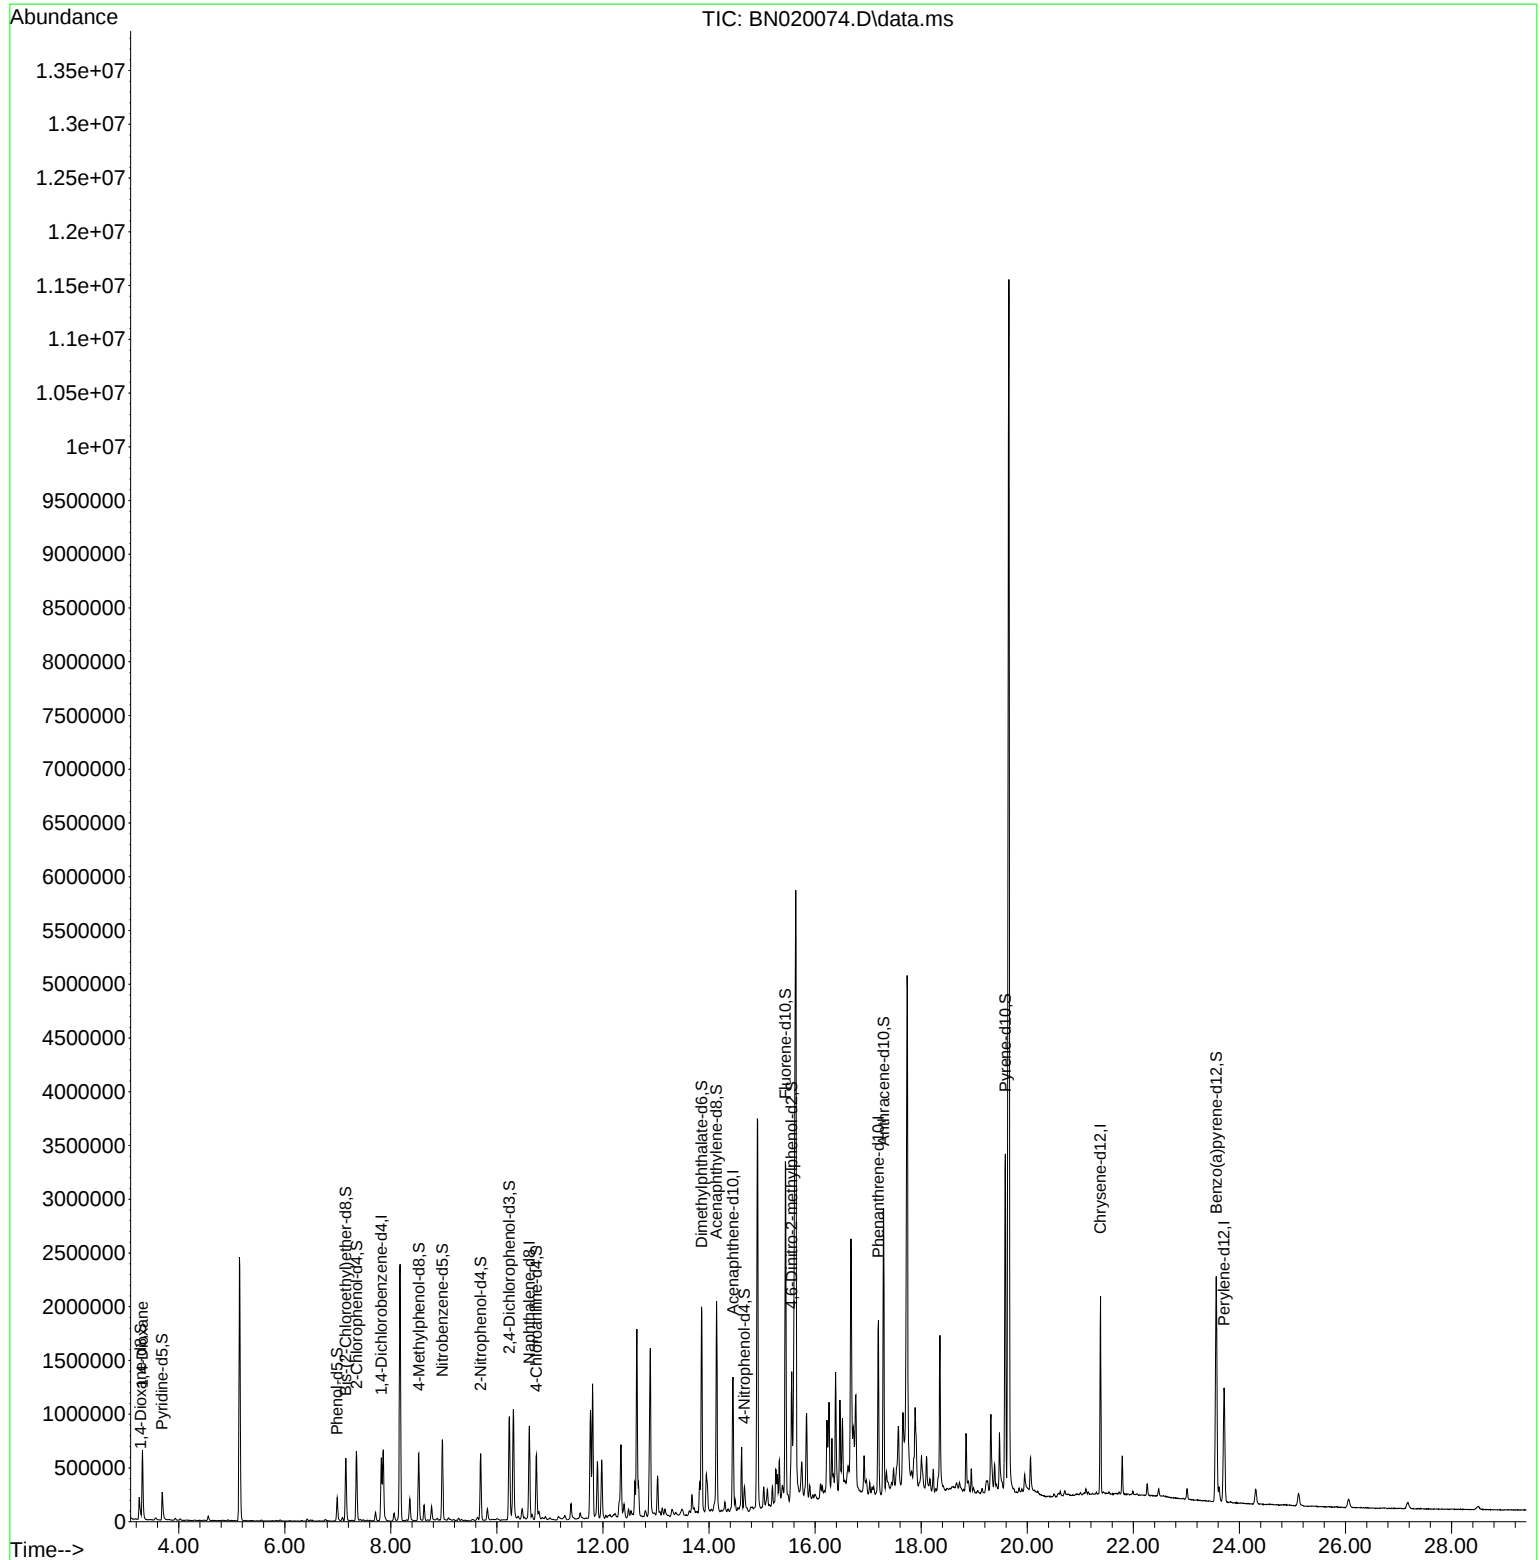

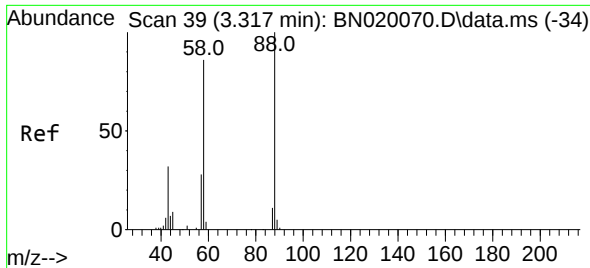

#2
 1,4-Dioxane
 Concen: 83.615 ng/uL
 RT: 3.317 min Scan# 39
 Delta R.T. 0.001 min
 Lab File: BN020074.D
 Acq: 09 Jun 2022 11:08

Instrument :
 BNA_N
 ClientSampleId :
 F5A56

Tgt Ion: 88 Resp: 317242

Ion	Ratio	Lower	Upper
88	100		
43	31.7	22.4	33.6
58	81.3	61.0	91.4

