

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020071.D
 Acq On : 09 Jun 2022 09:19
 Operator : CG/JU
 Sample : PB145381BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK381

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	45	rVB	34324	51594	1.43%	0.131%
2	3.687	98	102	120	rBV	459155	754653	20.98%	1.922%
3	4.028	156	160	165	rVB2	8683	13046	0.36%	0.033%
4	6.987	656	663	673	rBV	544427	878518	24.43%	2.237%
5	7.152	684	691	700	rBV	444466	718418	19.98%	1.829%
6	7.352	718	725	737	rBV	569087	920323	25.59%	2.344%
7	7.816	797	804	816	rBV	490023	826205	22.97%	2.104%
8	8.522	917	924	938	rBV	707271	1172194	32.60%	2.985%
9	8.969	993	1000	1014	rBV	555746	934462	25.98%	2.380%
10	9.693	1116	1123	1135	rBV	466283	781826	21.74%	1.991%
11	10.228	1207	1214	1226	rBV	674523	1156073	32.15%	2.944%
12	10.610	1271	1279	1287	rBV	766738	1327434	36.91%	3.380%
13	10.740	1293	1301	1317	rBV	785440	1358900	37.79%	3.460%
14	12.199	1544	1549	1557	rBV3	9660	17427	0.48%	0.044%
15	13.857	1824	1831	1844	rBV	1334923	1930524	53.68%	4.916%
16	14.140	1872	1879	1888	rBV	1511509	2217715	61.67%	5.647%
17	14.446	1924	1931	1945	rVB	1217120	1874155	52.11%	4.772%
18	14.640	1956	1964	1984	rBV	627375	986006	27.42%	2.511%
19	15.440	2093	2100	2113	rBV	1904547	2841212	79.01%	7.235%
20	15.557	2113	2120	2132	rVV	645710	933685	25.96%	2.378%
21	15.675	2136	2140	2145	rVB	22719	32514	0.90%	0.083%
22	16.222	2228	2233	2237	rBV3	6470	7499	0.21%	0.019%
23	16.969	2357	2360	2366	rBV5	3343	5911	0.16%	0.015%
24	17.187	2390	2397	2407	rBV	1553884	2251949	62.62%	5.734%
25	17.287	2407	2414	2428	rBV	2184736	3139149	87.29%	7.994%
26	17.775	2493	2497	2502	rBV4	2061	3723	0.10%	0.009%
27	18.092	2547	2551	2558	rBV3	4550	5512	0.15%	0.014%
28	19.145	2725	2730	2735	rBV2	27326	33750	0.94%	0.086%
29	19.216	2738	2742	2747	rBV	22968	31953	0.89%	0.081%
30	19.369	2765	2768	2772	rBV4	3139	4999	0.14%	0.013%
31	19.581	2798	2804	2827	rVV	2520958	3596193	100.00%	9.157%
32	20.139	2896	2899	2902	rBV4	3170	4953	0.14%	0.013%
33	20.369	2931	2938	2941	rBV9	3949	9117	0.25%	0.023%
34	20.592	2973	2976	2981	rVB4	9647	12157	0.34%	0.031%
35	21.375	3104	3109	3116	rBV	1834342	2486604	69.15%	6.332%
36	23.010	3383	3387	3395	rVB2	31262	48875	1.36%	0.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020071.D
Acq On : 09 Jun 2022 09:19
Operator : CG/JU
Sample : PB145381BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK381

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Title : SVOA CALIBRATION

37	23.557	3471	3480	3487	rBV2	1698105	3391383	94.30%	8.636%
38	23.710	3497	3506	3516	rBV	1112377	2343270	65.16%	5.967%
39	24.304	3603	3607	3614	rVB2	38119	74953	2.08%	0.191%
40	25.116	3739	3745	3752	rVB3	39848	92128	2.56%	0.235%




Sum of corrected areas: 39270962

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020071.D
Acq On : 09 Jun 2022 09:19
Operator : CG/JU
Sample : PB145381BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

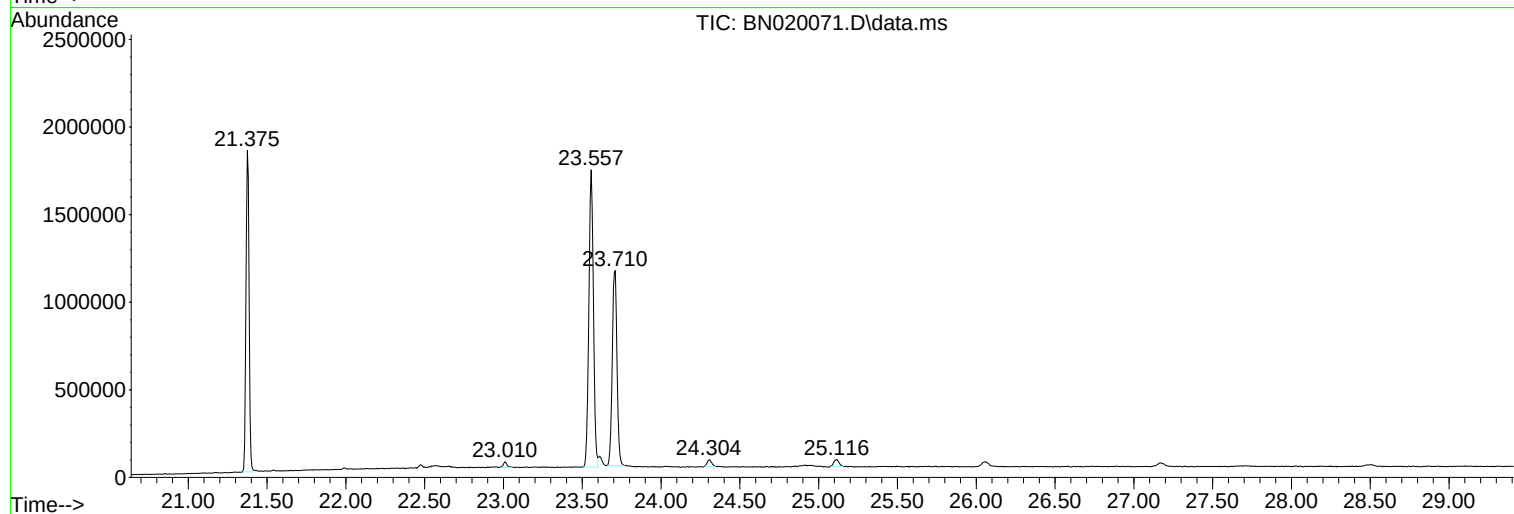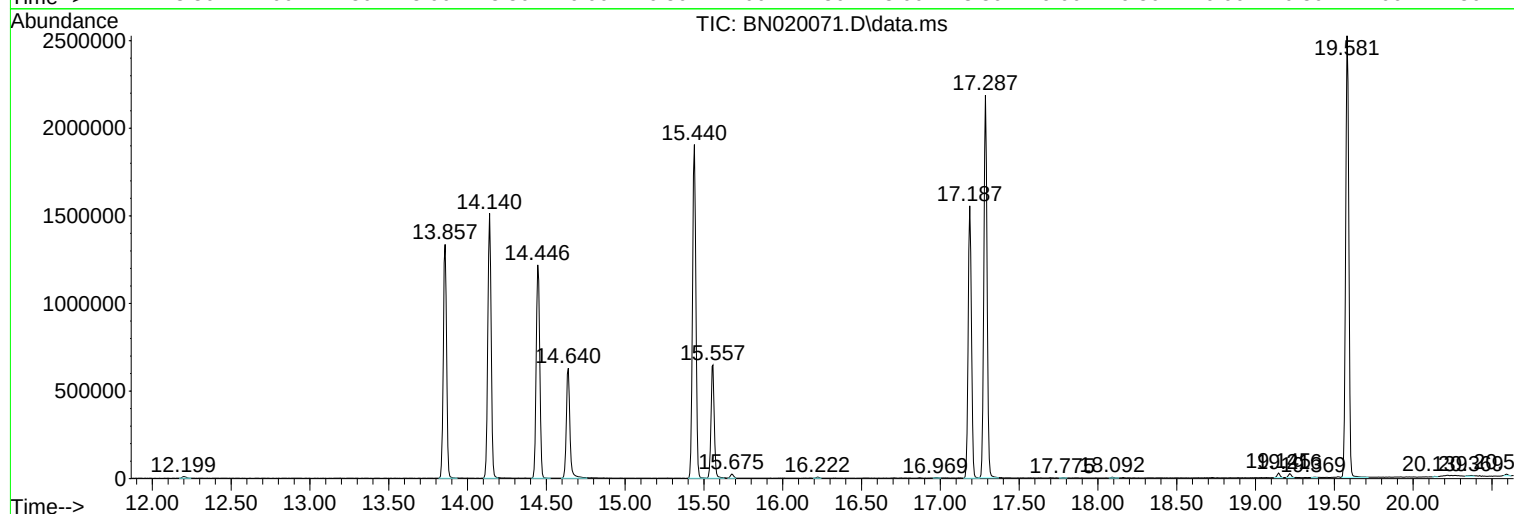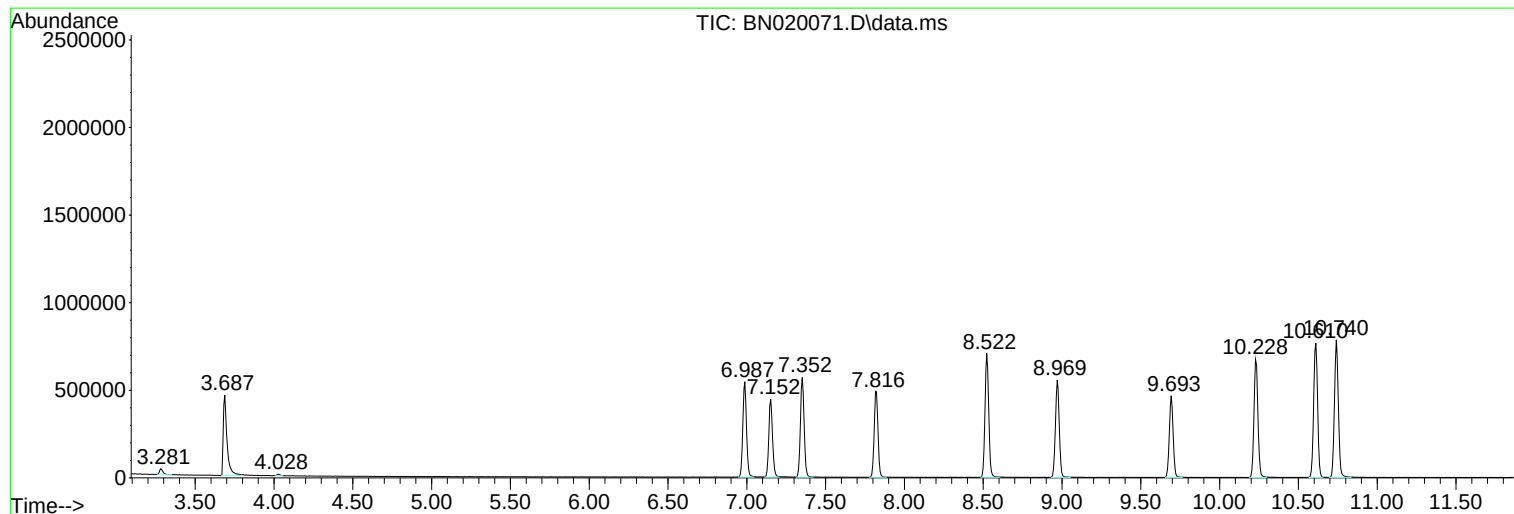

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020071.D
Acq On : 09 Jun 2022 09:19
Operator : CG/JU
Sample : PB145381BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020071.D
Acq On : 09 Jun 2022 09:19
Operator : CG/JU
Sample : PB145381BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc