

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020073.D
 Acq On : 09 Jun 2022 10:32
 Operator : CG/JU
 Sample : N3212-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	40	rVB	30395	43664	1.05%	0.110%
2	3.564	77	81	92	rVB2	12262	30239	0.73%	0.076%
3	3.687	99	102	119	rBV	153870	269891	6.51%	0.680%
4	3.934	139	144	150	rVB2	12306	22078	0.53%	0.056%
5	4.028	156	160	170	rVB2	11299	20195	0.49%	0.051%
6	4.558	245	250	262	rVB2	17055	31334	0.76%	0.079%
7	4.934	309	314	320	rBV3	5814	9710	0.23%	0.024%
8	5.546	415	418	426	rVB3	3083	5133	0.12%	0.013%
9	6.828	631	636	641	rBV7	3402	7227	0.17%	0.018%
10	6.987	656	663	674	rBV	137717	242235	5.85%	0.611%
11	7.152	684	691	705	rVB	452583	727900	17.57%	1.835%
12	7.352	717	725	734	rBV	470827	792684	19.13%	1.998%
13	7.464	739	744	750	rVB5	2887	5058	0.12%	0.013%
14	7.822	798	805	812	rVV	483482	803928	19.40%	2.026%
15	7.893	812	817	827	rVB	22345	40568	0.98%	0.102%
16	8.522	917	924	936	rBV	403838	655801	15.83%	1.653%
17	8.969	993	1000	1014	rBV	566215	959519	23.16%	2.418%
18	9.693	1116	1123	1134	rBV	452756	770972	18.61%	1.943%
19	10.228	1206	1214	1226	rBV	614225	1096414	26.46%	2.763%
20	10.610	1272	1279	1290	rVB	730941	1293596	31.22%	3.260%
21	10.740	1294	1301	1321	rBV	663922	1176326	28.39%	2.965%
22	12.199	1543	1549	1558	rBV	11500	19329	0.47%	0.049%
23	12.822	1649	1655	1659	rBV6	2677	5075	0.12%	0.013%
24	13.063	1691	1696	1701	rBV5	4495	8240	0.20%	0.021%
25	13.357	1740	1746	1751	rBV4	5096	9526	0.23%	0.024%
26	13.857	1824	1831	1841	rBV	1414969	2009894	48.51%	5.066%
27	14.140	1872	1879	1893	rBV	1494520	2279654	55.02%	5.745%
28	14.446	1924	1931	1939	rBV	1152936	1810830	43.70%	4.564%
29	14.640	1958	1964	1977	rBV	141975	239680	5.78%	0.604%
30	14.869	1998	2003	2007	rBV3	9292	12219	0.29%	0.031%
31	15.257	2063	2069	2078	rBV	126594	174149	4.20%	0.439%
32	15.440	2093	2100	2110	rBV	2009888	3006076	72.55%	7.576%
33	15.557	2113	2120	2128	rBV	683934	956867	23.09%	2.412%
34	15.675	2137	2140	2146	rVB	25248	35857	0.87%	0.090%
35	15.998	2191	2195	2201	rVB5	3453	6095	0.15%	0.015%
36	16.222	2229	2233	2238	rVB5	7162	9648	0.23%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020073.D
 Acq On : 09 Jun 2022 10:32
 Operator : CG/JU
 Sample : N3212-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	16.722	2312	2318	2320	rBV5	2302	4724	0.11%	0.012%
38	16.975	2357	2361	2366	rBV5	3414	5652	0.14%	0.014%
39	17.187	2390	2397	2406	rBV	1517486	2194173	52.96%	5.530%
40	17.287	2407	2414	2428	rVV	2449172	3611912	87.17%	9.103%
41	17.481	2444	2447	2451	rVB	6784	7739	0.19%	0.020%
42	17.781	2496	2498	2504	rVB5	2655	4316	0.10%	0.011%
43	17.863	2508	2512	2519	rVB5	10138	13451	0.32%	0.034%
44	18.087	2546	2550	2558	rBV2	54847	81458	1.97%	0.205%
45	18.163	2558	2563	2567	rVB	15421	22847	0.55%	0.058%
46	18.945	2691	2696	2701	rBV	53886	63742	1.54%	0.161%
47	19.145	2725	2730	2735	rBV	31538	43760	1.06%	0.110%
48	19.216	2738	2742	2746	rBV2	31572	46256	1.12%	0.117%
49	19.251	2746	2748	2752	rVB3	12378	14435	0.35%	0.036%
50	19.369	2764	2768	2774	rBV2	50306	70991	1.71%	0.179%
51	19.522	2790	2794	2798	rBV4	11789	15644	0.38%	0.039%
52	19.581	2798	2804	2818	rVV	2862698	4125068	99.56%	10.396%
53	20.063	2882	2886	2889	rBV6	2619	4492	0.11%	0.011%
54	20.575	2970	2973	2974	rBV3	5892	5923	0.14%	0.015%
55	20.592	2974	2976	2980	rVB2	13355	15157	0.37%	0.038%
56	21.375	3104	3109	3118	rBV	1825842	2448961	59.11%	6.172%
57	21.539	3135	3137	3142	rVB4	14533	14087	0.34%	0.036%
58	21.992	3212	3214	3219	rVB4	21295	22933	0.55%	0.058%
59	22.263	3255	3260	3268	rBV	149316	211402	5.10%	0.533%
60	22.475	3293	3296	3303	rVB2	39999	54511	1.32%	0.137%
61	23.010	3383	3387	3395	rVB2	62374	96581	2.33%	0.243%
62	23.557	3472	3480	3487	rBV2	2102409	4143358	100.00%	10.443%
63	23.710	3498	3506	3521	rVB	1162807	2410811	58.18%	6.076%
64	24.310	3603	3608	3616	rVB	78487	157572	3.80%	0.397%
65	25.116	3739	3745	3754	rVB3	75775	178070	4.30%	0.449%




Sum of corrected areas: 39677637

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020073.D
Acq On : 09 Jun 2022 10:32
Operator : CG/JU
Sample : N3212-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

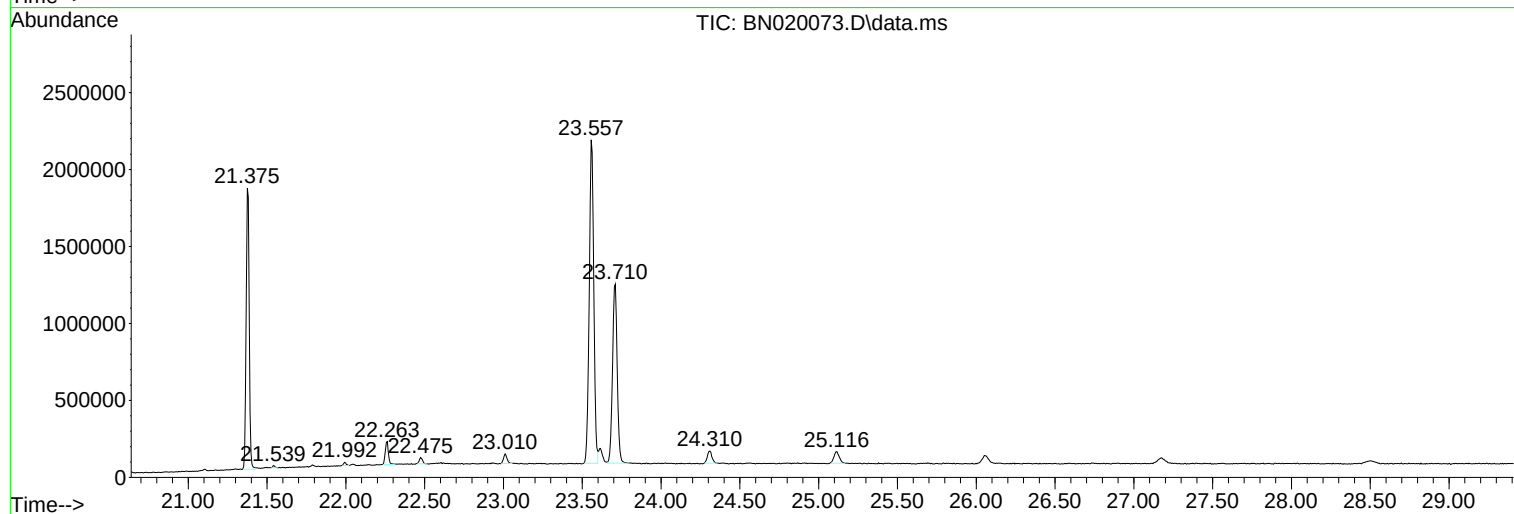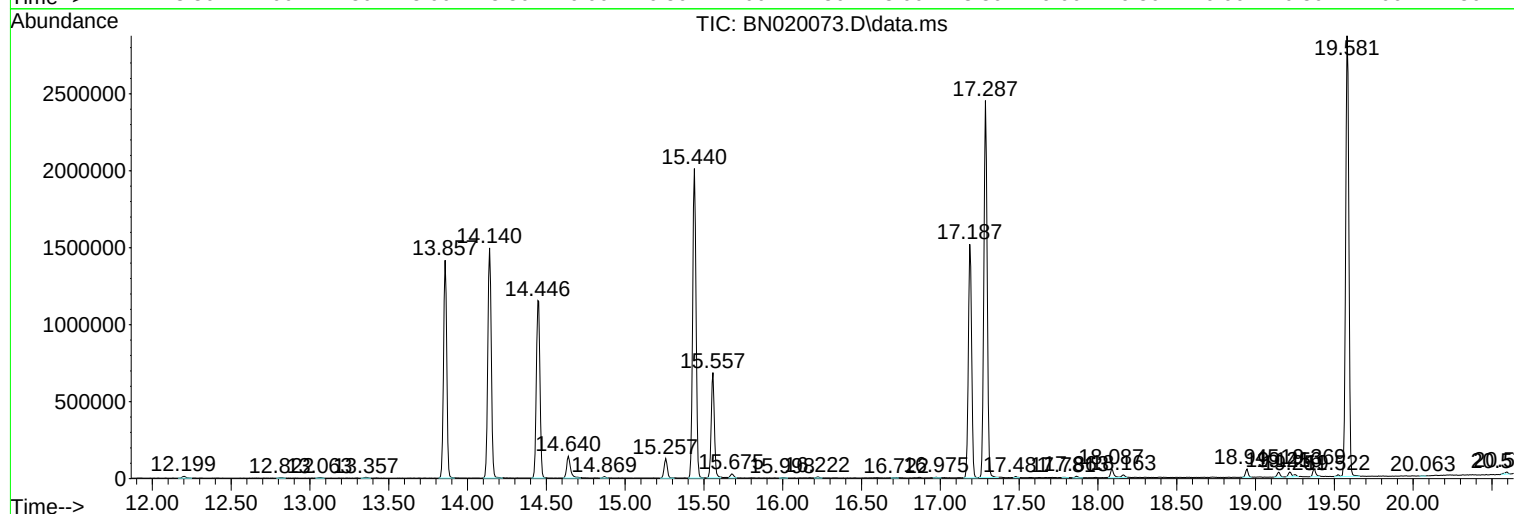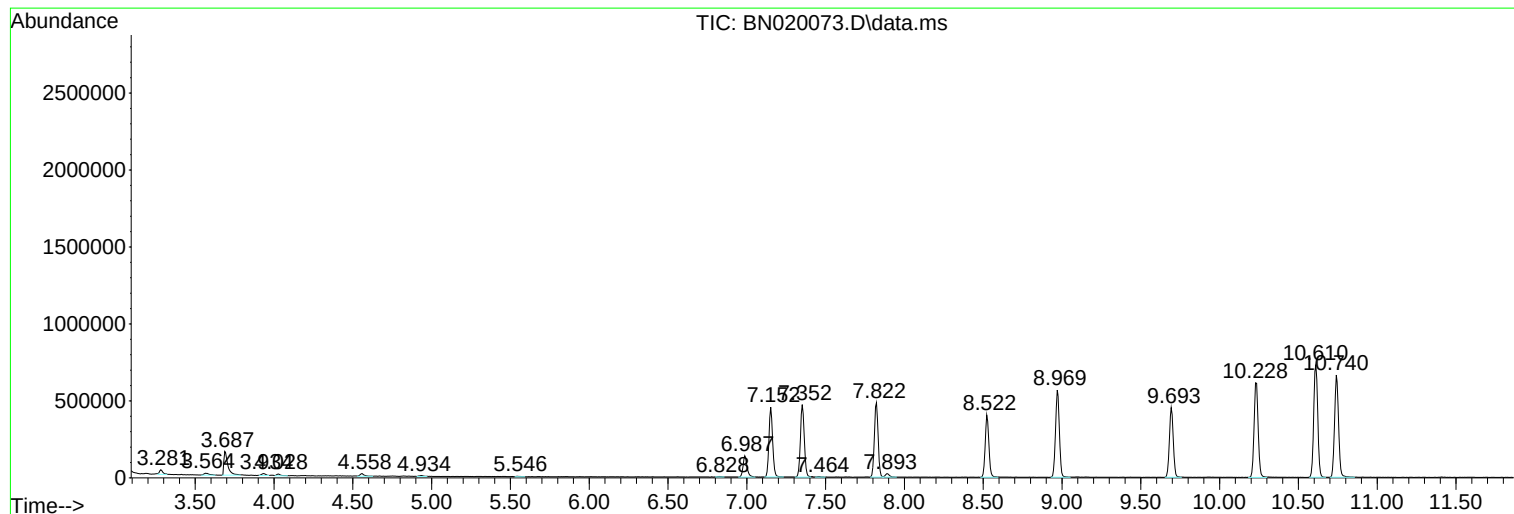

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020073.D
Acq On : 09 Jun 2022 10:32
Operator : CG/JU
Sample : N3212-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020073.D
Acq On : 09 Jun 2022 10:32
Operator : CG/JU
Sample : N3212-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc