

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020075.D
 Acq On : 09 Jun 2022 11:44
 Operator : CG/JU
 Sample : N3212-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN020075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	15	17	22	rVB4	6130	7556	0.17%	0.018%
2	3.281	29	33	36	rBV	31055	41189	0.92%	0.099%
3	3.317	36	39	47	rVB	33588	53670	1.19%	0.129%
4	3.564	77	81	90	rVB3	11688	24345	0.54%	0.058%
5	3.693	99	103	114	rBV	168922	282263	6.28%	0.676%
6	3.934	139	144	150	rVB2	15259	26185	0.58%	0.063%
7	4.028	156	160	168	rVB	11779	19332	0.43%	0.046%
8	4.393	220	222	229	rVB5	4183	6526	0.15%	0.016%
9	4.934	310	314	320	rBV3	7746	13252	0.29%	0.032%
10	6.987	657	663	673	rBV	129469	216800	4.82%	0.519%
11	7.152	681	691	699	rBV	477155	770603	17.14%	1.845%
12	7.228	700	704	708	rVB	5892	9275	0.21%	0.022%
13	7.352	717	725	734	rBV	431935	719396	16.00%	1.723%
14	7.458	741	743	749	rVB6	3439	4906	0.11%	0.012%
15	7.822	798	805	812	rBV	509270	836828	18.62%	2.004%
16	7.887	812	816	823	rVB	22399	36749	0.82%	0.088%
17	8.075	839	848	853	rBV7	5286	11582	0.26%	0.028%
18	8.522	916	924	938	rBV	378801	637818	14.19%	1.527%
19	8.634	938	943	950	rVB6	4395	8343	0.19%	0.020%
20	8.969	990	1000	1012	rBV	594439	1020943	22.71%	2.445%
21	9.099	1017	1022	1027	rVV3	4023	6086	0.14%	0.015%
22	9.693	1116	1123	1132	rBV	435158	739912	16.46%	1.772%
23	9.928	1160	1163	1169	rBV4	3334	6353	0.14%	0.015%
24	10.234	1208	1215	1223	rBV	621386	1074602	23.90%	2.573%
25	10.305	1223	1227	1235	rVV2	9368	19253	0.43%	0.046%
26	10.393	1237	1242	1247	rBV5	4332	7599	0.17%	0.018%
27	10.610	1268	1279	1287	rVB	799322	1342762	29.87%	3.216%
28	10.740	1292	1301	1318	rBV	748367	1341100	29.83%	3.212%
29	11.404	1408	1414	1419	rBV7	4768	10137	0.23%	0.024%
30	11.510	1427	1432	1439	rBV7	9057	20247	0.45%	0.048%
31	11.804	1478	1482	1485	rBV3	4516	7001	0.16%	0.017%
32	11.851	1485	1490	1491	rVV2	5098	8146	0.18%	0.020%
33	11.869	1491	1493	1497	rVV3	6490	9159	0.20%	0.022%
34	11.916	1497	1501	1508	rVB4	4385	8345	0.19%	0.020%
35	12.122	1530	1536	1541	rVB7	3551	8041	0.18%	0.019%
36	12.199	1541	1549	1553	rBV2	14150	25591	0.57%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020075.D
 Acq On : 09 Jun 2022 11:44
 Operator : CG/JU
 Sample : N3212-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

37	12.640	1618	1624	1633	rVB	56660	84341	1.88%	0.202%
38	12.810	1648	1653	1658	rBV5	3349	5708	0.13%	0.014%
39	12.893	1661	1667	1674	rBV3	5175	11853	0.26%	0.028%
40	12.969	1674	1680	1687	rVB5	3750	7095	0.16%	0.017%
41	13.040	1687	1692	1697	rBV3	13022	28470	0.63%	0.068%
42	13.087	1697	1700	1709	rVB2	12166	20372	0.45%	0.049%
43	13.293	1730	1735	1741	rBV	17053	26641	0.59%	0.064%
44	13.357	1743	1746	1753	rVB4	3870	6027	0.13%	0.014%
45	13.857	1824	1831	1842	rBV	1567276	2264576	50.38%	5.423%
46	13.998	1853	1855	1860	rVB2	4916	6279	0.14%	0.015%
47	14.140	1868	1879	1888	rBV	1624450	2456278	54.64%	5.882%
48	14.363	1914	1917	1922	rVB6	2933	4846	0.11%	0.012%
49	14.445	1925	1931	1940	rVV	1219528	1886456	41.96%	4.517%
50	14.640	1956	1964	1973	rBV	139269	235324	5.23%	0.564%
51	14.869	1999	2003	2007	rBV4	5575	8354	0.19%	0.020%
52	14.981	2019	2022	2025	rBV3	3705	5651	0.13%	0.014%
53	15.028	2025	2030	2037	rVB	7083	13956	0.31%	0.033%
54	15.134	2045	2048	2051	rBV4	5736	7313	0.16%	0.018%
55	15.187	2051	2057	2059	rVV4	6613	11922	0.27%	0.029%
56	15.222	2059	2063	2065	rVV2	10412	16243	0.36%	0.039%
57	15.257	2065	2069	2085	rVV	88268	151687	3.37%	0.363%
58	15.381	2085	2090	2093	rVV7	3385	5160	0.11%	0.012%
59	15.440	2093	2100	2110	rVV	2224318	3317531	73.80%	7.944%
60	15.557	2114	2120	2135	rBV	607095	905921	20.15%	2.169%
61	15.681	2136	2141	2147	rVB	29881	48744	1.08%	0.117%
62	15.804	2159	2162	2166	rVB5	3272	4984	0.11%	0.012%
63	15.892	2173	2177	2182	rVB	25765	32082	0.71%	0.077%
64	16.022	2197	2199	2204	rVV5	4769	6051	0.13%	0.014%
65	16.128	2210	2217	2221	rVV8	8070	19472	0.43%	0.047%
66	16.192	2221	2228	2231	rVV3	16833	32005	0.71%	0.077%
67	16.222	2231	2233	2241	rVB4	12729	14915	0.33%	0.036%
68	16.334	2247	2252	2255	rBV4	6851	11634	0.26%	0.028%
69	16.375	2257	2259	2263	rVB5	4413	4611	0.10%	0.011%
70	16.522	2281	2284	2288	rBV6	2463	4504	0.10%	0.011%
71	16.681	2308	2311	2313	rBV4	4620	6063	0.13%	0.015%
72	16.869	2339	2343	2349	rBV5	7225	10403	0.23%	0.025%
73	16.957	2354	2358	2365	rVV5	8342	18339	0.41%	0.044%
74	17.187	2390	2397	2407	rVV	1524045	2266788	50.43%	5.428%
75	17.287	2407	2414	2426	rBV2	2547926	3860139	85.87%	9.244%
76	17.475	2443	2446	2452	rVB	6038	8611	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
 Data File : BN020075.D
 Acq On : 09 Jun 2022 11:44
 Operator : CG/JU
 Sample : N3212-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F5A54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
 Title : SVOA CALIBRATION

77	17.563	2456	2461	2464	rBV6	4788	9053	0.20%	0.022%
78	17.781	2495	2498	2500	rBV3	4463	4796	0.11%	0.011%
79	17.869	2508	2513	2518	rVB7	9810	15007	0.33%	0.036%
80	18.092	2545	2551	2559	rBV	105651	179586	3.99%	0.430%
81	18.163	2559	2563	2567	rVB	19049	29726	0.66%	0.071%
82	18.728	2655	2659	2661	rVB4	3385	4549	0.10%	0.011%
83	18.945	2691	2696	2702	rBV	41141	54320	1.21%	0.130%
84	19.145	2726	2730	2735	rBV2	41704	57697	1.28%	0.138%
85	19.216	2737	2742	2746	rVV	38016	54182	1.21%	0.130%
86	19.251	2746	2748	2751	rVB3	7054	7116	0.16%	0.017%
87	19.369	2763	2768	2776	rBV2	46518	78855	1.75%	0.189%
88	19.522	2790	2794	2798	rBV4	15309	20245	0.45%	0.048%
89	19.580	2798	2804	2821	rVV	3113823	4495343	100.00%	10.765%
90	20.592	2971	2976	2980	rBV4	14419	26381	0.59%	0.063%
91	21.098	3058	3062	3070	rBV	146566	234166	5.21%	0.561%
92	21.375	3104	3109	3120	rBV	1826366	2488959	55.37%	5.960%
93	22.257	3255	3259	3264	rBV	134713	178852	3.98%	0.428%
94	23.010	3384	3387	3393	rVB2	41144	62668	1.39%	0.150%
95	23.563	3472	3481	3488	rBV2	2033074	4166516	92.69%	9.978%
96	23.710	3498	3506	3516	rVB2	1102187	2274416	50.59%	5.447%
97	25.110	3741	3744	3754	rVB2	45485	97280	2.16%	0.233%




Sum of corrected areas: 41758957

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020075.D
Acq On : 09 Jun 2022 11:44
Operator : CG/JU
Sample : N3212-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

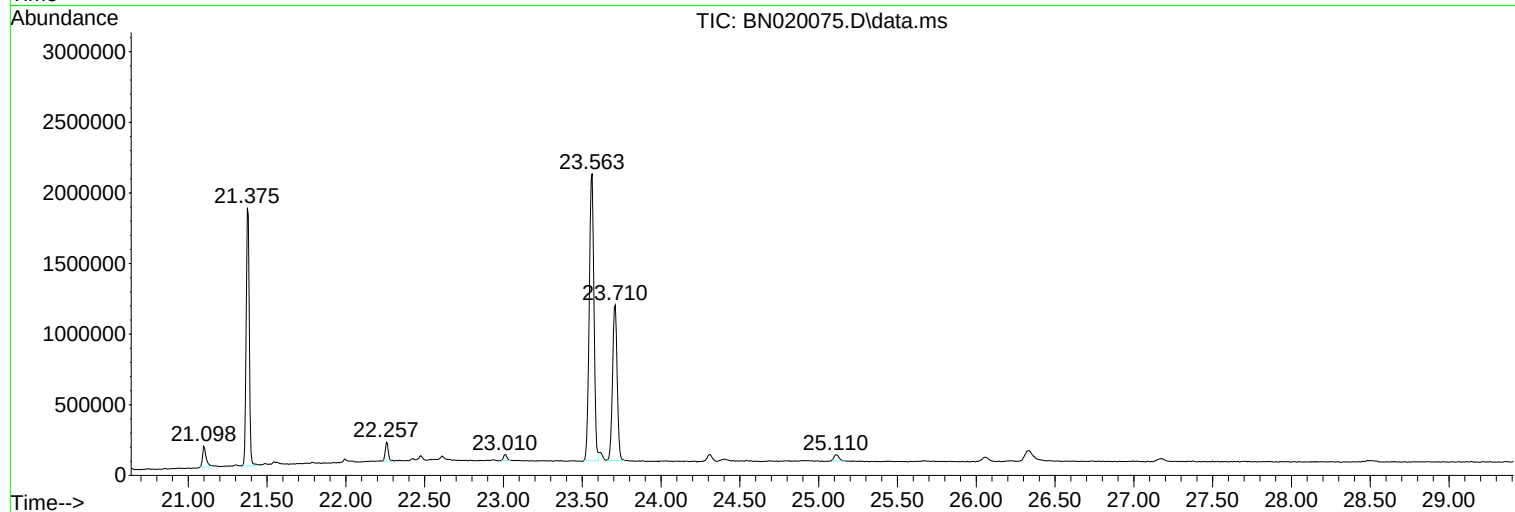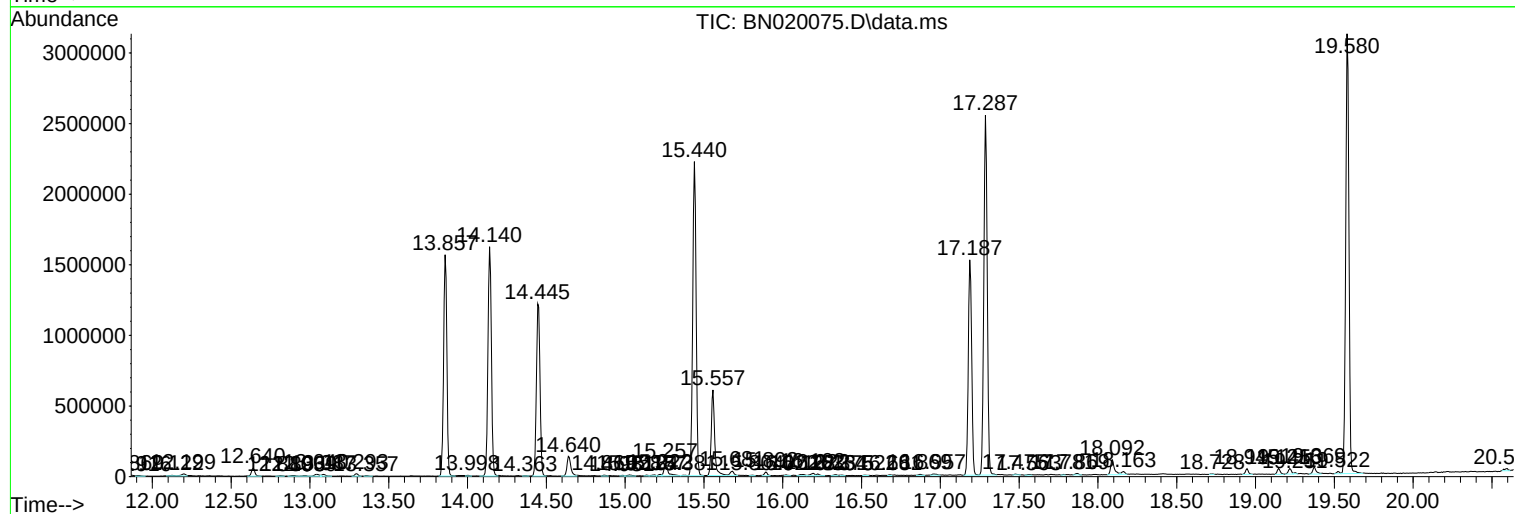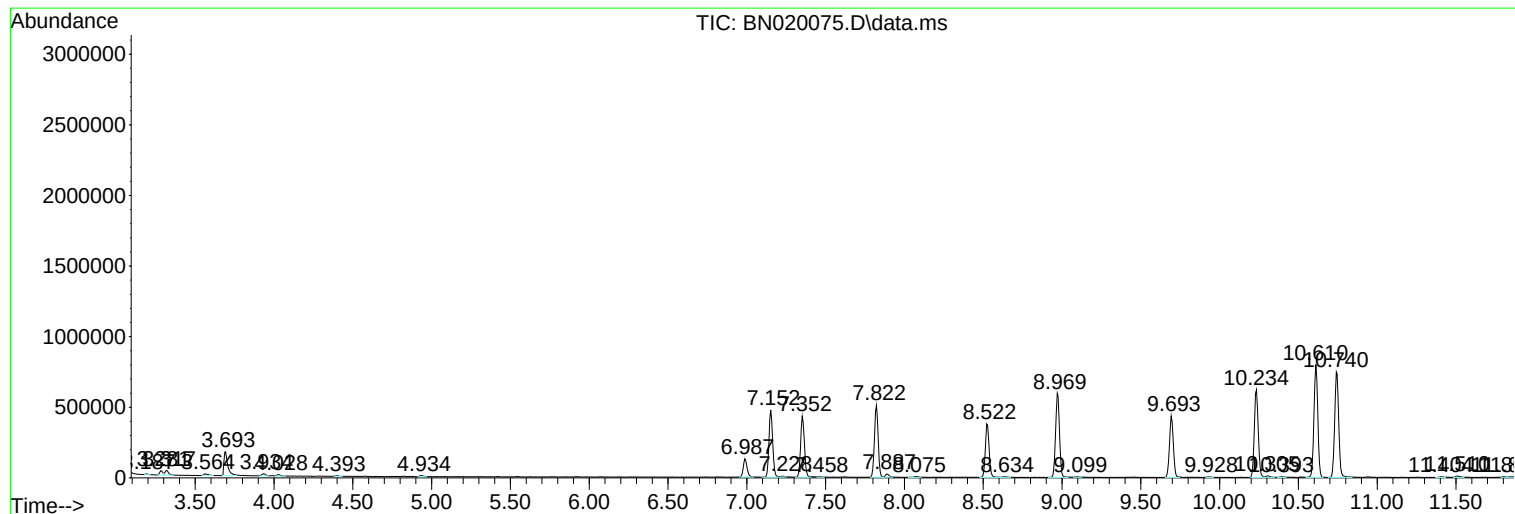

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020075.D
Acq On : 09 Jun 2022 11:44
Operator : CG/JU
Sample : N3212-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060922\
Data File : BN020075.D
Acq On : 09 Jun 2022 11:44
Operator : CG/JU
Sample : N3212-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F5A54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN060622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc