
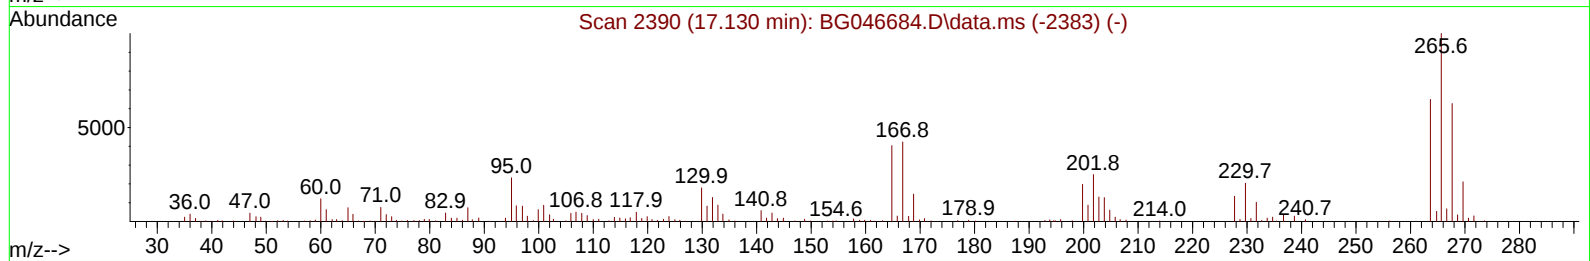
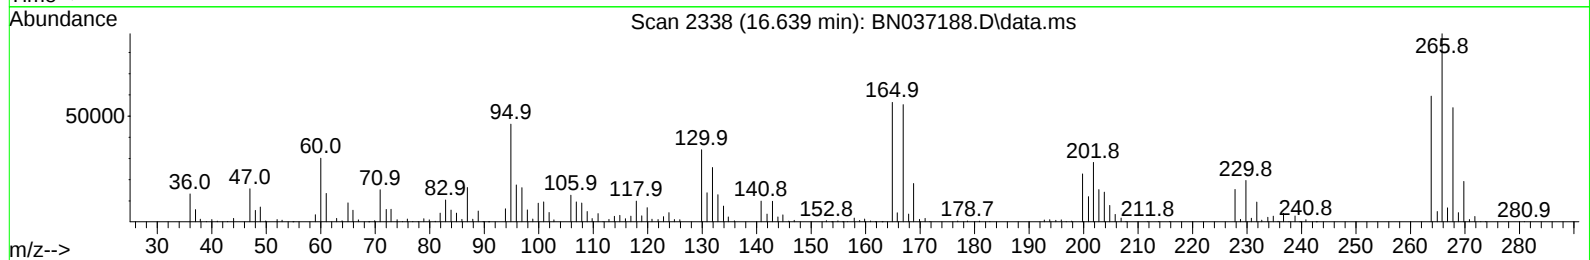


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037188.D
Acq On : 09 Jun 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:37:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

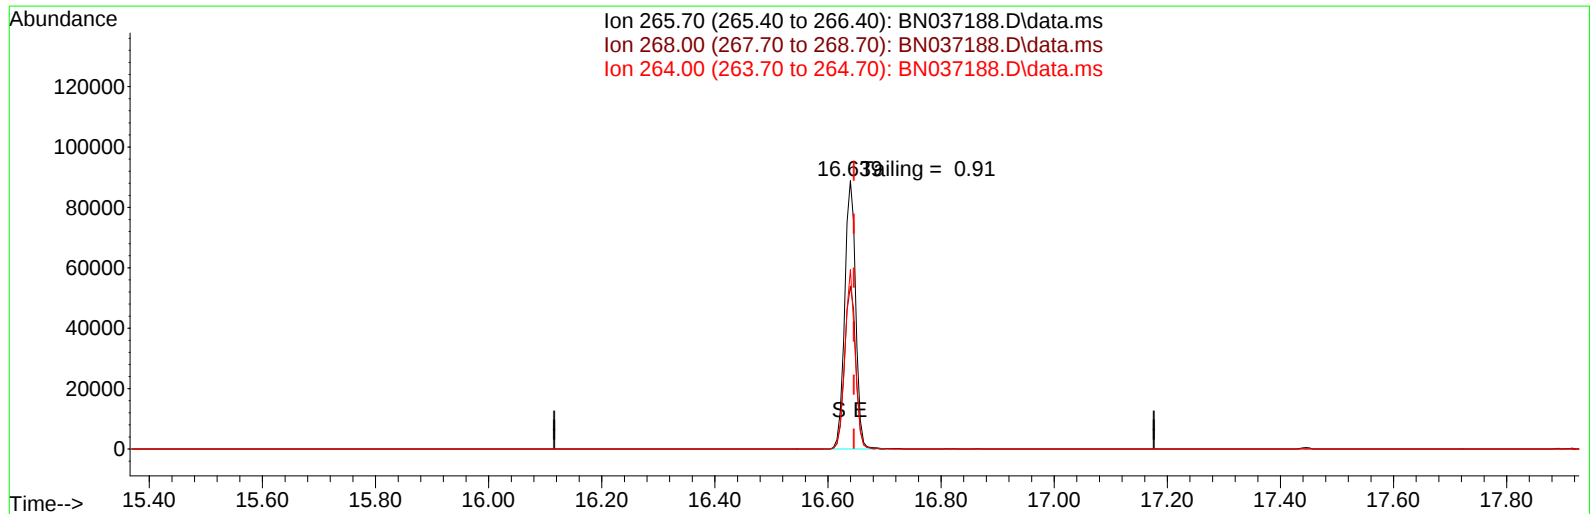

TIC: BN037188.D\data.ms

(70) Pentachlorophenol (C)




16.639min (-0.007) 18937.43 ng

response 119636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.72
264.00	61.60	66.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN060925\
Data File : BN037188.D
Acq On : 09 Jun 2025 10:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 14:33:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 04 02:36:29 2025
Response via : Initial Calibration

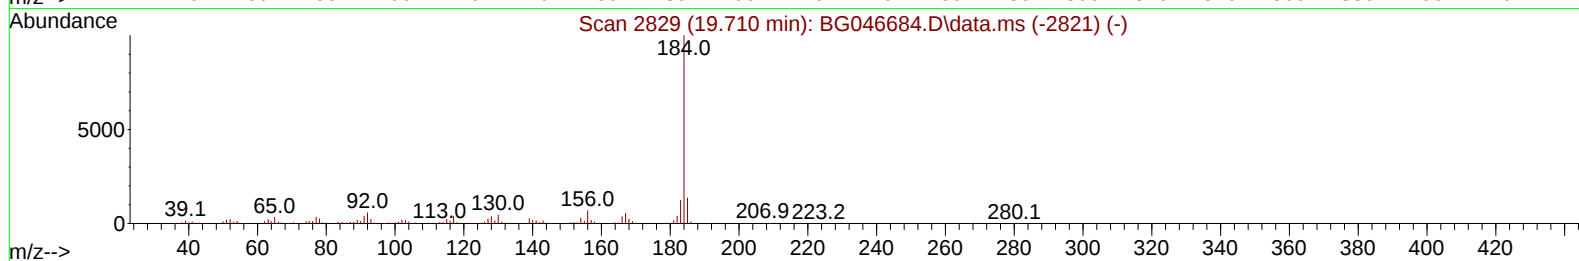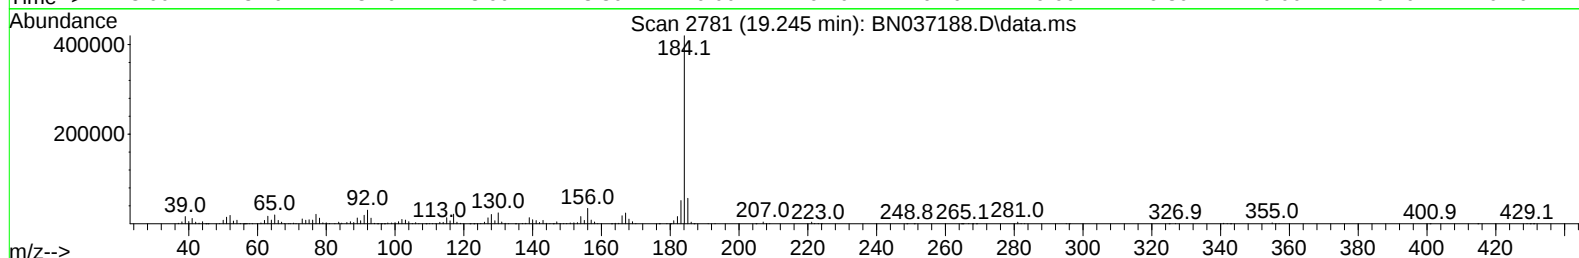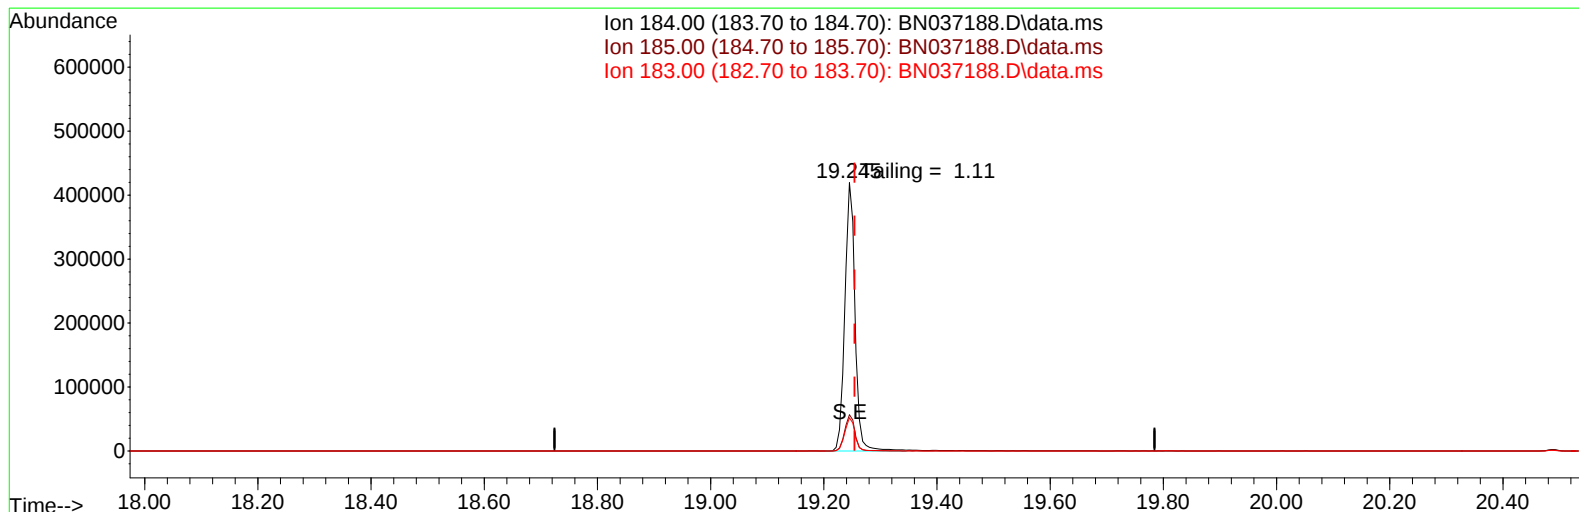

TIC: BN037188.D\data.ms

(77) Benzidine

19.245min (-0.009) 0.00 ng

response 528346

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.53
183.00	13.20	12.40
0.00	0.00	0.00