


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN061020\
 Data File : BN010820.D
 Acq On : 10 Jun 2020 16:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 10 15:14:26 2020

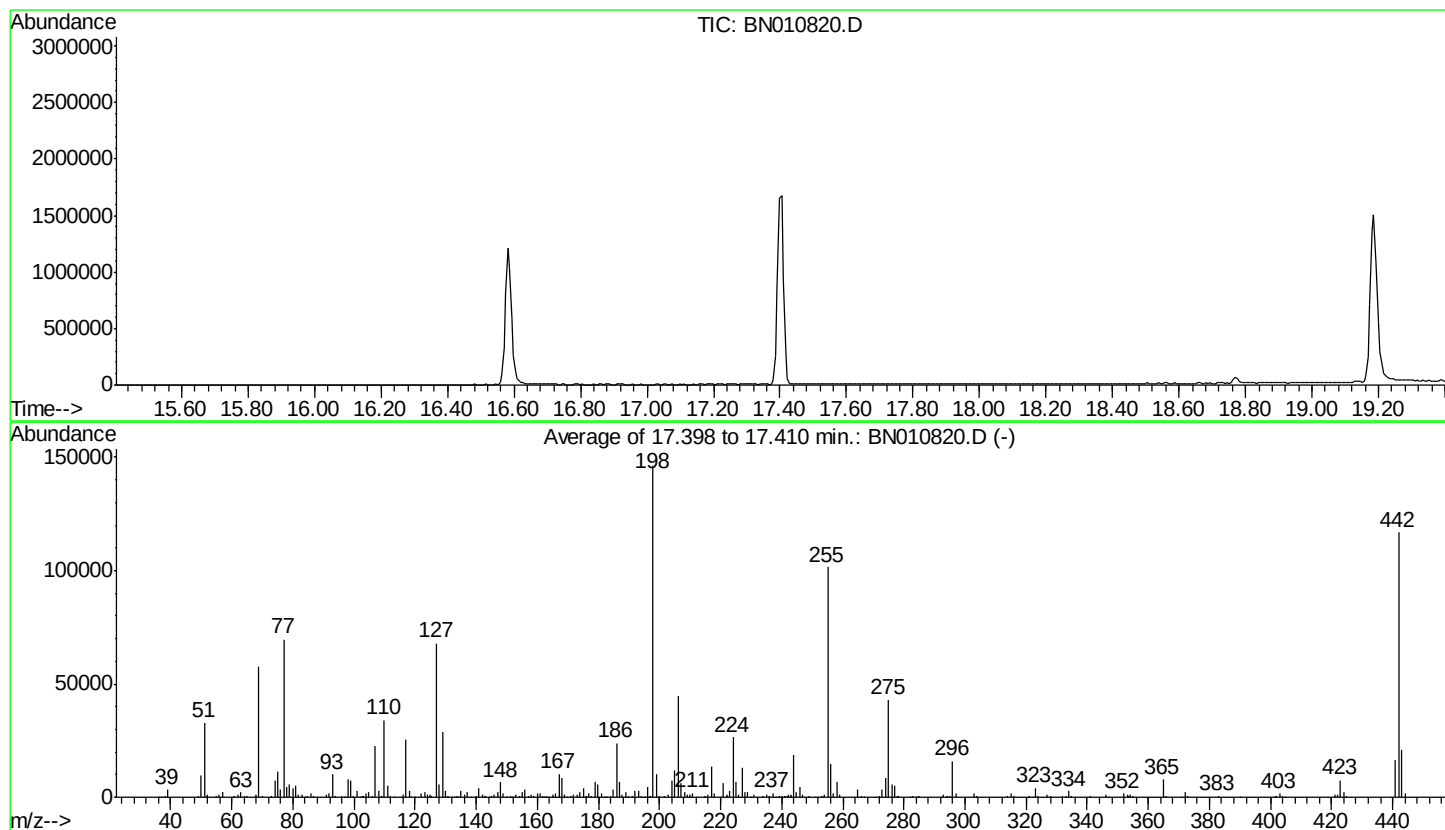

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	33058	PASS
68	69	0.00	2	1.8	1026	PASS
69	198	0.00	100	39.4	57594	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	46.5	68069	PASS
197	198	0.00	2	0.6	815	PASS
198	198	100	100	100.0	146328	PASS
199	198	5	9	7.1	10424	PASS
275	198	10	60	29.5	43133	PASS
365	198	1	100	5.4	7907	PASS
441	198	0.01	100	11.3	16548	PASS
442	198	50	100	79.9	116885	PASS
443	442	15	24	17.8	20860	PASS