

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014876.D
 Acq On : 10 Jun 2021 23:48
 Operator : CG/JU
 Sample : M2596-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5W4

Manual Integrations
 APPROVED

mohammad
 6/11/2021 2:13:42 PM

Quant Time: Jun 11 01:49:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 10 11:55:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	134971	20.00	ng/ul	0.00
20) Naphthalene-d8	10.475	136	546276	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.346	164	399209	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	890030	20.00	ng/ul	0.00
79) Chrysene-d12	21.298	240	1079643	20.00	ng/ul	0.00
88) Perylene-d12	23.557	264	1254104	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.211	96	12912m	3.90	ng/uL	0.00
4) Pyridine-d5	3.623	84	60985m	7.31	ng/ul	0.00
7) Phenol-d5	6.869	99	63960	4.84	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	148166	22.55	ng/ul	0.00
11) 2-Chlorophenol-d4	7.228	132	187573	22.92	ng/ul	0.00
15) 4-Methylphenol-d8	8.405	113	129509	12.60	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	123180	29.93	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	136362	30.83	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.110	165	249751	24.76	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	294202	24.74	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	972273	30.66	ng/ul	0.00
49) Acenaphthylene-d8	14.040	160	1118897	30.51	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	24034m	4.77	ng/ul	0.02
60) Fluorene-d10	15.345	176	833751	30.51	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	120175	24.69	ng/ul	0.00
73) Anthracene-d10	17.198	188	1414312	34.02	ng/ul	0.00
81) Pyrene-d10	19.504	212	1860130	36.54	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.416	264	2284674	34.20	ng/ul	0.00
Target Compounds						
59) Diethylphthalate	15.175	149	33766	1.12	ng/ul#	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014876.D
Acq On : 10 Jun 2021 23:48
Operator : CG/JU
Sample : M2596-18
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BG5W4

Manual Integrations
APPROVED

mohammad
6/11/2021 2:13:42 PM


Quant Time: Jun 11 01:49:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 10 11:55:23 2021
Response via : Initial Calibration

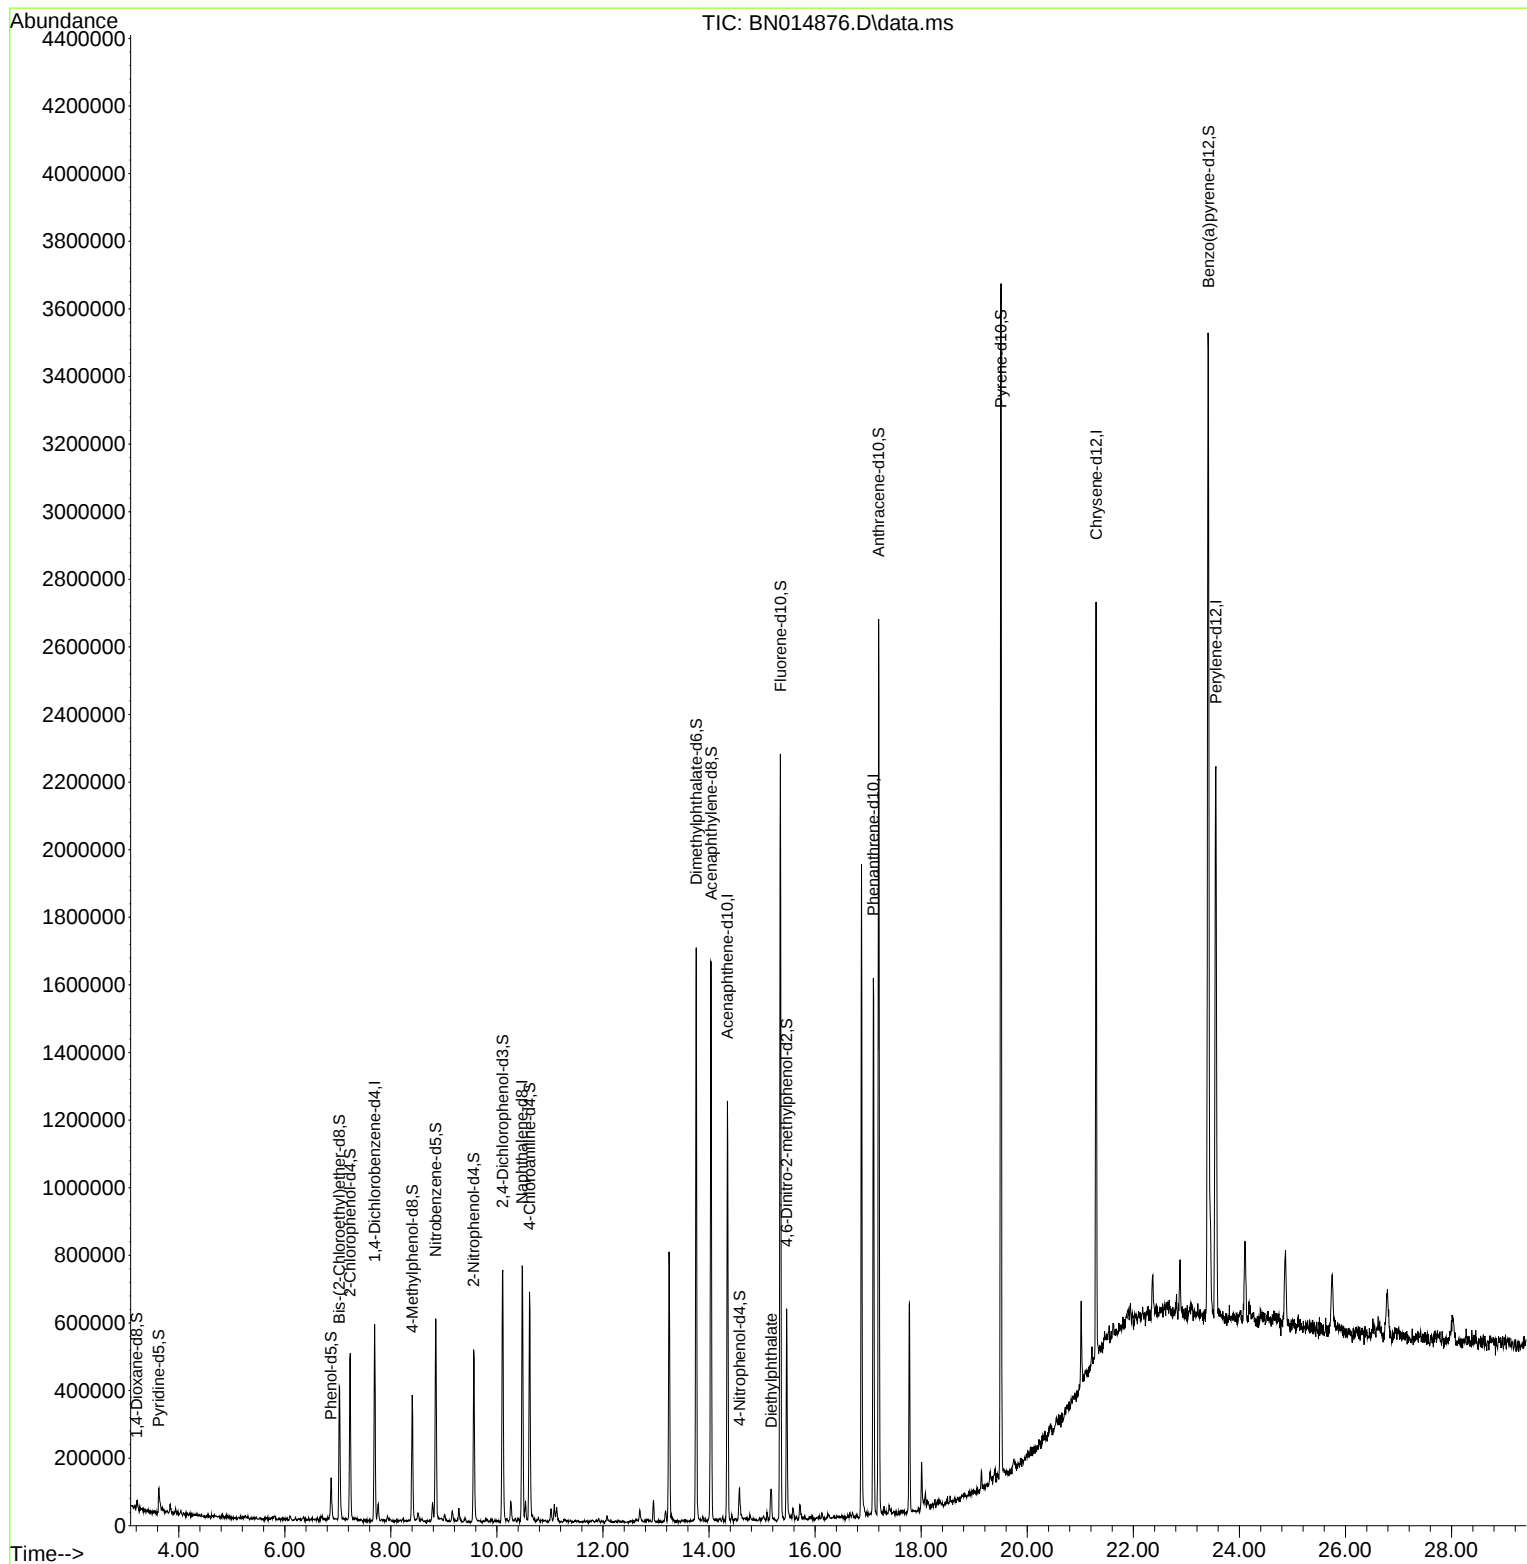

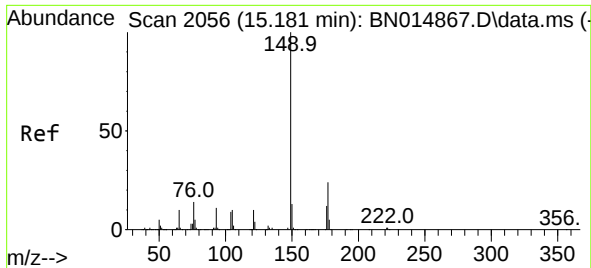

#59
 Diethylphthalate
 Concen: 1.12 ng/ul
 RT: 15.175 min Scan# 2055
 Delta R.T. -0.006 min
 Lab File: BN014876.D
 Acq: 10 Jun 2021 23:48

Instrument :
 BNA_N
 ClientSampleId :
 BG5W4

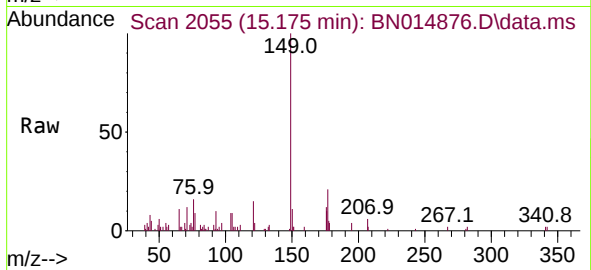

Tgt Ion	Ratio	Lower	Upper
149	100		
177	26.1	20.6	31.0
150	10.8	11.4	17.2#

Manual Integrations
 APPROVED

mohammad
 6/11/2021 2:13:42 PM

