

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
 Data File : BN014878.D
 Acq On : 11 Jun 2021 00:59
 Operator : CG/JU
 Sample : M2618-04DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

Manual Integrations
 APPROVED

mohammad
 6/11/2021 2:13:48 PM

Quant Time: Jun 11 01:50:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 10 11:55:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	164379	20.00	ng/ul	0.00
20) Naphthalene-d8	10.481	136	653772	20.00	ng/ul	# 0.00
38) Acenaphthene-d10	14.346	164	476156	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	1091935	20.00	ng/ul	# 0.00
79) Chrysene-d12	21.298	240	1293711	20.00	ng/ul	0.00
88) Perylene-d12	23.557	264	1383224	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.223	96	6635m	1.64	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	
7) Phenol-d5	6.875	99	74624	4.64	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.028	67	37175m	4.64	ng/ul	0.00
11) 2-Chlorophenol-d4	7.228	132	58399	5.86	ng/ul	0.00
15) 4-Methylphenol-d8	8.411	113	61677m	4.93	ng/ul	0.01
21) Nitrobenzene-d5	8.852	128	29481	5.99	ng/ul	0.00
24) 2-Nitrophenol-d4	9.569	143	32252m	6.09	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.105	165	64005	5.30	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	65776m	4.62	ng/ul	0.01
46) Dimethylphthalate-d6	13.757	166	214179	5.66	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	245417	5.61	ng/ul	0.00
54) 4-Nitrophenol-d4	14.575	143	21063m	3.50	ng/ul	0.02
60) Fluorene-d10	15.345	176	188250	5.78	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	17372m	2.91	ng/ul	0.00
73) Anthracene-d10	17.198	188	307467	6.03	ng/ul	0.00
81) Pyrene-d10	19.498	212	399141	6.54	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	507366	6.89	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.192	149	2045532m	57.10	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN061021\
Data File : BN014878.D
Acq On : 11 Jun 2021 00:59
Operator : CG/JU
Sample : M2618-04DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BG5R7DL

Manual Integrations
APPROVED

mohammad
6/11/2021 2:13:48 PM


Quant Time: Jun 11 01:50:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN052521.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 10 11:55:23 2021
Response via : Initial Calibration

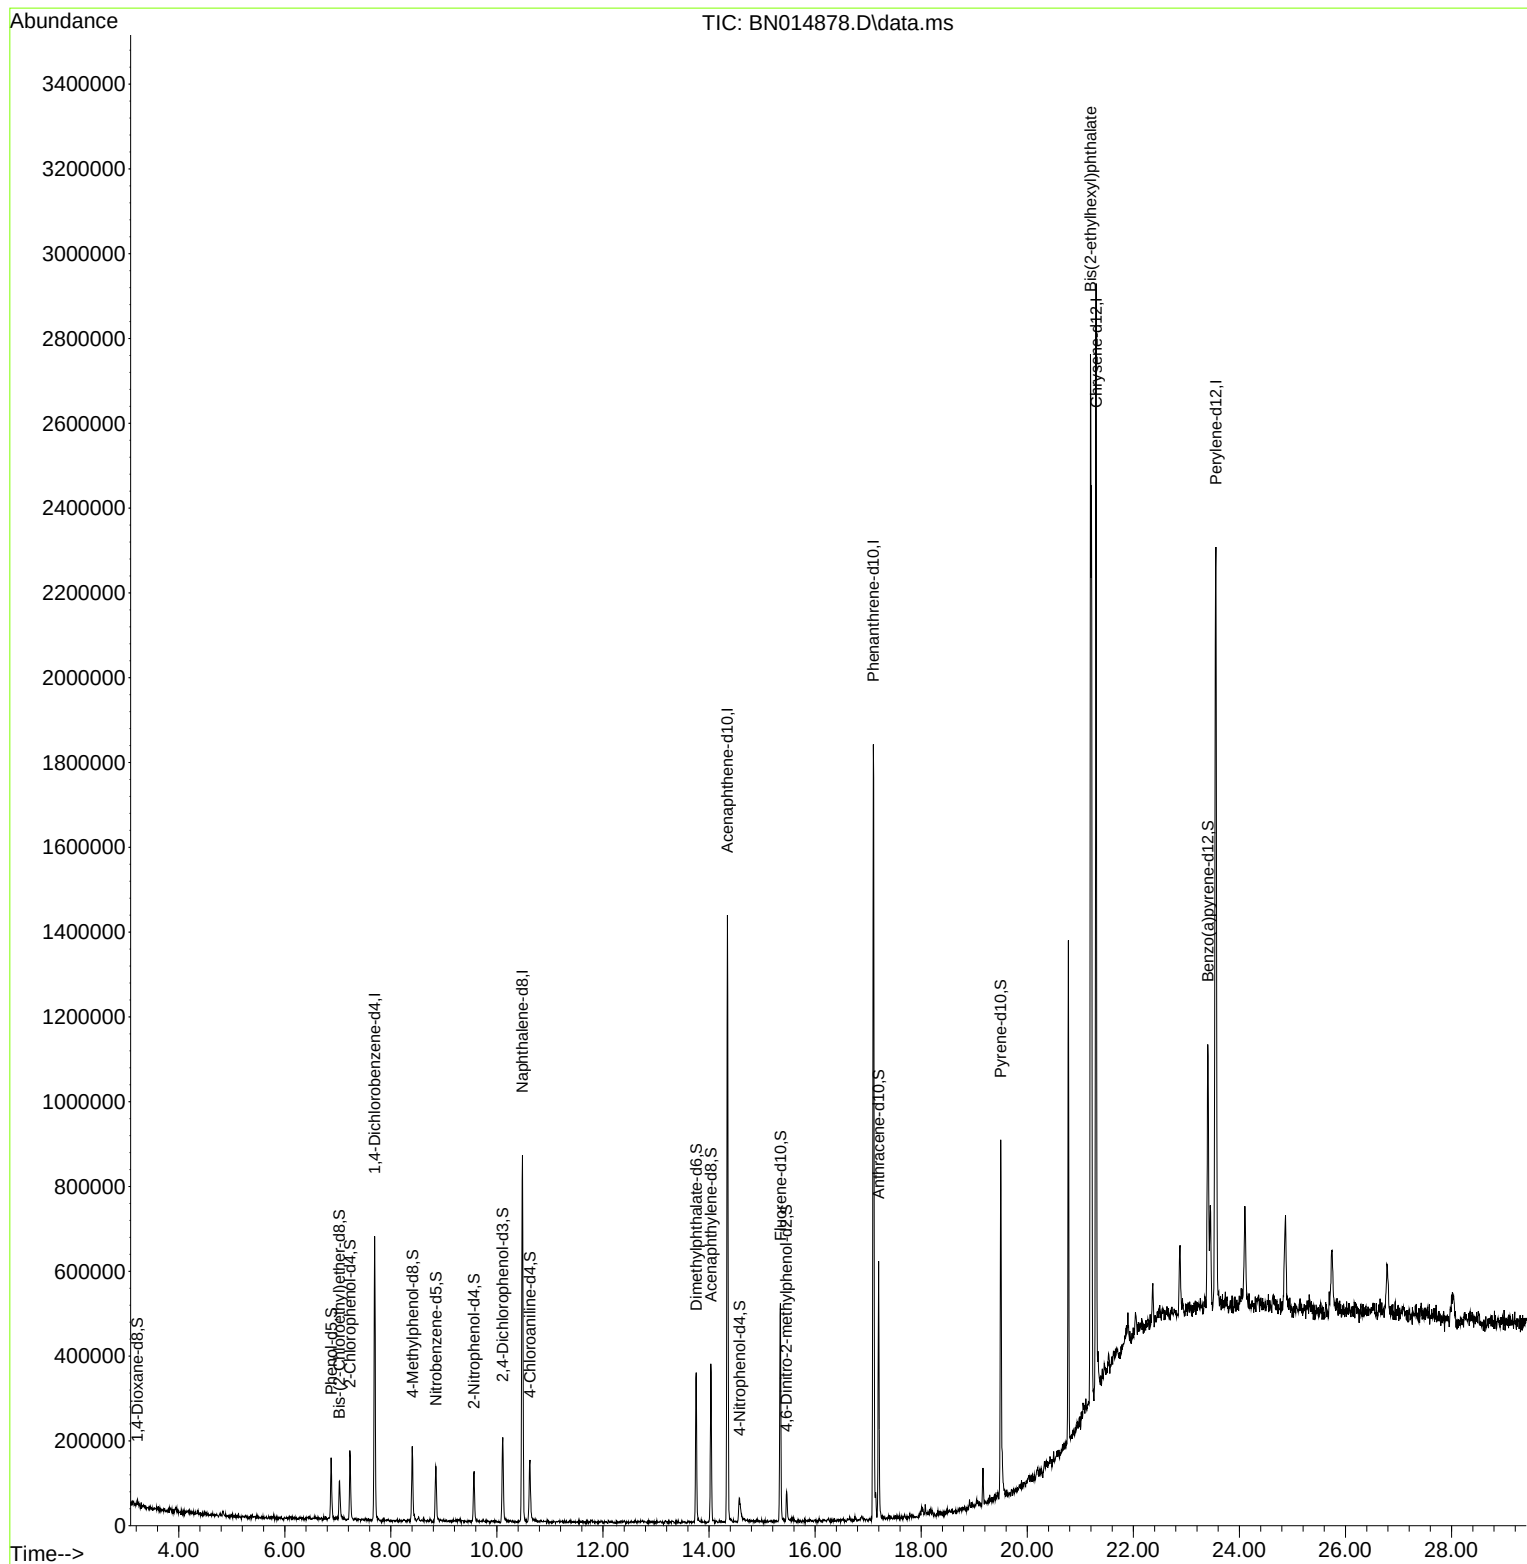

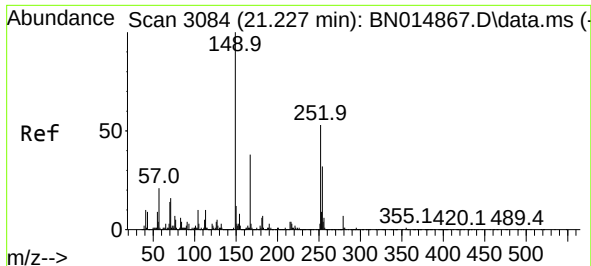

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 57.10 ng/ul m
 RT: 21.192 min Scan# 3078
 Delta R.T. -0.035 min
 Lab File: BN014878.D
 Acq: 11 Jun 2021 00:59

Instrument :
 BNA_N
 ClientSampleId :
 BG5R7DL

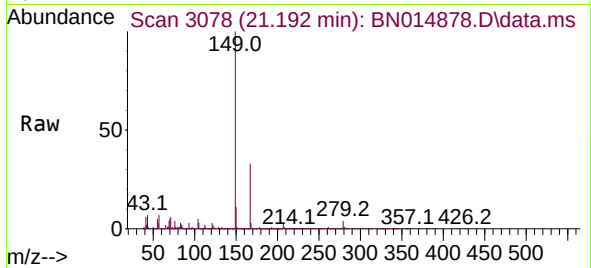

Tgt Ion:149 Resp: 2045532
 Ion Ratio Lower Upper
 149 100
 167 33.2 30.7 46.1
 279 3.8 5.1 7.7#

Manual Integrations
 APPROVED

mohammad
 6/11/2021 2:13:48 PM

